

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
 Data File : BM007390.D
 Acq On : 03 Sep 2016 04:46
 Operator : UM/SJ
 Sample : H4655-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0024

Quant Time: Sep 03 05:16:50 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 03 01:45:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	173484	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	816020	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	572026	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1530551	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	2196383	20.00	ng/ul	0.00
83) Perylene-d12	23.61	264	2279625	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	13046	3.84	ng/uL	0.00
5) Phenol-d5	6.96	99	283728	17.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	169943	19.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	228317	18.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	244634	17.12	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	121748	20.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	140879	20.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	259240	18.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	311596	17.93	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1047125	21.22	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1186149	20.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	168912	18.13	ng/ul	0.00
57) Fluorene-d10	15.42	176	908733	21.29	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	165336	17.18	ng/ul	0.00
70) Anthracene-d10	17.27	188	1577458	22.06	ng/ul	0.00
76) Pyrene-d10	19.56	212	2102789	22.90	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	2422873	23.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	370833	7.54	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
Data File : BM007390.D
Acq On : 03 Sep 2016 04:46
Operator : UM/SJ
Sample : H4655-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0024

Quant Time: Sep 03 05:16:50 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 03 01:45:38 2016
Response via : Initial Calibration

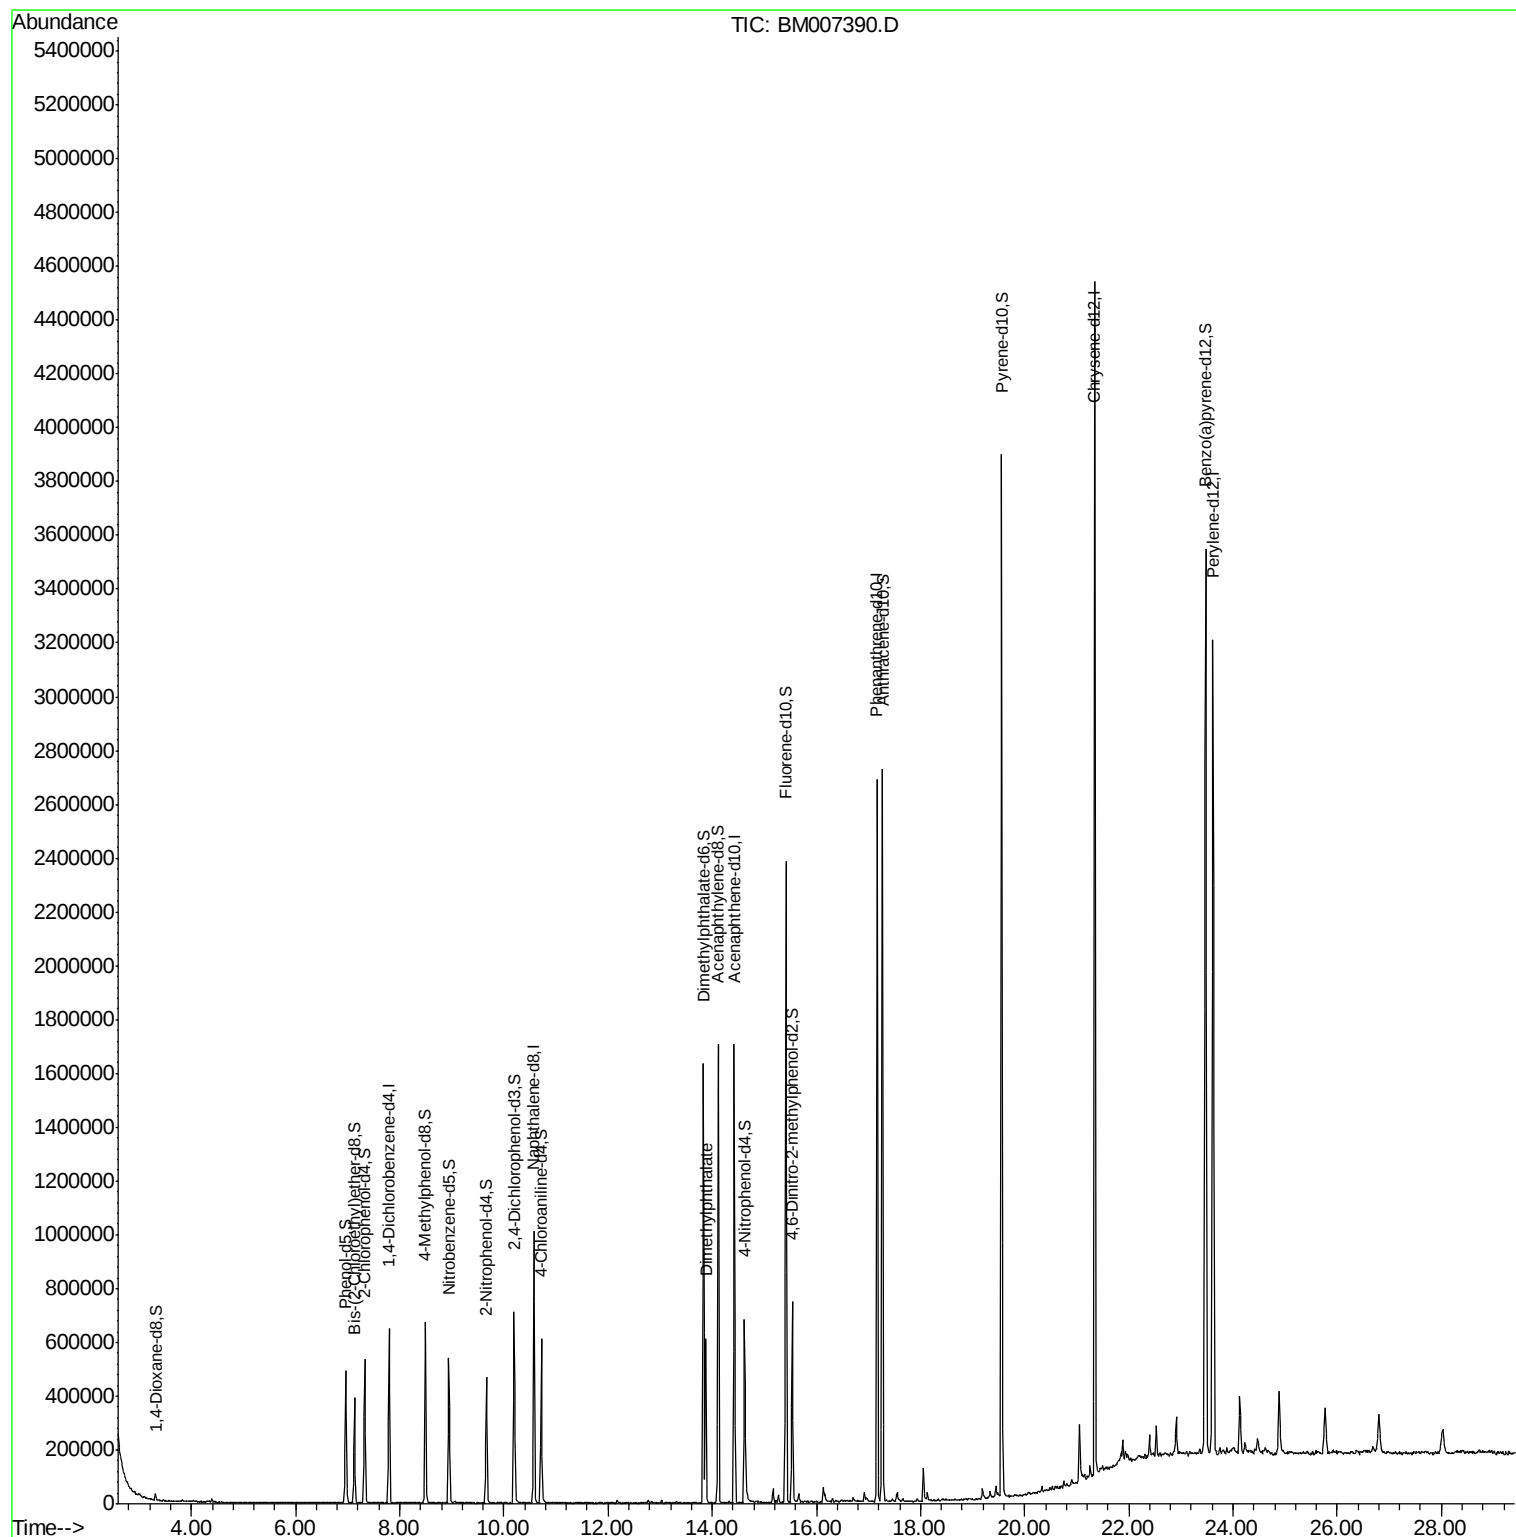

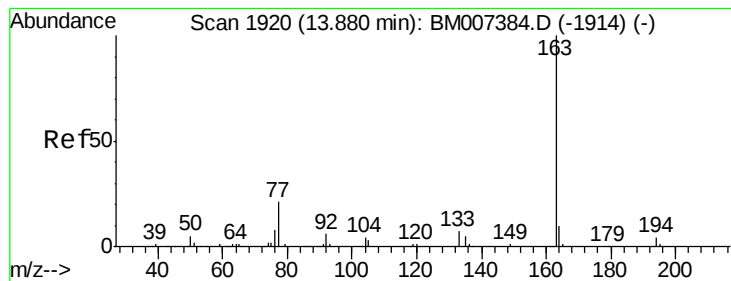

#44

Dimethylphthalate

Concen: 7.54 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. 0.00 min

Lab File: BM007390.D


Acq: 03 Sep 2016 04:46

Instrument :

BNA_M

ClientSampleId :

C0024

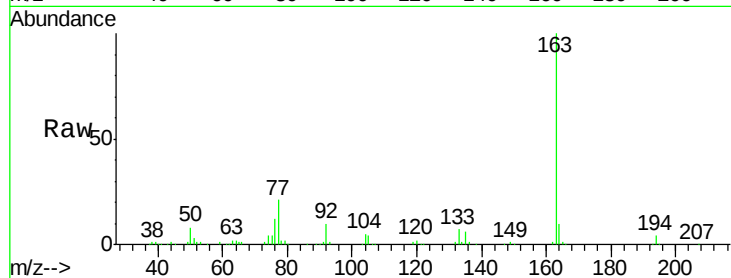


Tgt Ion:163 Resp: 370833

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 9.7 7.8 11.8

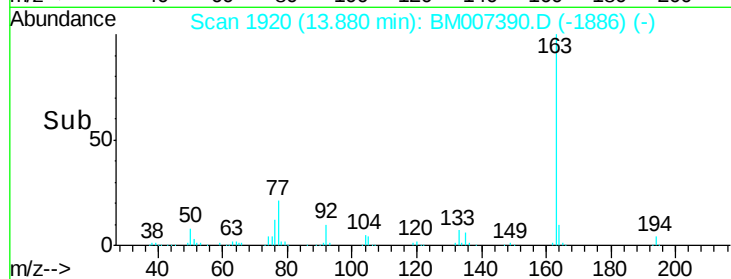

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

