

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
 Data File : BM007402.D
 Acq On : 03 Sep 2016 11:58
 Operator : UM/SJ
 Sample : H4639-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD389

Manual Integrations
 APPROVED

sohil
 9/6/2016 1:16:40 PM

Quant Time: Sep 05 03:49:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 05 01:45:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	228891	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1042222	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	693221	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1768867	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2312033	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	2179042	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	15044	3.36	ng/uL	0.00
5) Phenol-d5	6.96	99	371361	17.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	204677	18.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	291543	18.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	306684	16.26	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	155730	20.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	183449	20.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	339219	19.07	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	172349	7.77	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1193538	19.96	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1437652	20.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	173816	15.40	ng/ul	0.00
57) Fluorene-d10	15.42	176	1070887	20.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	190172	17.10	ng/ul	0.00
70) Anthracene-d10	17.27	188	1711880	20.72	ng/ul	0.00
76) Pyrene-d10	19.56	212	2301312	23.80	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	2219174	22.11	ng/ul	0.00

Target Compounds

					Qvalue
28) Naphthalene	10.63	128	99890	1.93 ng/ul	100
34) 2-Methylnaphthalene	12.24	142	80991	1.91 ng/ul	91
44) Dimethylphthalate	13.88	163	591782	9.93 ng/ul	99
53) Dibenzofuran	14.82	168	110139	1.59 ng/ul	94
69) Phenanthrene	17.21	178	463477	4.88 ng/ul	99
74) Fluoranthene	19.23	202	1160596	9.74 ng/ul	99
77) Pyrene	19.59	202	795892	6.42 ng/ul	99
80) Benzo(a)anthracene	21.33	228	499333	3.66 ng/ul	97
82) Chrysene	21.39	228	1089752	8.83 ng/ul	97
85) Benzo(b)fluoranthene	22.94	252	1126415	8.74 ng/ul	98
86) Benzo(k)fluoranthene	22.98	252	312502m	2.62 ng/ul	
88) Benzo(a)pyrene	23.52	252	270987	2.20 ng/ul	98
89) Indeno(1,2,3-cd)pyrene	25.91	276	219149	1.45 ng/ul	99
91) Benzo(g,h,i)perylene	26.61	276	182090	1.42 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090316\
Data File : BM007402.D
Acq On : 03 Sep 2016 11:58
Operator : UM/SJ
Sample : H4639-12
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BD389

Manual Integrations
APPROVED

sohil
9/6/2016 1:16:40 PM

Quant Time: Sep 05 03:49:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 05 01:45:04 2016
Response via : Initial Calibration

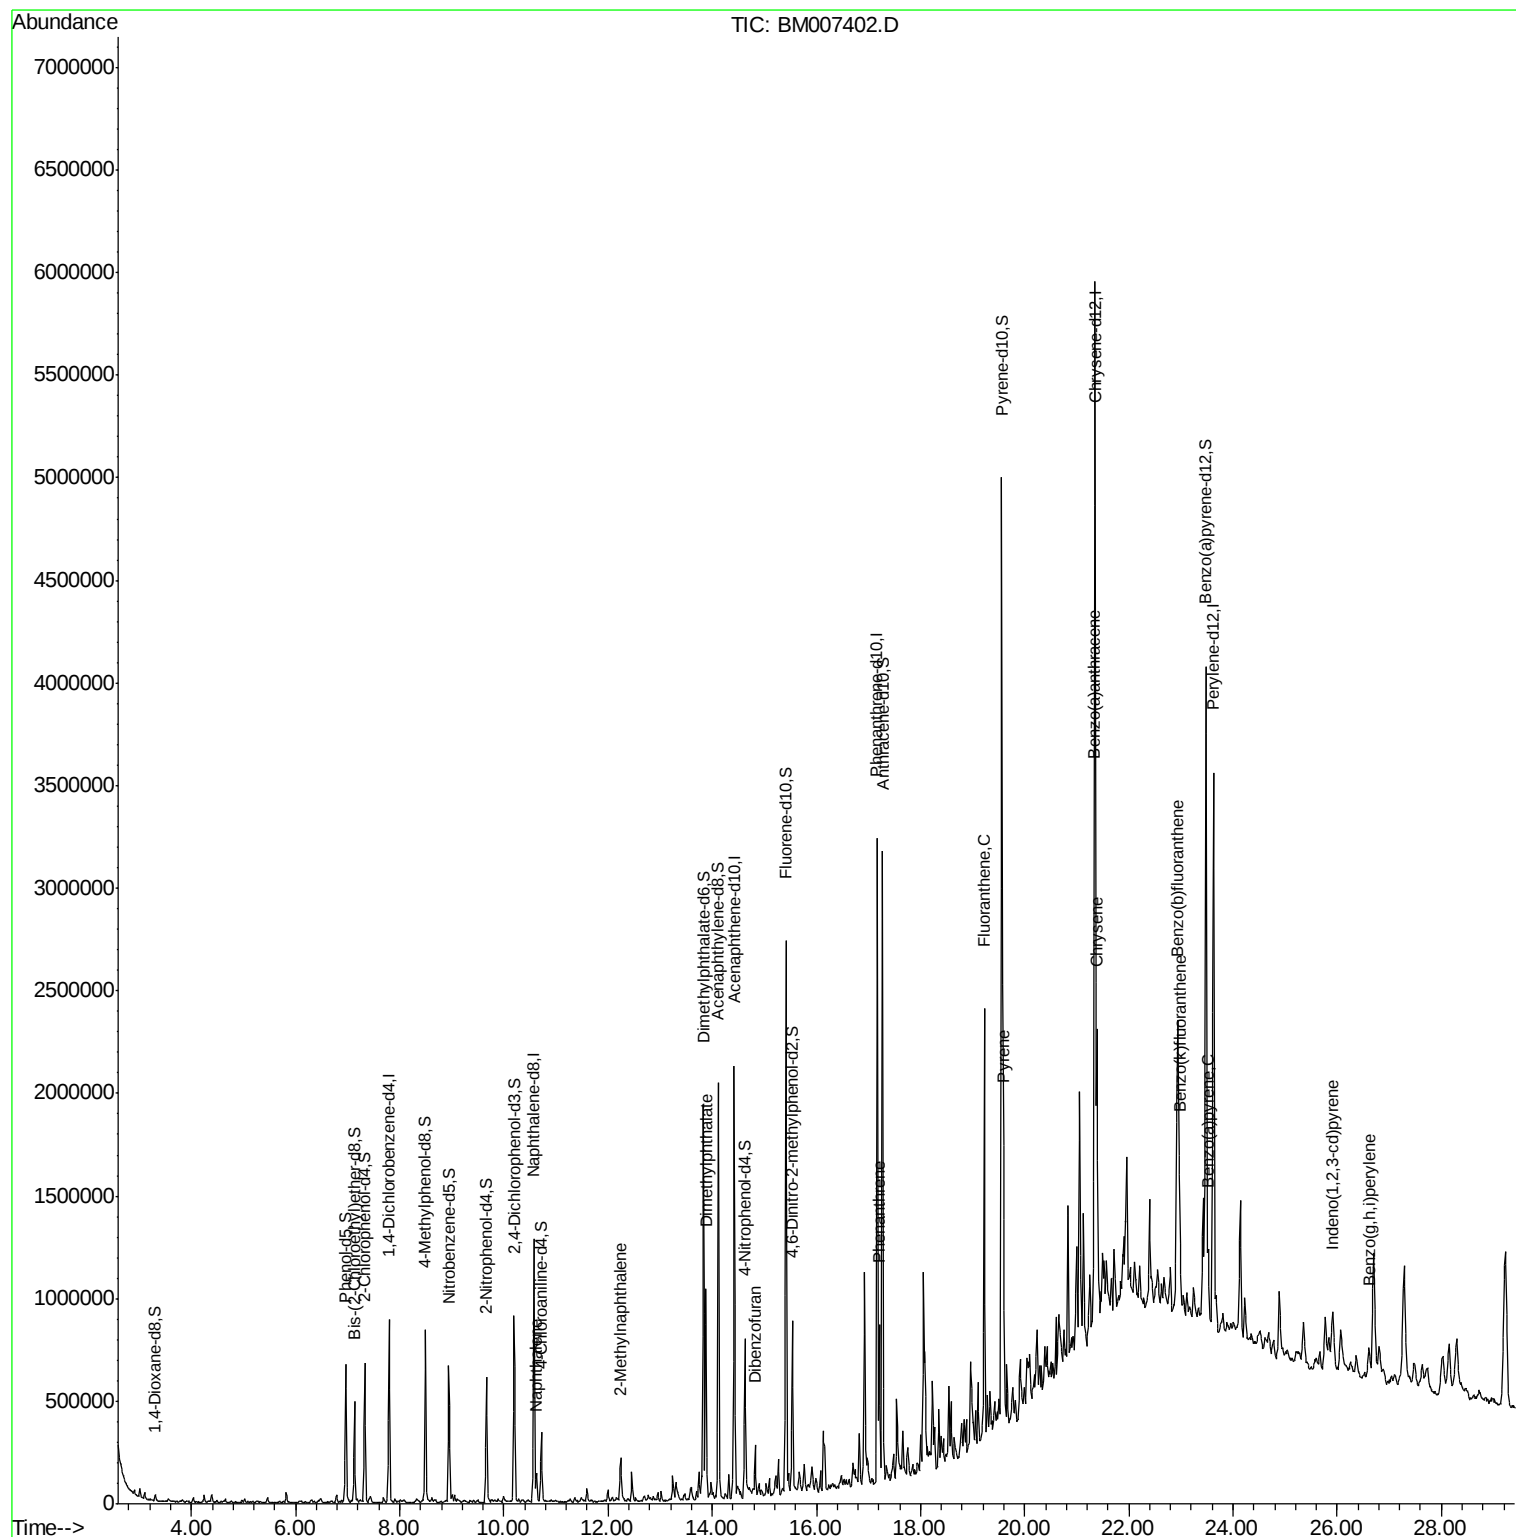

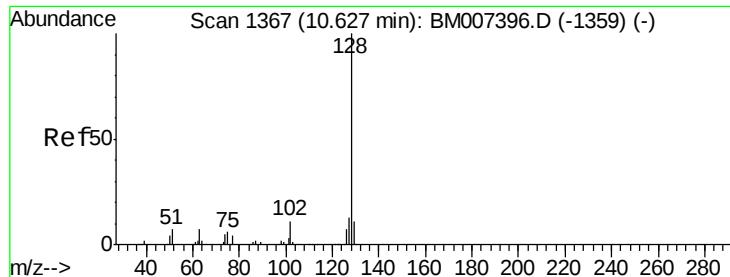





#28
Naphthalene
Concen: 1.93 ng/ul
RT: 10.63 min Scan# 1367
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Instrument :
BNA_M
ClientSampleId :
BD389

Tgt Ion	Ratio	Resp Lower	Resp Upper
128	100		
129	10.8	8.6	12.8
127	13.0	10.6	15.8




Manual Integrations
APPROVED


sohil
9/6/2016 1:16:40 PM

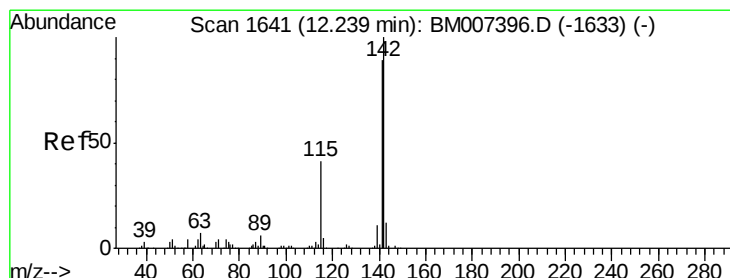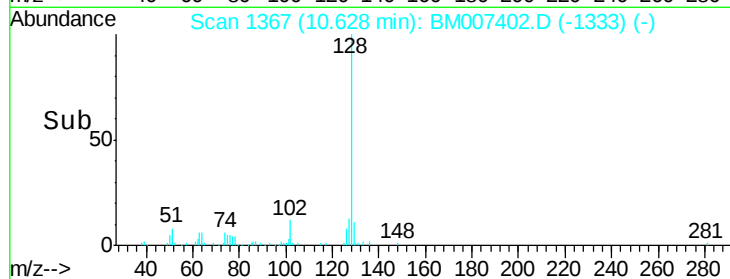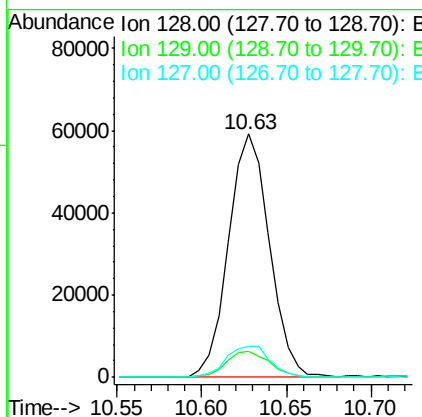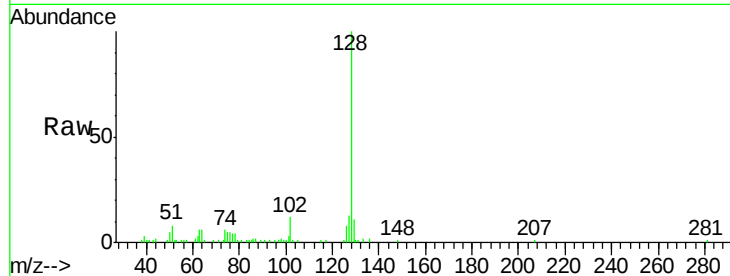

#34
2-Methylnaphthalene
Concen: 1.91 ng/ul
RT: 12.24 min Scan# 1641
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Tgt Ion	Ratio	Resp Lower	Resp Upper
142	100		
141	97.3	71.3	106.9

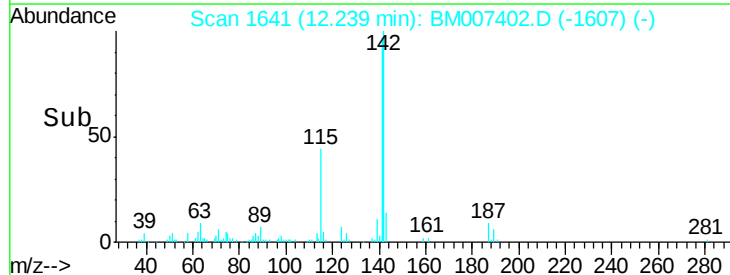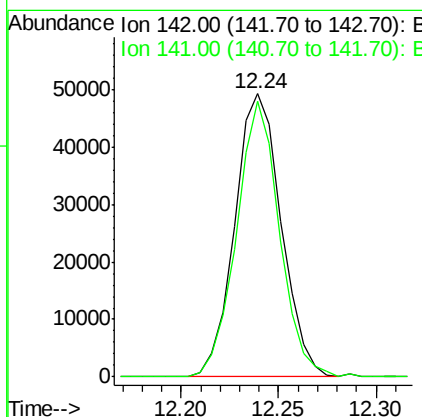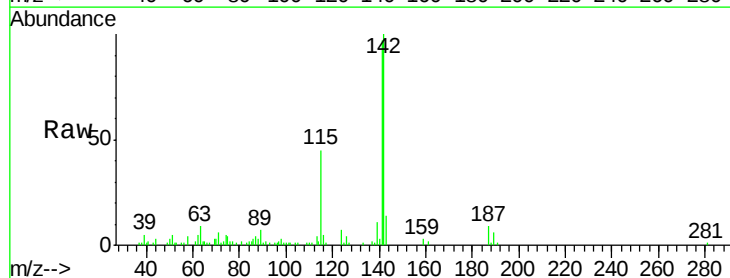

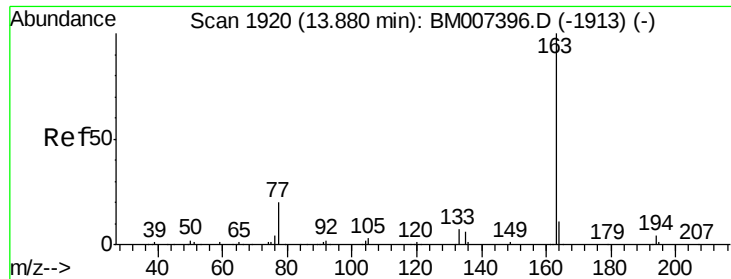





#44
Dimethylphthalate
Concen: 9.93 ng/ul
RT: 13.88 min Scan# 1920
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Instrument :
BNA_M
ClientSampleId :
BD389

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.2
164	10.1	7.8	11.8




Manual Integrations
APPROVED


sohil
9/6/2016 1:16:40 PM

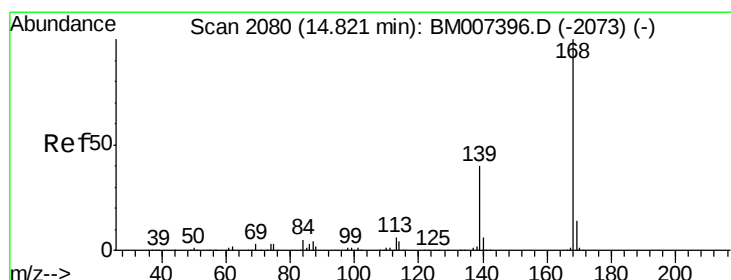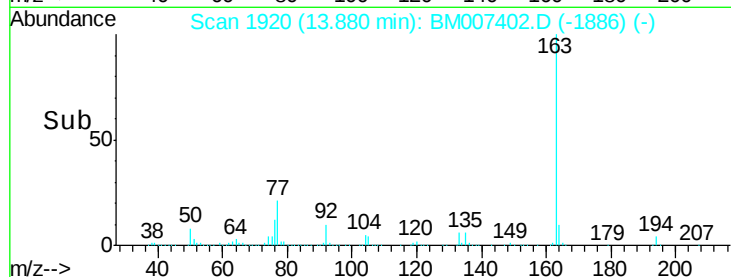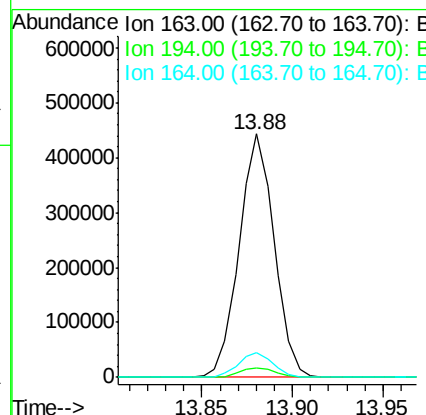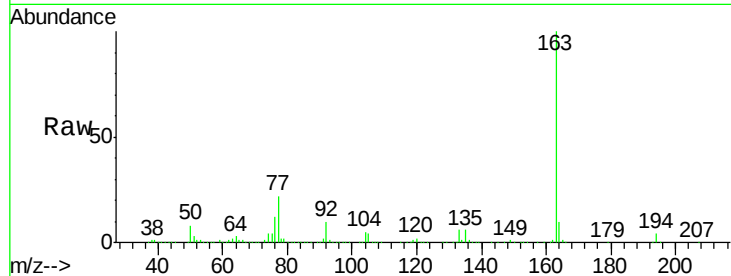

#53
Dibenzofuran
Concen: 1.59 ng/ul
RT: 14.82 min Scan# 2080
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Tgt Ion	Ratio	Lower	Upper
168	100		
139	41.2	30.1	45.1

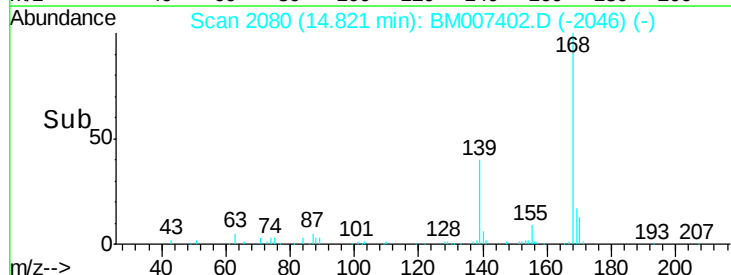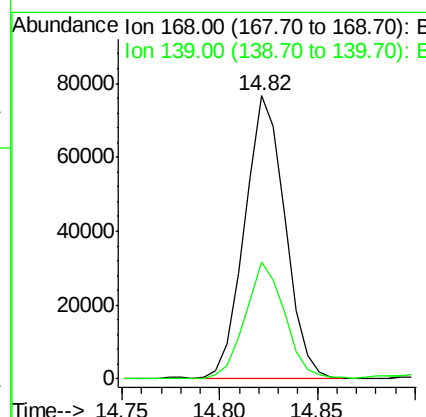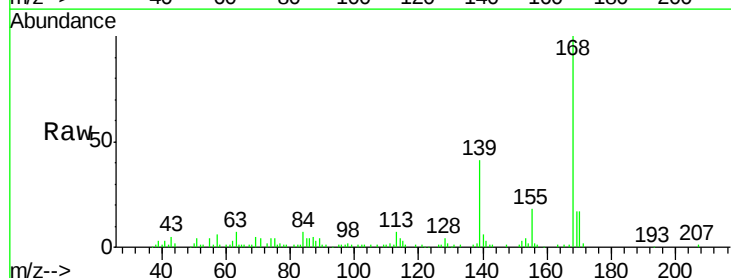

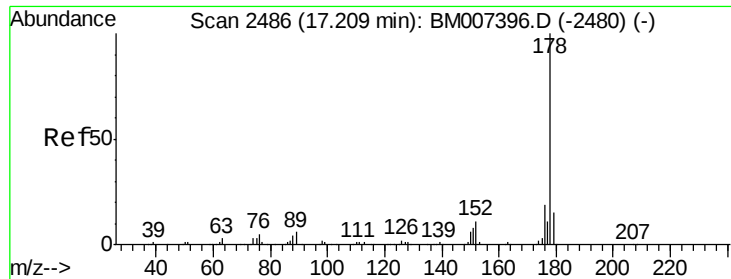





#69
Phenanthrene
Concen: 4.88 ng/ul
RT: 17.21 min Scan# 2486
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Instrument :
BNA_M
ClientSampleId :
BD389

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.8	12.2	18.2
176	18.9	15.1	22.7




Manual Integrations
APPROVED


sohil
9/6/2016 1:16:40 PM

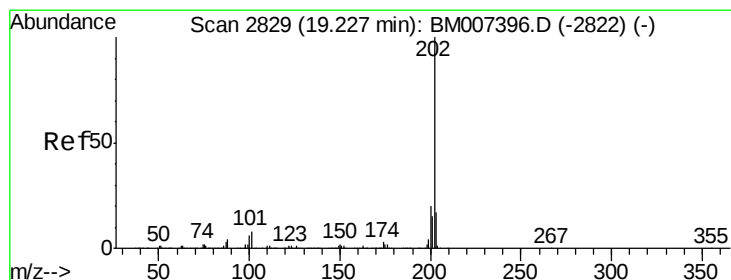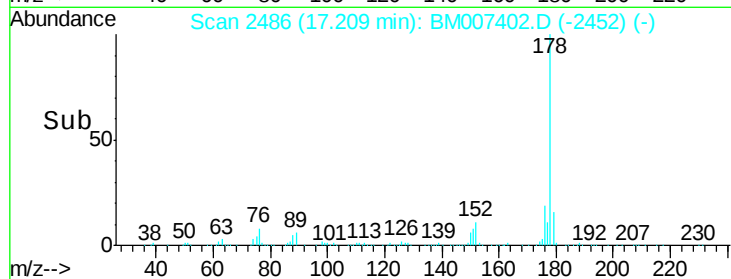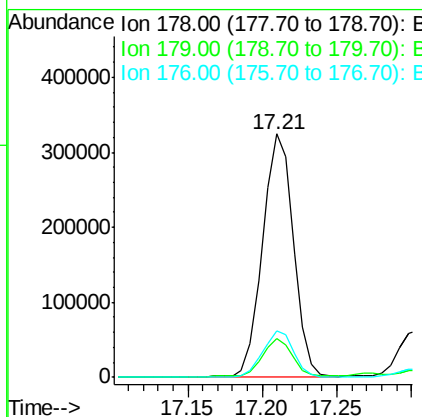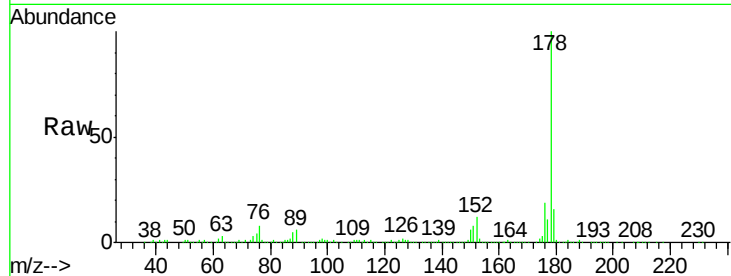

#74
Fluoranthene
Concen: 9.74 ng/ul
RT: 19.23 min Scan# 2829
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.2	6.9	10.3
100	6.2	5.4	8.0

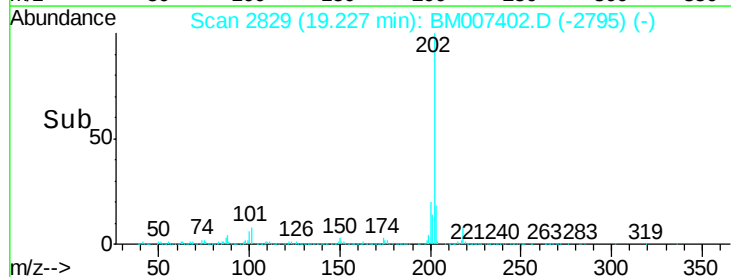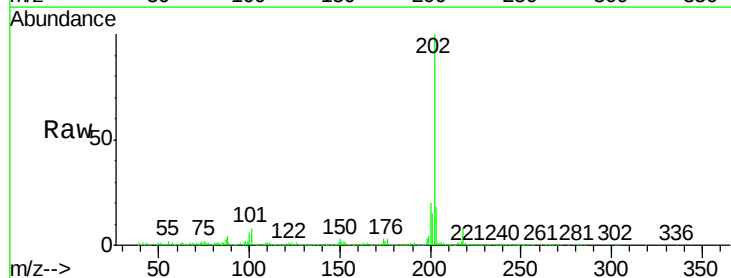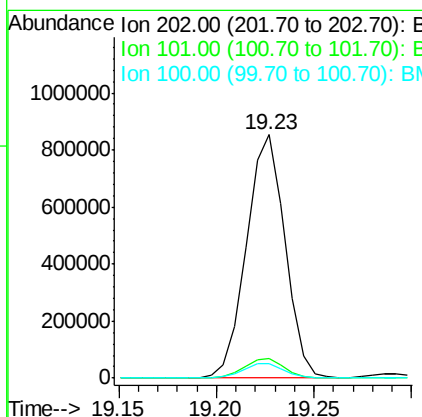

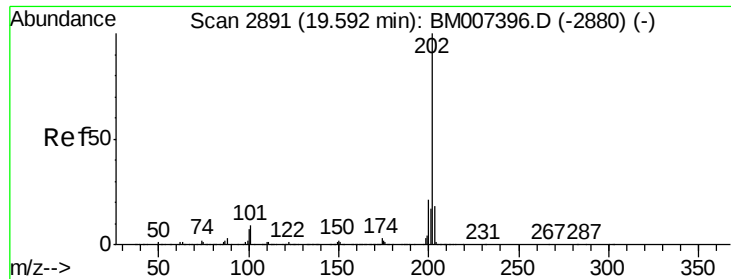

#77

Pyrene

Concen: 6.42 ng/ul

RT: 19.59 min Scan# 2891

Delta R.T. 0.00 min

Lab File: BM007402.D

Acq: 03 Sep 2016 11:58

Instrument :

BNA_M





ClientSampleId :

BD389

Tgt Ion:	202	Resp:	795892
Ion Ratio	Lower	Upper	
202	100		
101	10.2	8.4	12.6
100	7.9	6.9	10.3

Manual Integrations
APPROVED

sohil
9/6/2016 1:16:40 PM

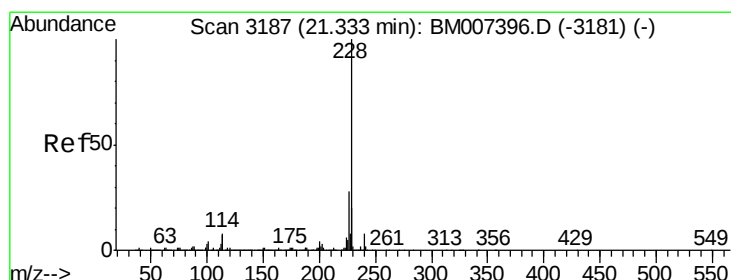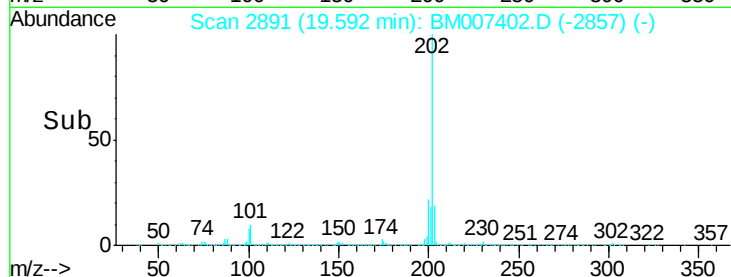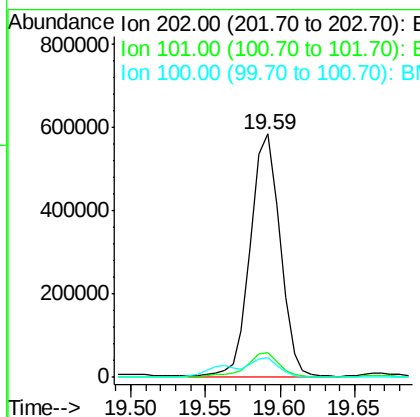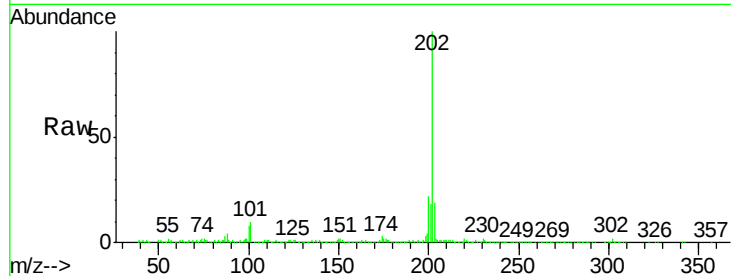

#80

Benzo(a)anthracene

Concen: 3.66 ng/ul




RT: 21.33 min Scan# 3187


Delta R.T. 0.00 min

Lab File: BM007402.D

Acq: 03 Sep 2016 11:58

Tgt Ion:	228	Resp:	499333
Ion Ratio	Lower	Upper	
228	100		
229	22.2	15.6	23.4
226	28.2	21.8	32.8

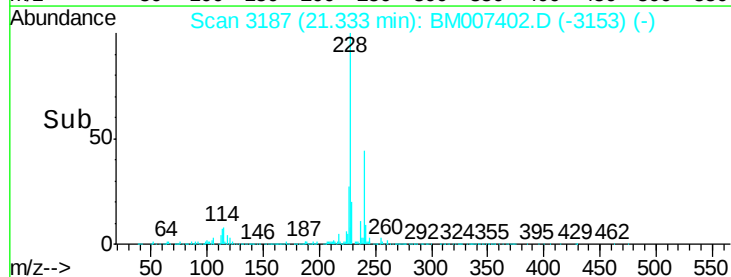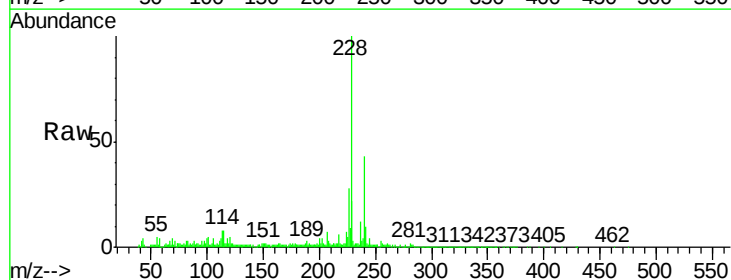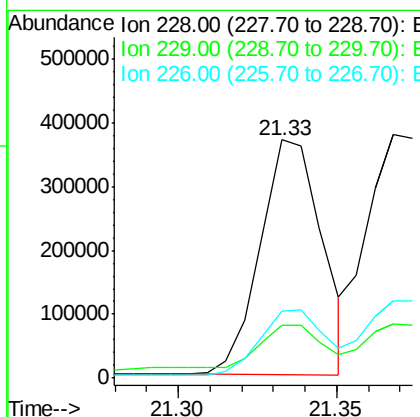

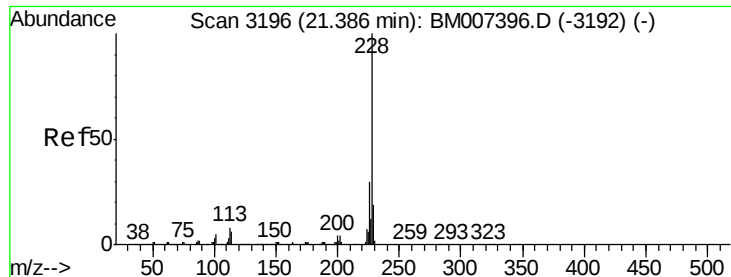

#82

Chrysene

Concen: 8.83 ng/ul

RT: 21.39 min Scan# 3196

Delta R.T. 0.00 min

Lab File: BM007402.D

Acq: 03 Sep 2016 11:58

Instrument :

BNA_M

ClientSampleId :

BD389

Tgt Ion:228 Resp: 1089752

Ion Ratio Lower Upper

228 100


226 30.1 23.4 35.2

229 21.4 15.5 23.3

Manual Integrations
APPROVED

sohil




9/6/2016 1:16:40 PM

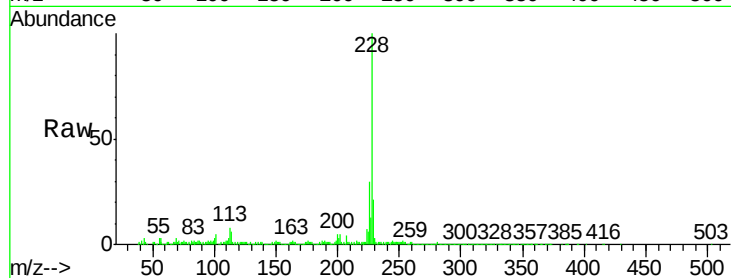

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

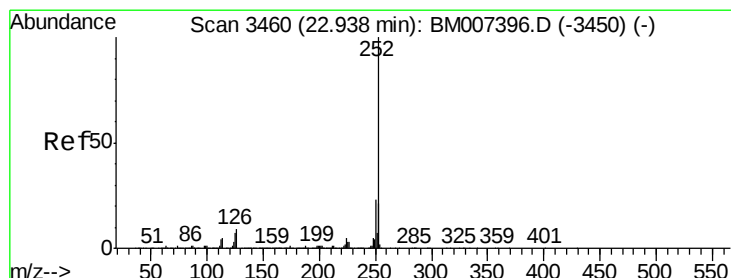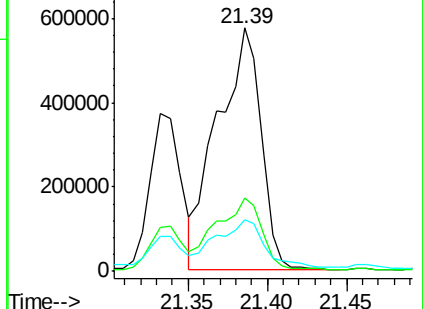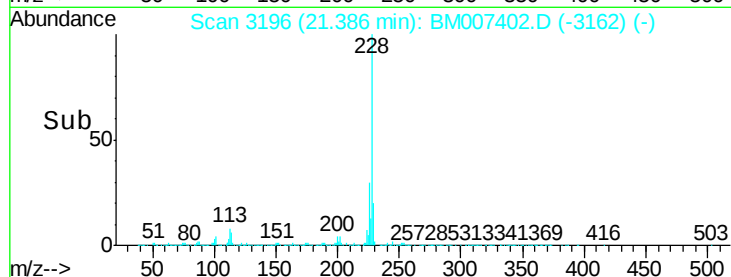

#85

Benzo(b)fluoranthene

Concen: 8.74 ng/ul

RT: 22.94 min Scan# 3460

Delta R.T. 0.00 min

Lab File: BM007402.D

Acq: 03 Sep 2016 11:58


Tgt Ion:252 Resp: 1126415

Ion Ratio Lower Upper

252 100

253 22.6 17.1 25.7



125 7.8 5.8 8.8

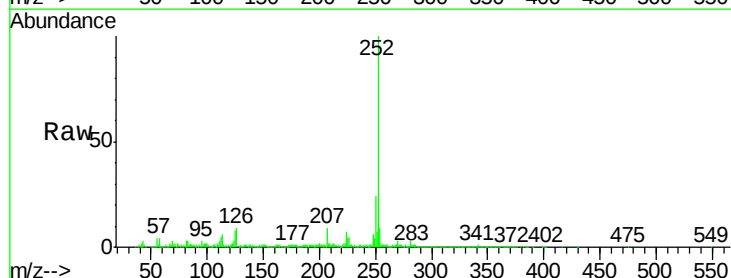


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

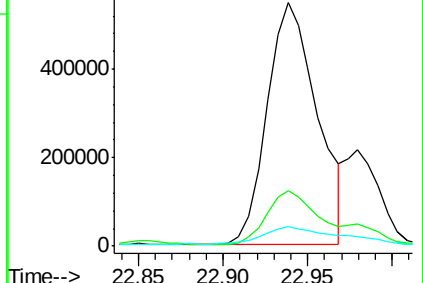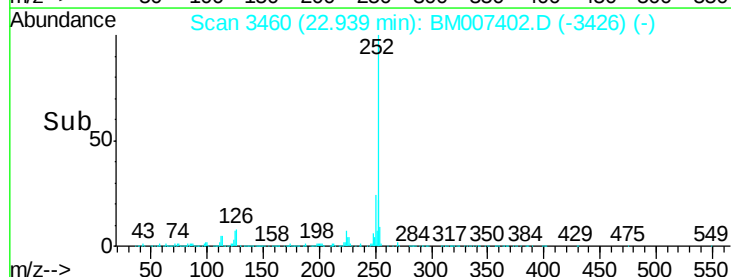

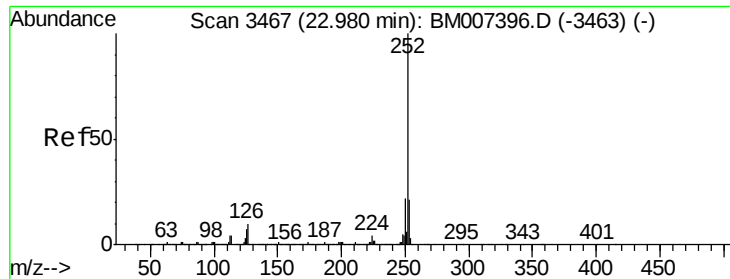





#86
Benzo(k)fluoranthene
Concen: 2.62 ng/ul m
RT: 22.98 min Scan# 3467
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Instrument :
BNA_M
ClientSampleId :
BD389

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.6	26.4
125	9.7	5.7	8.5




Manual Integrations
APPROVED


sohil
9/6/2016 1:16:40 PM

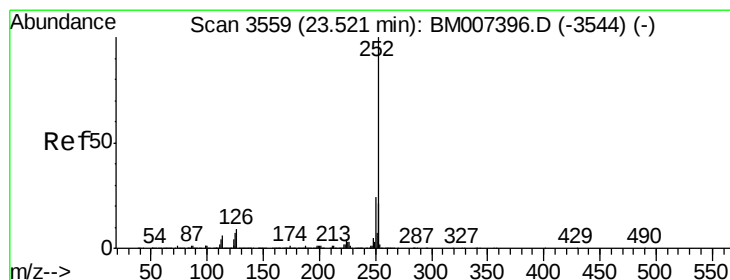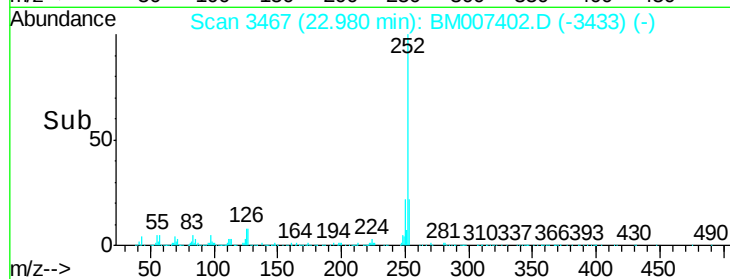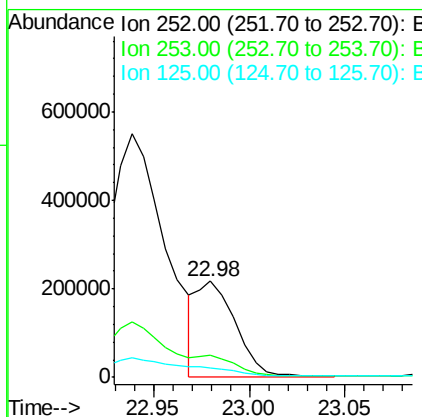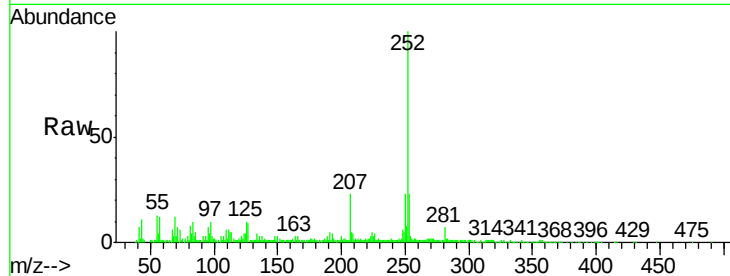

#88
Benzo(a)pyrene
Concen: 2.20 ng/ul
RT: 23.52 min Scan# 3559
Delta R.T. 0.00 min
Lab File: BM007402.D
Acq: 03 Sep 2016 11:58

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.7	26.5
125	9.4	6.6	9.8

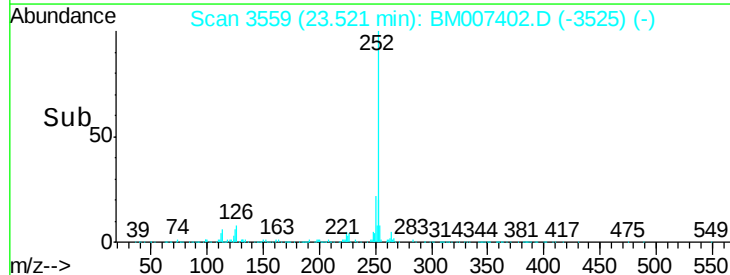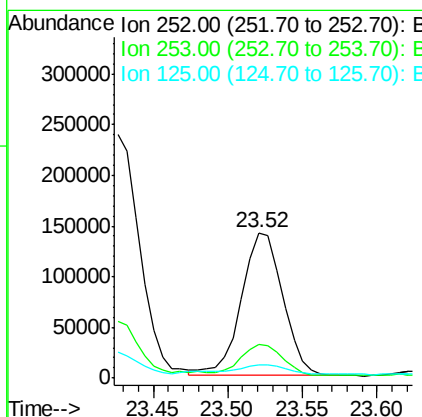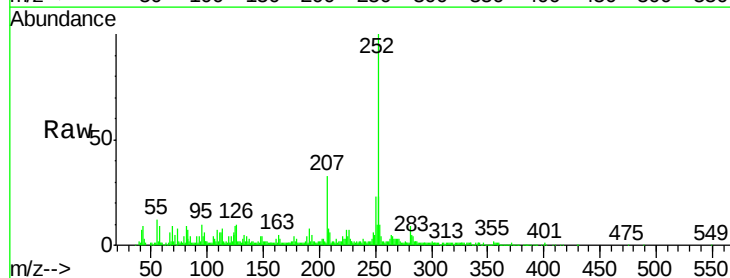

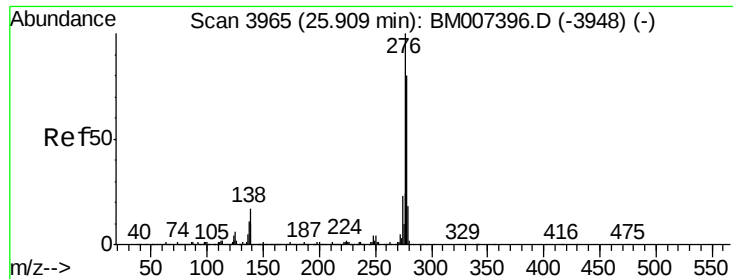

#89

Indeno(1,2,3-cd)pyrene

Concen: 1.45 ng/ul

RT: 25.91 min Scan# 3965

Delta R.T. 0.00 min

Lab File: BM007402.D

Acq: 03 Sep 2016 11:58

Instrument :

BNA_M





ClientSampled :

BD389

Tgt Ion:	276	Resp:	219149
Ion Ratio		Lower	Upper
276	100		
138	16.2	13.9	20.9
277	25.2	20.1	30.1

Manual Integrations
APPROVED

sohil
9/6/2016 1:16:40 PM

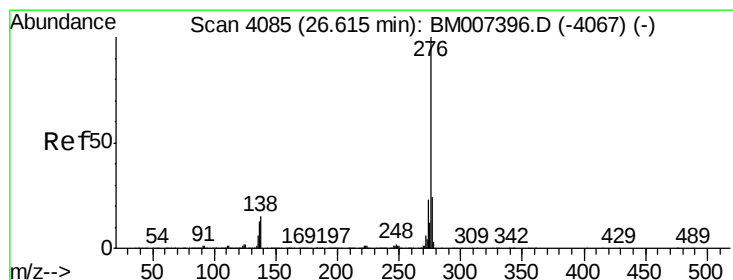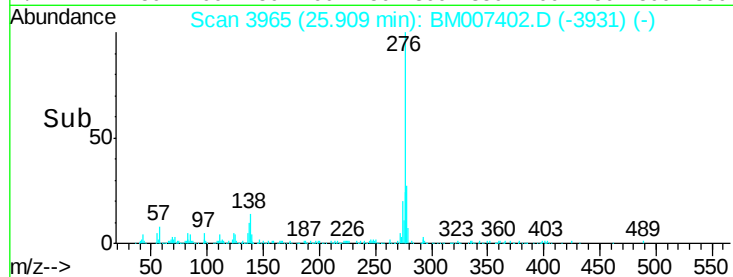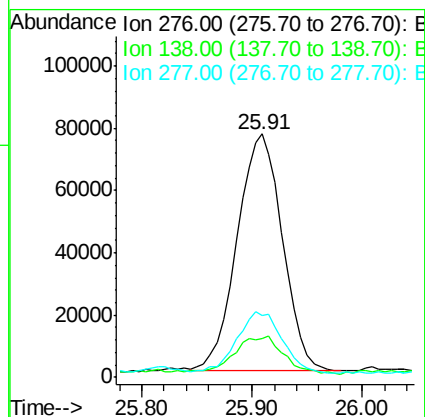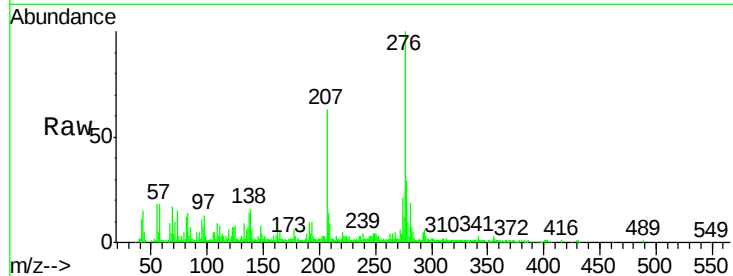

#91

Benzo(g,h,i)perylene

Concen: 1.42 ng/ul

RT: 26.61 min Scan# 4084

Delta R.T. -0.01 min

Lab File: BM007402.D

Acq: 03 Sep 2016 11:58

Tgt Ion:	276	Resp:	182090
Ion Ratio		Lower	Upper
276	100		
138	16.2	13.5	20.3
277	24.4	19.3	28.9

