

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
 Data File : BM022505.D
 Acq On : 03 Sep 2019 16:30
 Operator : HP/JU
 Sample : K4555-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TW-10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	359	364	376	rBV	152613	233440	15.07%	3.907%
2	6.710	627	633	645	rBV	68258	137152	8.85%	2.296%
3	7.040	683	689	704	rBV	345116	539130	34.80%	9.024%
4	7.504	763	768	776	rBB	75993	118052	7.62%	1.976%
5	7.810	814	820	832	rBB	338230	526663	33.99%	8.815%
6	8.681	962	968	987	rBV	178824	373630	24.12%	6.254%
7	10.287	1235	1241	1259	rBB	54289	125103	8.07%	2.094%
8	12.769	1657	1663	1681	rBV	537108	860629	55.55%	14.405%
9	14.175	1896	1902	1913	rBV	92286	157704	10.18%	2.640%
10	15.686	2153	2159	2176	rBV	442261	769169	49.64%	12.874%
11	16.945	2368	2373	2388	rBV2	83630	167635	10.82%	2.806%
12	19.580	2816	2821	2831	rBV	1304010	1549349	100.00%	25.932%
13	21.162	3085	3090	3101	rBV	122153	207787	13.41%	3.478%
14	23.345	3456	3461	3474	rBV2	94525	209192	13.50%	3.501%


Sum of corrected areas: 5974635

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
Data File : BM022505.D
Acq On : 03 Sep 2019 16:30
Operator : HP/JU
Sample : K4555-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

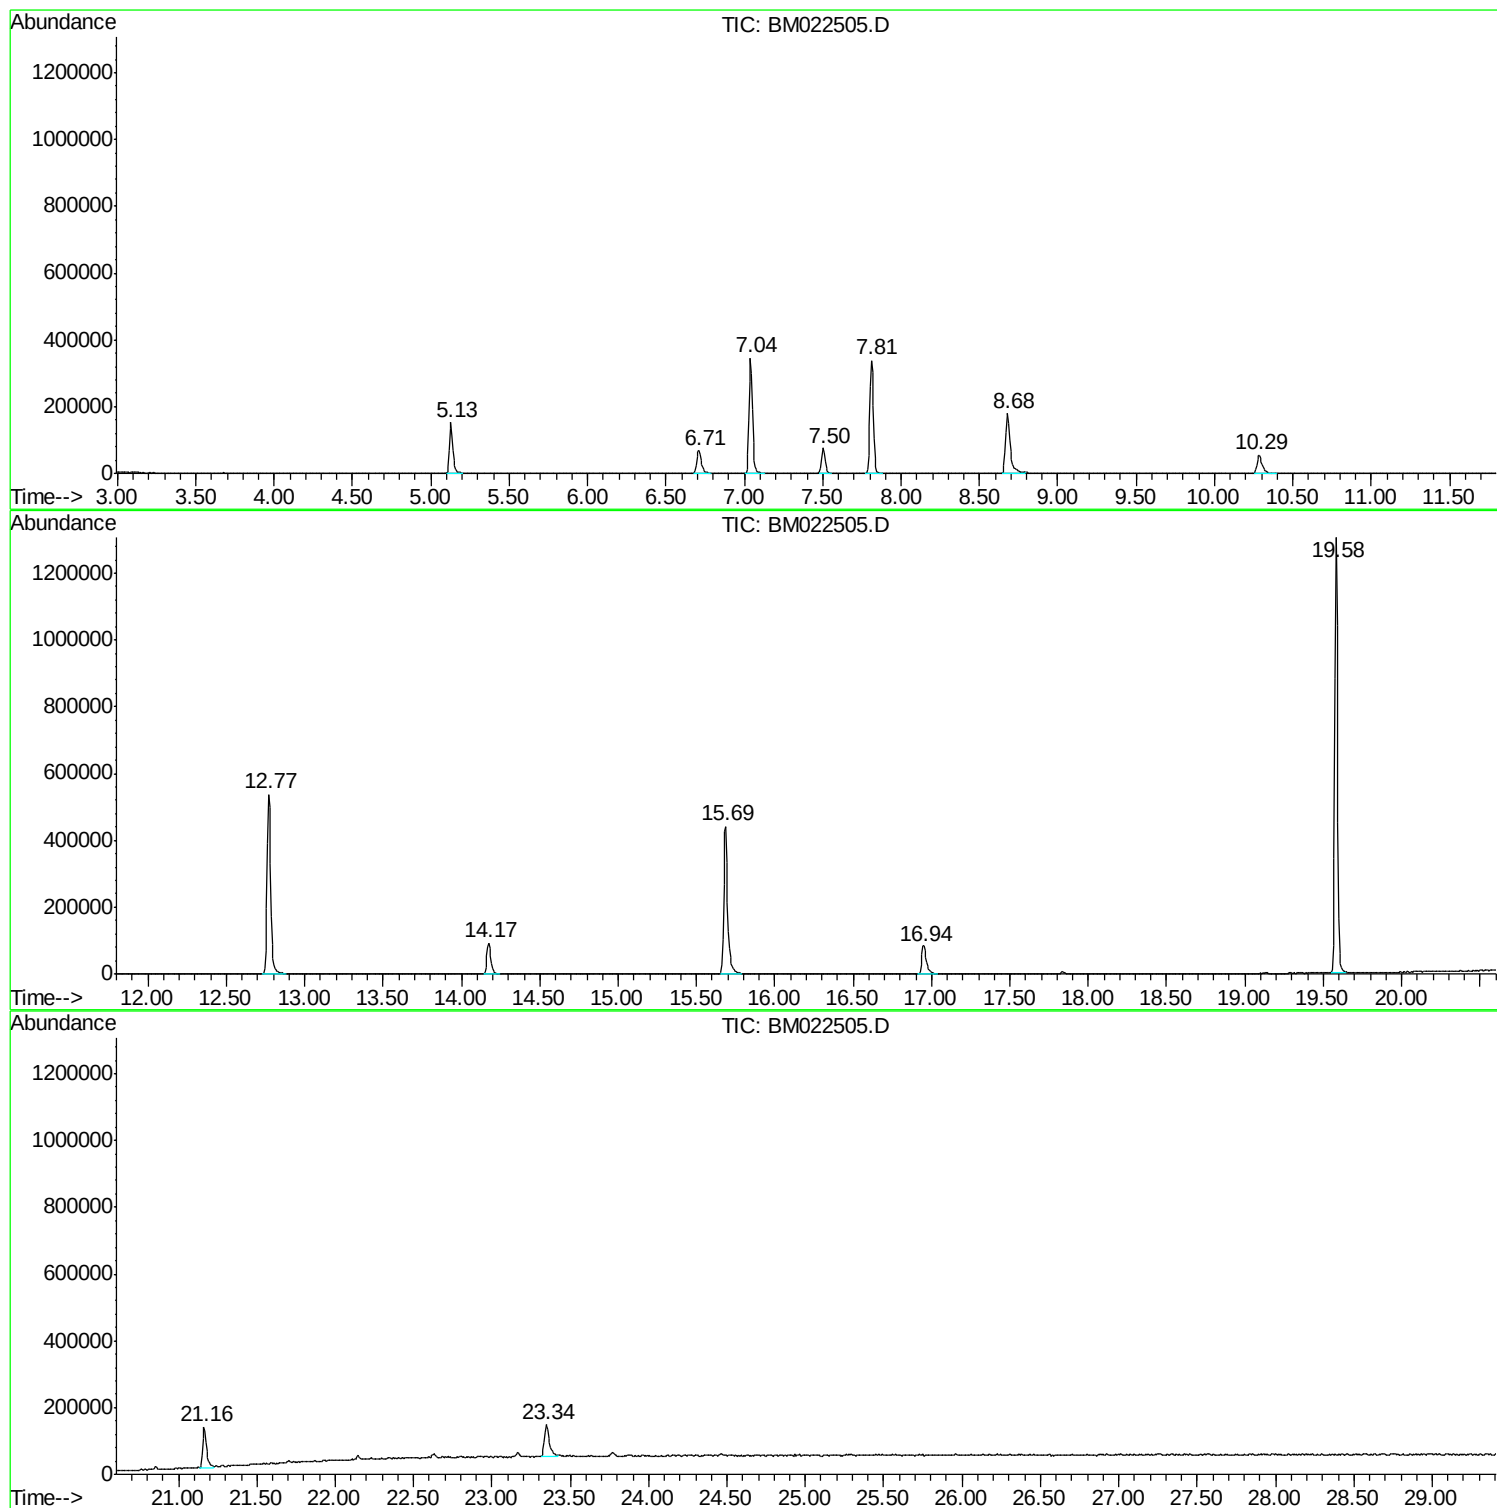

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
Data File : BM022505.D
Acq On : 03 Sep 2019 16:30
Operator : HP/JU
Sample : K4555-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-10










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	91.34 ng	539130	1,4-Dichlorobenzene-d4	7.50

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3H-1,2-Dithiol-3-one, 5-methyl-			132	C4H4OS2	003620-08-4	14
2	1,3,4-Thiadiazole-2(3H)-thione, ...			132	C3H4N2S2	029490-19-5	14
3	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	14
4	1H-Benzimidazole, 2-methyl-			132	C8H8N2	000615-15-6	14
5	1,3-Cyclopentanedione, 2-chloro-			132	C5H5ClO2	014203-19-1	10

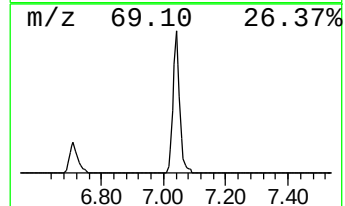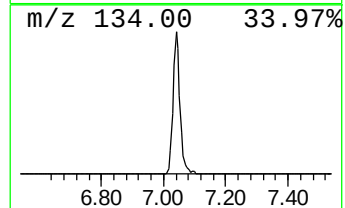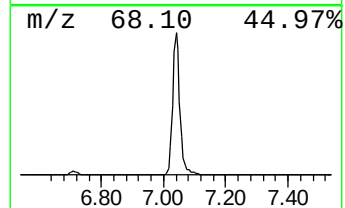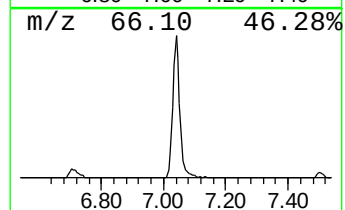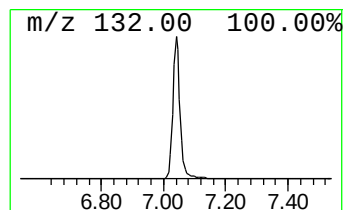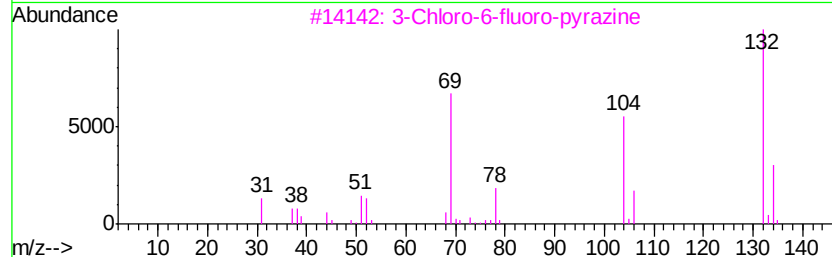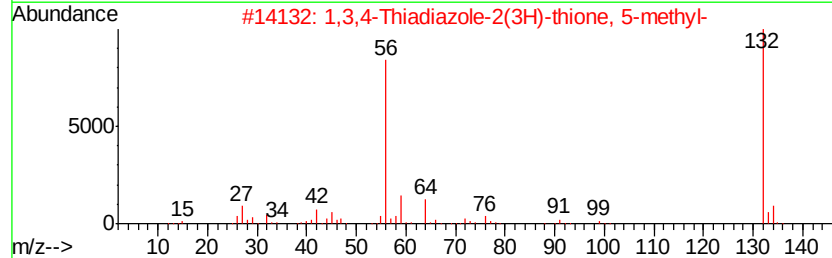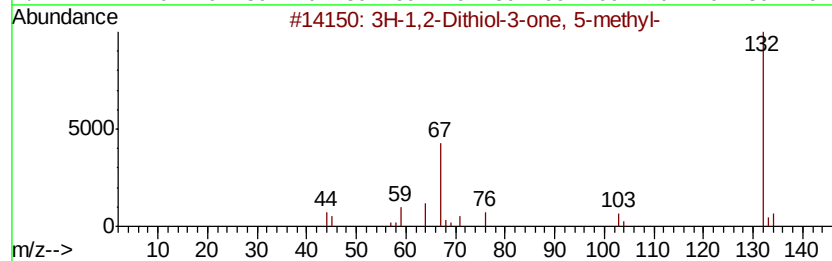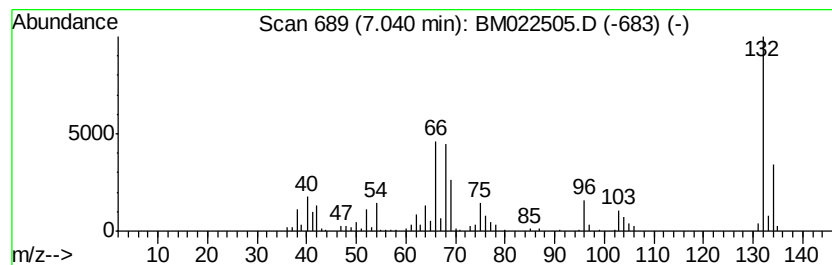

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090319\
Data File : BM022505.D
Acq On : 03 Sep 2019 16:30
Operator : HP/JU
Sample : K4555-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.04	7.04	91.3	ng	539130	1	7.50	118052	20.0