

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
 Data File : BM022507.D
 Acq On : 03 Sep 2019 17:43
 Operator : HP/JU
 Sample : K4555-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TW-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	359	364	378	rBV	149876	238847	15.18%	3.973%
2	6.704	627	632	651	rBV	75383	147766	9.39%	2.458%
3	7.040	683	689	703	rBV	337731	533257	33.90%	8.871%
4	7.504	763	768	776	rBB	76899	117276	7.45%	1.951%
5	7.810	814	820	831	rBB	331050	520966	33.12%	8.667%
6	8.681	961	968	988	rBV	180265	369552	23.49%	6.148%
7	10.281	1234	1240	1256	rBV	55386	126099	8.02%	2.098%
8	12.769	1657	1663	1677	rBV	516344	855447	54.38%	14.231%
9	14.174	1896	1902	1913	rBB2	92109	160829	10.22%	2.676%
10	15.680	2153	2158	2179	rBB	434463	751680	47.78%	12.505%
11	16.945	2368	2373	2387	rBV2	93872	168000	10.68%	2.795%
12	19.580	2816	2821	2833	rBV	1358705	1573180	100.00%	26.171%
13	21.162	3085	3090	3101	rBV	137040	220547	14.02%	3.669%
14	23.344	3456	3461	3472	rVB	110345	227705	14.47%	3.788%


Sum of corrected areas: 6011151

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
Data File : BM022507.D
Acq On : 03 Sep 2019 17:43
Operator : HP/JU
Sample : K4555-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

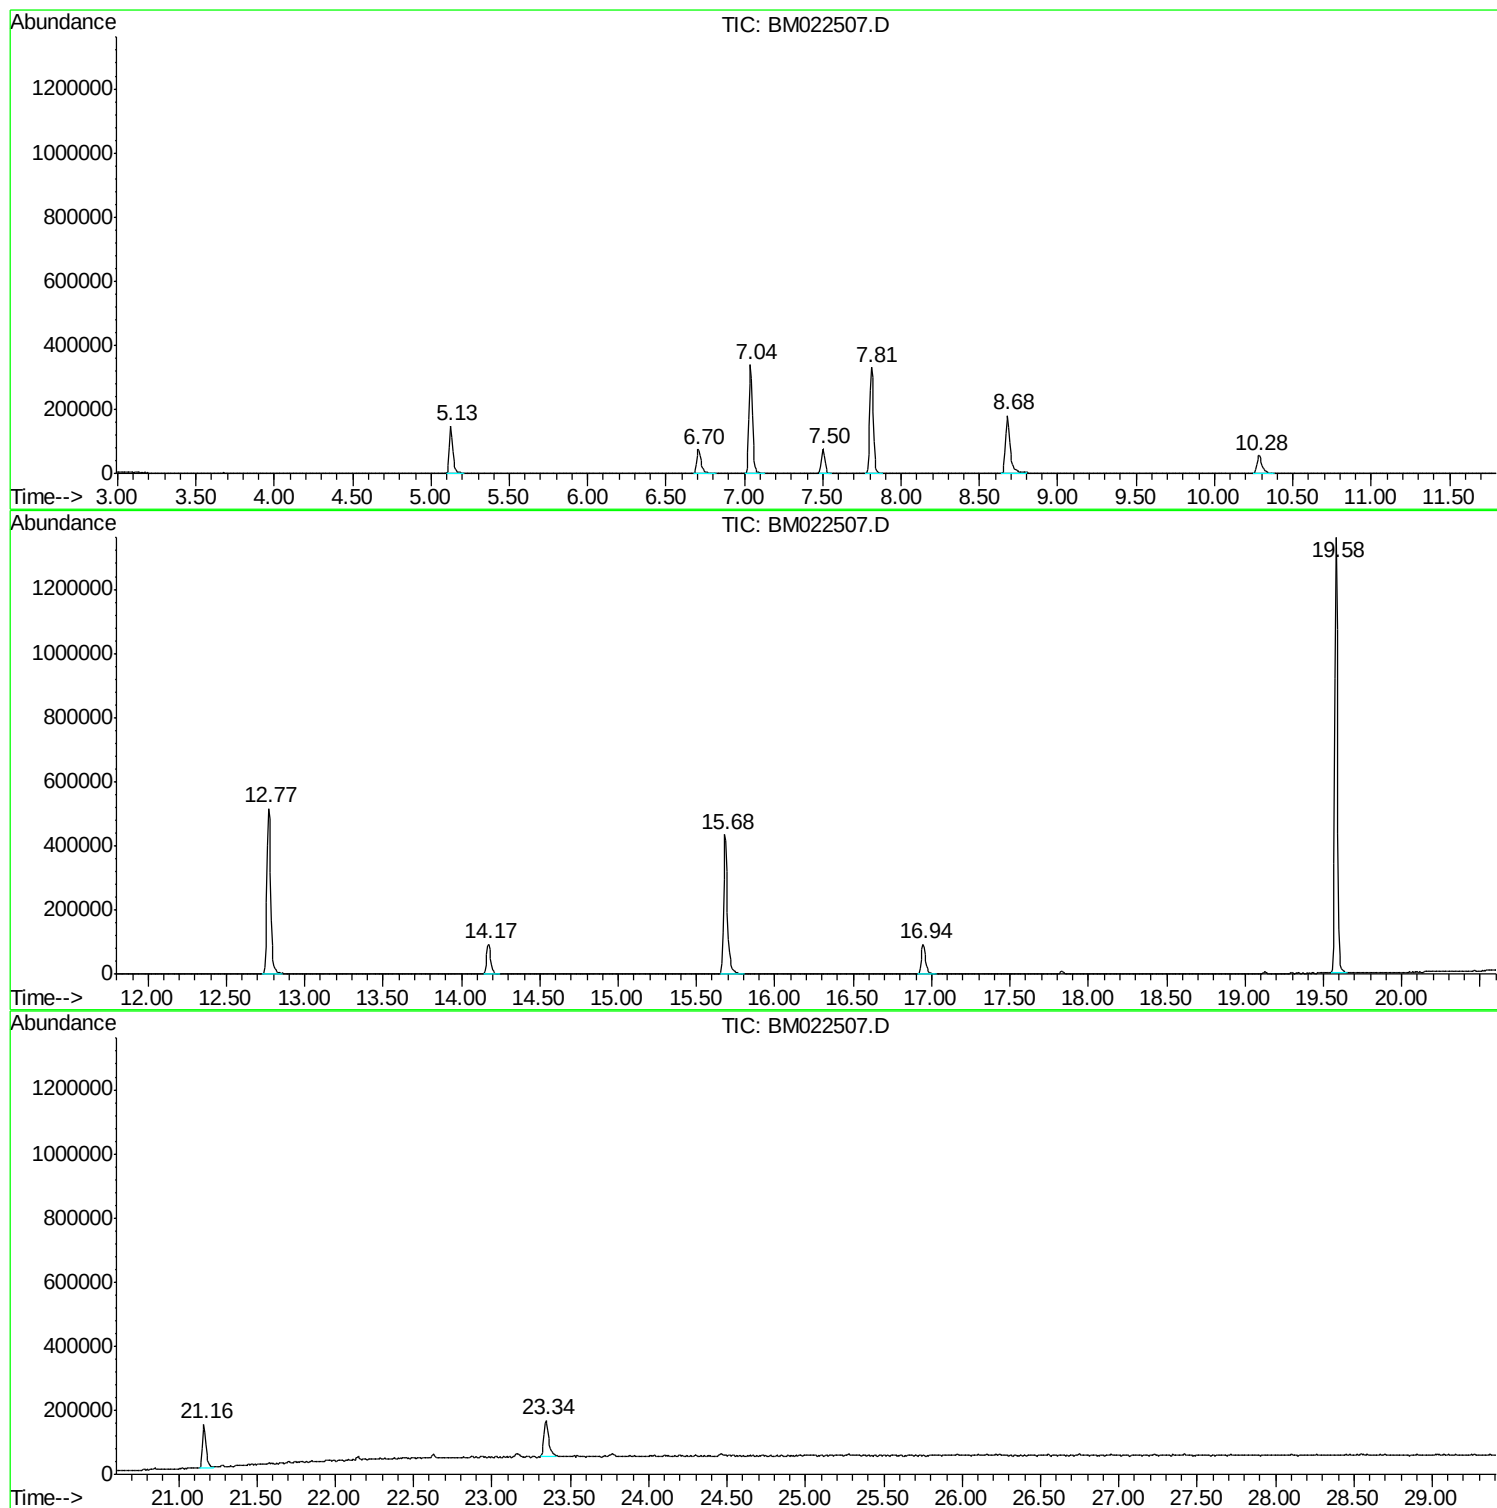

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
Data File : BM022507.D
Acq On : 03 Sep 2019 17:43
Operator : HP/JU
Sample : K4555-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	90.94 ng	533257	1,4-Dichlorobenzene-d4	7.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	14
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
5		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10

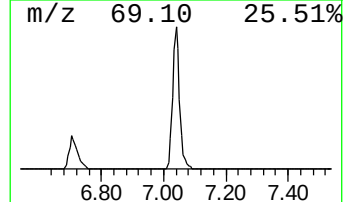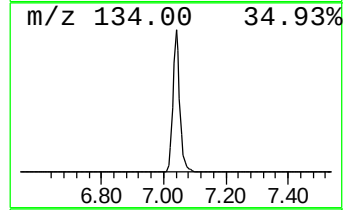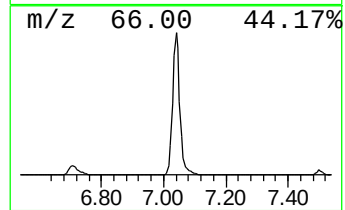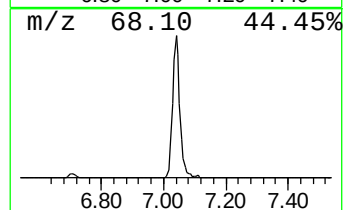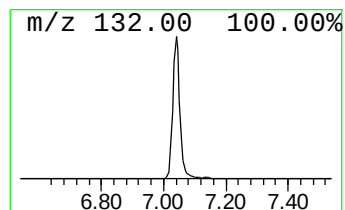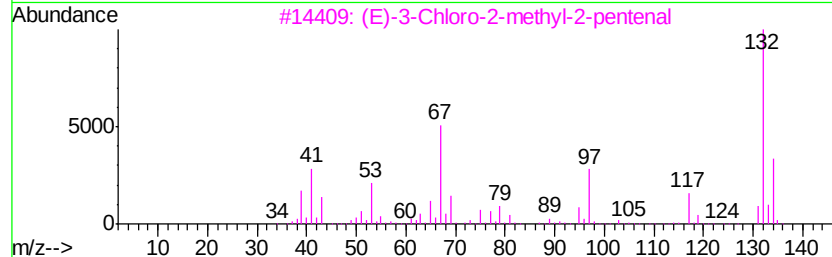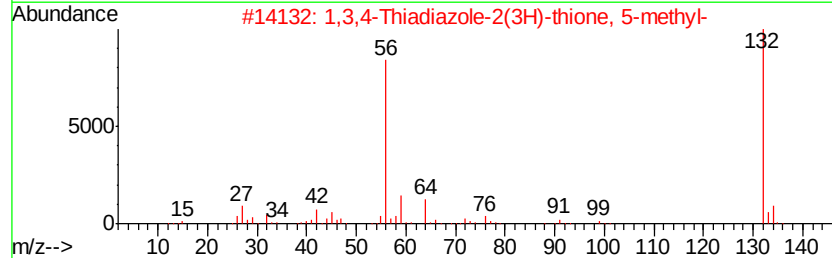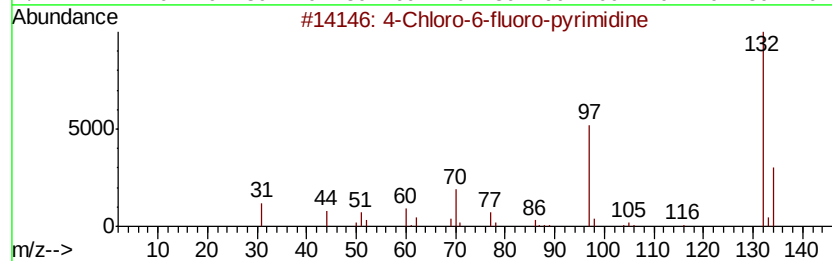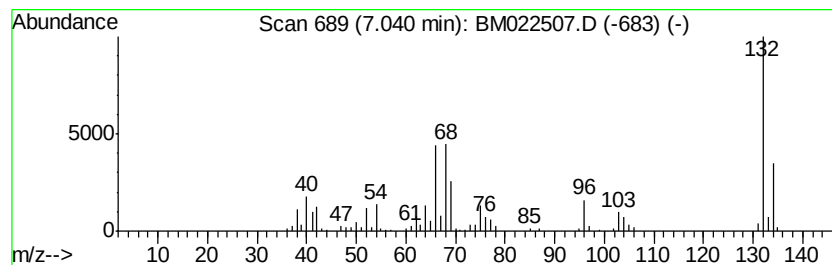

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090319\
Data File : BM022507.D
Acq On : 03 Sep 2019 17:43
Operator : HP/JU
Sample : K4555-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.04	7.04	90.9	ng	533257	1	7.50	117276	20.0