

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
 Data File : BM022508.D
 Acq On : 03 Sep 2019 18:20
 Operator : HP/JU
 Sample : K4555-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TW-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	359	364	378	rBV	173046	274304	16.79%	4.142%
2	6.704	627	632	647	rBV	87215	169184	10.35%	2.554%
3	7.039	683	689	705	rBV	391074	607963	37.21%	9.179%
4	7.504	763	768	776	rBB	86878	130839	8.01%	1.975%
5	7.810	814	820	831	rBB	369402	580897	35.55%	8.771%
6	8.681	961	968	994	rBV	204024	423851	25.94%	6.399%
7	10.280	1234	1240	1253	rBV	63313	140399	8.59%	2.120%
8	12.769	1657	1663	1681	rBV	611333	971488	59.45%	14.668%
9	14.168	1896	1901	1914	rBB	103029	179776	11.00%	2.714%
10	15.680	2153	2158	2175	rBV	503893	856393	52.41%	12.930%
11	16.945	2368	2373	2392	rBV	105683	190201	11.64%	2.872%
12	19.580	2816	2821	2832	rBV	1394071	1634031	100.00%	24.671%
13	21.162	3085	3090	3100	rBV	135940	228439	13.98%	3.449%
14	23.344	3455	3461	3474	rBV	110653	235521	14.41%	3.556%


Sum of corrected areas: 6623286

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
Data File : BM022508.D
Acq On : 03 Sep 2019 18:20
Operator : HP/JU
Sample : K4555-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

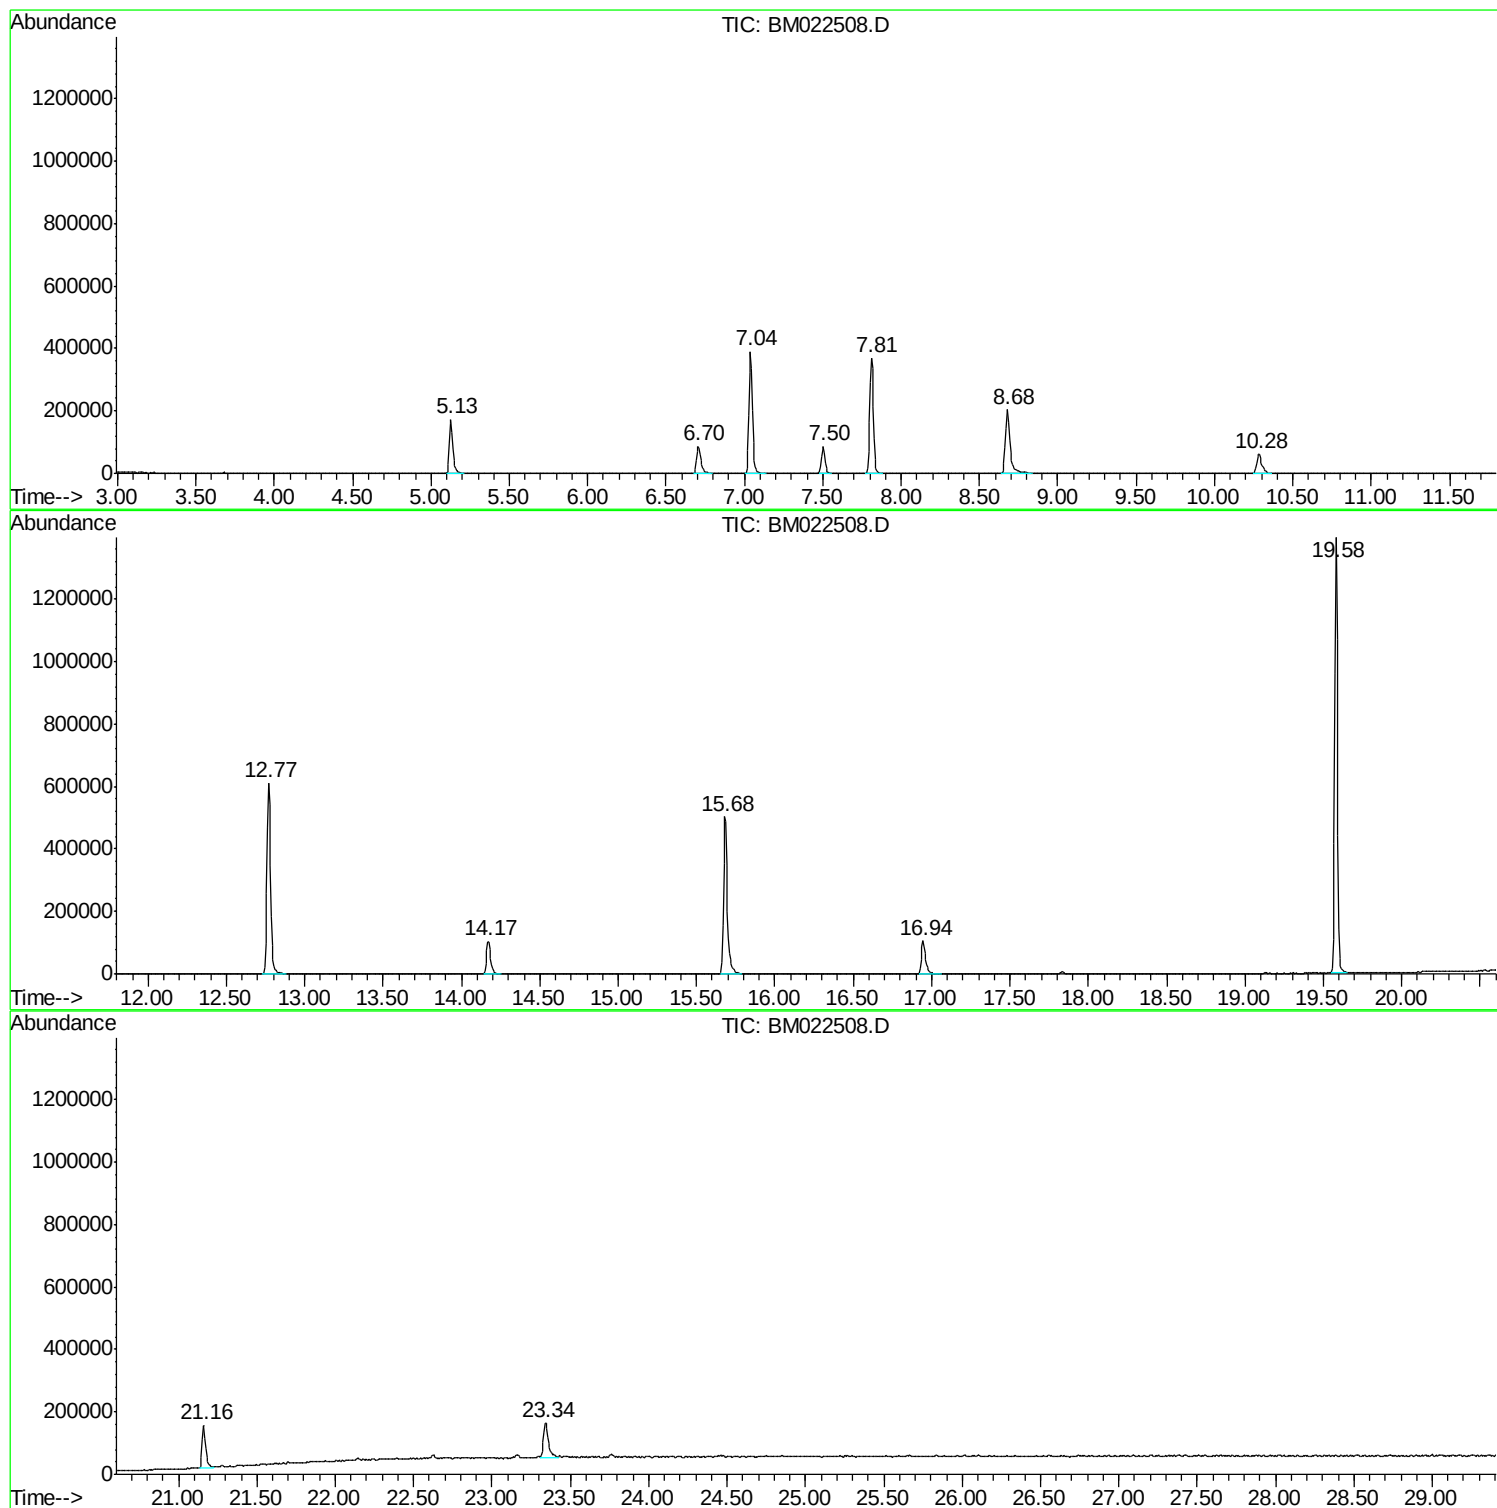

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
Data File : BM022508.D
Acq On : 03 Sep 2019 18:20
Operator : HP/JU
Sample : K4555-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-6










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	92.93 ng	607963	1,4-Dichlorobenzene-d4	7.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	14
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10

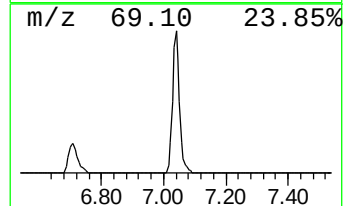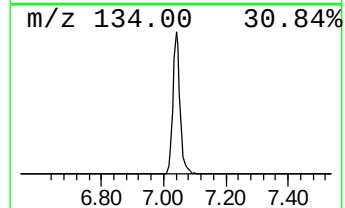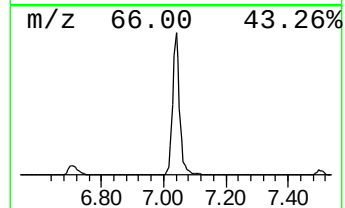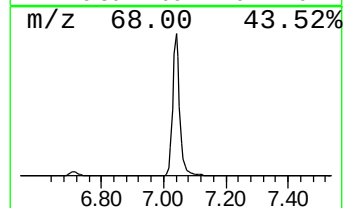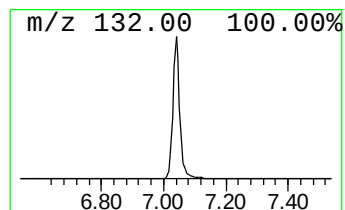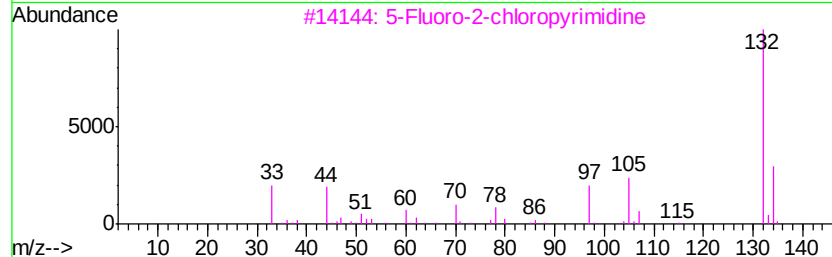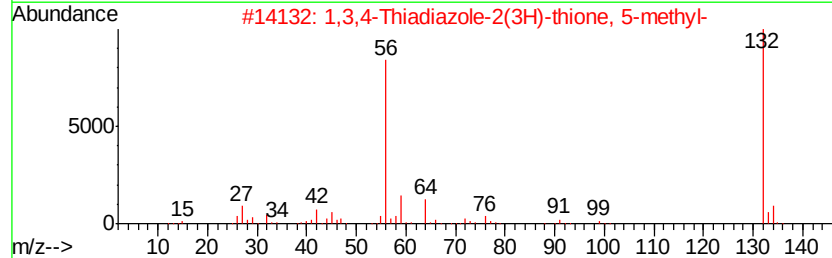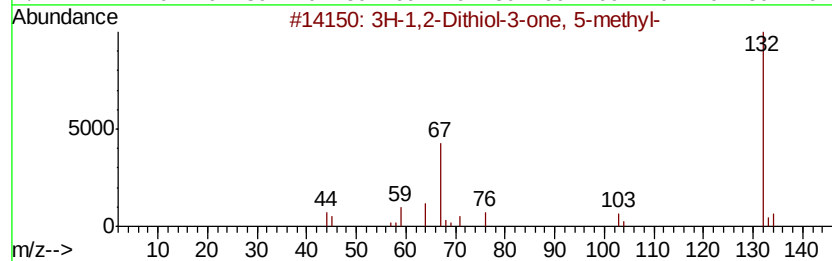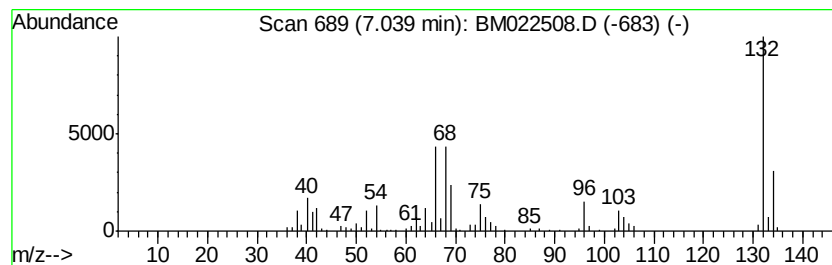

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090319\
Data File : BM022508.D
Acq On : 03 Sep 2019 18:20
Operator : HP/JU
Sample : K4555-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.04	7.04	92.9	ng	607963	1	7.50	130839	20.0