


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090319\
 Data File : BM022493.D
 Acq On : 03 Sep 2019 09:05
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 02 03:54:42 2019

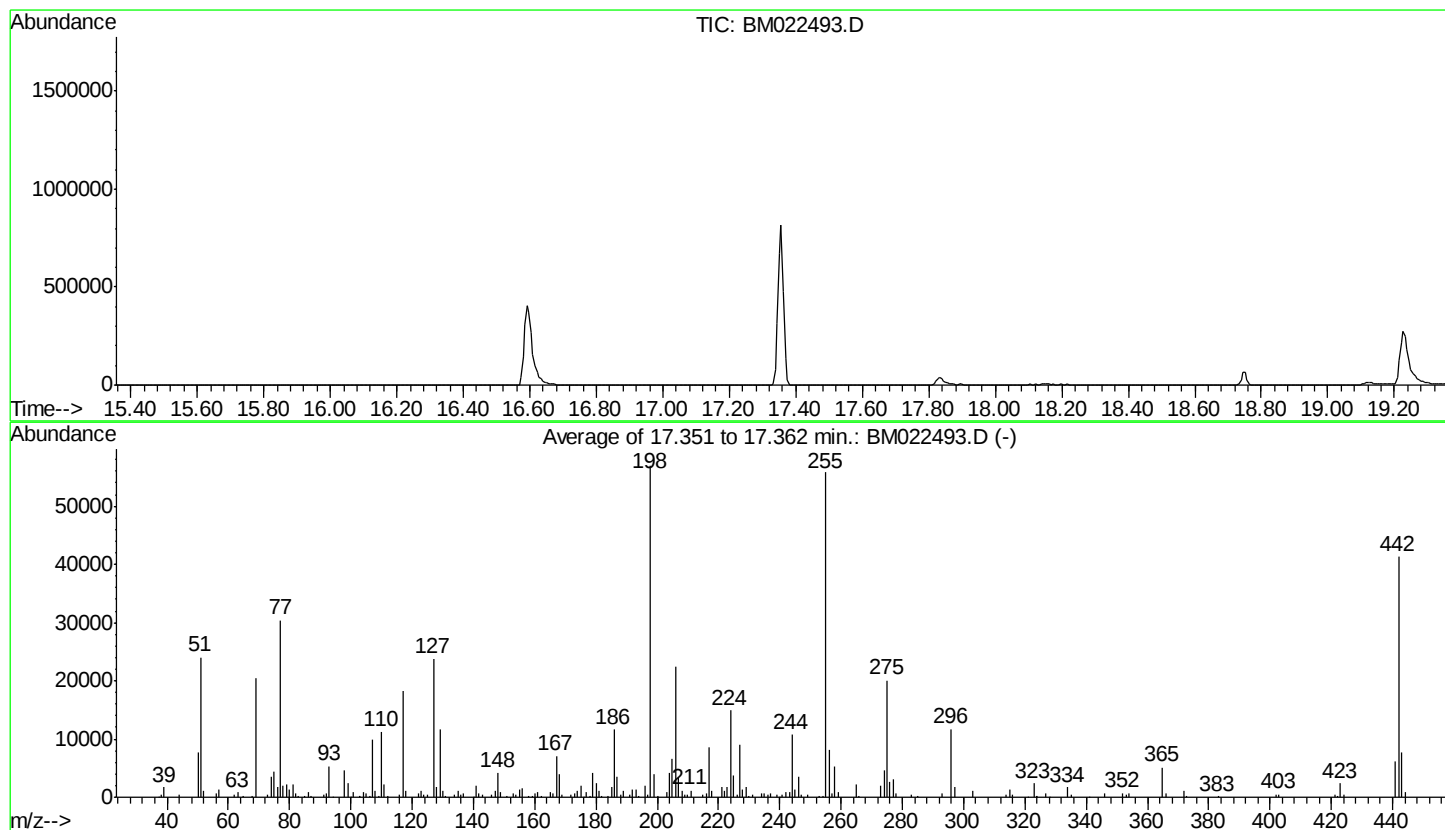

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	23971	PASS
68	69	0.00	2	1.5	306	PASS
69	198	0.00	100	36.1	20553	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	23761	PASS
197	198	0.00	2	0.8	461	PASS
198	198	100	100	100.0	56962	PASS
199	198	5	9	7.1	4053	PASS
275	198	10	60	35.2	20043	PASS
365	198	1	100	9.0	5103	PASS
441	198	0.01	100	11.0	6248	PASS
442	198	50	100	72.5	41277	PASS
443	442	15	24	18.8	7747	PASS