

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090320\
 Data File : BM027311.D
 Acq On : 03 Sep 2020 11:22
 Operator : JU/CG
 Sample : L3840-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA6

Quant Time: Sep 03 11:55:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 03 09:55:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	105410	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	400443	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	285973	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	667968	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	789882	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	902474	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.14	96	9615	5.17	ng/uL	0.00
5) Phenol-d5	6.76	99	150700	17.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	118013	21.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	127148	19.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	125996	18.36	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	64307	20.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	70479	19.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	137703	18.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	170003	20.90	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	573775	25.29	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	581620	21.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	60290	15.75	ng/ul	0.00
58) Fluorene-d10	15.22	176	452396	23.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.34	200	74349	17.06	ng/ul	0.00
71) Anthracene-d10	17.06	188	780180	24.61	ng/ul	0.00
79) Pyrene-d10	19.37	212	960433	21.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	1169537	23.25	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	90452	3.841	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090320\
Data File : BM027311.D
Acq On : 03 Sep 2020 11:22
Operator : JU/CG
Sample : L3840-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA6

Quant Time: Sep 03 11:55:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 03 09:55:00 2020
Response via : Initial Calibration

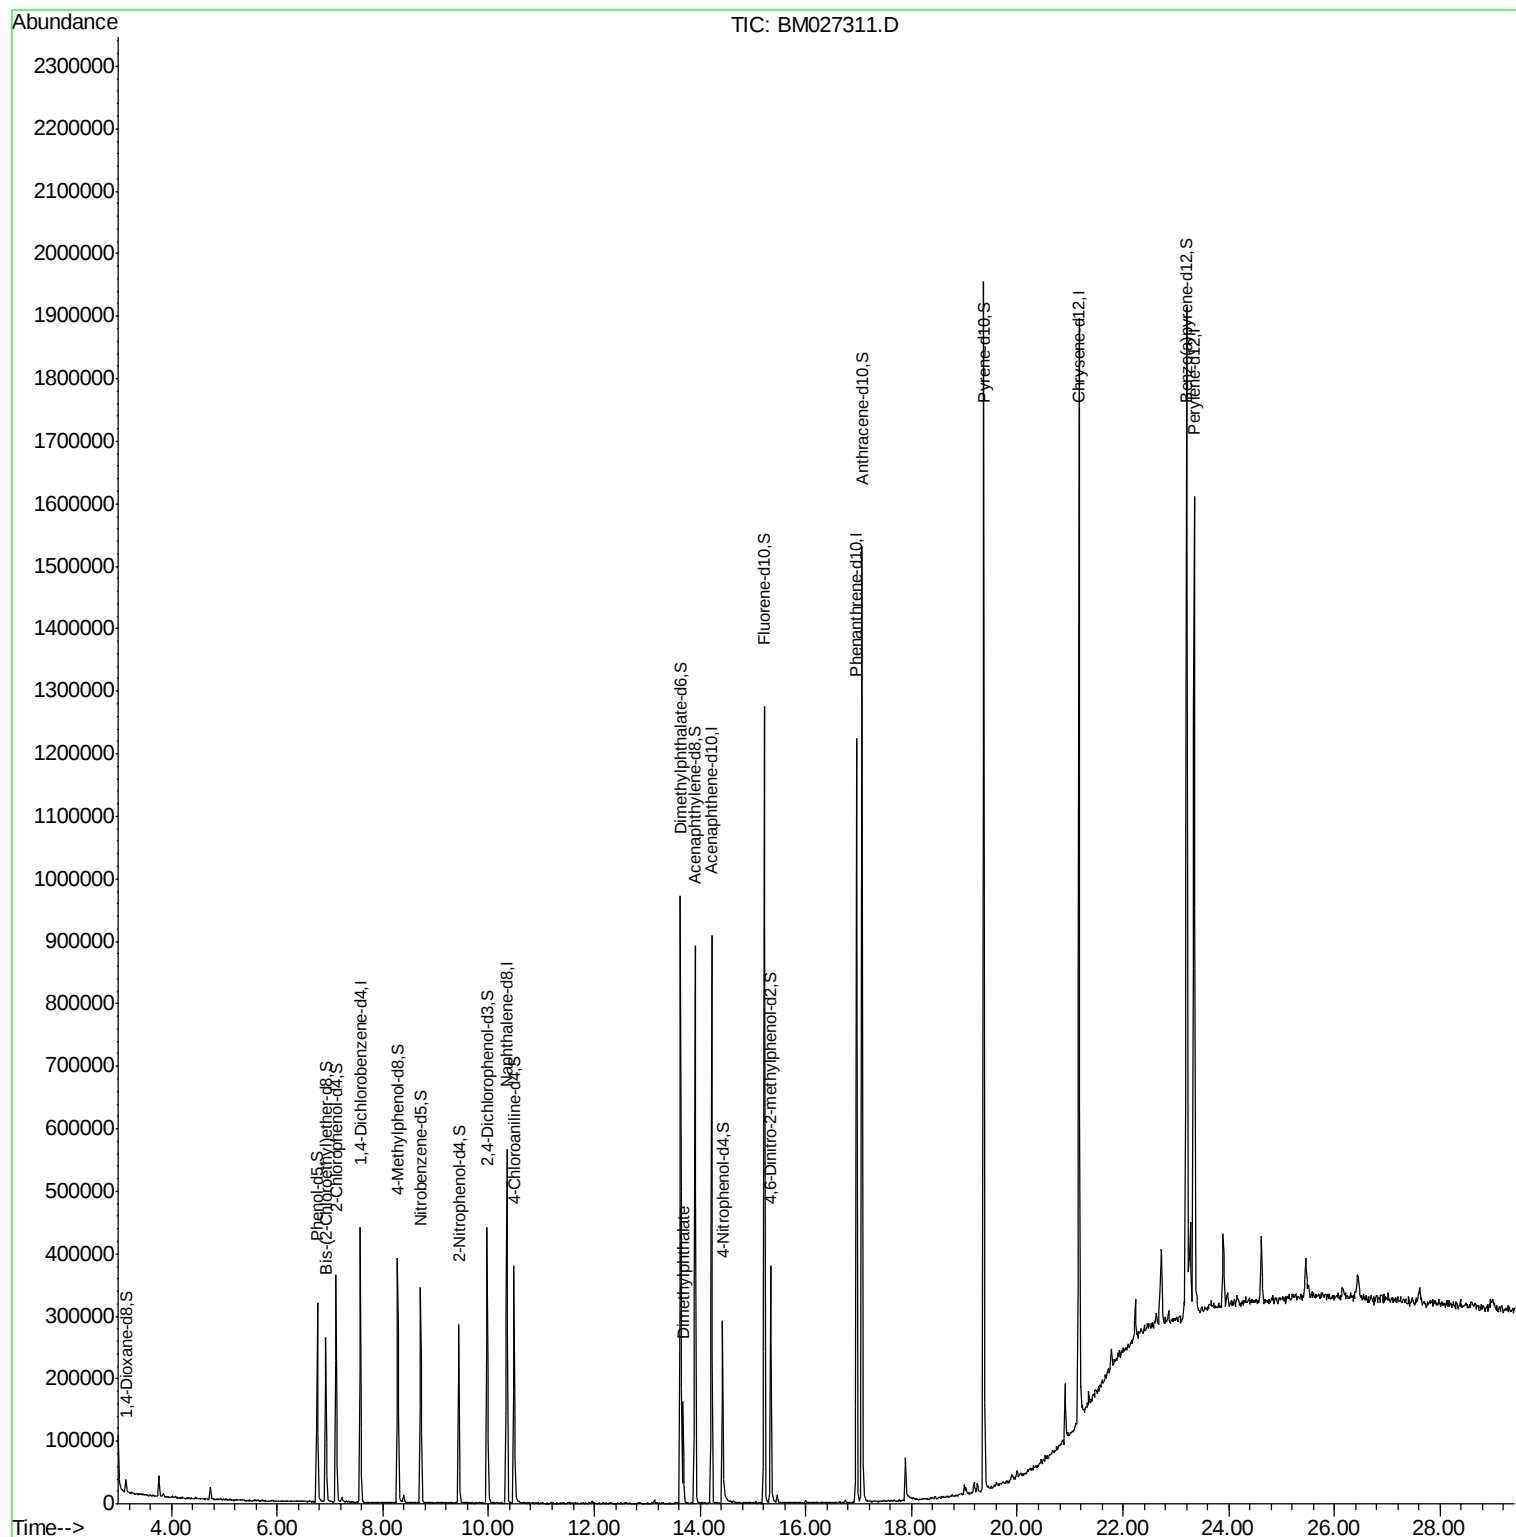

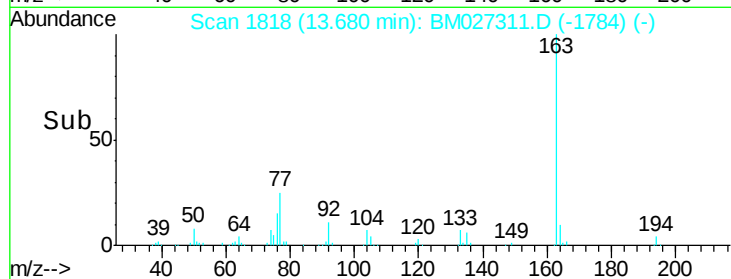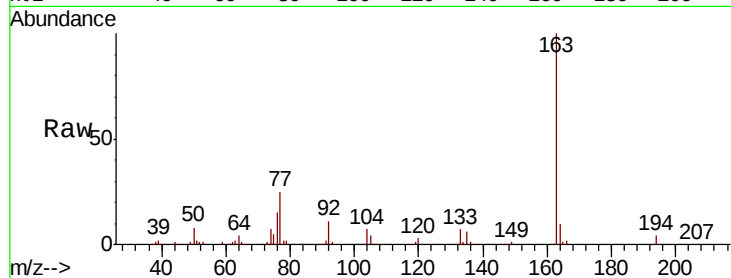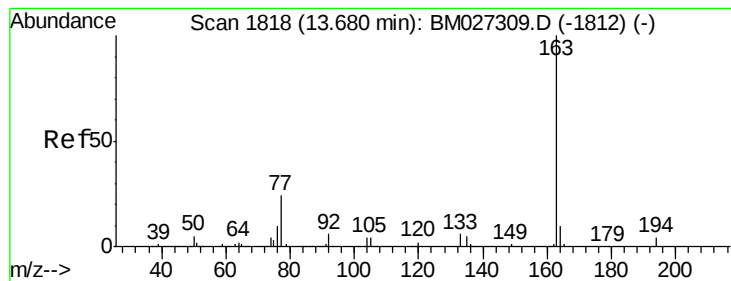

#45

Dimethylphthalate

Concen: 3.841 ng/ul

RT: 13.68 min Scan# 1818

Delta R.T. -0.00 min

Lab File: BM027311.D

Acq: 03 Sep 2020 11:22

Instrument :

BNA_M

ClientSampleId :

C0AA6

Tot Ion:163 Resp: 90452

Ion Ratio Lower Upper

163 100

194 3.9 3.5 5.3

164 10.1 8.2 12.2

