

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090320\
 Data File : BM027314.D
 Acq On : 03 Sep 2020 13:12
 Operator : JU/CG
 Sample : L3840-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE5

Quant Time: Sep 03 13:56:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 03 09:55:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	131524	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	496952	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	346030	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	771483	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	784833	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	778253	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	23422	10.09	ng/uL	0.00
5) Phenol-d5	6.76	99	362719	34.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	262731	38.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	303750	36.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	302445	35.32	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	148400	37.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	166522	36.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	329148	35.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	392429	38.88	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1110889	40.46	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1328862	40.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	123971	26.77	ng/ul	0.00
58) Fluorene-d10	15.22	176	959817	40.51	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.34	200	129462	25.72	ng/ul	0.00
71) Anthracene-d10	17.06	188	1522974	41.59	ng/ul	0.00
79) Pyrene-d10	19.36	212	1743760	38.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	1682285	38.77	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	118082	4.144	ng/ul	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090320\
Data File : BM027314.D
Acq On : 03 Sep 2020 13:12
Operator : JU/CG
Sample : L3840-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE5

Quant Time: Sep 03 13:56:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 03 09:55:00 2020
Response via : Initial Calibration

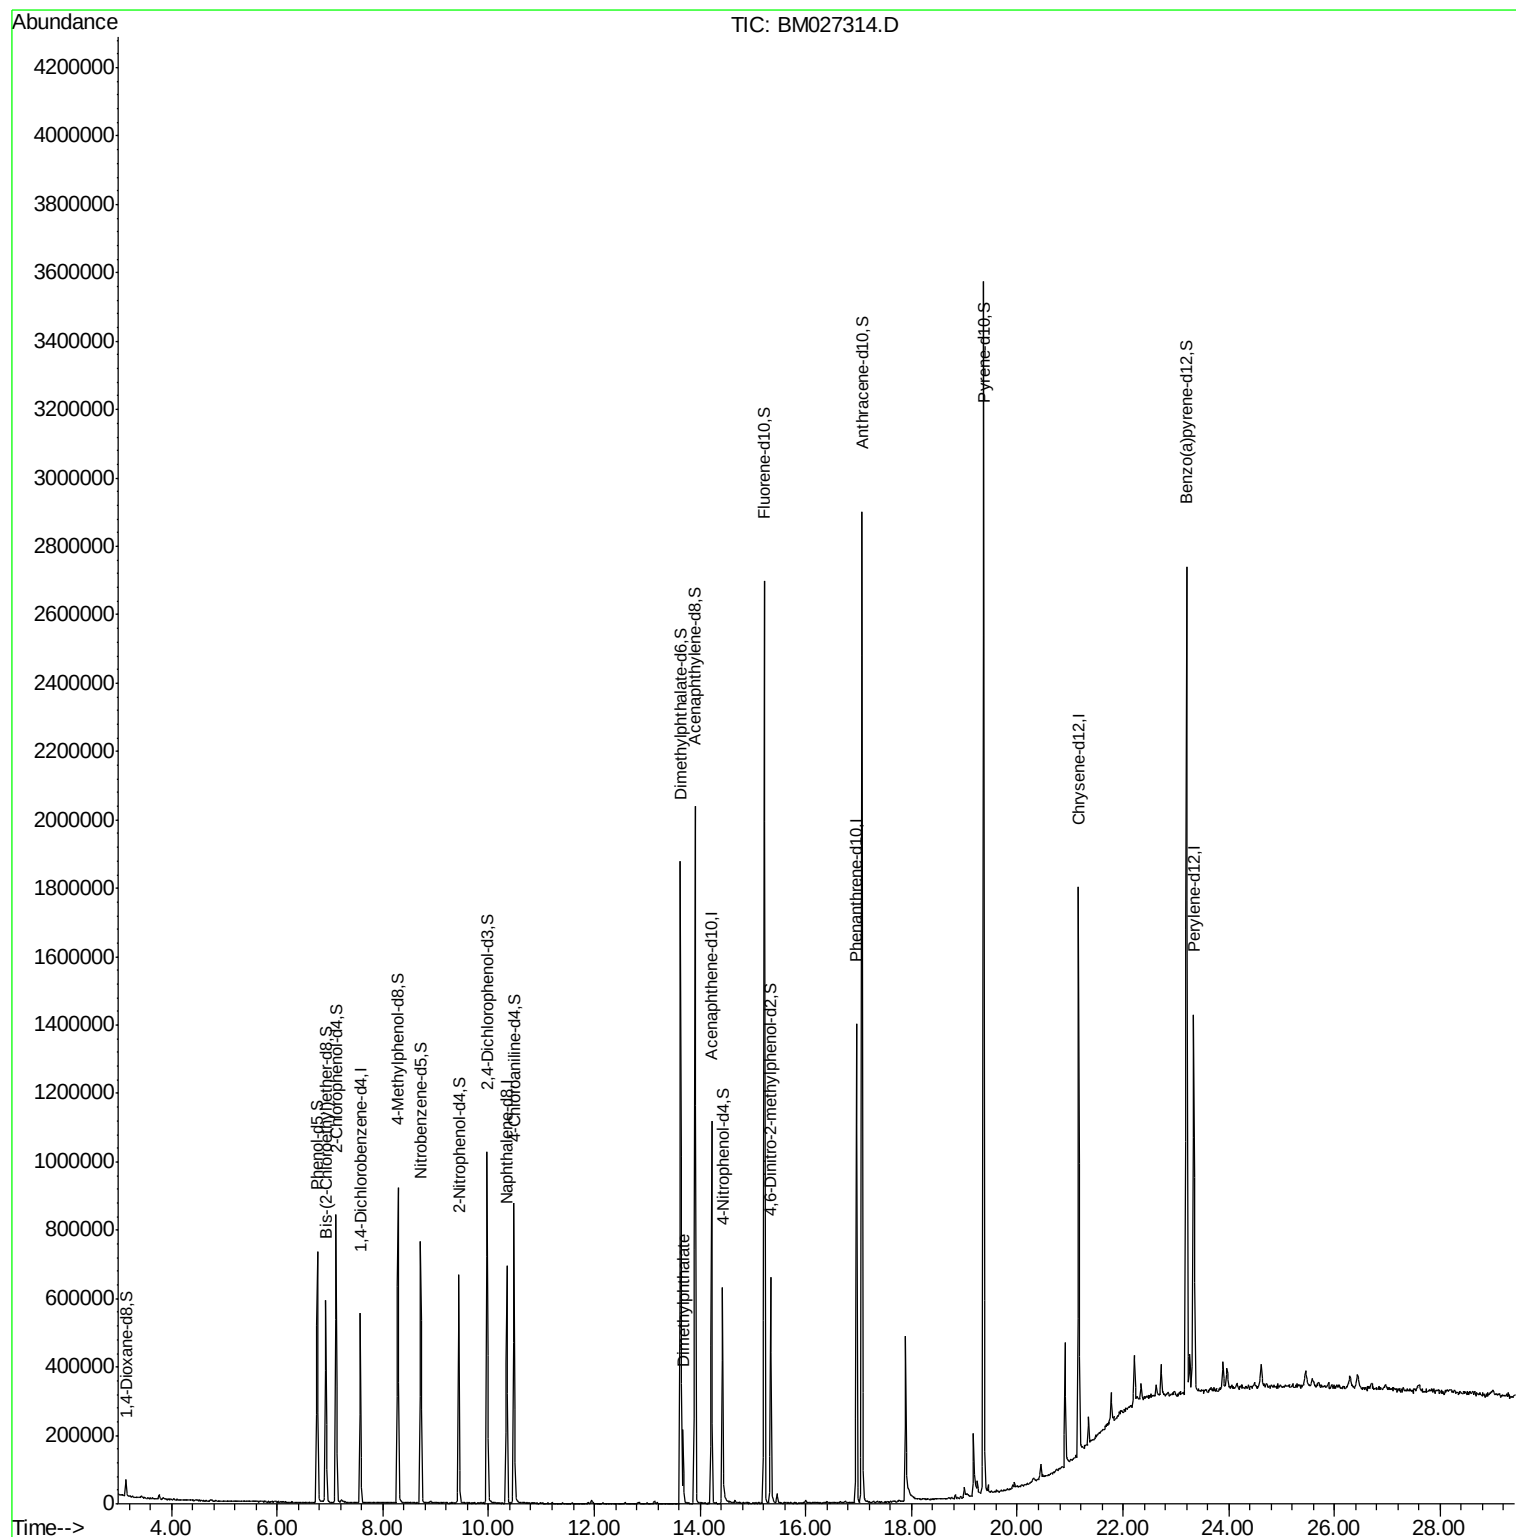

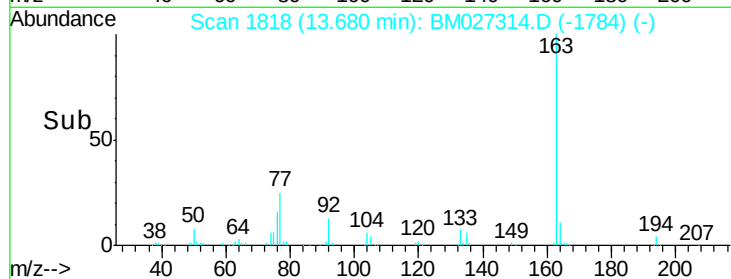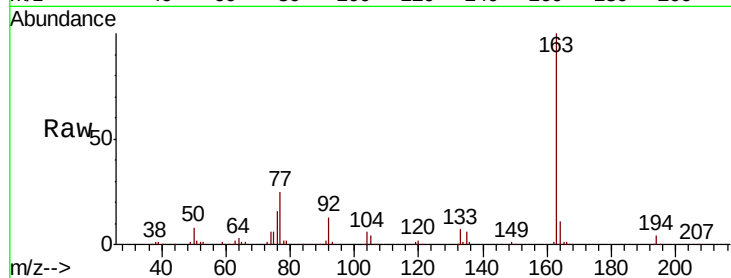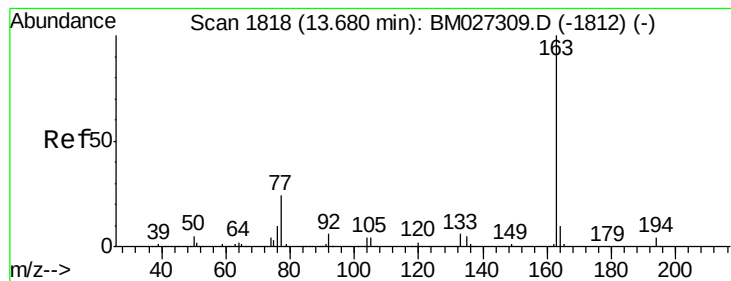

#45

Dimethylphthalate

Concen: 4.144 ng/ul

RT: 13.68 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM027314.D

Acq: 03 Sep 2020 13:12

Instrument :

BNA_M

ClientSampleId :

C0AE5

Tot Ion:163 Resp: 118082

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 11.3 8.2 12.2

