

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090320\
 Data File : BM027317.D
 Acq On : 03 Sep 2020 15:01
 Operator : JU/CG
 Sample : L3840-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD2

Quant Time: Sep 03 15:34:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 03 09:55:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	130958	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	493546	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	350421	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	786829	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	798185	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	769731	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.14	96	21861	9.45	ng/uL	0.00
5) Phenol-d5	6.76	99	345519	32.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	246917	35.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	281636	34.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	284718	33.40	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	137881	34.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	157852	34.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	310262	33.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	354301	35.35	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1047561	37.68	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1239640	37.71	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	123804	26.40	ng/ul	0.00
58) Fluorene-d10	15.22	176	900088	37.51	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.34	200	127191	24.78	ng/ul	0.00
71) Anthracene-d10	17.06	188	1437121	38.48	ng/ul	0.00
79) Pyrene-d10	19.36	212	1627526	35.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	1527561	35.60	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	205423	7.119	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090320\
Data File : BM027317.D
Acq On : 03 Sep 2020 15:01
Operator : JU/CG
Sample : L3840-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Quant Time: Sep 03 15:34:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 03 09:55:00 2020
Response via : Initial Calibration

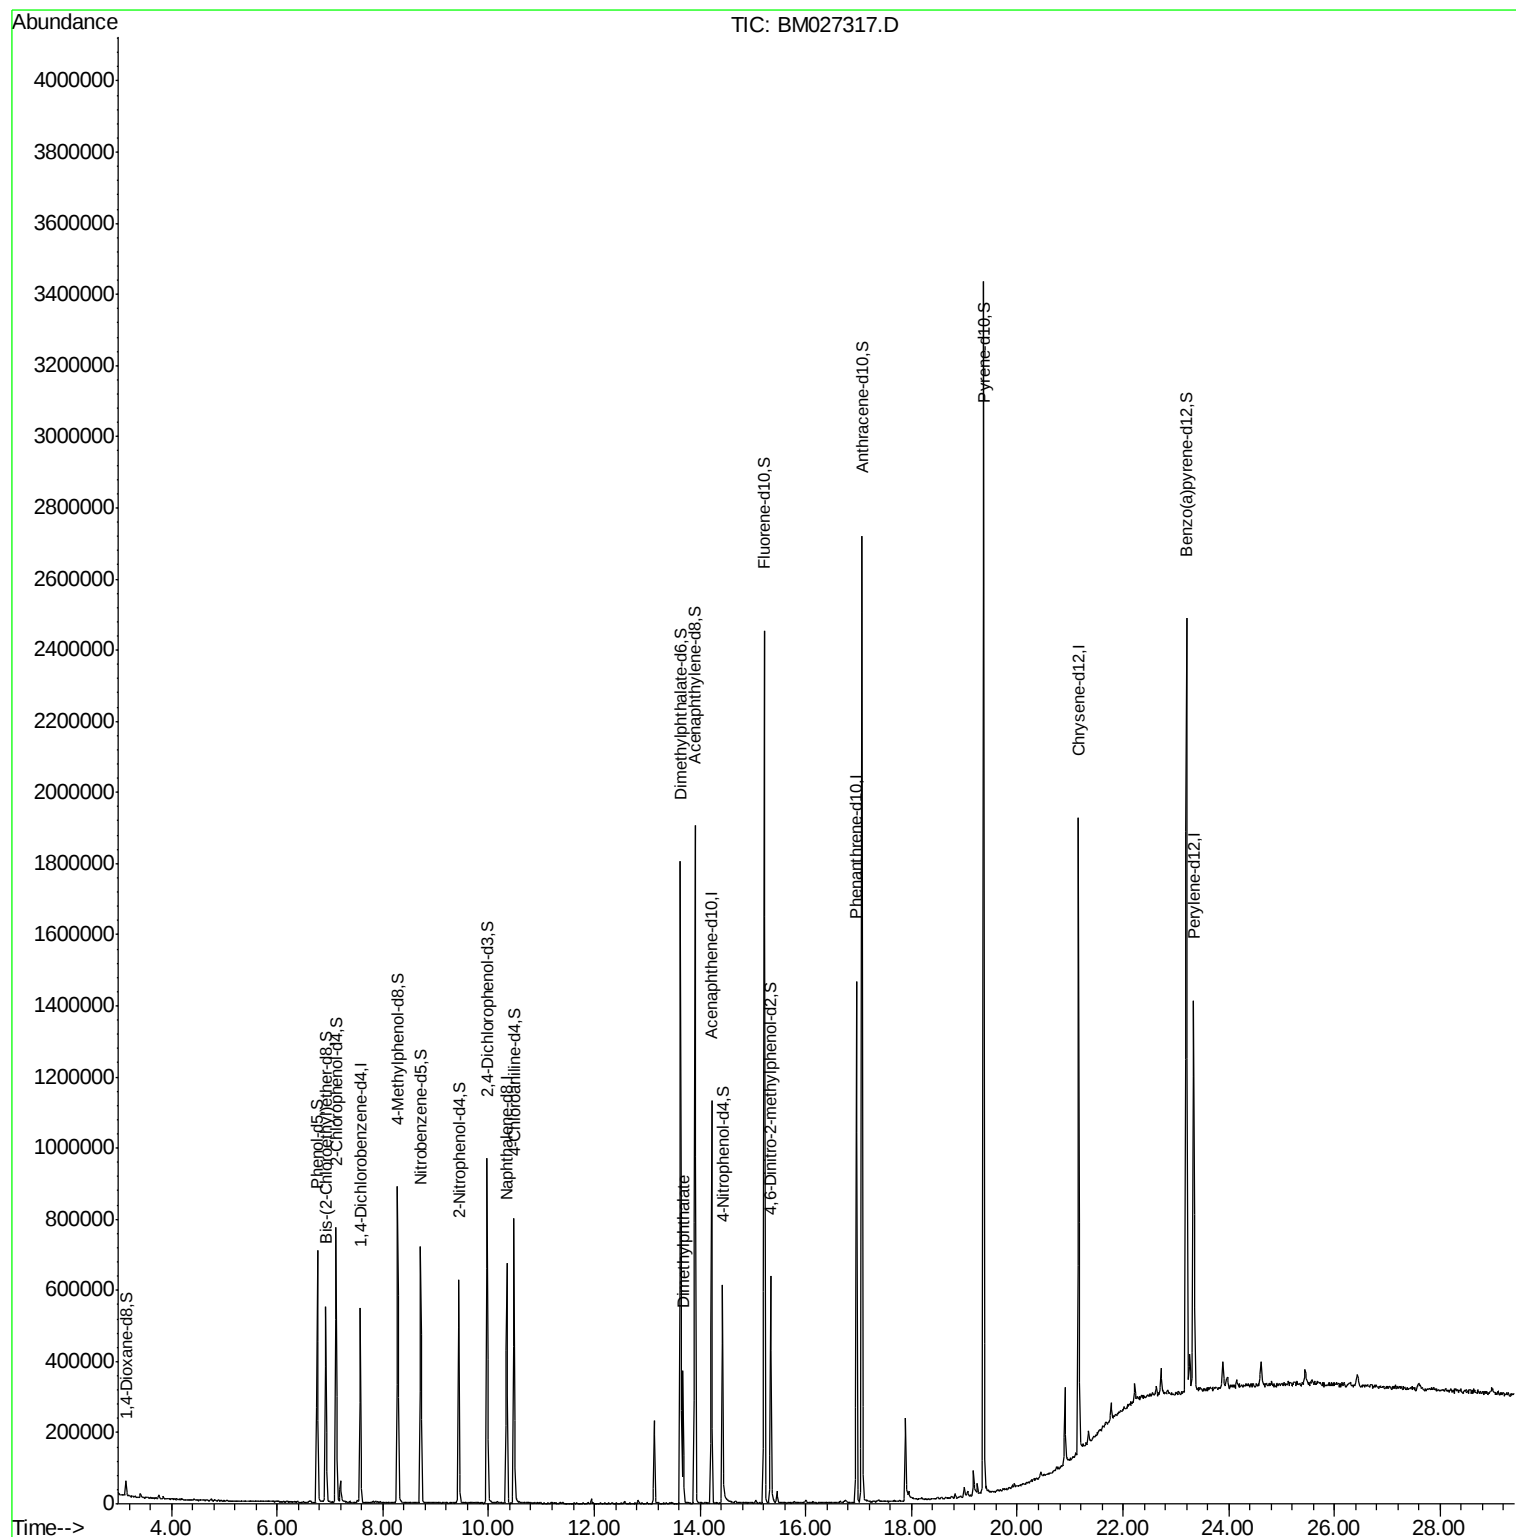

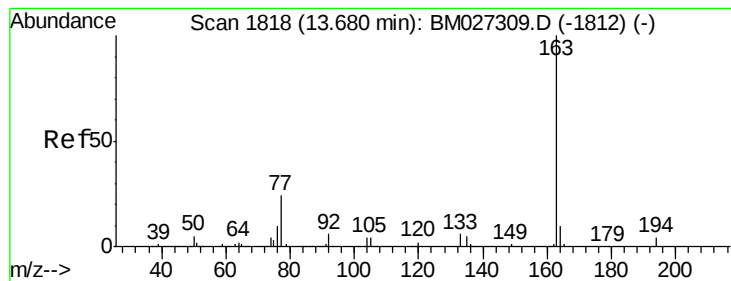

#45

Dimethylphthalate

Concen: 7.119 ng/ul

RT: 13.68 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM027317.D

Acq: 03 Sep 2020 15:01

Instrument :

BNA_M

ClientSampleId :

C0AD2


Tot Ion:163 Resp: 205423

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 10.0 8.2 12.2

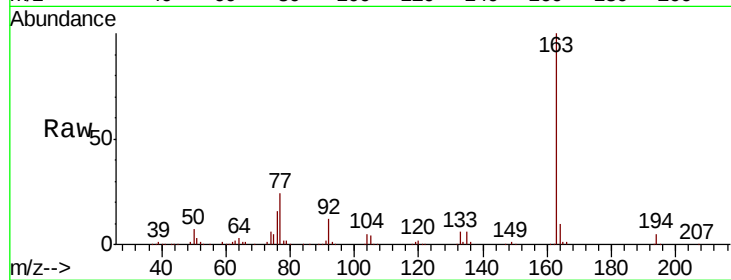

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

