


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
Data File : BM032067.D
Acq On : 04 Sep 2021 08:39
Operator : CG/JU
Sample : M3486-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AY9

Manual Integrations
APPROVED

mohammad
9/7/2021 11:38:12 AM

Quant Time: Sep 06 01:27:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 16:21:27 2021
Response via : Initial Calibration

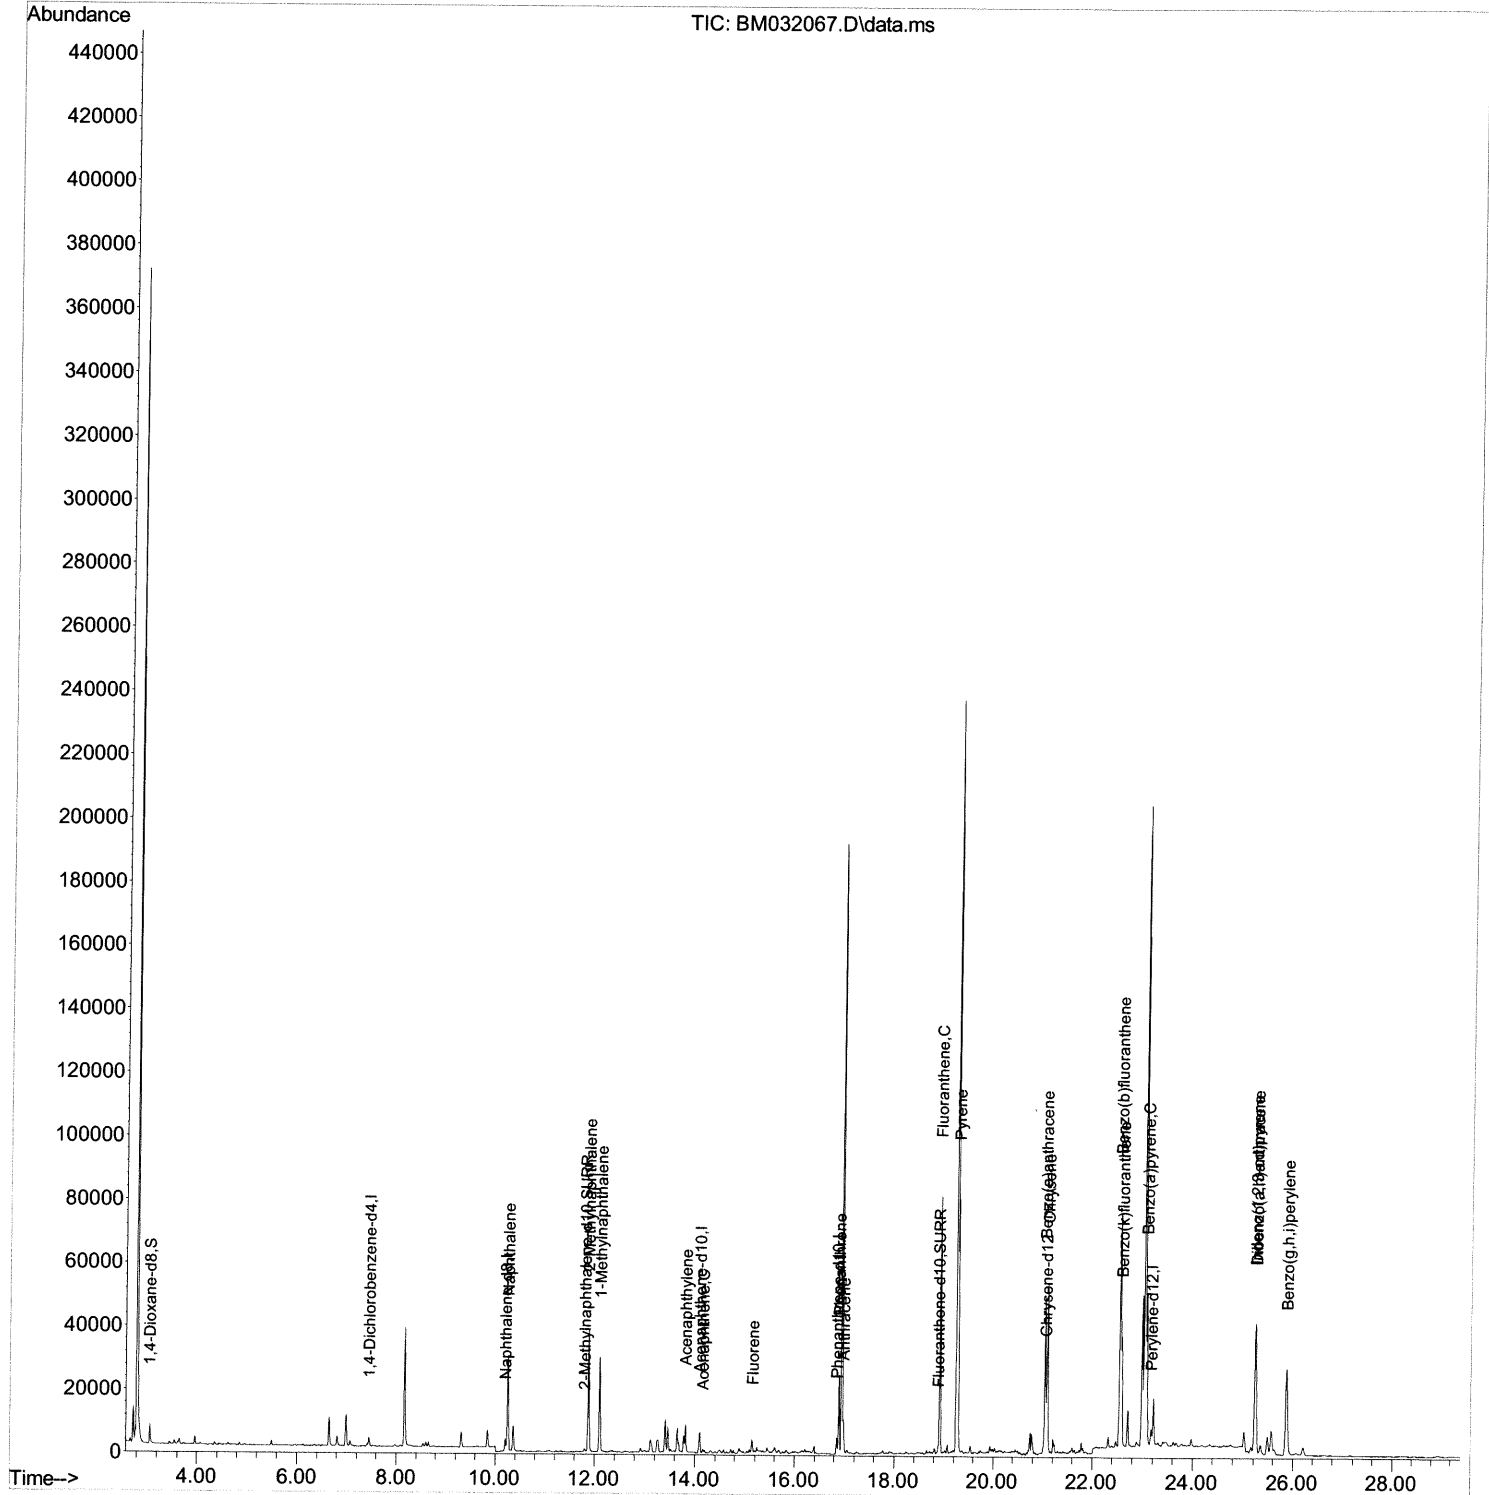

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
 Data File : BM032067.D
 Acq On : 04 Sep 2021 08:39
 Operator : CG/JU
 Sample : M3486-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AY9

Manual Integrations
 APPROVED

mohammad
 9/7/2021 11:38:12 AM

Quant Time: Sep 06 05:39:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 16:21:27 2021
 Response via : Initial Calibration

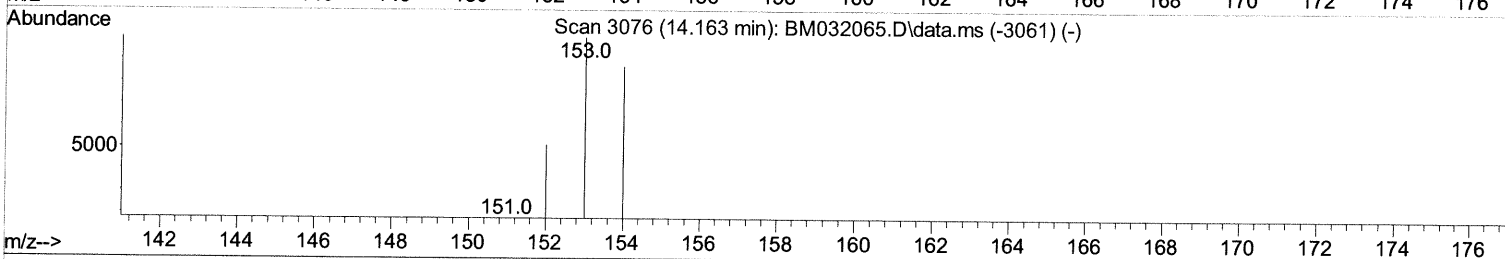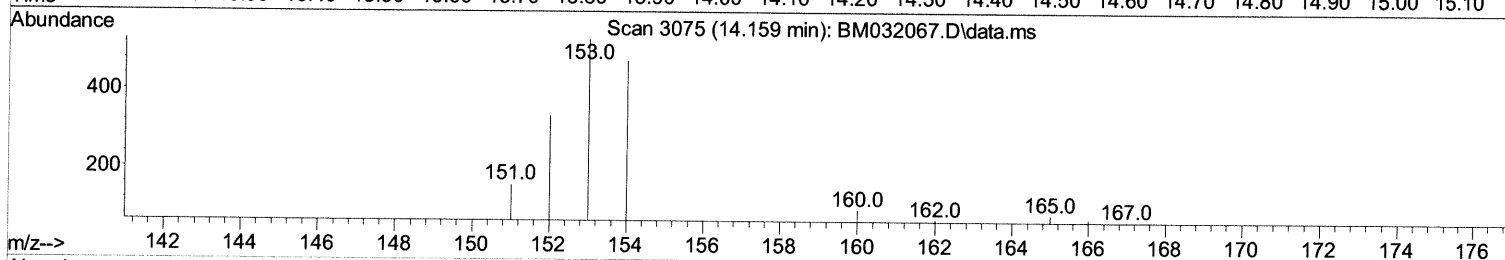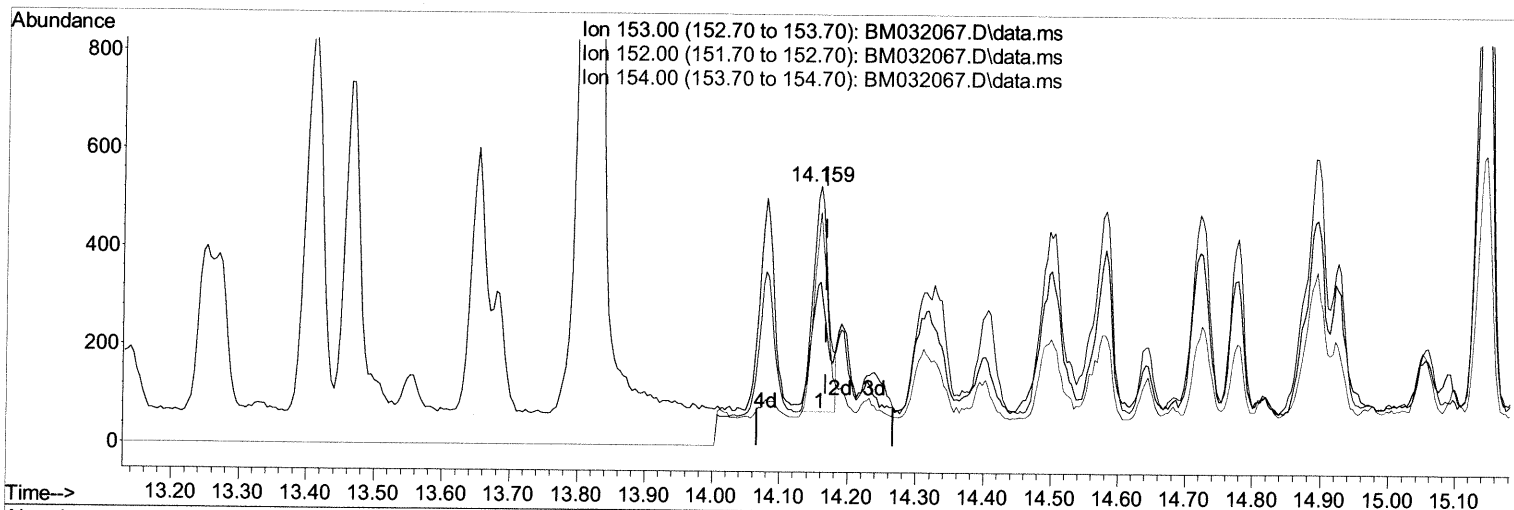

TIC: BM032067.D\data.ms

(11) Acenaphthene (C)

14.159min (-0.008) 0.07 ng/ul

response 715

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	51.20	63.02#
154.00	88.10	90.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
 Data File : BM032067.D
 Acq On : 04 Sep 2021 08:39
 Operator : CG/JU
 Sample : M3486-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AY9

Manual Integrations
 APPROVED

mohammad
 9/7/2021 11:38:12 AM

Quant Time: Sep 06 01:27:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 16:21:27 2021
 Response via : Initial Calibration

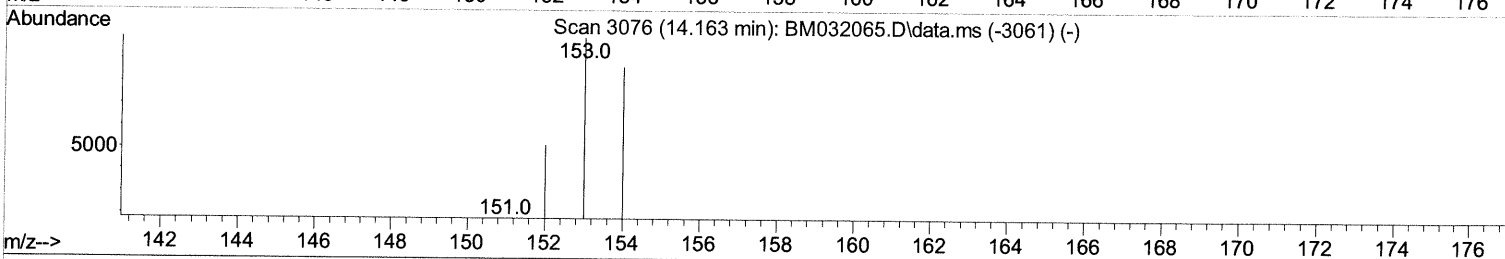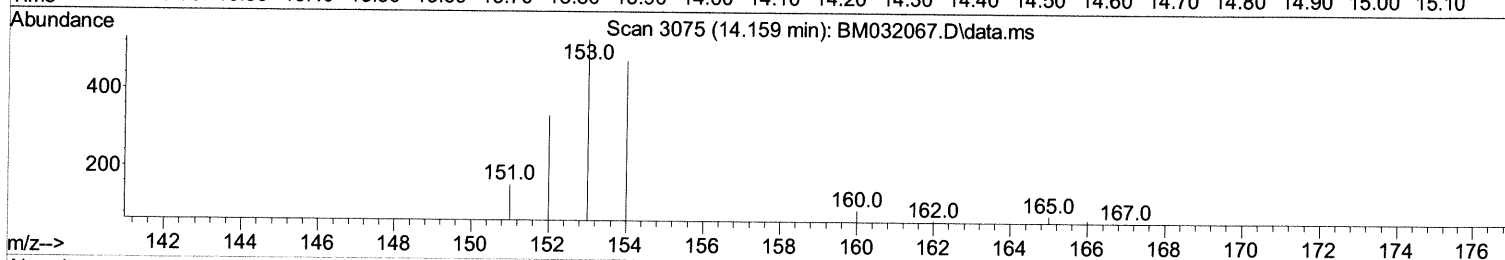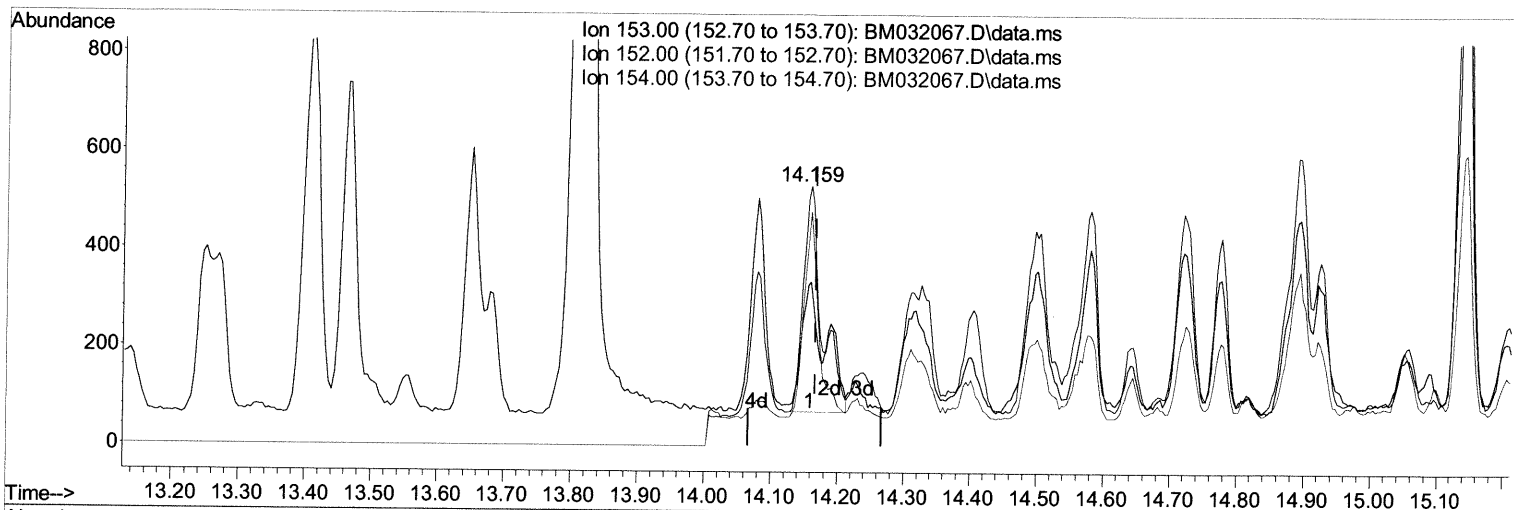

TIC: BM032067.D\data.ms

(11) Acenaphthene (C)

14.159min (-0.008) 0.09 ng/ul m 09/08/21 JU

response 899

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	51.20	63.02#
154.00	88.10	90.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
 Data File : BM032067.D
 Acq On : 04 Sep 2021 08:39
 Operator : CG/JU
 Sample : M3486-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AY9

Manual Integrations
 APPROVED

mohammad
 9/7/2021 11:38:12 AM

Quant Time: Sep 06 05:39:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 16:21:27 2021
 Response via : Initial Calibration

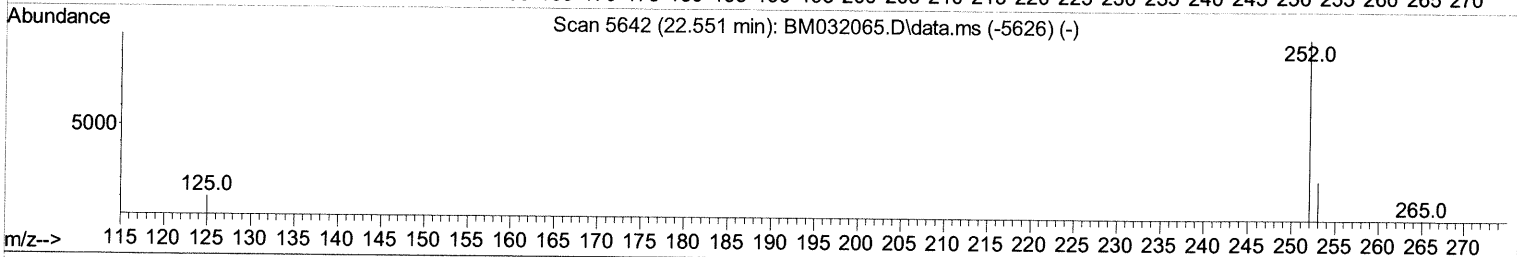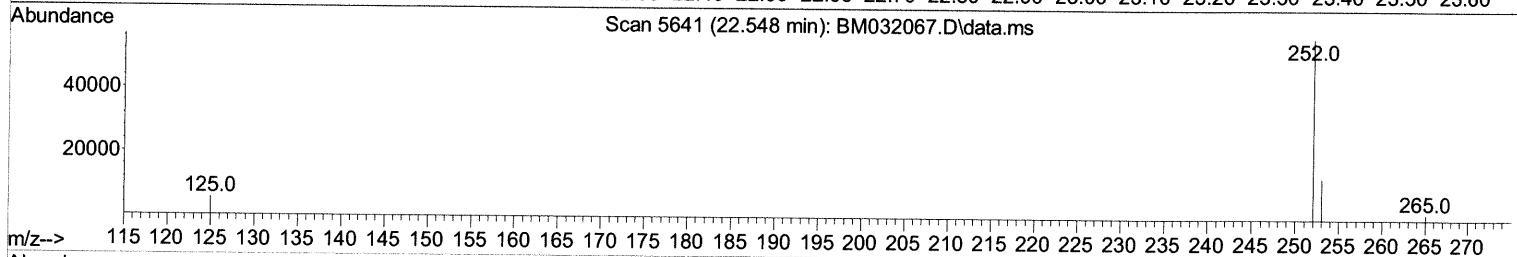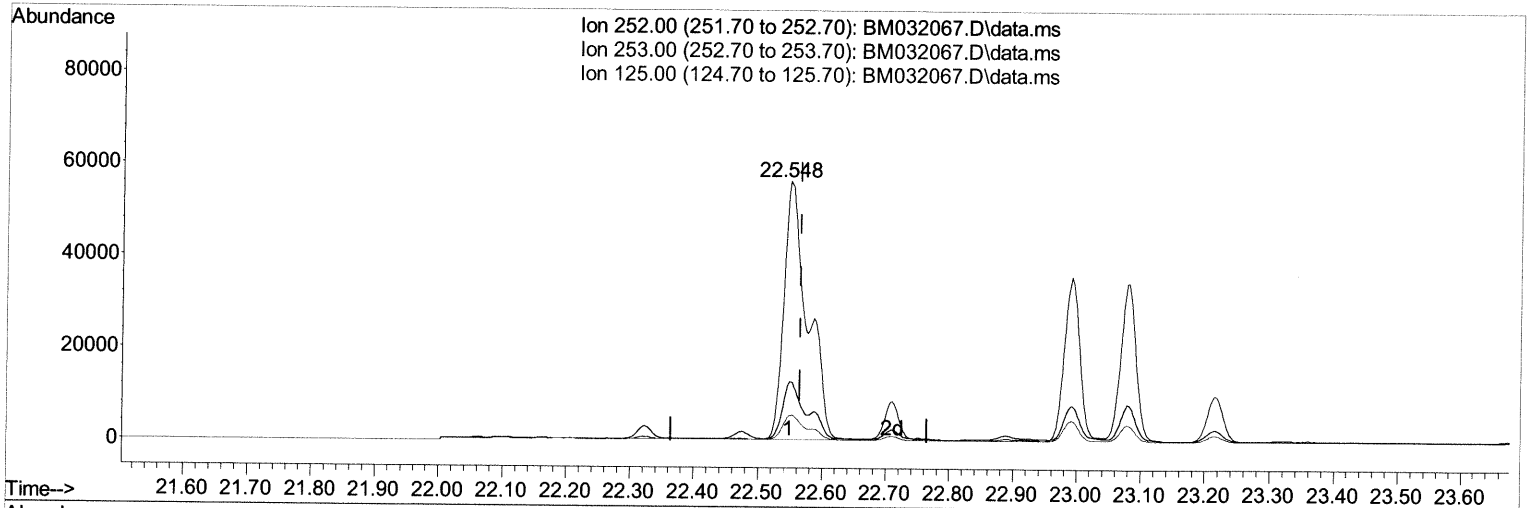

TIC: BM032067.D\data.ms

(24) Benzo(b)fluoranthene

22.548min (-0.017) 5.78 ng/ul

response 145029

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.50	22.92
125.00	14.20	9.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
 Data File : BM032067.D
 Acq On : 04 Sep 2021 08:39
 Operator : CG/JU
 Sample : M3486-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AY9

Manual Integrations
 APPROVED

mohammad
 9/7/2021 11:38:12 AM

Quant Time: Sep 06 01:27:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 16:21:27 2021
 Response via : Initial Calibration

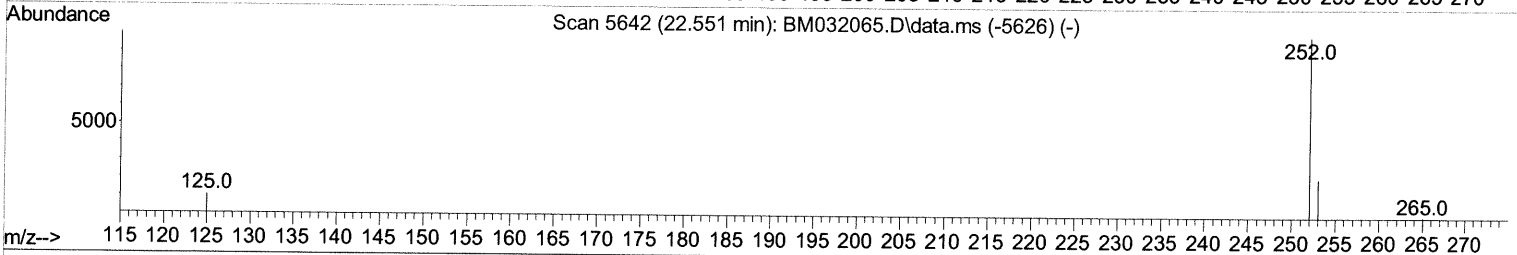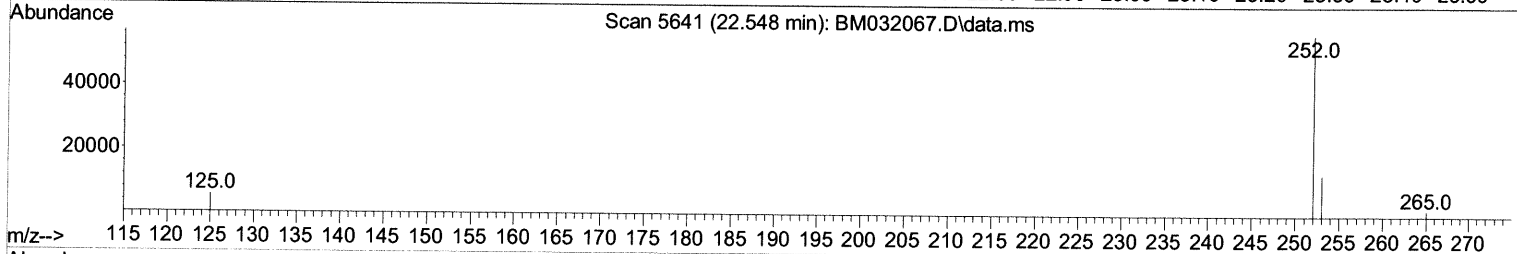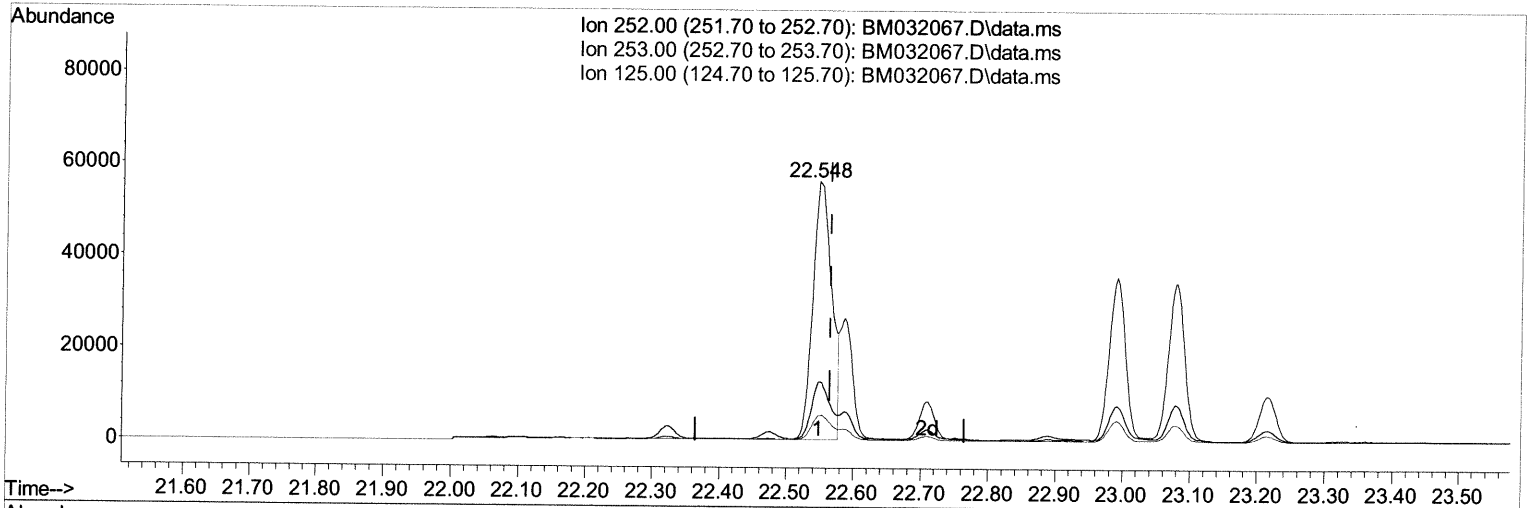

TIC: BM032067.D\data.ms

(24) Benzo(b)fluoranthene

22.548min (-0.017) 4.35 ng/ul m 09/08/21 ju

response 109256

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.50	22.92
125.00	14.20	9.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
Data File : BM032067.D
Acq On : 04 Sep 2021 08:39
Operator : CG/JU
Sample : M3486-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AY9

Manual Integrations
APPROVED

mohammad
9/7/2021 11:38:12 AM

Quant Time: Sep 06 05:39:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 16:21:27 2021
Response via : Initial Calibration

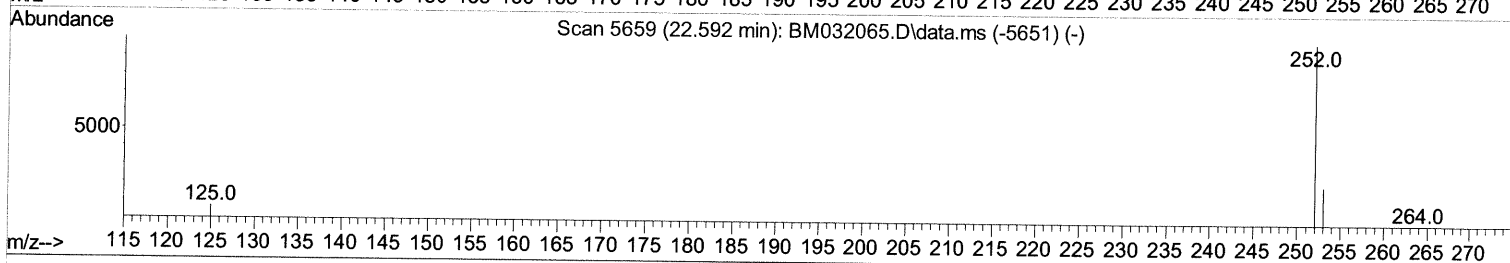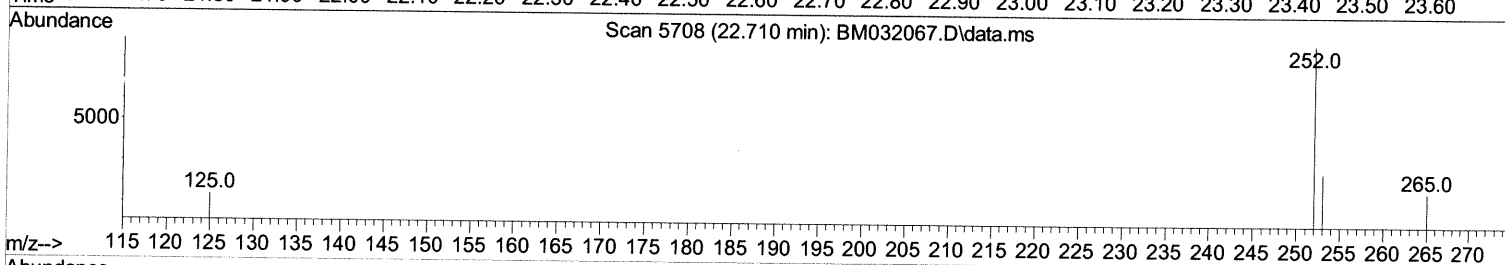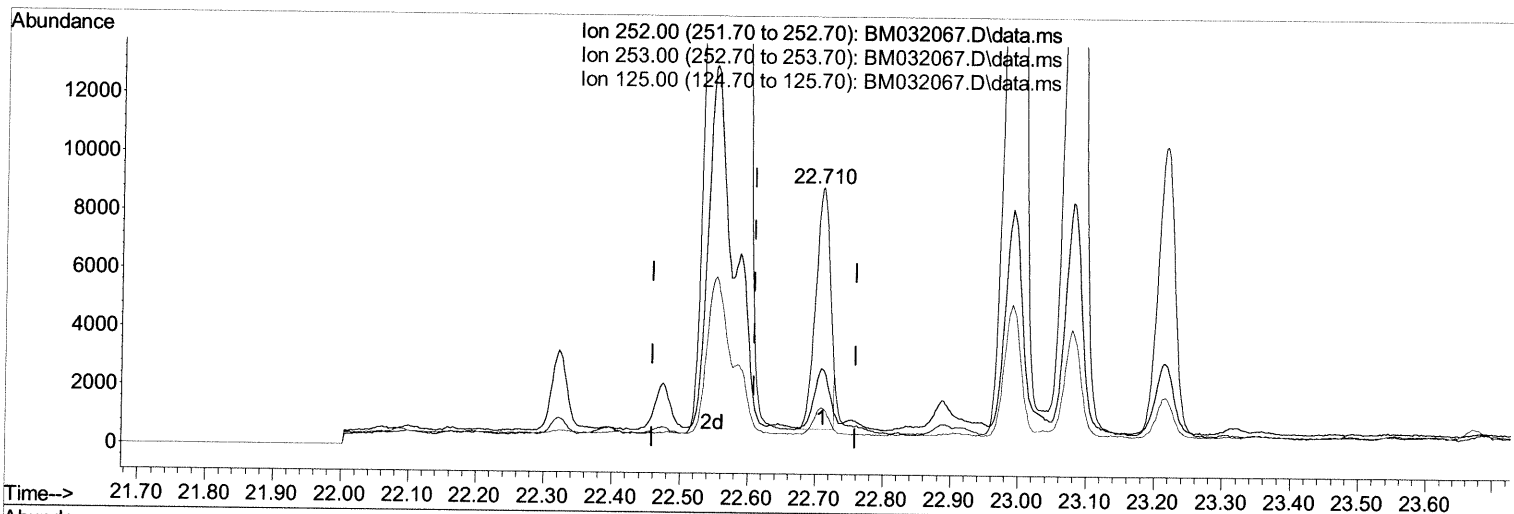

TIC: BM032067.D\data.ms

(25) Benzo(k) fluoranthene

22.710min (+ 0.101) 0.48 ng/ul

response 12335

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.50	30.41
125.00	13.70	15.47
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
 Data File : BM032067.D
 Acq On : 04 Sep 2021 08:39
 Operator : CG/JU
 Sample : M3486-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AY9

Manual Integrations
 APPROVED

mohammad
 9/7/2021 11:38:12 AM

Quant Time: Sep 06 01:27:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 16:21:27 2021
 Response via : Initial Calibration

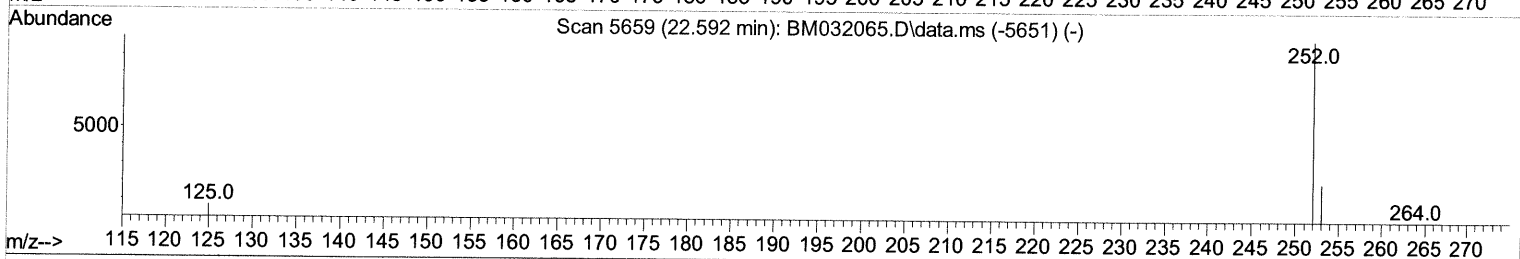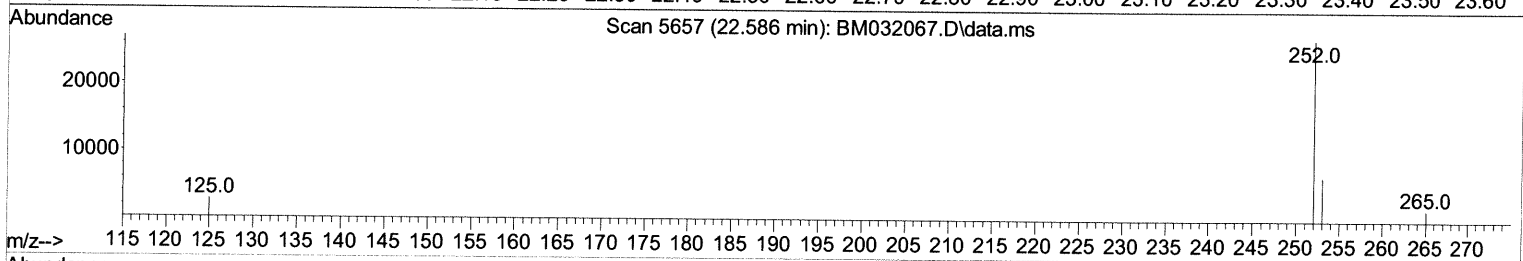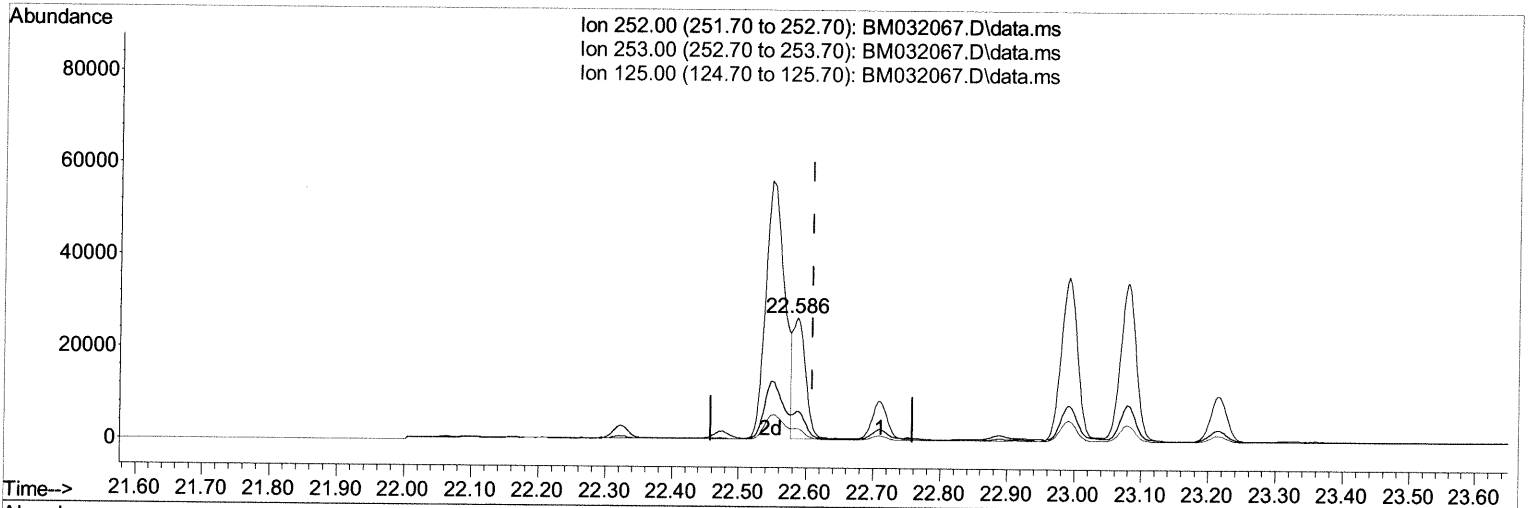

TIC: BM032067.D\data.ms

(25) Benzo(k)fluoranthene

22.586min (-0.022) 1.34 ng/ul m 09/08/21 JU

response 34696

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.50	24.64#
125.00	13.70	10.41#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
 Data File : BM032067.D
 Acq On : 04 Sep 2021 08:39
 Operator : CG/JU
 Sample : M3486-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AY9

Manual Integrations
 APPROVED

mohammad
 9/7/2021 11:38:12 AM

Quant Time: Sep 06 01:27:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 16:21:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.452	152	1545	0.400	ng/ul	0.00
4) Naphthalene-d8	10.207	136	5165	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.094	164	3189	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.851	188	5915	0.400	ng/ul	-0.01
17) Chrysene-d12	21.059	240	5074	0.400	ng/ul	-0.01
23) Perylene-d12	23.170	264	5459	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	3979	2.345	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.803	152	1247	0.156	ng/ul	-0.02
18) Fluoranthene-d10	18.888	212	2510	0.169	ng/ul	-0.02
Target Compounds						
					Qvalue	
5) Naphthalene	10.252	128	40480	2.954	ng/ul	95
7) 2-Methylnaphthalene	11.875	142	27558	2.882	ng/ul	99
8) 1-Methylnaphthalene	12.100	142	20637	2.192	ng/ul	98
10) Acenaphthylene	13.814	152	6877	0.534	ng/ul	100
11) Acenaphthene	14.159	153	899m	0.085	ng/ul	> 09/06/21 JU
12) Fluorene	15.156	166	1246	0.102	ng/ul#	75
15) Phenanthrene	16.893	178	26101	1.450	ng/ul	97
16) Anthracene	16.986	178	10190	0.645	ng/ul	99
19) Fluoranthene	18.919	202	68573	3.127	ng/ul	100
20) Pyrene	19.285	202	67108	2.969	ng/ul	99
21) Benzo(a)anthracene	21.044	228	40247	2.171	ng/ul	99
22) Chrysene	21.095	228	54827	2.575	ng/ul	99
24) Benzo(b)fluoranthene	22.548	252	109256m	4.353	ng/ul	> 09/06/21 JU
25) Benzo(k)fluoranthene	22.586	252	34696m	1.340	ng/ul	>
26) Benzo(a)pyrene	23.078	252	57695	2.631	ng/ul#	82
27) Indeno(1,2,3-cd)pyrene	25.237	276	60806	2.035	ng/ul#	96
28) Dibenzo(a,h)anthracene	25.242	278	14702	0.612	ng/ul	94
29) Benzo(g,h,i)perylene	25.872	276	52035	1.957	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed