

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
 Data File : BM032088.D
 Acq On : 04 Sep 2021 22:10
 Operator : CG/JU
 Sample : M3517-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Quant Time: Sep 06 04:14:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 16:21:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.448	152	1882	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.203	136	6146	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.095	164	2314	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.851	188	4563	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.064	240	3985	0.400	ng/ul	# 0.00
23) Perylene-d12	23.176	264	5218	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.061	96	8029	3.884	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.804	152	2095	0.220	ng/ul	-0.02
18) Fluoranthene-d10	18.892	212	4011	0.343	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.253	128	786	0.048	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090321\
Data File : BM032088.D
Acq On : 04 Sep 2021 22:10
Operator : CG/JU
Sample : M3517-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB8


Quant Time: Sep 06 04:14:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM090321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 16:21:27 2021
Response via : Initial Calibration

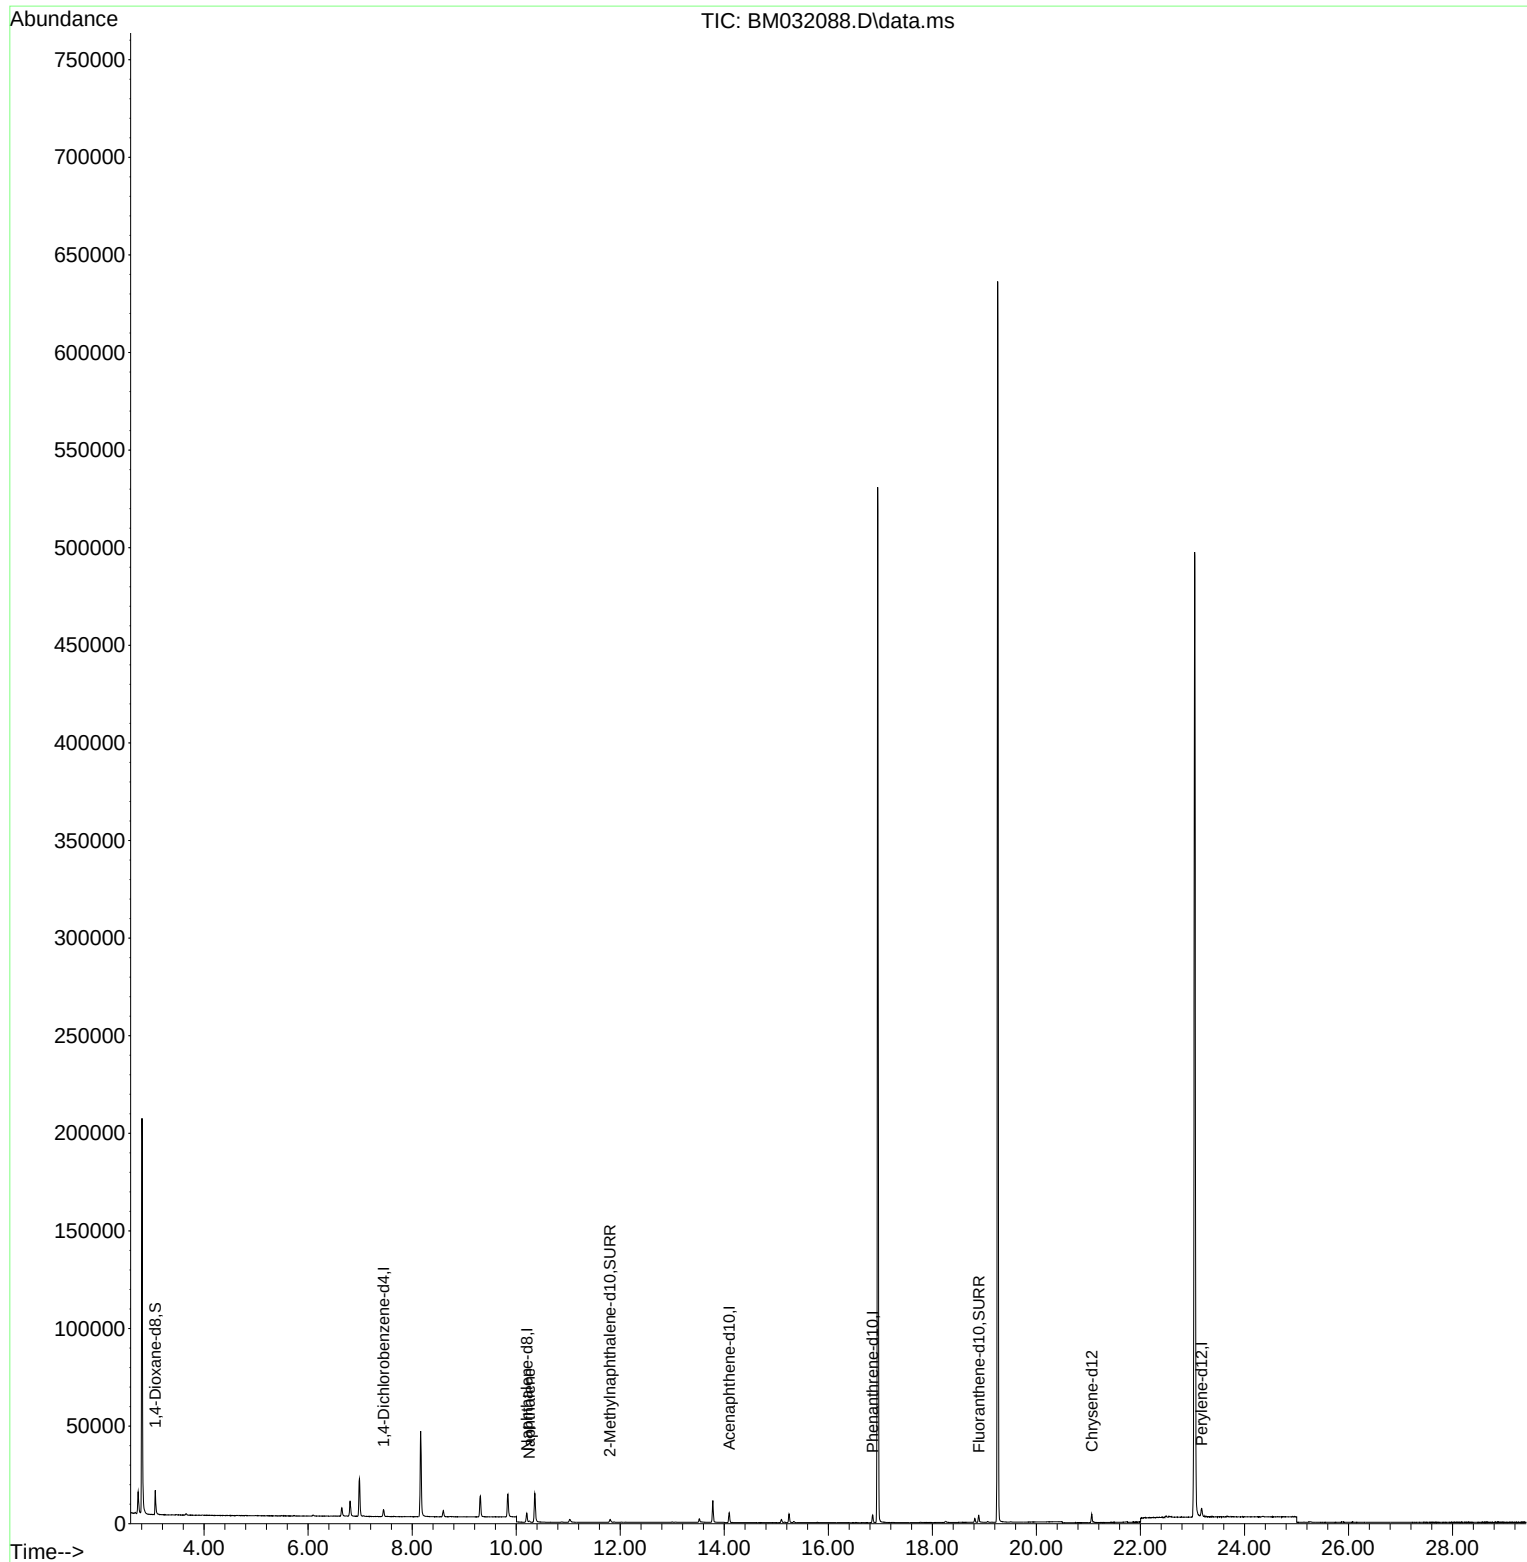

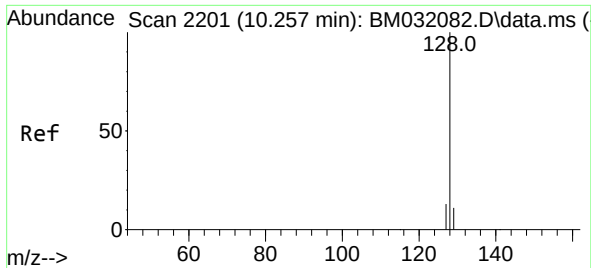

#5
Naphthalene
Concen: 0.048 ng/ul
RT: 10.253 min Scan# 2200
Delta R.T. -0.018 min
Lab File: BM032088.D
Acq: 04 Sep 2021 22:10

Instrument :
BNA_M
ClientSampleId :
C0AB8

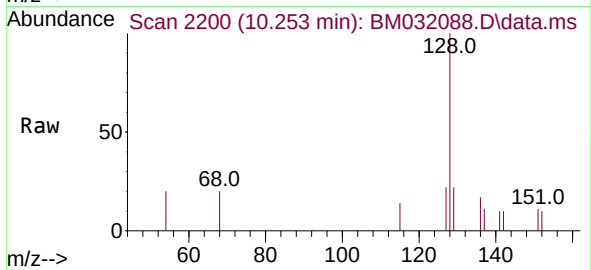

Tgt Ion:	128	Resp:	786
Ion	Ratio	Lower	Upper
128	100		
129	21.8	10.9	16.3#
127	21.6	12.4	18.6#

