
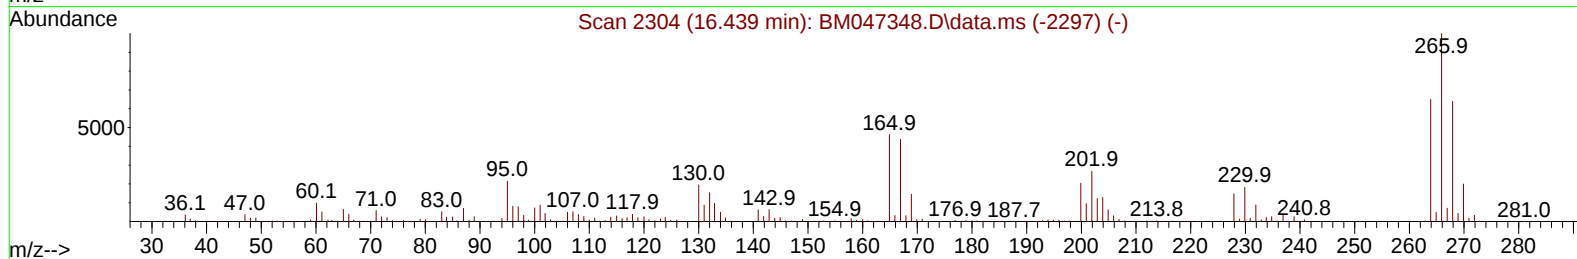
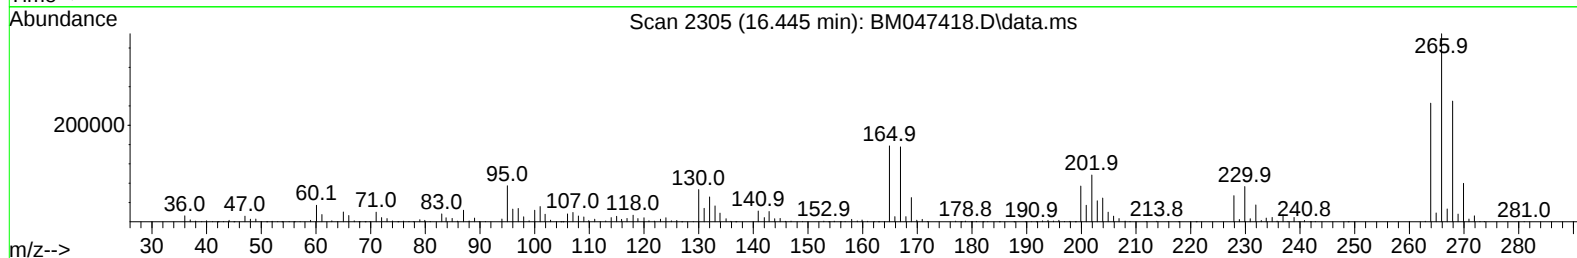


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090324\
Data File : BM047418.D
Acq On : 03 Sep 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:59:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

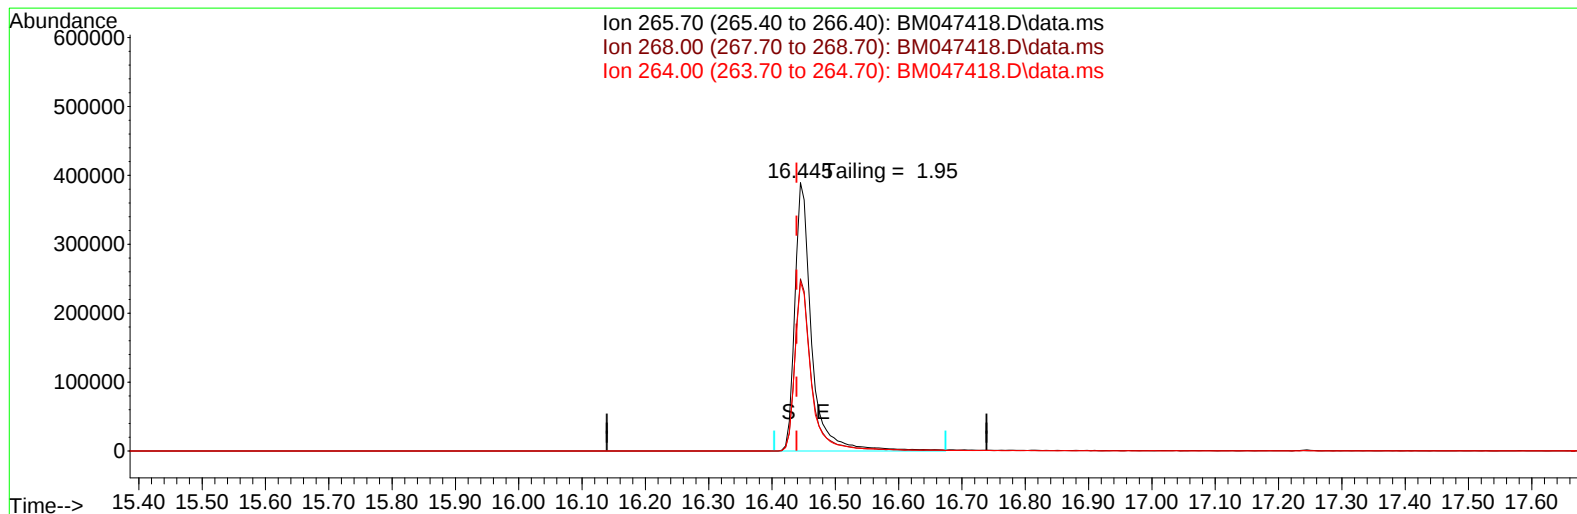

TIC: BM047418.D\data.ms

(70) Pentachlorophenol (C)




16.445min (+ 0.006) 682751.52 ng

response 720722

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.18
264.00	64.90	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090324\
Data File : BM047418.D
Acq On : 03 Sep 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:59:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

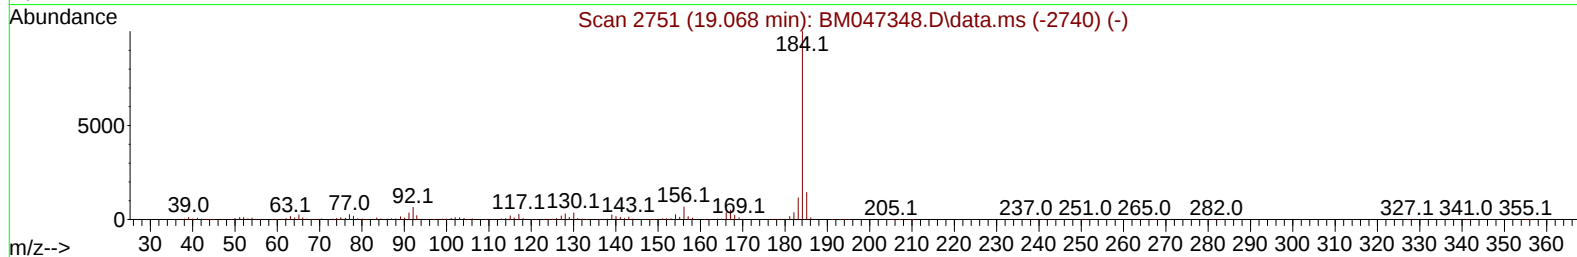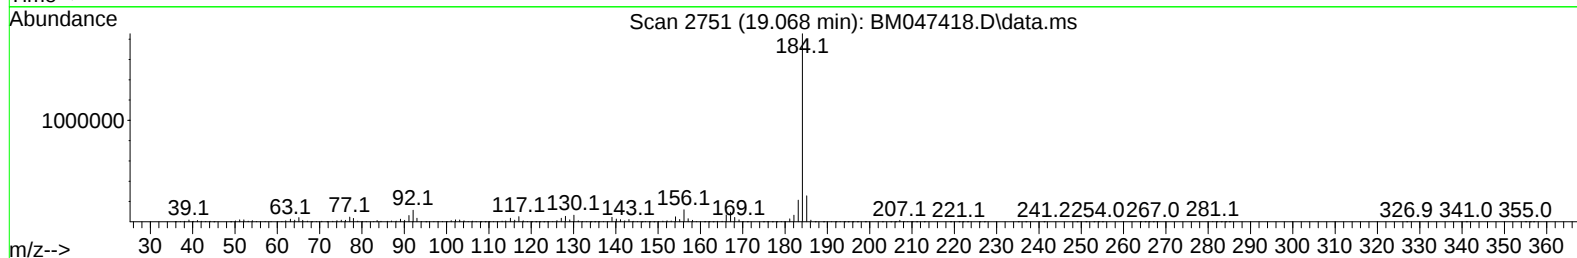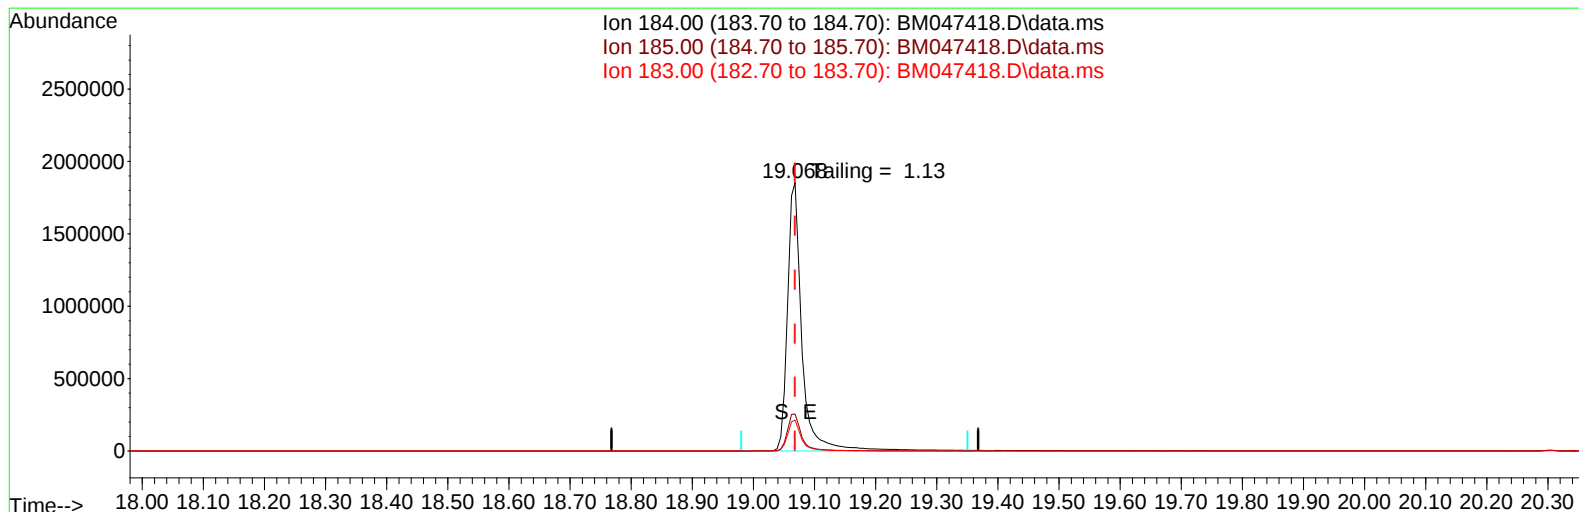

TIC: BM047418.D\data.ms

(77) Benzidine**19.068min (+ 0.000) 65892.32 ng****response 3068706**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.82
183.00	11.50	11.53
0.00	0.00	0.00