


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090324\
Data File : BM047418.D
Acq On : 03 Sep 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

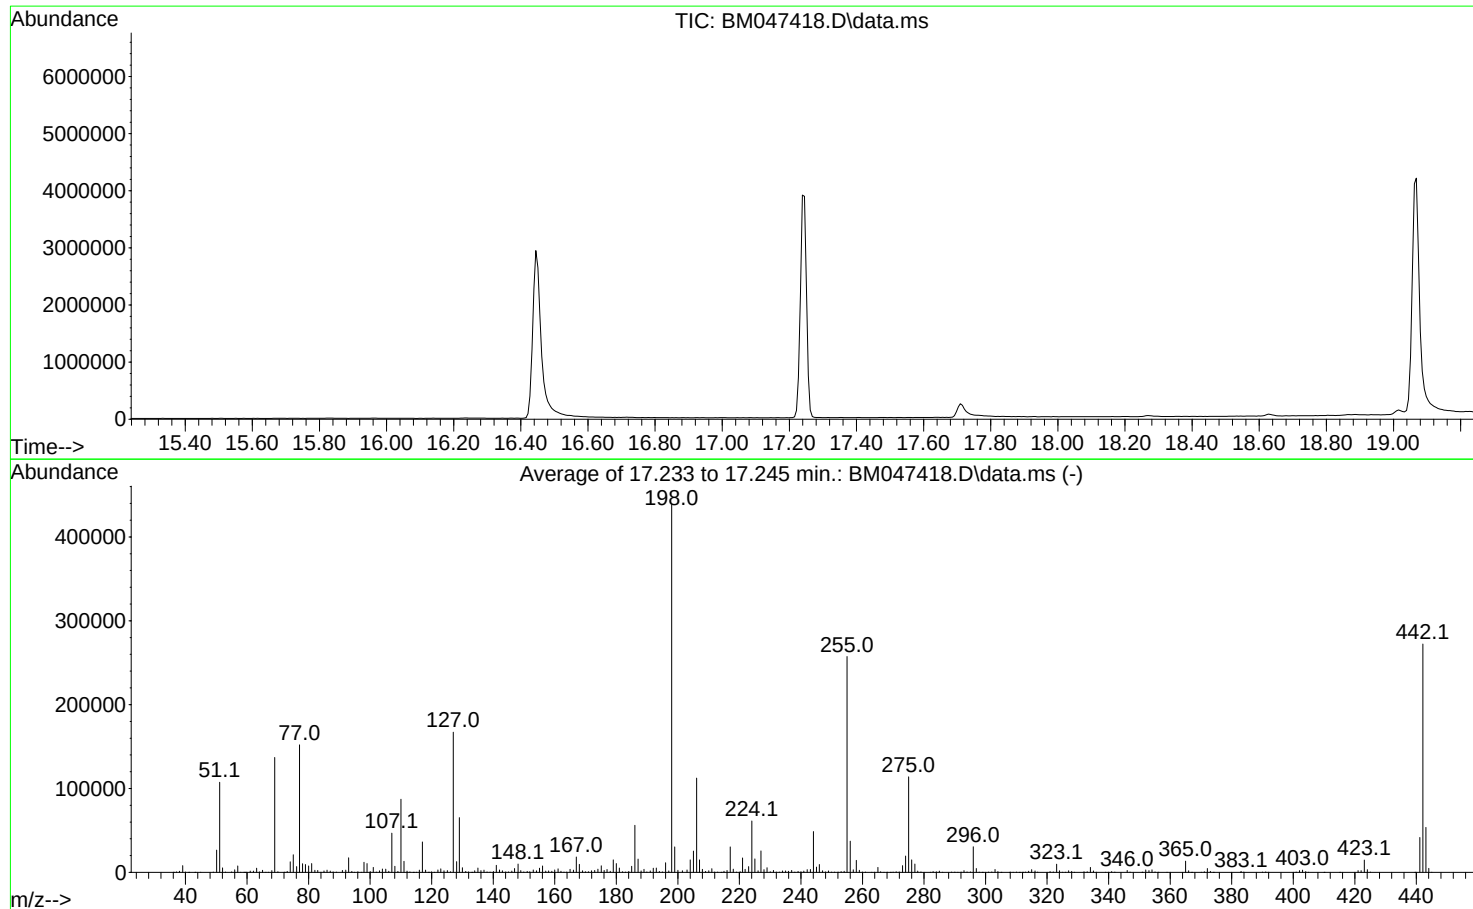




AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.5	107388	PASS
68	69	0.00	2	1.6	2140	PASS
69	198	0.00	100	31.2	137043	PASS
70	69	0.00	2	0.6	813	PASS
127	198	10	80	38.1	167251	PASS
197	198	0.00	2	0.4	1743	PASS
198	198	100	100	100.0	438699	PASS
199	198	5	9	6.9	30341	PASS
275	198	10	60	26.0	113925	PASS
365	198	1	100	3.1	13445	PASS
441	198	0.01	100	9.5	41696	PASS
442	442	50	100	100.0	272379	PASS
443	442	15	24	19.7	53544	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090324\
Data File : BM047418.D
Acq On : 03 Sep 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 03 12:59:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

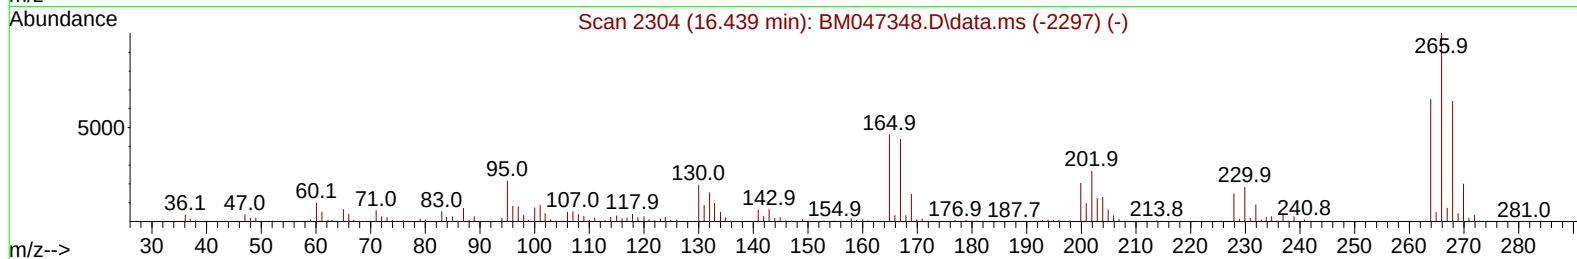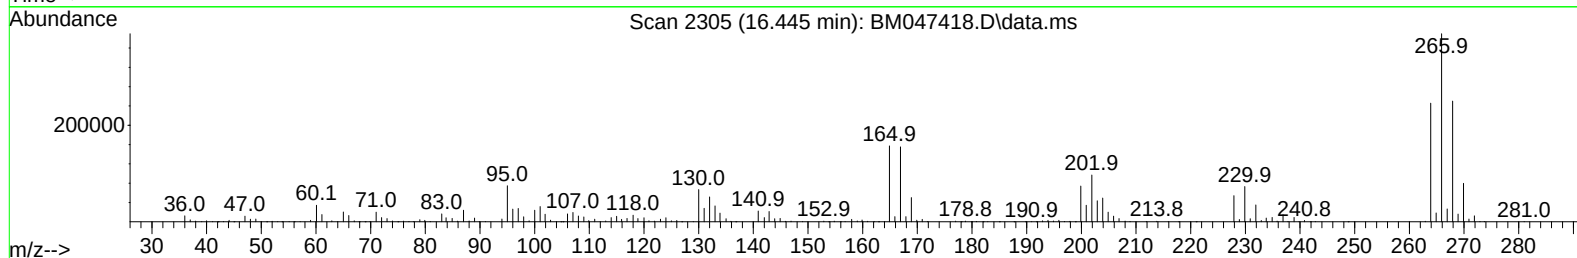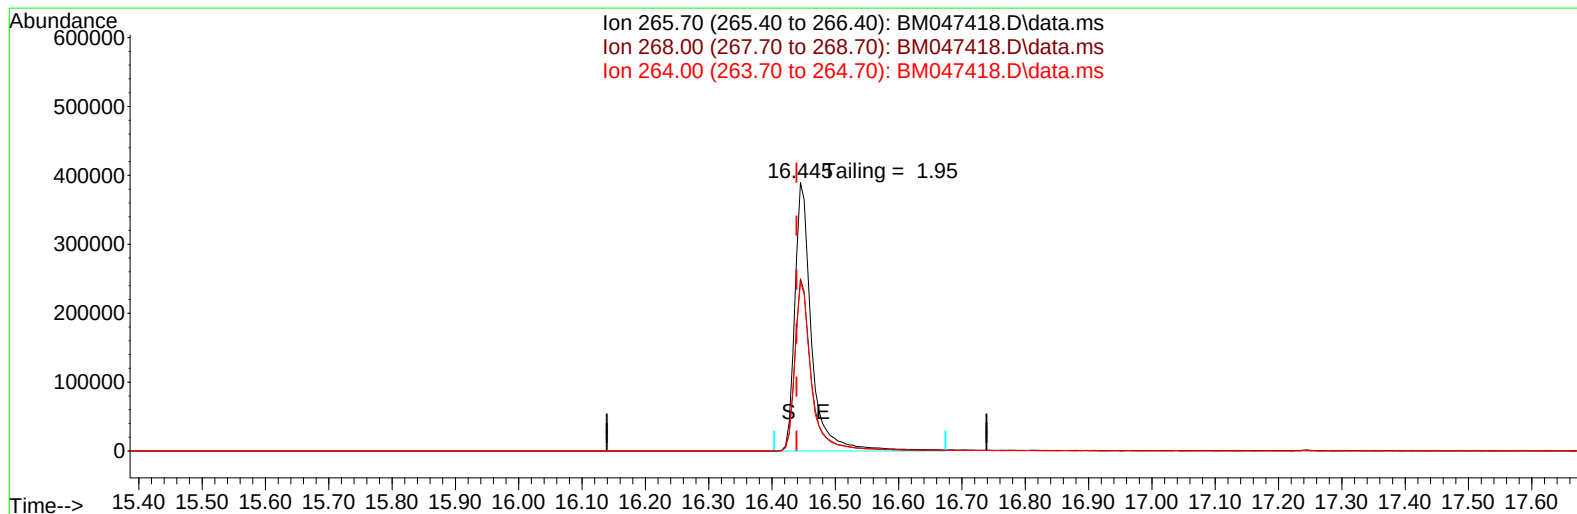

TIC: BM047418.D\data.ms

(70) Pentachlorophenol (C)

16.445min (+ 0.006) 682751.52 ng




response 720722

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.18
264.00	64.90	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090324\
Data File : BM047418.D
Acq On : 03 Sep 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 03 12:59:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

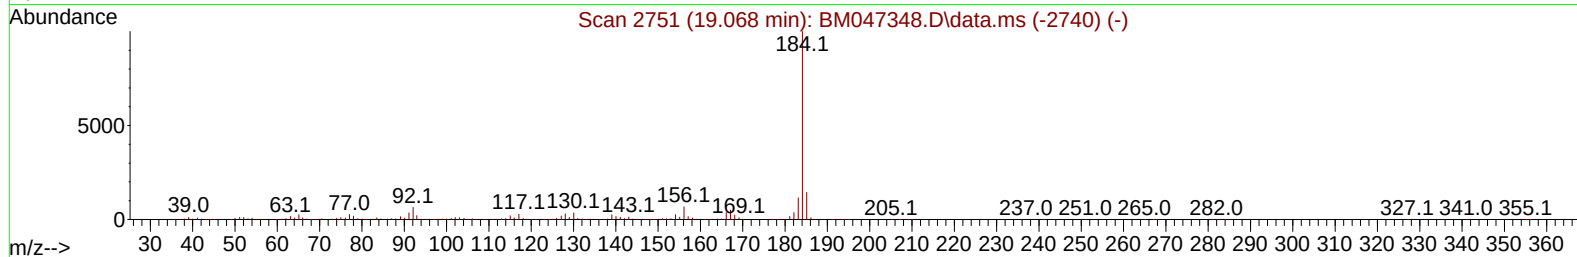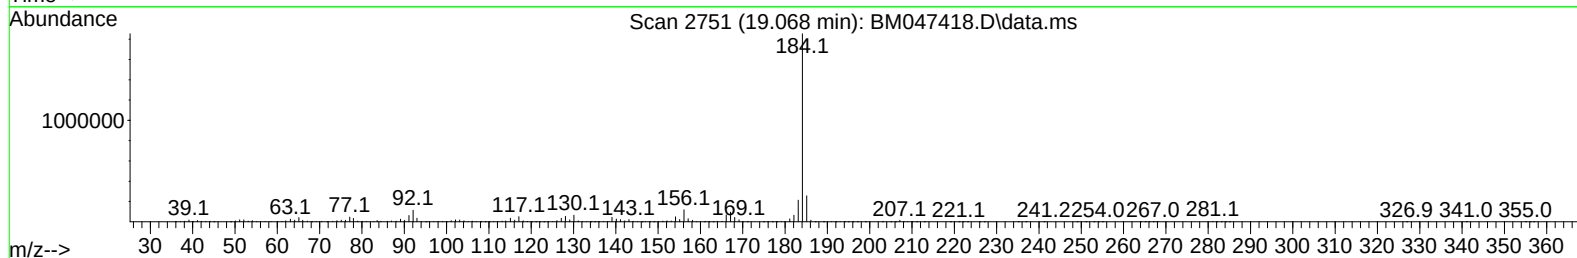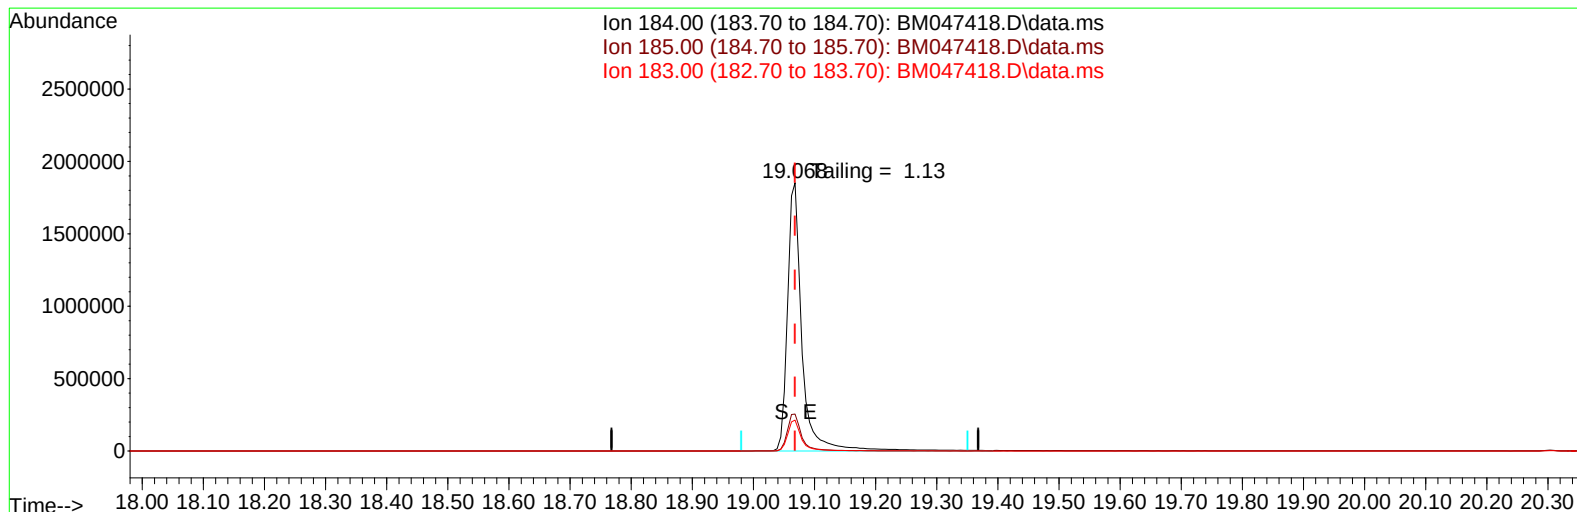

TIC: BM047418.D\data.ms

(77) Benzidine

19.068min (+ 0.000) 65892.32 ng

response 3068706

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.82
183.00	11.50	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/3/2024	BNA_M	<u>BM047418.D</u>
Compound Name	Response	Retention Time
DDT	1587192	20.303
DDD	38105	19.868
DDE	3563	19.345
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41668	1628860	2.56

Instrument :
BNA_M
ClientSampleId :
DFTPP