
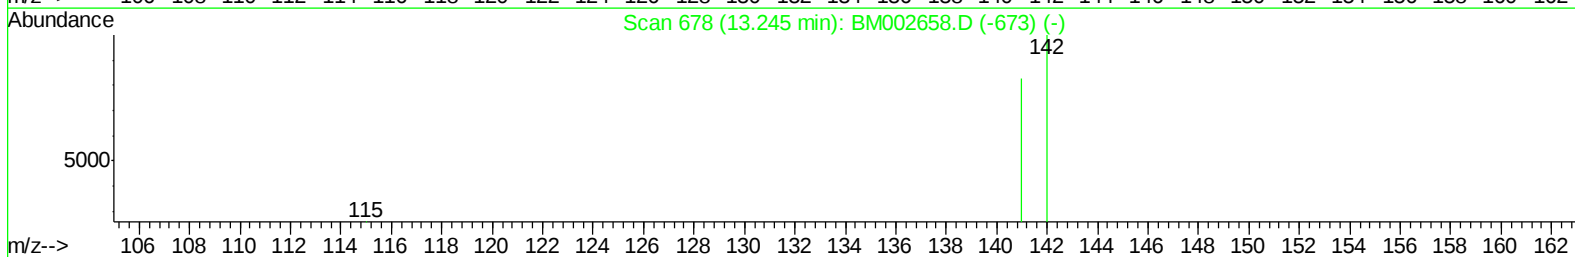
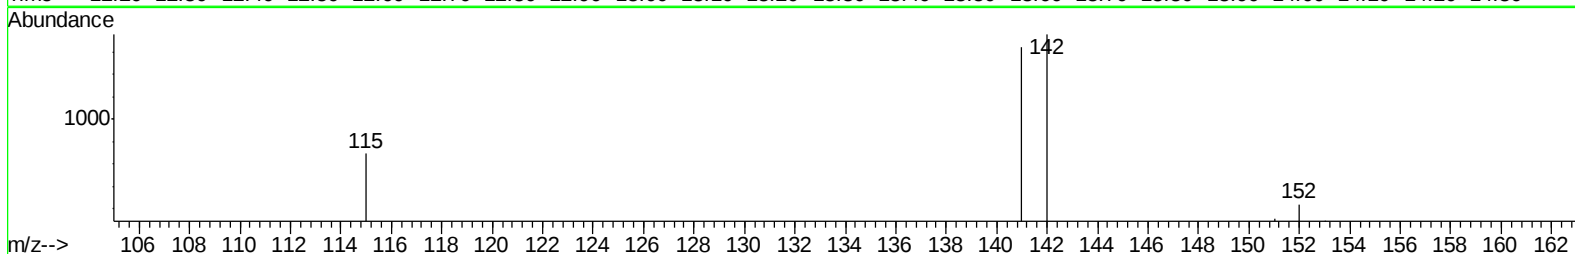


Data Path : Z:\HPCHEM1\BNA_M\Data\BM090415\
Data File : BM002672.D
Acq On : 04 Sep 2015 13:40
Operator : UM/IZ
Sample : MDL-02-S
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Sep 04 14:11:23 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 04 04:35:12 2015
Response via : Initial Calibration

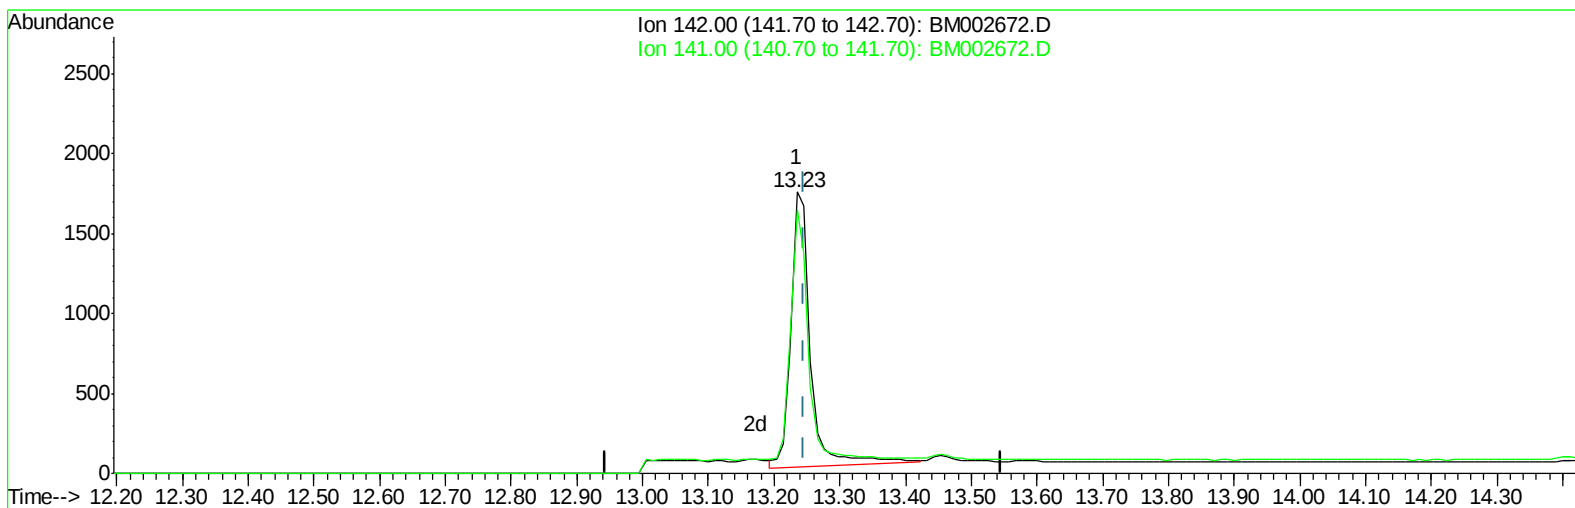

TIC: BM002672.D

(7) 2-Methylnaphthalene




13.235min (-0.010) 0.07ng/ul

response 3576

Ion	Exp%	Act%
142.00	100	100
141.00	87.90	94.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM090415\
Data File : BM002672.D
Acq On : 04 Sep 2015 13:40
Operator : UM/IZ
Sample : MDL-02-S
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Sep 04 14:11:23 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 04 04:35:12 2015
Response via : Initial Calibration

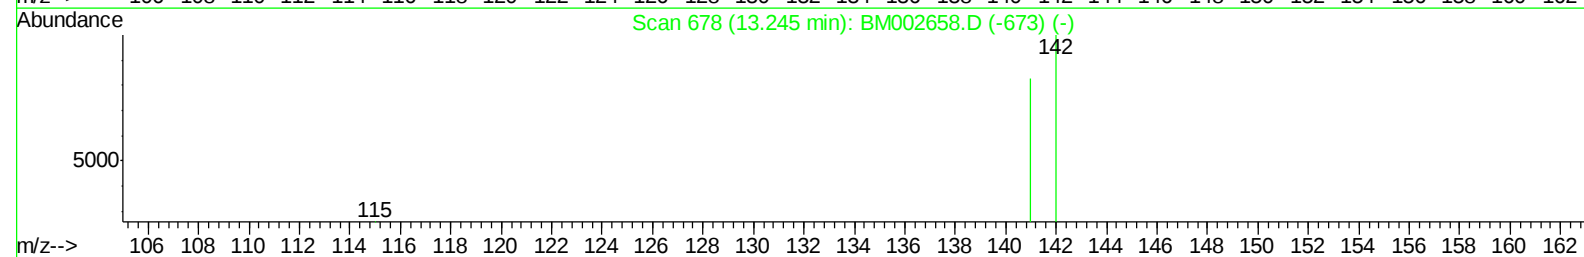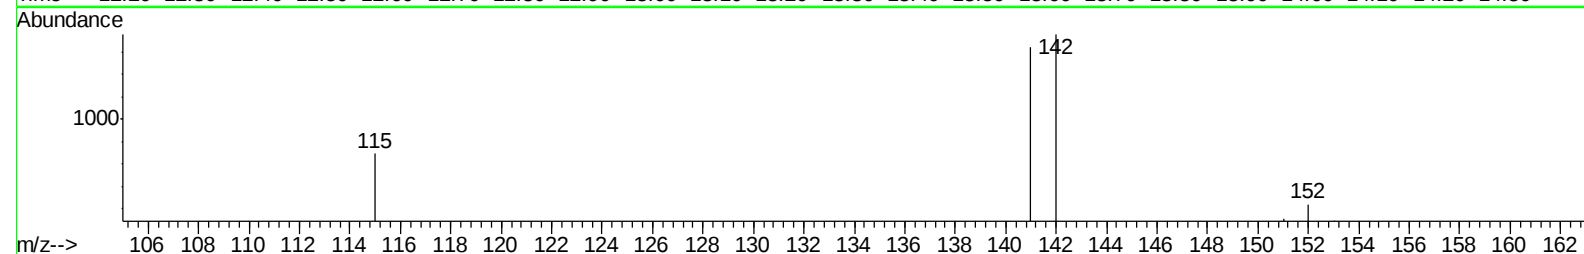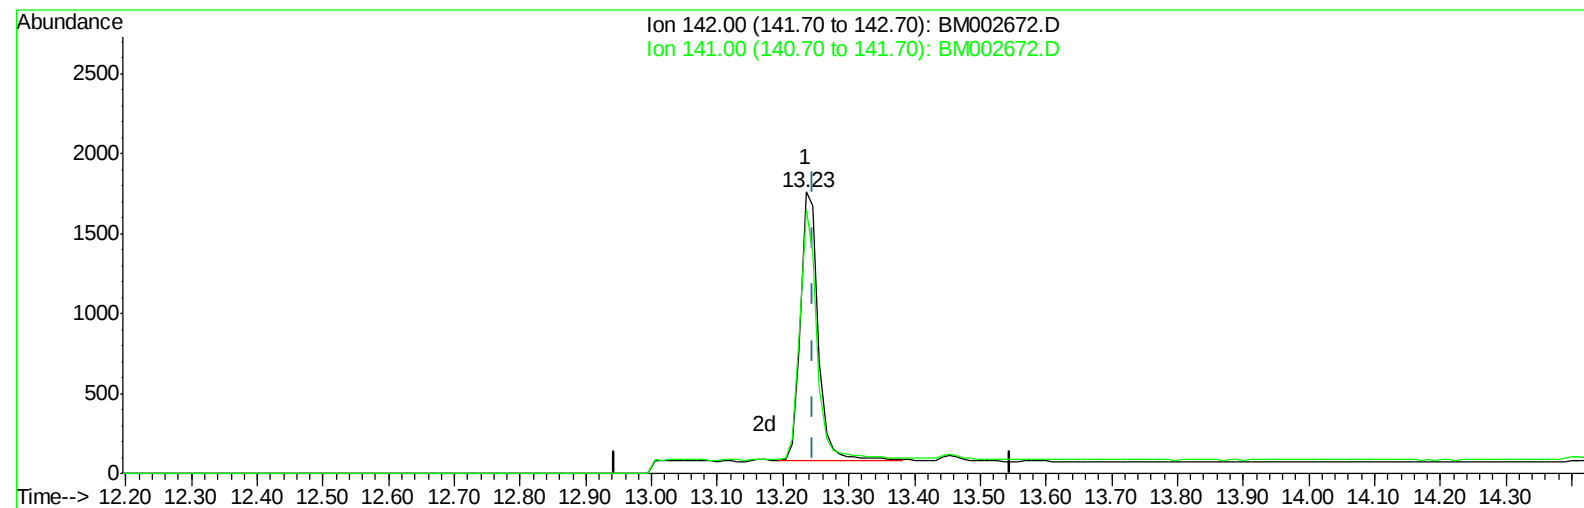

TIC: BM002672.D

(7) 2-Methylnaphthalene

13.235min (-0.010) 0.06ng/ul m

response 3181

Ion	Exp%	Act%
142.00	100	100
141.00	87.90	106.48#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM090415\
 Data File : BM002672.D
 Acq On : 04 Sep 2015 13:40
 Operator : UM/IZ
 Sample : MDL-02-S
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Sep 04 14:12:49 2015

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Sep 04 04:35:12 2015

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.78	152	7897	0.40	ng/ul	0.00
4) Naphthalene-d8	11.64	136	29904	0.40	ng/ul	0.00
8) Acenaphthene-d10	15.36	164	11964	0.40	ng/ul	0.00
12) Phenanthrene-d10	18.08	188	21530	0.40	ng/ul	0.00
18) Chrysene-d12	22.16	240	19467	0.40	ng/ul	0.00
22) Perylene-d12	24.77	264	19311	0.40	ng/ul	-0.01

System Monitoring Compounds

2) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
6) 2-Methylnaphthalene-d10	13.17	152	17806	0.44	ng/ul	0.00
16) Fluoranthene-d10	20.03	212	24468	0.50	ng/ul	-0.01

Target Compounds

					Qvalue
5) Naphthalene	11.69	128	4987	0.06	ng/ul 97
7) 2-Methylnaphthalene	13.23	142	3181m	0.06	ng/ul
9) Acenaphthylene	15.09	152	4192	0.07	ng/ul 98
10) Acenaphthene	15.42	153	2911	0.07	ng/ul 96
11) Fluorene	16.39	166	3008	0.06	ng/ul 91
14) Phenanthrene	18.11	178	4388	0.07	ng/ul 97
15) Anthracene	18.20	178	4100	0.06	ng/ul 96
17) Fluoranthene	20.07	202	4700	0.07	ng/ul 89
19) Pyrene	20.42	202	4795	0.07	ng/ul# 96
20) Benzo(a)anthracene	22.14	228	4453	0.07	ng/ul# 93
21) Chrysene	22.19	228	4259	0.07	ng/ul# 91
23) Benzo(b)fluoranthene	23.96	252	5039	0.07	ng/ul# 67
24) Benzo(k)fluoranthene	24.01	252	4207	0.07	ng/ul# 65
25) Benzo(a)pyrene	24.66	252	4231	0.07	ng/ul# 60
26) Indeno(1,2,3-cd)pyrene	27.54	276	5198	0.07	ng/ul 99
27) Dibenzo(a,h)anthracene	27.54	278	4120	0.07	ng/ul# 80
28) Benzo(g,h,i)perylene	28.40	276	4447	0.07	ng/ul# 84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM090415\
Data File : BM002672.D
Acq On : 04 Sep 2015 13:40
Operator : UM/IZ
Sample : MDL-02-S
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Sep 04 14:12:49 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 04 04:35:12 2015
Response via : Initial Calibration

