

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090415\
 Data File : BM002672.D
 Acq On : 04 Sep 2015 13:40
 Operator : UM/IZ
 Sample : MDL-02-S
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-02-S

Quant Time: Sep 04 14:12:49 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 04 04:35:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.78	152	7897	0.40	ng/ul	0.00
4) Naphthalene-d8	11.64	136	29904	0.40	ng/ul	0.00
8) Acenaphthene-d10	15.36	164	11964	0.40	ng/ul	0.00
12) Phenanthrene-d10	18.08	188	21530	0.40	ng/ul	0.00
18) Chrysene-d12	22.16	240	19467	0.40	ng/ul	0.00
22) Perylene-d12	24.77	264	19311	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
6) 2-Methylnaphthalene-d10	13.17	152	17806	0.44	ng/ul	0.00
16) Fluoranthene-d10	20.03	212	24468	0.50	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Naphthalene	11.69	128	4987	0.06	ng/ul	97
7) 2-Methylnaphthalene	13.23	142	3181m	0.06	ng/ul	
9) Acenaphthylene	15.09	152	4192	0.07	ng/ul	98
10) Acenaphthene	15.42	153	2911	0.07	ng/ul	96
11) Fluorene	16.39	166	3008	0.06	ng/ul	91
14) Phenanthrene	18.11	178	4388	0.07	ng/ul	97
15) Anthracene	18.20	178	4100	0.06	ng/ul	96
17) Fluoranthene	20.07	202	4700	0.07	ng/ul	89
19) Pyrene	20.42	202	4795	0.07	ng/ul#	96
20) Benzo(a)anthracene	22.14	228	4453	0.07	ng/ul#	93
21) Chrysene	22.19	228	4259	0.07	ng/ul#	91
23) Benzo(b)fluoranthene	23.96	252	5039	0.07	ng/ul#	67
24) Benzo(k)fluoranthene	24.01	252	4207	0.07	ng/ul#	65
25) Benzo(a)pyrene	24.66	252	4231	0.07	ng/ul#	60
26) Indeno(1,2,3-cd)pyrene	27.54	276	5198	0.07	ng/ul	99
27) Dibenzo(a,h)anthracene	27.54	278	4120	0.07	ng/ul#	80
28) Benzo(g,h,i)perylene	28.40	276	4447	0.07	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090415\
Data File : BM002672.D
Acq On : 04 Sep 2015 13:40
Operator : UM/IZ
Sample : MDL-02-S
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-02-S

Quant Time: Sep 04 14:12:49 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 04 04:35:12 2015
Response via : Initial Calibration

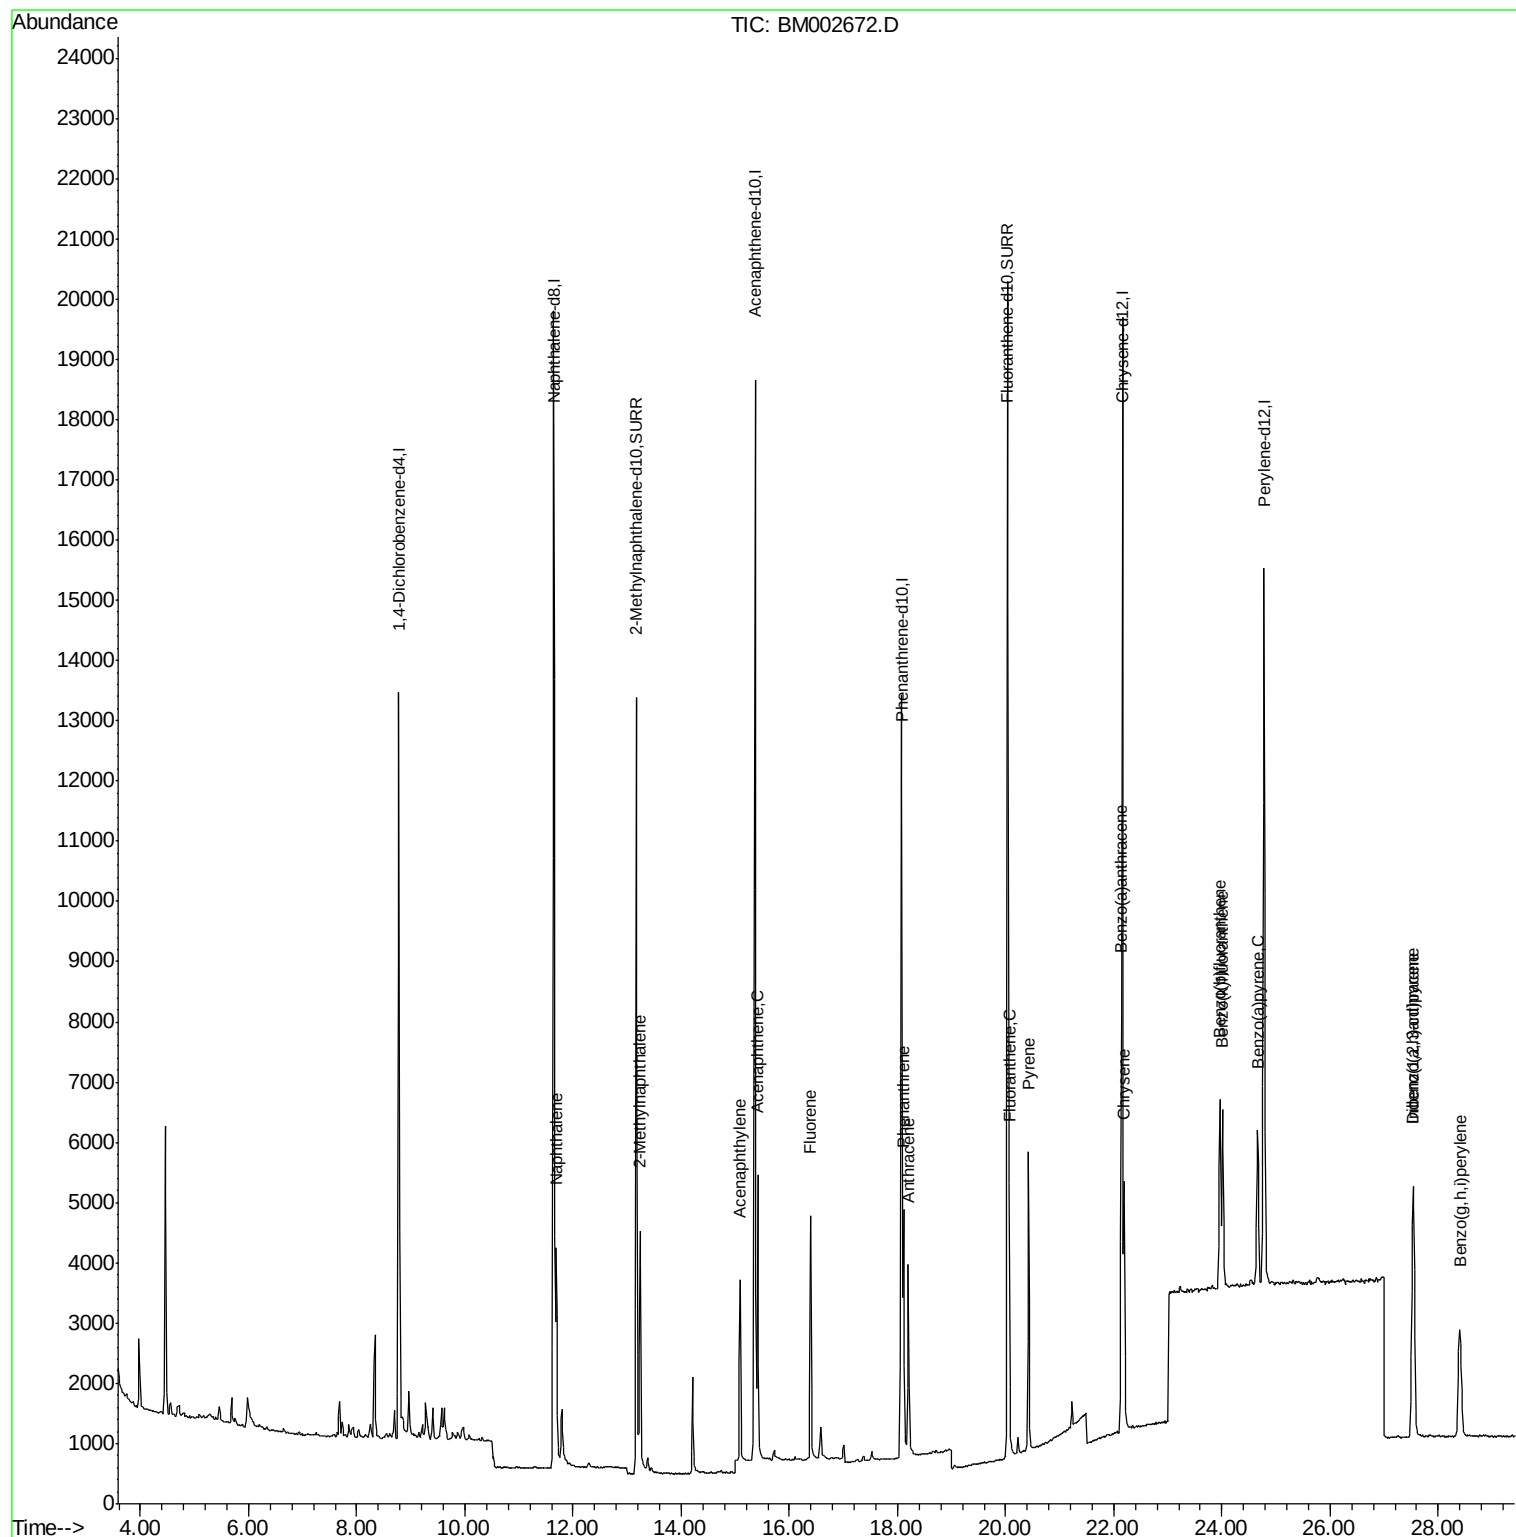

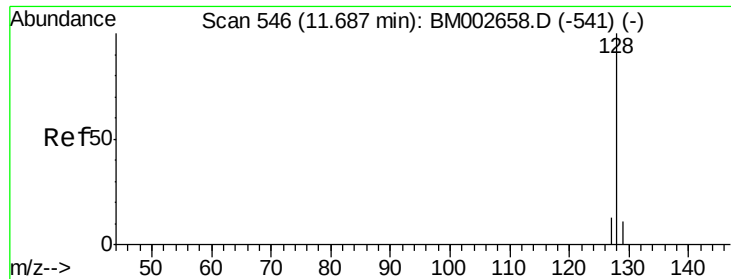

#5

Naphthalene

Concen: 0.06 ng/ul

RT: 11.69 min Scan# 546

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S


Tgt Ion:128 Resp: 4987

Ion Ratio Lower Upper

128 100

129 13.5 9.8 14.8




127 14.5 10.7 16.1



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

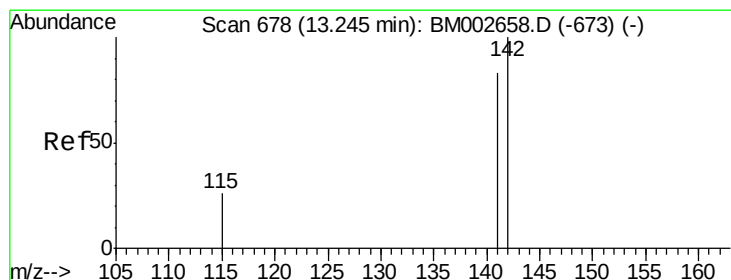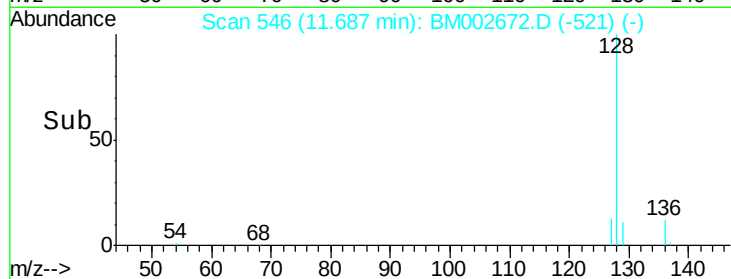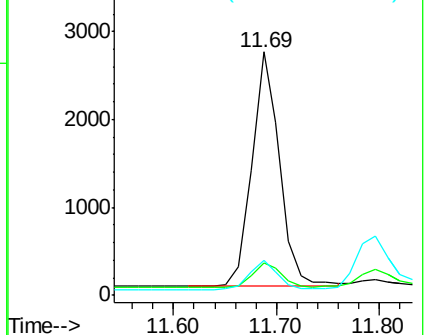

#7

2-Methylnaphthalene

Concen: 0.06 ng/ul m

RT: 13.23 min Scan# 677

Delta R.T. -0.01 min

Lab File: BM002672.D


Acq: 04 Sep 2015 13:40

Tgt Ion:142 Resp: 3181

Ion Ratio Lower Upper



142 100


141 106.5 70.3 105.5#

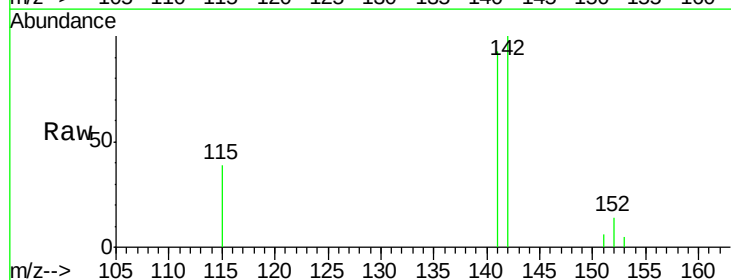

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

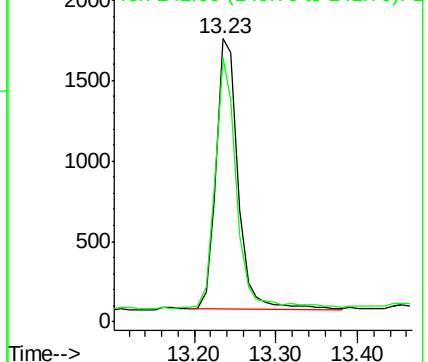



#9

Acenaphthylene

Concen: 0.07 ng/ul

RT: 15.09 min Scan# 852

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S





Tgt Ion:152 Resp: 4192

Ion Ratio Lower Upper

152 100

151 20.6 16.8 25.2

153 15.8 11.3 16.9

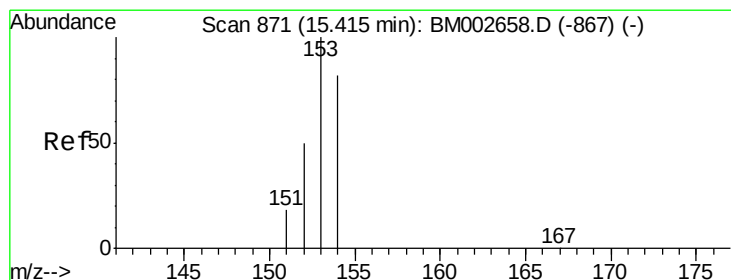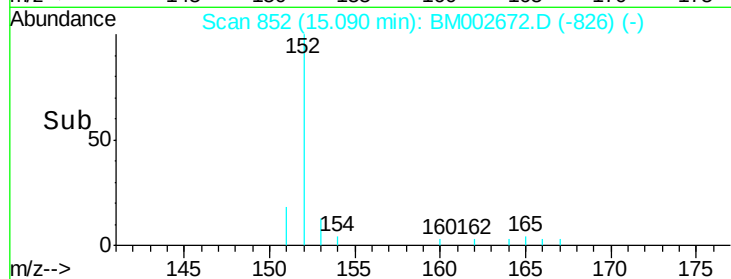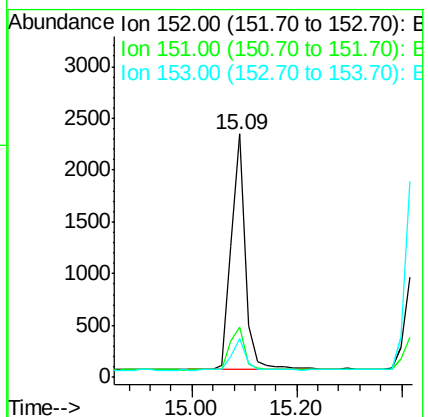

#10

Acenaphthene

Concen: 0.07 ng/ul

RT: 15.42 min Scan# 871

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40




Tgt Ion:153 Resp: 2911


Ion Ratio Lower Upper

153 100

152 51.1 42.3 63.5

154 84.6 64.7 97.1



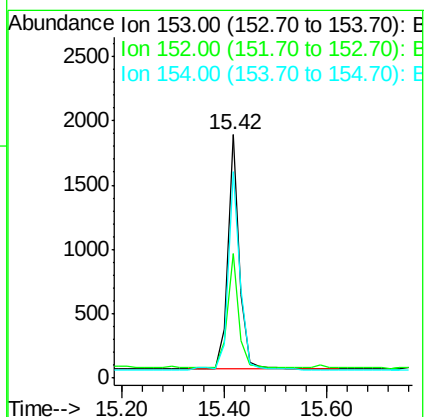



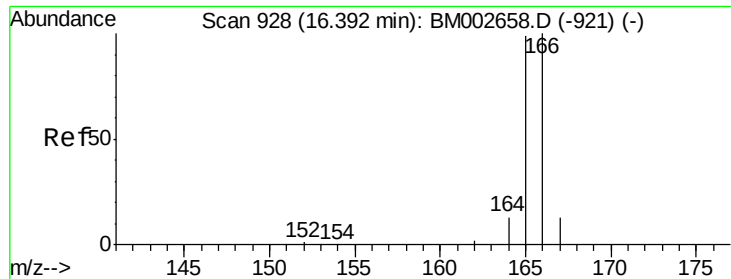

#11
Fluorene
 Concen: 0.06 ng/ul
 RT: 16.39 min Scan# 928
 Delta R.T. 0.00 min
 Lab File: BM002672.D
 Acq: 04 Sep 2015 13:40




Instrument :
 BNA_M
 ClientSampleId :
 MDL-02-S


Tgt Ion:166 Resp: 3008
 Ion Ratio Lower Upper
 166 100
 165 99.6 87.6 131.4
 167 16.1 11.1 16.7

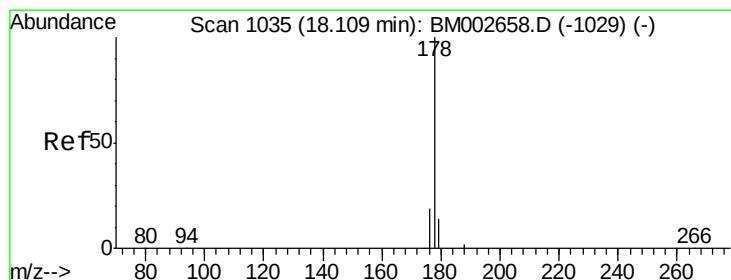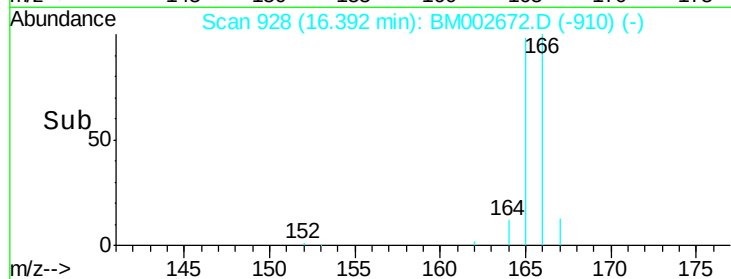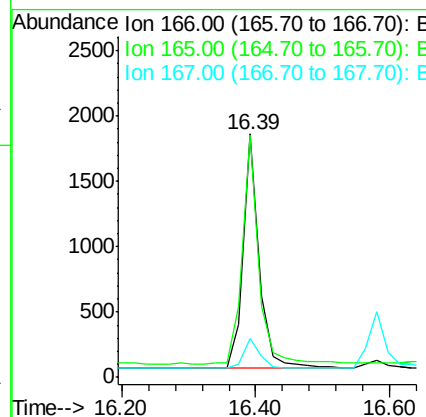

#14
Phenanthrene
 Concen: 0.07 ng/ul
 RT: 18.11 min Scan# 1035
 Delta R.T. 0.00 min
 Lab File: BM002672.D
 Acq: 04 Sep 2015 13:40

Tgt Ion:178 Resp: 4388
 Ion Ratio Lower Upper
 178 100
 176 20.9 16.2 24.4
 179 18.4 12.8 19.2

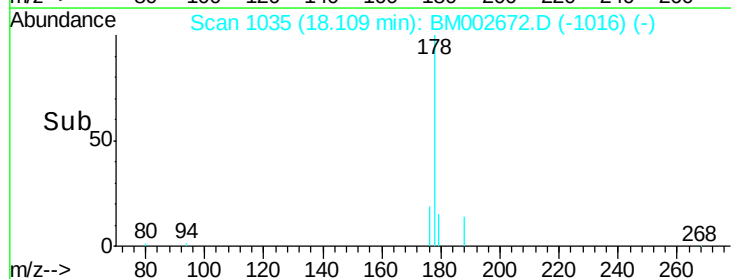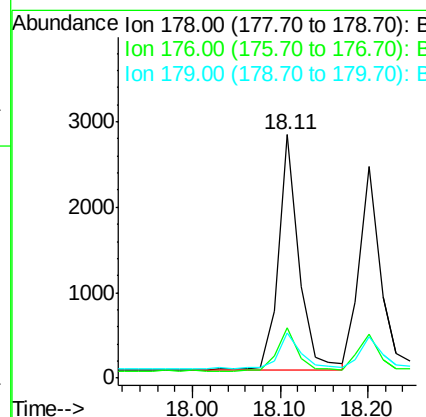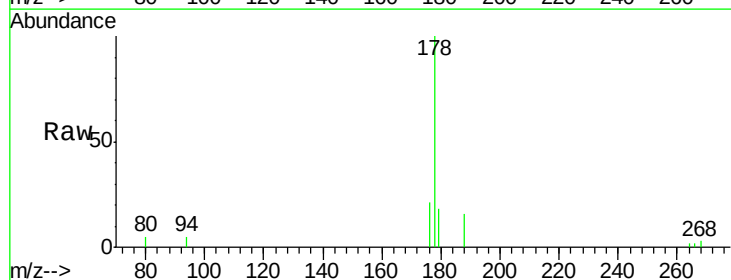

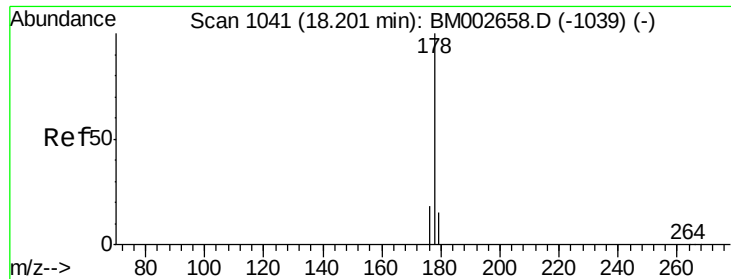

#15

Anthracene

Concen: 0.06 ng/ul

RT: 18.20 min Scan# 1041

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S


Tgt Ion:178 Resp: 4100

Ion Ratio Lower Upper

178 100

176 20.5 15.8 23.8




179 19.4 13.3 19.9



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

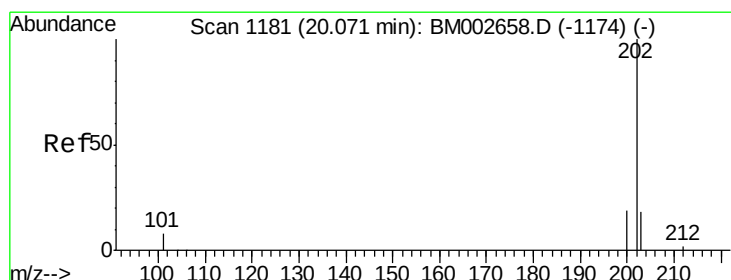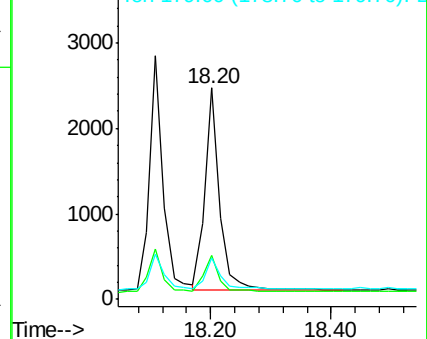

#17

Fluoranthene

Concen: 0.07 ng/ul

RT: 20.07 min Scan# 1181

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40


Tgt Ion:202 Resp: 4700

Ion Ratio Lower Upper

202 100

101 9.3 0.0 33.1



203 22.5 0.0 37.2




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

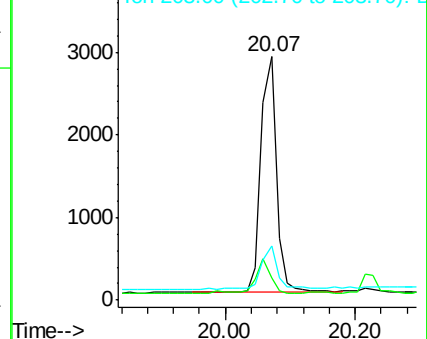

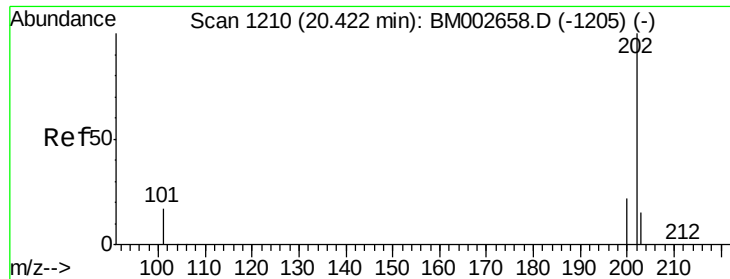

#19

Pyrene

Concen: 0.07 ng/ul

RT: 20.42 min Scan# 1210

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S


Tgt Ion:202 Resp: 4795

Ion Ratio Lower Upper

202 100

200 22.2 18.0 27.0




203 21.0 13.8 20.6#

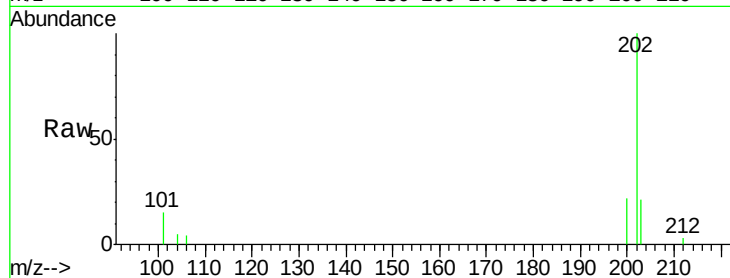

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

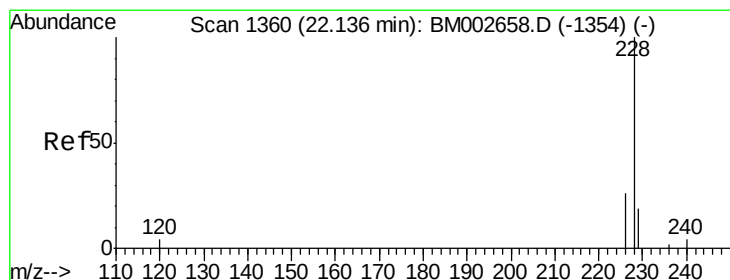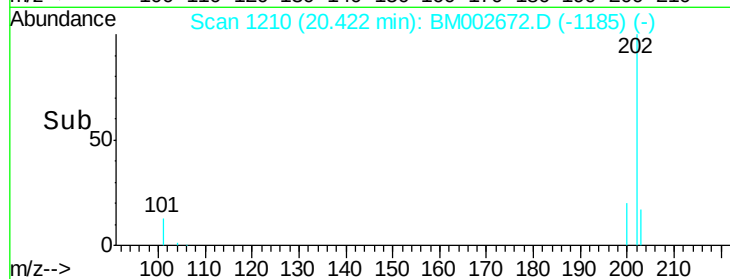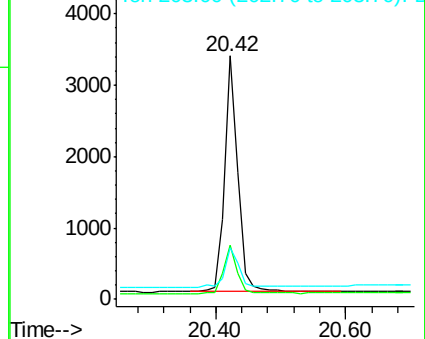

#20

Benzo(a)anthracene

Concen: 0.07 ng/ul

RT: 22.14 min Scan# 1360

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40


Tgt Ion:228 Resp: 4453

Ion Ratio Lower Upper

228 100

226 29.7 23.0 34.4



229 25.0 15.2 22.8#

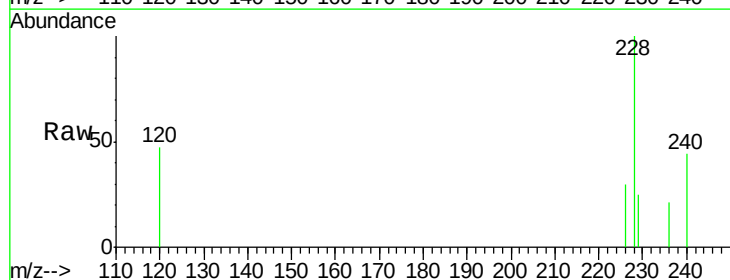


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

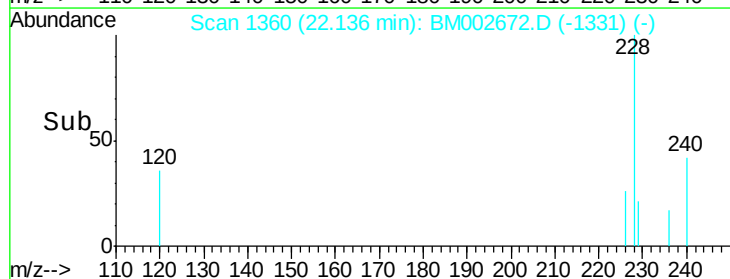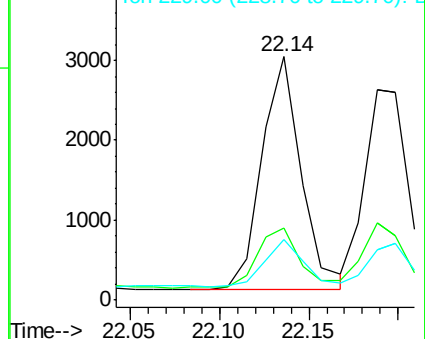

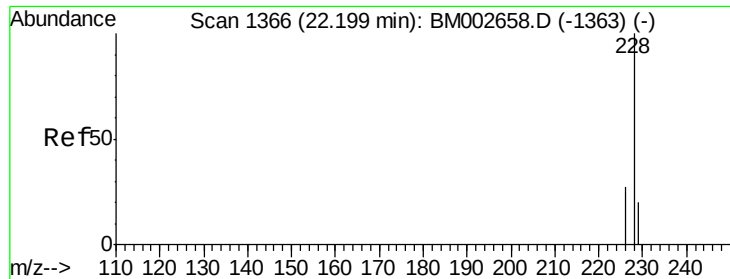

#21

Chrysene

Concen: 0.07 ng/ul

RT: 22.19 min Scan# 1365

Delta R.T. -0.01 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S


Tgt Ion:228 Resp: 4259

Ion Ratio Lower Upper

228 100

226 36.7 25.7 38.5




229 24.0 15.2 22.8#

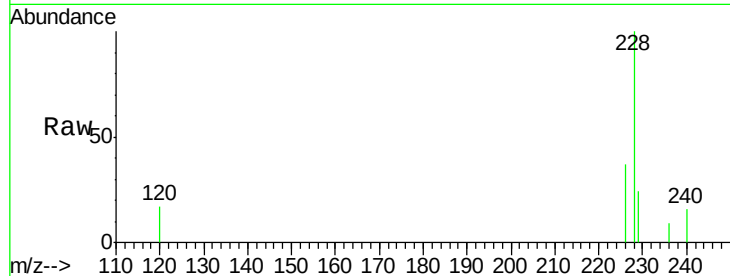

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

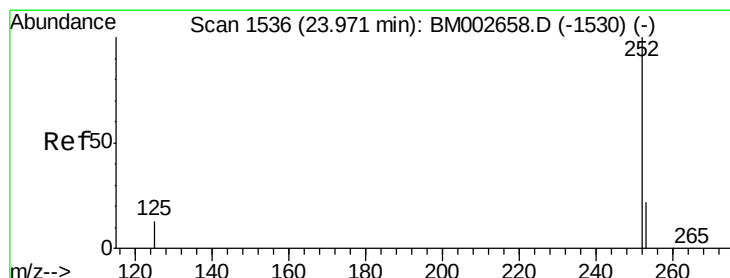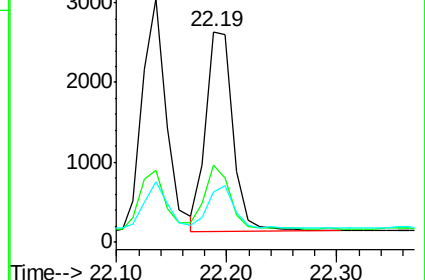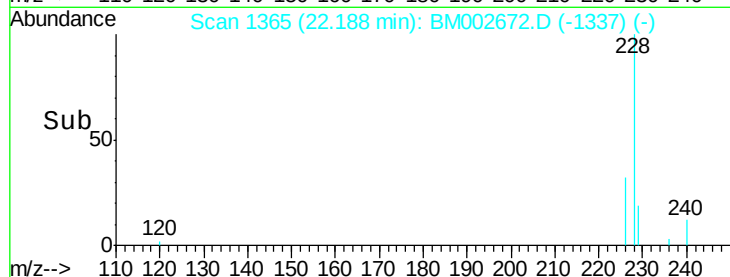

#23

Benzo(b)fluoranthene

Concen: 0.07 ng/ul

RT: 23.96 min Scan# 1535

Delta R.T. -0.01 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40


Tgt Ion:252 Resp: 5039

Ion Ratio Lower Upper

252 100

253 37.5 0.0 48.0



125 36.7 0.0 36.6#

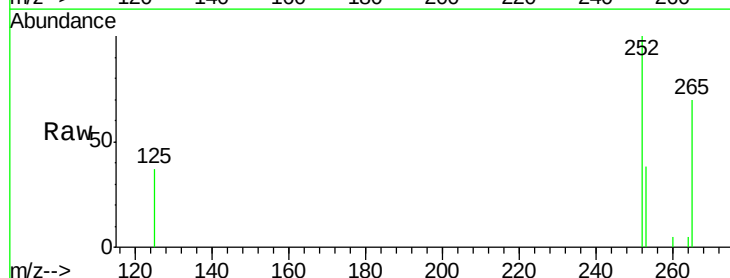


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

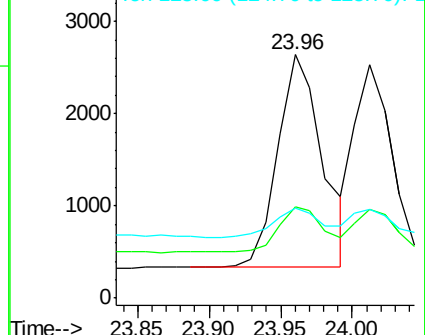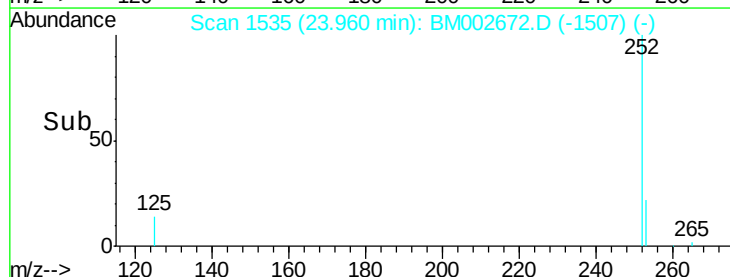

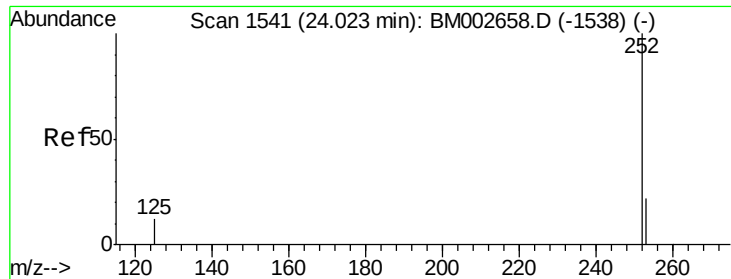

#24

Benzo(k)fluoranthene

Concen: 0.07 ng/ul

RT: 24.01 min Scan# 1540

Delta R.T. -0.01 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S





Tgt Ion:252 Resp: 4207

Ion Ratio Lower Upper

252 100

253 38.1 20.8 31.2#

125 38.2 12.2 18.4#

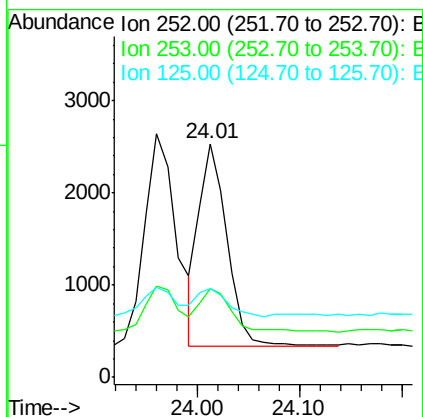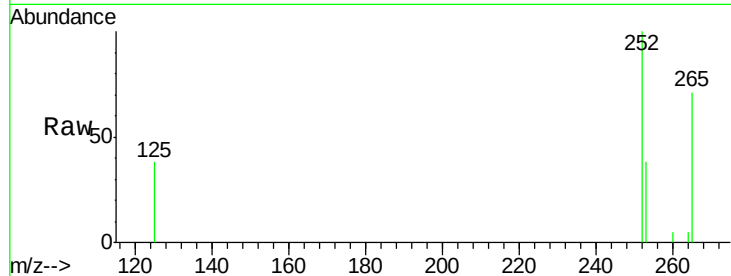

#25

Benzo(a)pyrene

Concen: 0.07 ng/ul

RT: 24.66 min Scan# 1602

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40




Tgt Ion:252 Resp: 4231


Ion Ratio Lower Upper

252 100

253 41.6 21.8 32.8#

125 44.1 14.5 21.7#

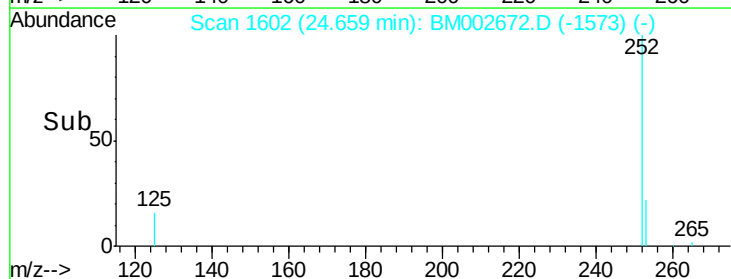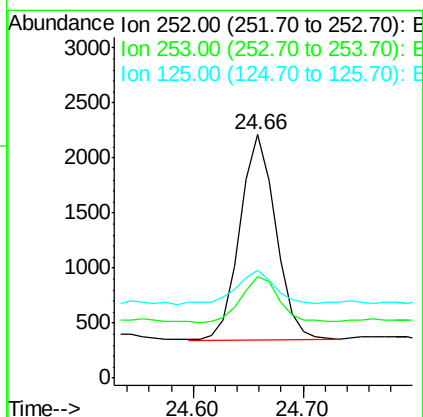



#26

Indeno(1,2,3-cd)pyrene

Concen: 0.07 ng/ul

RT: 27.54 min Scan# 1878

Delta R.T. 0.00 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S


Tgt Ion:276 Resp: 5198

Ion Ratio Lower Upper

276 100

138 33.8 27.5 41.3




277 24.9 19.3 28.9

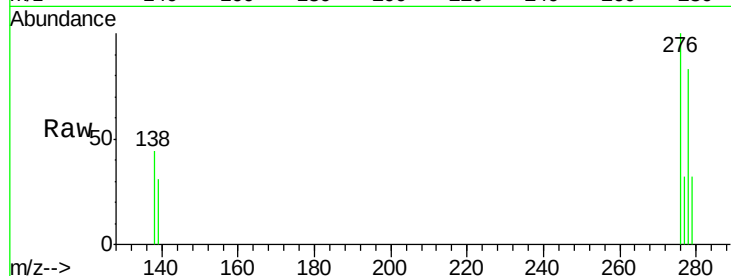

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

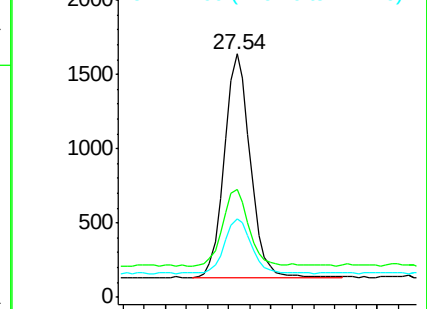

#27

Dibenzo(a,h)anthracene

Concen: 0.07 ng/ul

RT: 27.54 min Scan# 1878

Delta R.T. -0.01 min

Lab File: BM002672.D

Acq: 04 Sep 2015 13:40


Tgt Ion:278 Resp: 4120

Ion Ratio Lower Upper

278 100

139 37.7 21.7 32.5#



279 38.1 21.9 32.9#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

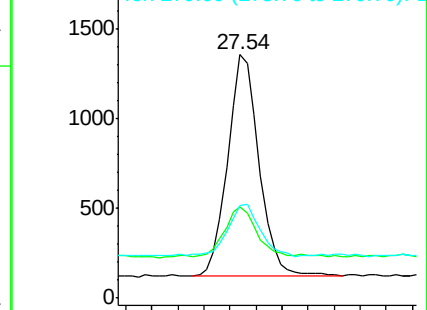

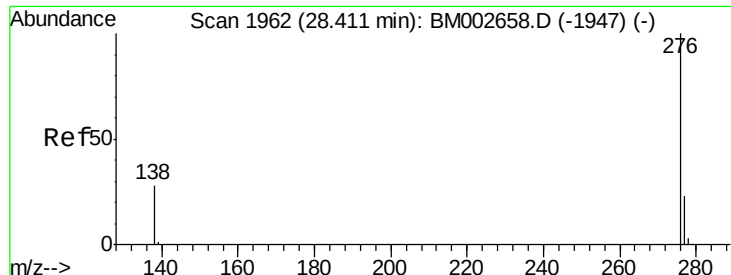

#28

Benzo(g,h,i)perylene

Concen: 0.07 ng/ul

RT: 28.40 min Scan# 1961

Delta R.T. -0.01 min

Lab File: BM002672.D


Acq: 04 Sep 2015 13:40

Instrument :

BNA_M

ClientSampleId :

MDL-02-S




Tgt Ion: 276 Resp: 4447

Ion Ratio Lower Upper

276 100

277 33.9 21.3 31.9#

138 41.6 25.5 38.3#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

