


Data Path : Z:\HPCHEM1\BNA_M\Data\BM090415\
 Data File : BM002668.D
 Acq On : 04 Sep 2015 11:14
 Operator : UM/IZ
 Sample : DFTPP12
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP12

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 04 04:35:12 2015

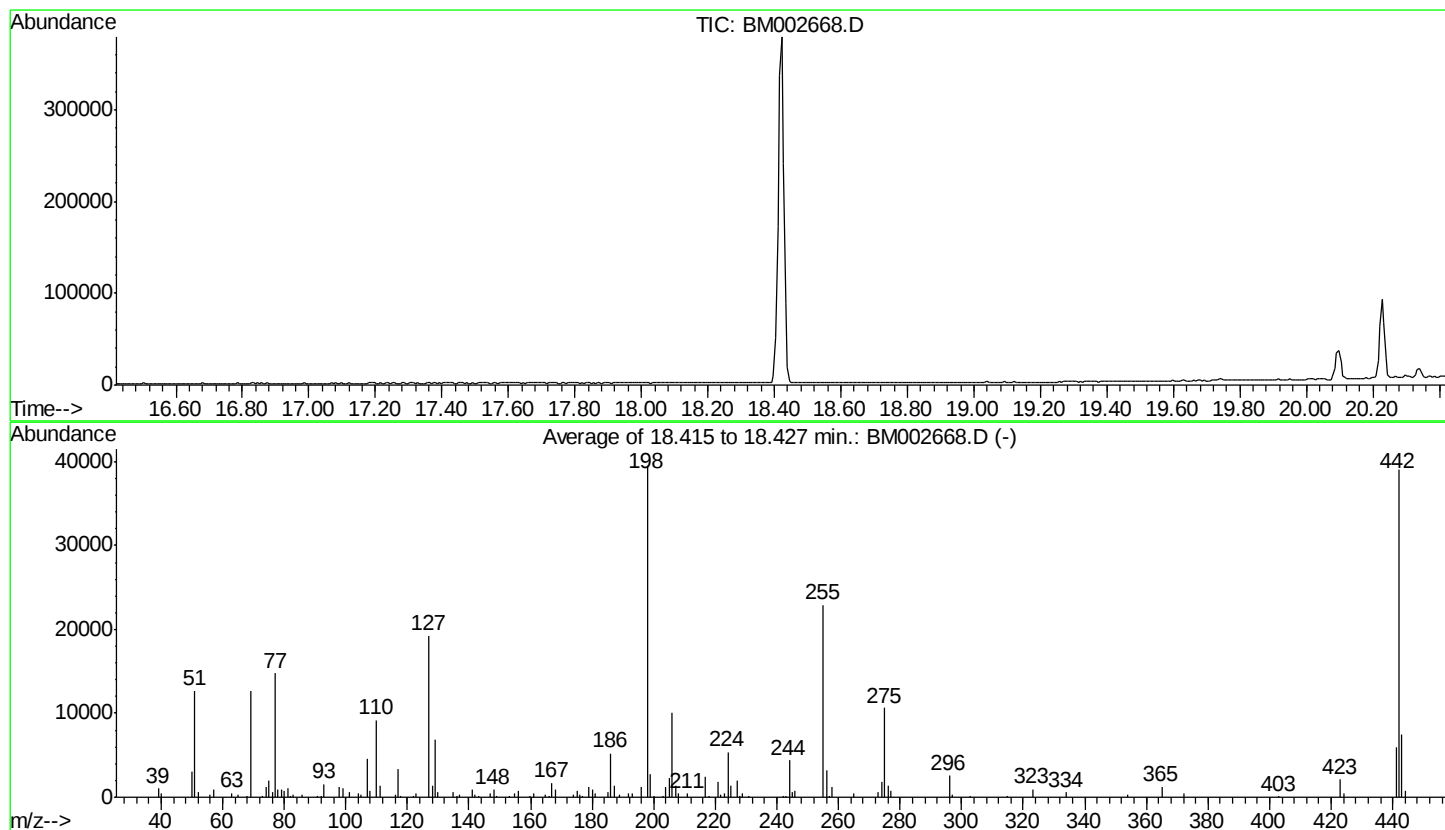

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	12685	PASS
68	69	0.00	2	0.9	115	PASS
69	198	0.00	100	32.1	12682	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	19234	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	39525	PASS
199	198	5	9	7.0	2761	PASS
275	198	10	60	27.0	10670	PASS
365	198	1	100	3.1	1224	PASS
441	443	0.01	100	79.3	5976	PASS
442	198	50	100	98.9	39077	PASS
443	442	15	24	19.3	7539	PASS

m/z	Abundance
39.00	1289.0
40.00	480.0
44.00	1811.0
50.00	3551.0
51.10	15185.0
52.00	866.0
55.90	480.0
57.00	1074.0
63.10	506.0
65.00	370.0
69.00	15305.0
73.00	305.0
74.00	1520.0
75.00	2425.0
76.00	774.0
77.10	17416.0
78.00	1131.0
78.90	1083.0
80.00	981.0
81.00	1260.0
82.00	319.0
83.00	359.0
85.90	418.0
90.90	362.0
91.90	304.0
93.00	1795.0
98.00	1518.0
99.00	1208.0
101.00	775.0
103.90	405.0
105.00	407.0
107.00	5317.0
107.90	871.0
110.00	10454.0
110.90	1419.0
116.00	341.0
117.00	3815.0
117.90	335.0
121.90	323.0
122.90	603.0
127.00	21816.0
128.00	1536.0
129.00	7844.0
129.90	609.0
135.00	754.0
136.90	413.0
141.00	1022.0
141.90	382.0
147.00	604.0
148.00	989.0
153.00	441.0
154.90	533.0
156.00	848.0
160.90	396.0
164.90	410.0
167.00	1836.0
168.00	1054.0
174.00	408.0
175.00	758.0
176.00	400.0
176.90	357.0
178.90	1306.0
180.00	1092.0
180.90	526.0
185.00	657.0
186.00	5555.0
187.00	1461.0
189.00	320.0
192.00	412.0
192.90	401.0
196.00	1174.0
197.90	43048.0
198.90	3070.0
204.00	1335.0
205.00	2361.0
206.00	10360.0
207.00	2130.0
208.00	460.0
210.90	388.0
216.90	2721.0
221.00	1923.0
221.70	465.0
223.00	559.0
224.00	5576.0
225.00	1576.0
227.00	2092.0
227.90	390.0
228.90	447.0
243.00	366.0
244.00	4394.0
244.90	599.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

245.90	761.0
255.00	23376.0
256.00	3297.0
256.90	305.0
258.00	1190.0
264.90	512.0
272.90	533.0
274.00	1801.0
275.00	10481.0
276.00	1529.0
277.00	866.0
296.00	2463.0
297.00	338.0
323.00	916.0
334.00	570.0
364.90	1045.0
372.00	536.0
423.00	1850.0
424.00	409.0
441.00	5005.0
442.00	32608.0
443.00	6478.0
443.90	640.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

m/z	Abundance
39.00	1125.0
40.00	469.0
44.00	1712.0
50.00	3602.0
51.00	14750.0
52.00	724.0
56.00	396.0
57.00	1081.0
63.10	658.0
65.00	358.0
68.00	345.0
69.00	14494.0
74.00	1405.0
75.00	2274.0
76.00	774.0
77.10	17120.0
78.10	1190.0
79.00	1145.0
80.00	905.0
81.00	1163.0
81.90	354.0
82.90	345.0
86.00	351.0
90.90	336.0
92.00	317.0
93.00	1859.0
98.00	1346.0
99.00	1268.0
101.00	698.0
104.00	465.0
105.00	394.0
107.00	5237.0
107.90	843.0
110.00	10864.0
111.00	1674.0
116.10	400.0
117.00	3988.0
121.80	353.0
123.00	541.0
127.00	22656.0
128.00	1711.0
129.00	7833.0
130.00	715.0
135.00	663.0
136.00	336.0
137.00	353.0
141.00	946.0
141.90	321.0
143.00	355.0
146.90	502.0
148.00	1014.0
149.00	334.0
155.00	629.0
156.00	900.0
159.90	305.0
160.90	451.0
164.90	430.0
166.00	356.0
167.00	1961.0
167.90	1055.0
174.00	638.0
175.00	858.0
176.00	337.0
176.90	321.0
179.00	1623.0
180.00	1220.0
180.90	545.0
184.90	749.0
186.00	6277.0
187.00	1713.0
189.00	407.0
191.90	484.0
192.90	666.0
196.00	1429.0
197.90	46640.0
198.90	3165.0
199.90	305.0
202.90	334.0
204.00	1372.0
205.00	2672.0
206.00	11663.0
207.00	2233.0
208.00	443.0
211.00	478.0
216.90	2904.0
217.90	376.0
221.00	2168.0
222.90	614.0
224.00	6426.0
225.00	1389.0
227.00	2364.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

228.00	307.0
228.90	489.0
231.00	382.0
241.90	327.0
244.00	5246.0
245.00	765.0
245.90	817.0
255.00	27376.0
256.00	3842.0
258.00	1402.0
264.90	544.0
272.90	786.0
274.00	2249.0
275.00	12646.0
276.00	1699.0
276.90	865.0
296.00	3004.0
297.00	514.0
302.90	392.0
314.90	438.0
323.00	1111.0
334.00	713.0
354.00	451.0
365.00	1477.0
372.00	585.0
403.00	439.0
423.00	2548.0
424.00	469.0
441.00	7086.0
442.00	46584.0
443.00	9070.0
444.00	826.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

m/z	Abundance
39.00	732.0
39.90	383.0
44.00	1665.0
50.00	1946.0
51.00	8121.0
52.00	426.0
57.00	582.0
63.00	338.0
69.00	8248.0
74.00	836.0
75.00	1331.0
76.00	460.0
77.10	9827.0
78.00	587.0
79.00	602.0
80.00	448.0
80.90	653.0
92.90	1051.0
98.00	817.0
99.00	726.0
100.90	336.0
104.00	312.0
107.00	3165.0
108.00	545.0
110.00	6253.0
111.00	905.0
117.00	2143.0
122.90	362.0
127.00	13230.0
128.00	994.0
129.00	4845.0
130.00	406.0
135.00	393.0
141.00	656.0
146.90	306.0
148.00	648.0
154.90	350.0
156.00	581.0
161.00	367.0
167.00	1336.0
167.90	557.0
175.00	544.0
179.00	942.0
180.00	596.0
180.90	331.0
185.00	513.0
186.00	3766.0
187.00	942.0
192.00	350.0
192.90	372.0
196.00	998.0
198.00	28888.0
198.90	2049.0
204.00	965.0
205.00	1741.0
206.00	8038.0
207.00	1732.0
207.90	357.0
210.90	313.0
217.00	1823.0
221.00	1196.0
221.70	404.0
222.90	386.0
224.00	4056.0
225.00	999.0
227.00	1648.0
228.90	331.0
244.00	3535.0
245.00	545.0
245.90	619.0
255.00	18120.0
256.00	2492.0
258.00	947.0
265.00	370.0
272.90	604.0
273.90	1516.0
275.00	8885.0
276.00	1089.0
277.00	648.0
296.00	2226.0
323.00	838.0
334.00	418.0
354.00	305.0
365.00	1151.0
372.00	438.0
423.00	2010.0
424.00	351.0
441.00	5837.0
442.00	38040.0
443.00	7070.0
444.00	615.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

m/z	Abundance
44.00	1758.0
207.00	602.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12