

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027338.D
 Acq On : 04 Sep 2020 19:56
 Operator : JU/CG
 Sample : L3840-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Quant Time: Sep 05 00:59:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 05 00:52:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	132646	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	532761	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	400538	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	958088	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1263515	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1355630	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	9896	3.32	ng/uL	0.00
5) Phenol-d5	6.76	99	162548	14.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	124296	17.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	131795	16.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	138661	15.55	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	68859	17.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	77349	17.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	148153	15.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	182110	16.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	612622	19.22	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	646913	17.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	62059	11.06	ng/ul	0.00
58) Fluorene-d10	15.21	176	501256	17.56	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	76492	12.47	ng/ul	0.00
71) Anthracene-d10	17.06	188	808495	17.84	ng/ul	0.00
79) Pyrene-d10	19.36	212	1092958	19.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1392569	19.15	ng/ul	0.00

Target Compounds


					Ovalue
45) Dimethylphthalate	13.67	163	253537	7.549	ng/ul 99
77) Fluoranthene	19.02	202	229713	3.398	ng/ul 99
80) Pyrene	19.39	202	294384	3.851	ng/ul 99
83) Benzo(a)anthracene	21.14	228	380852	4.652	ng/ul 98
85) Chrysene	21.20	228	592393	7.323	ng/ul 99
88) Benzo(b)fluoranthene	22.73	252	182860	2.043	ng/ul 99
89) Benzo(k)fluoranthene	22.73	252	182973	2.039	ng/ul 99
91) Benzo(a)pyrene	23.24	252	322231	3.859	ng/ul 99
92) Indeno(1,2,3-cd)pyrene	25.49	276	140683	1.283	ng/ul 95
94) Benzo(g,h,i)perylene	26.14	276	113996	1.244	ng/ul 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027338.D
Acq On : 04 Sep 2020 19:56
Operator : JU/CG
Sample : L3840-20
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB8

Quant Time: Sep 05 00:59:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 05 00:52:50 2020
Response via : Initial Calibration

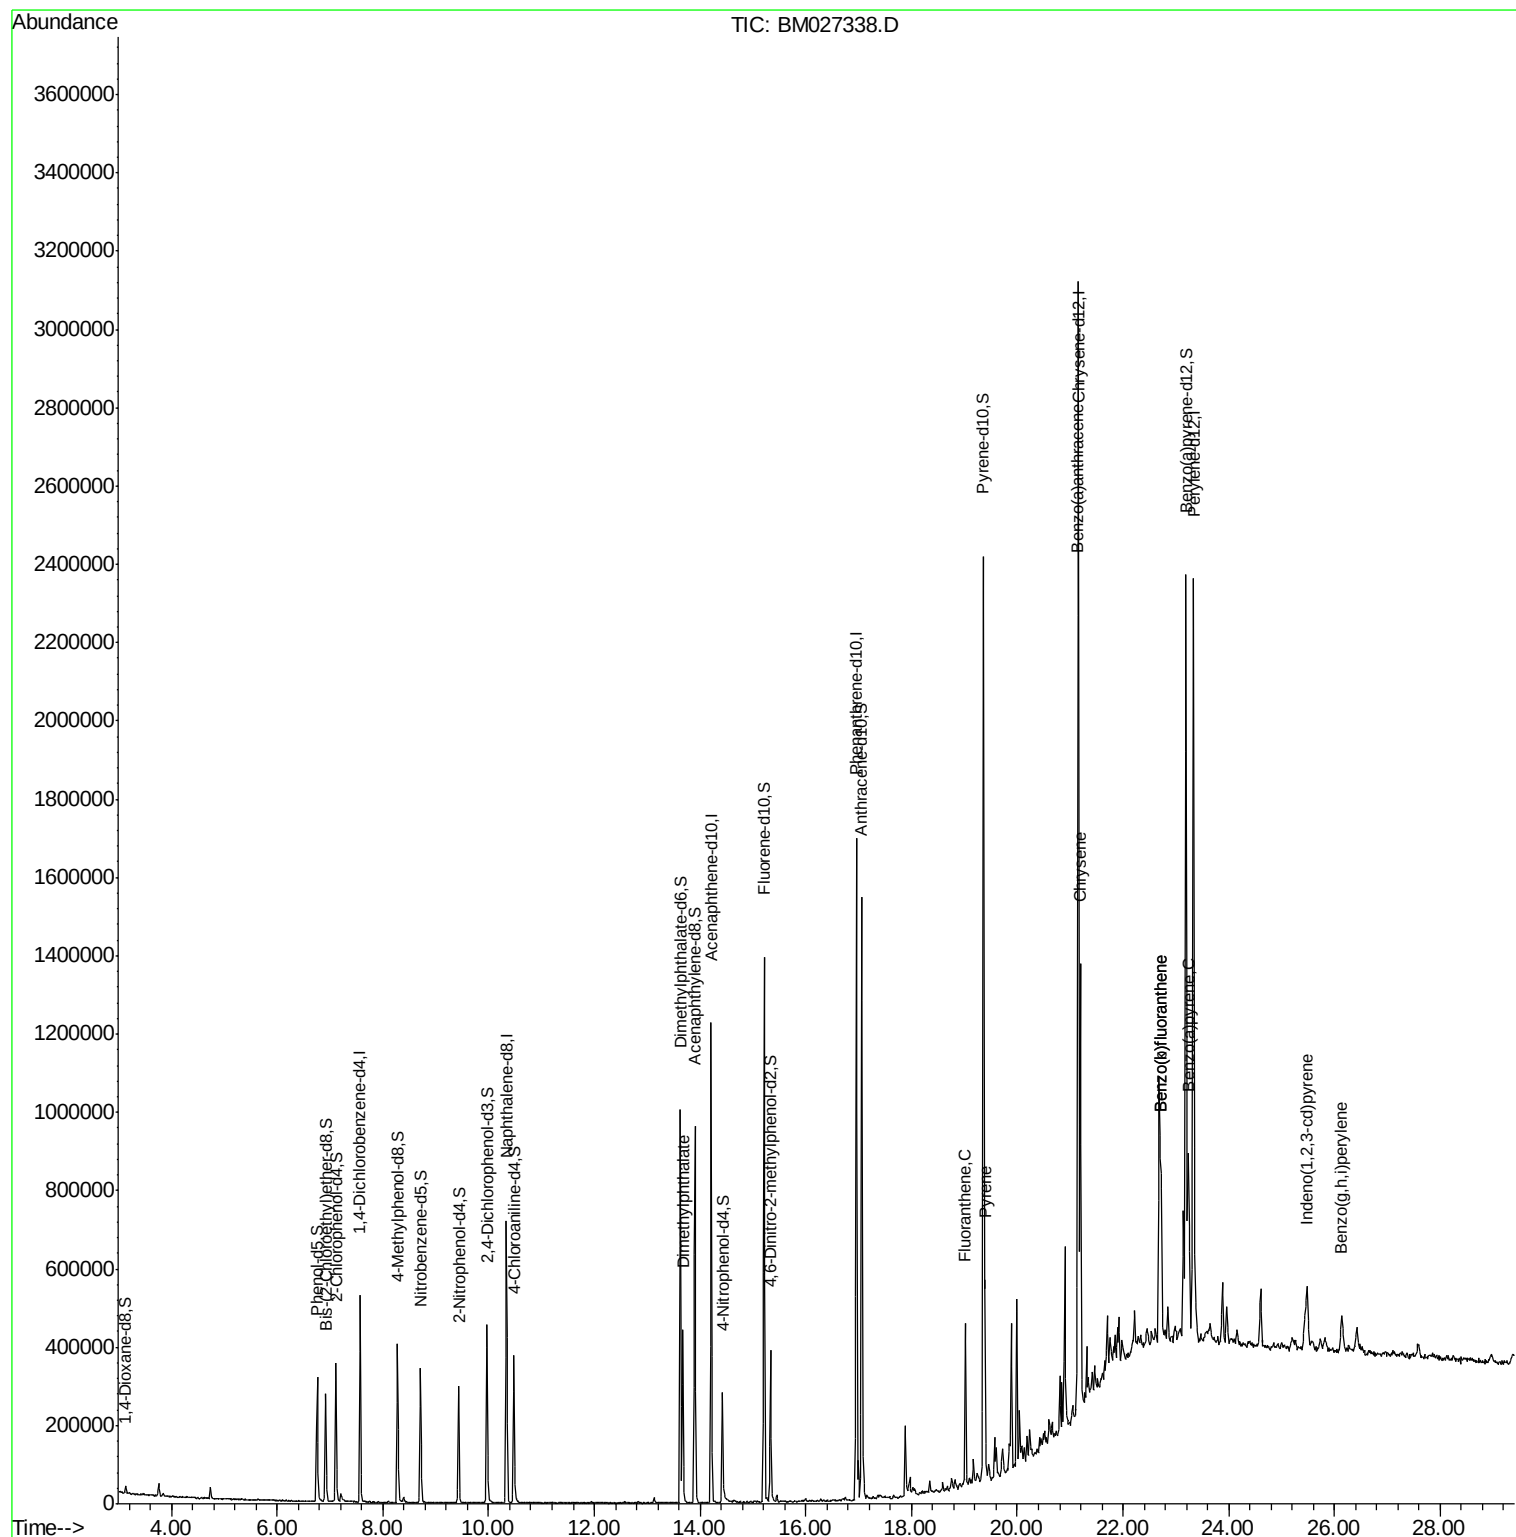

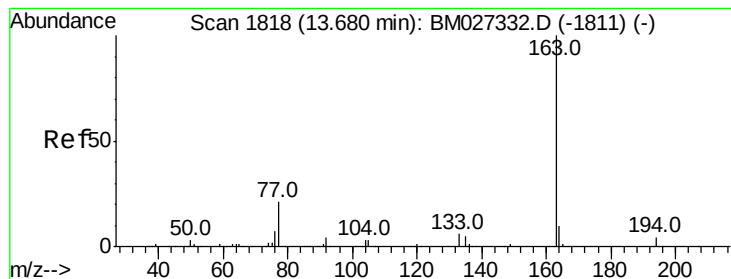

#45

Dimethylphthalate

Concen: 7.549 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56

Instrument :

BNA_M

ClientSampleId :

C0AB8


Tot Ion:163 Resp: 253537

Ion Ratio Lower Upper

163 100

194 3.9 3.3 4.9




164 9.8 8.1 12.1

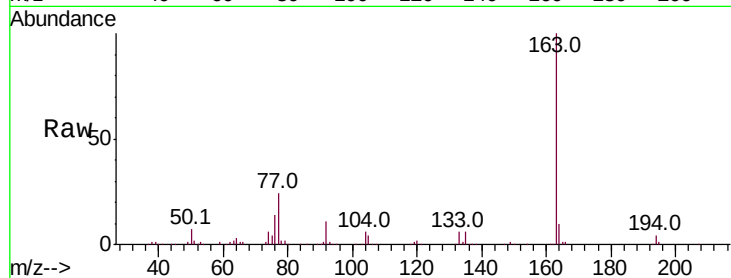

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

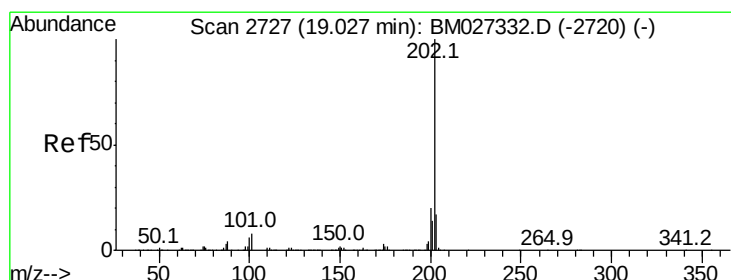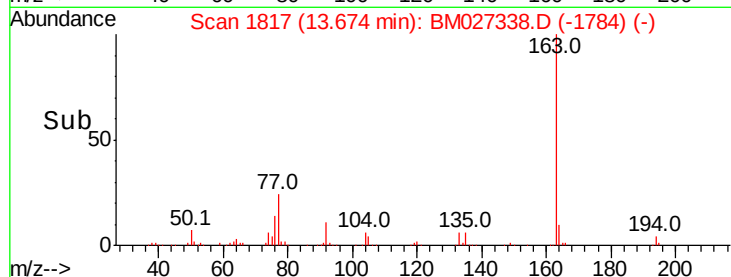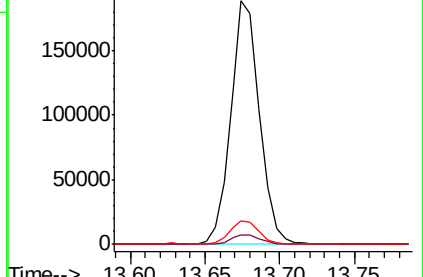

#77

Fluoranthene

Concen: 3.398 ng/ul

RT: 19.02 min Scan# 2726

Delta R.T. -0.01 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56


Tgt Ion:202 Resp: 229713

Ion Ratio Lower Upper

202 100

101 7.4 6.2 9.2



100 6.2 5.0 7.6

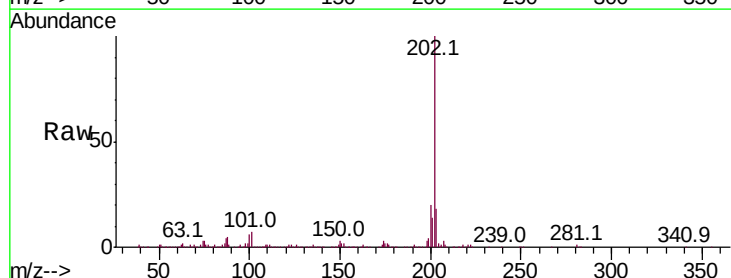


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E



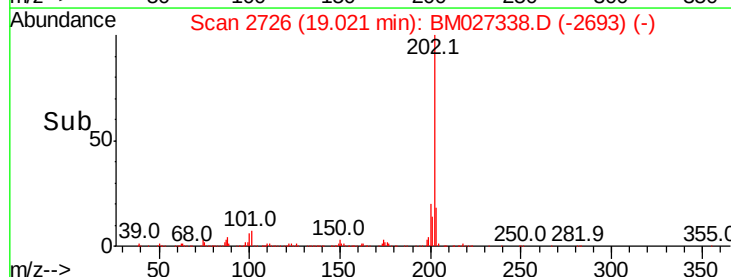
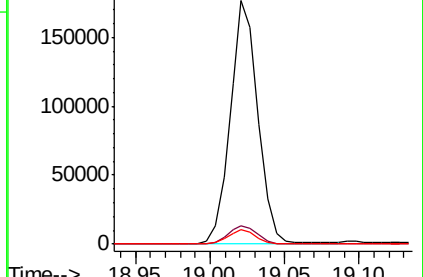


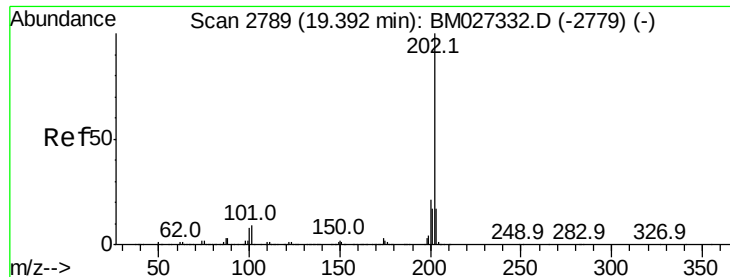

#80
Pvrene
Concen: 3.851 ng/ul
RT: 19.39 min Scan# 2788
Delta R.T. -0.01 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56




Instrument :
BNA_M
ClientSampleId :
C0AB8


Tot Ion:	202	Resp:	294384
Ion	Ratio	Lower	Upper
202	100		
101	8.7	7.1	10.7
100	8.4	6.1	9.1

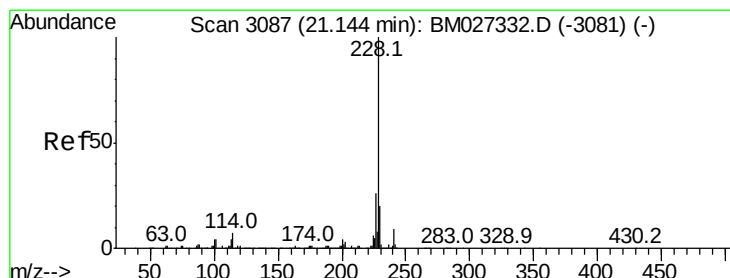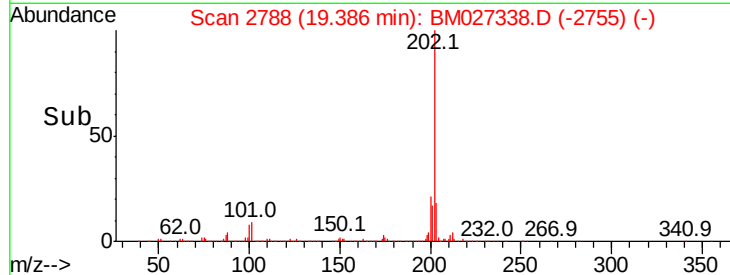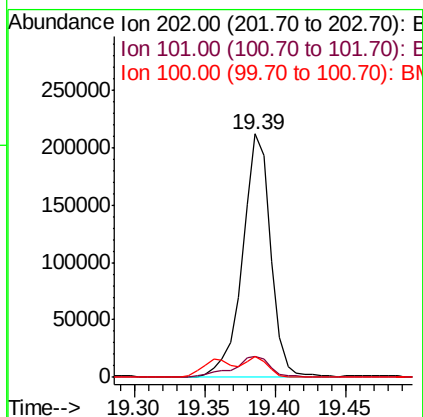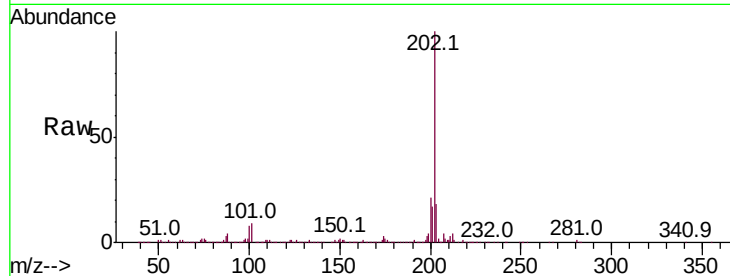

#83
Benzo(a)anthracene
Concen: 4.652 ng/ul
RT: 21.14 min Scan# 3087
Delta R.T. -0.01 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56

Tgt Ion:	228	Resp:	380852
Ion	Ratio	Lower	Upper
228	100		
229	20.5	15.8	23.6
226	26.1	21.5	32.3

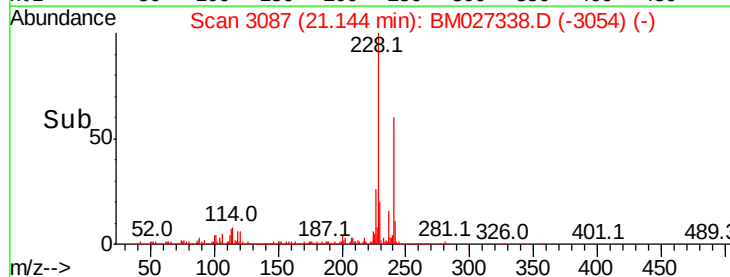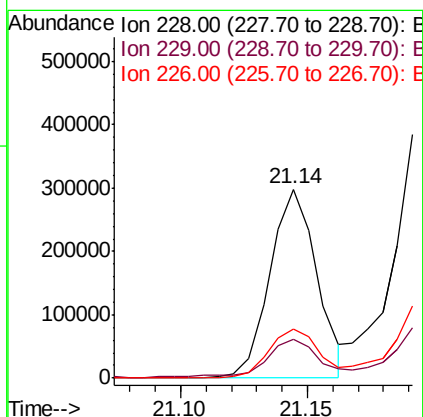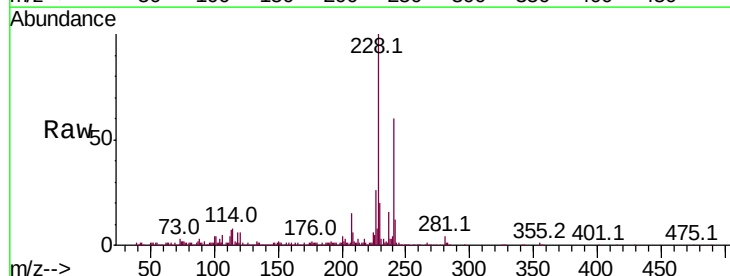

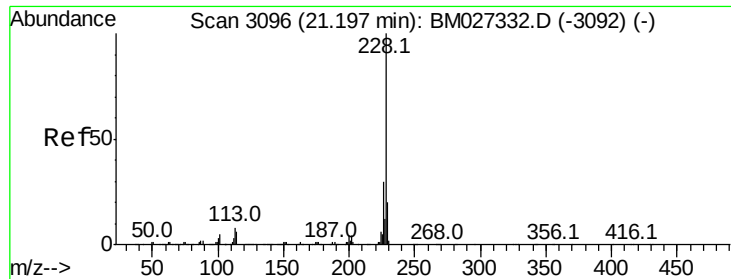

#85

Chrysene

Concen: 7.323 ng/ul

RT: 21.20 min Scan# 3096

Delta R.T. -0.00 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56

Instrument :

BNA_M

ClientSampleId :

C0AB8


Tot Ion:228 Resp: 592393

Ion Ratio Lower Upper

228 100

226 29.0 23.4 35.2




229 20.3 15.8 23.8

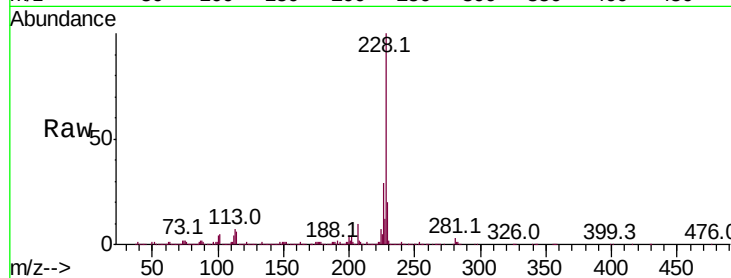

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

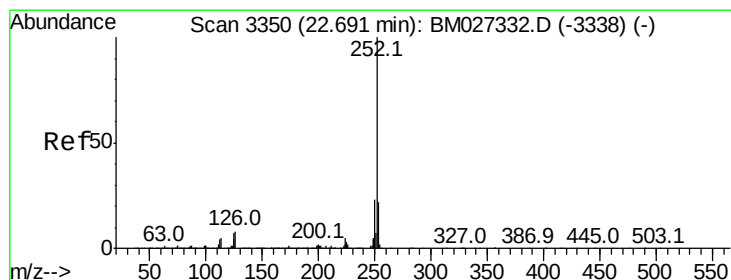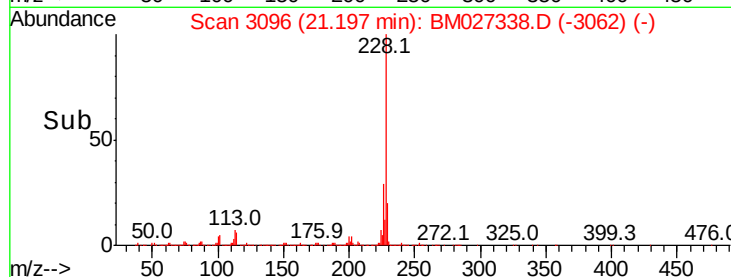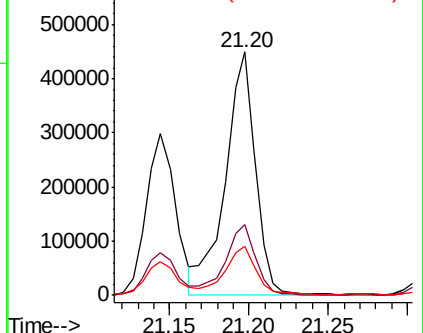

#88

Benzo(b)fluoranthene

Concen: 2.043 ng/ul

RT: 22.73 min Scan# 3356

Delta R.T. 0.03 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56


Tgt Ion:252 Resp: 182860

Ion Ratio Lower Upper

252 100

253 22.5 17.7 26.5



125 7.2 5.1 7.7

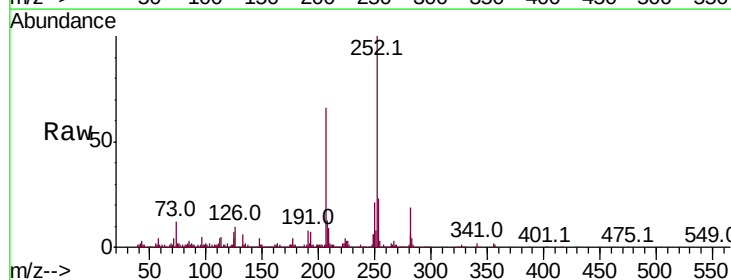


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

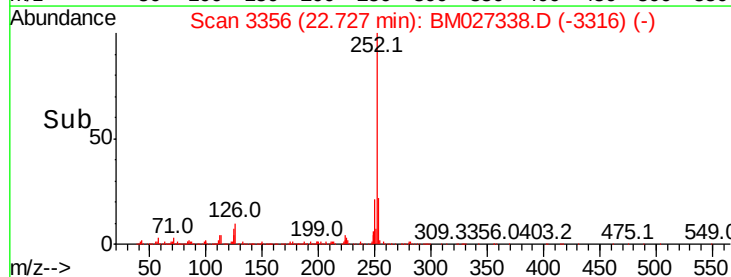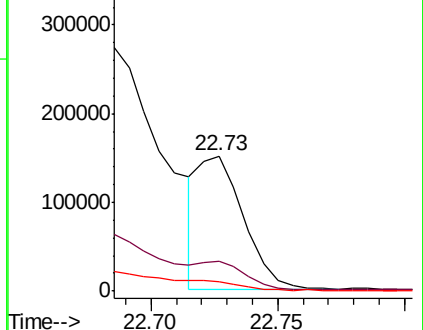

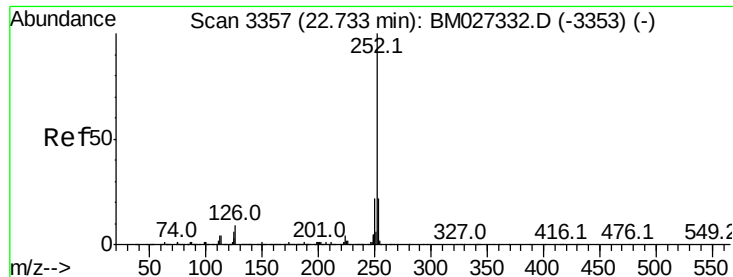

#89

Benzo(k)fluoranthene

Concen: 2.039 ng/ul

RT: 22.73 min Scan# 3356

Delta R.T. -0.01 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56

Instrument :

BNA_M

ClientSampleId :

C0AB8





Tot Ion:252 Resp: 182973

Ion Ratio Lower Upper

252 100

253 22.5 17.4 26.0

125 7.2 5.6 8.4

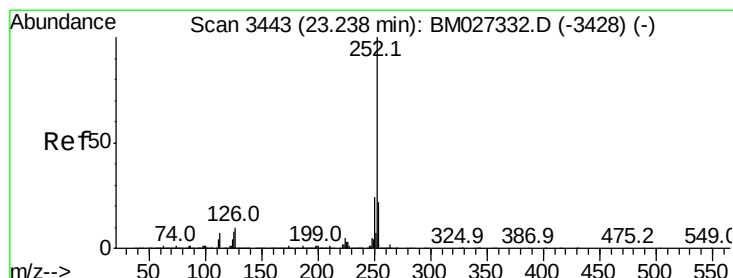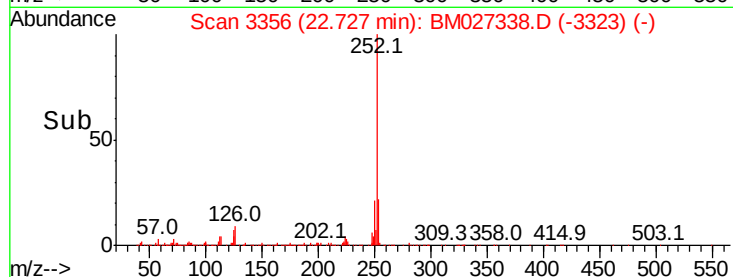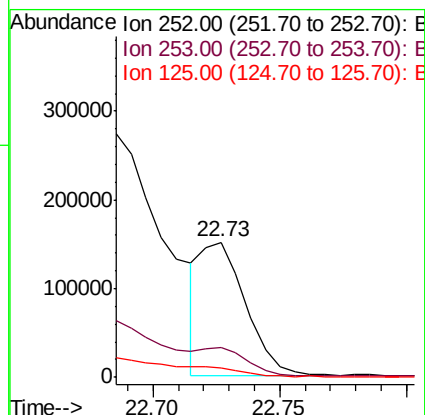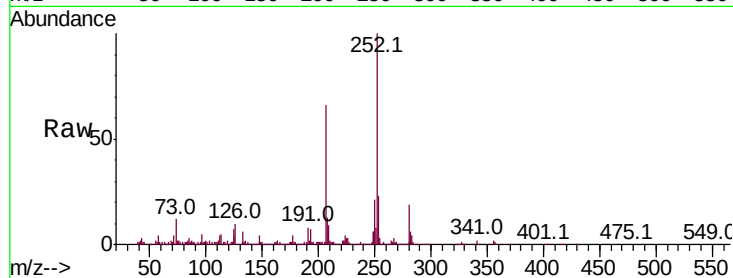

#91

Benzo(a)pyrene

Concen: 3.859 ng/ul

RT: 23.24 min Scan# 3443

Delta R.T. -0.00 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56




Tgt Ion:252 Resp: 322231


Ion Ratio Lower Upper

252 100

253 22.4 17.5 26.3

125 8.7 6.6 10.0


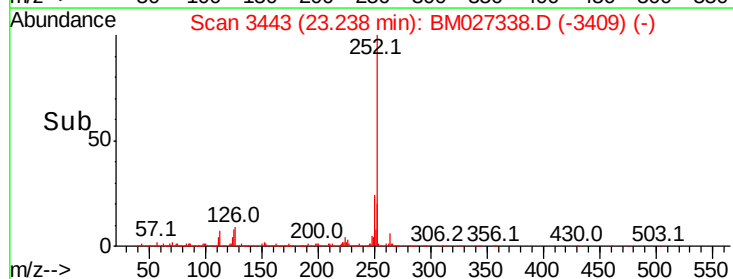
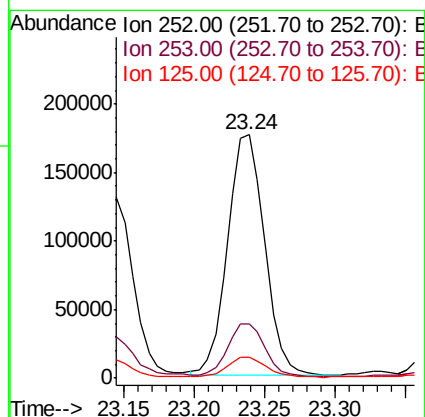
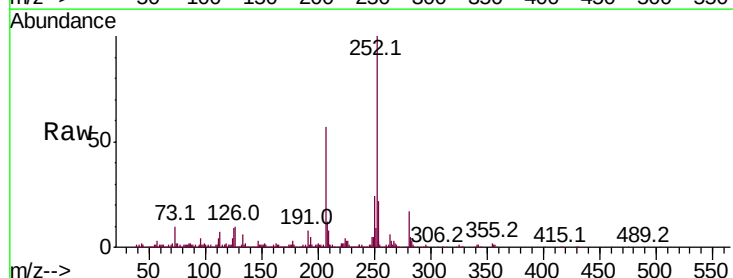


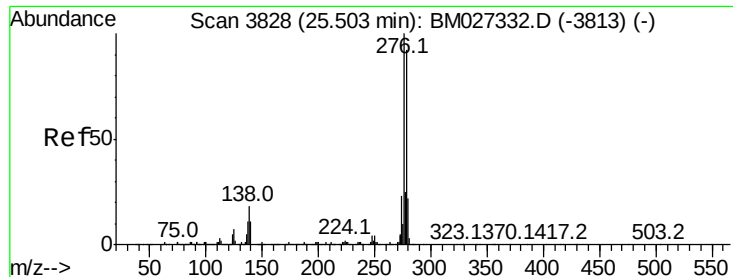

#92
 Indeno(1,2,3-cd)pyrene
 Concen: 1.283 ng/ul
 RT: 25.49 min Scan# 3825
 Delta R.T. -0.01 min
 Lab File: BM027338.D
 Acq: 04 Sep 2020 19:56

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Tot Ion:	276	Resp:	140683
Ion	Ratio	Lower	Upper
276	100		
138	15.0	14.0	21.0
277	27.0	20.1	30.1

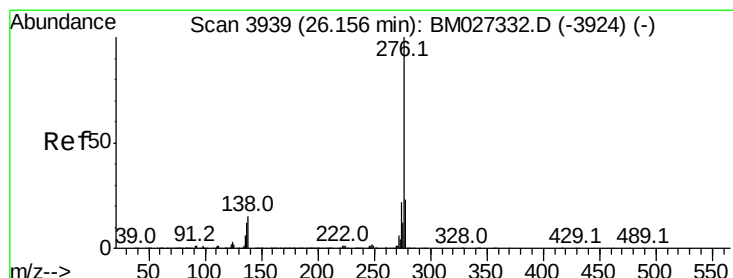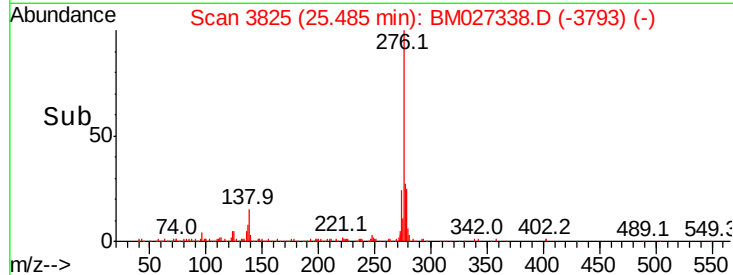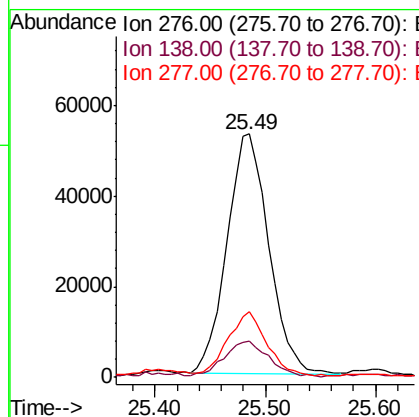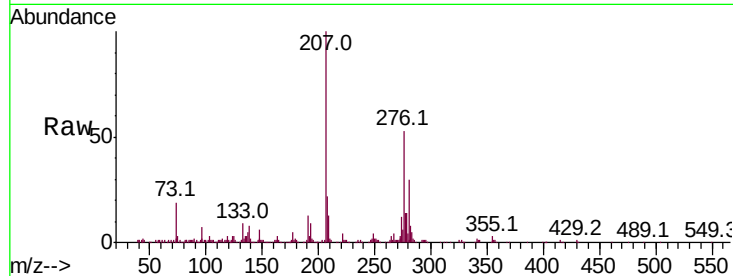

#94
 Benzo(g,h,i)perylene
 Concen: 1.244 ng/ul
 RT: 26.14 min Scan# 3936
 Delta R.T. -0.02 min
 Lab File: BM027338.D
 Acq: 04 Sep 2020 19:56

Tgt Ion:	276	Resp:	113996
Ion	Ratio	Lower	Upper
276	100		
138	13.6	12.2	18.2
277	25.7	18.6	28.0

