

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027343.D
 Acq On : 04 Sep 2020 22:59
 Operator : JU/CG
 Sample : L3843-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Quant Time: Sep 05 01:00:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 05 00:52:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	133719	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	534204	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	401338	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	959631	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1170170	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1272927	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	7896	2.63	ng/uL	0.00
5) Phenol-d5	6.76	99	110613	10.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	93238	12.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	91118	11.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	95007	10.57	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	49587	12.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	51811	11.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	97386	10.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	120403	10.73	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	448088	14.03	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	422545	11.71	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	36217	6.44	ng/ul	0.00
58) Fluorene-d10	15.21	176	341554	11.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	47109	7.67	ng/ul	0.00
71) Anthracene-d10	17.06	188	544510	12.00	ng/ul	0.00
79) Pyrene-d10	19.36	212	676004	12.97	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	766639	11.23	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	129103	3.836	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027343.D
Acq On : 04 Sep 2020 22:59
Operator : JU/CG
Sample : L3843-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Time: Sep 05 01:00:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 05 00:52:50 2020
Response via : Initial Calibration

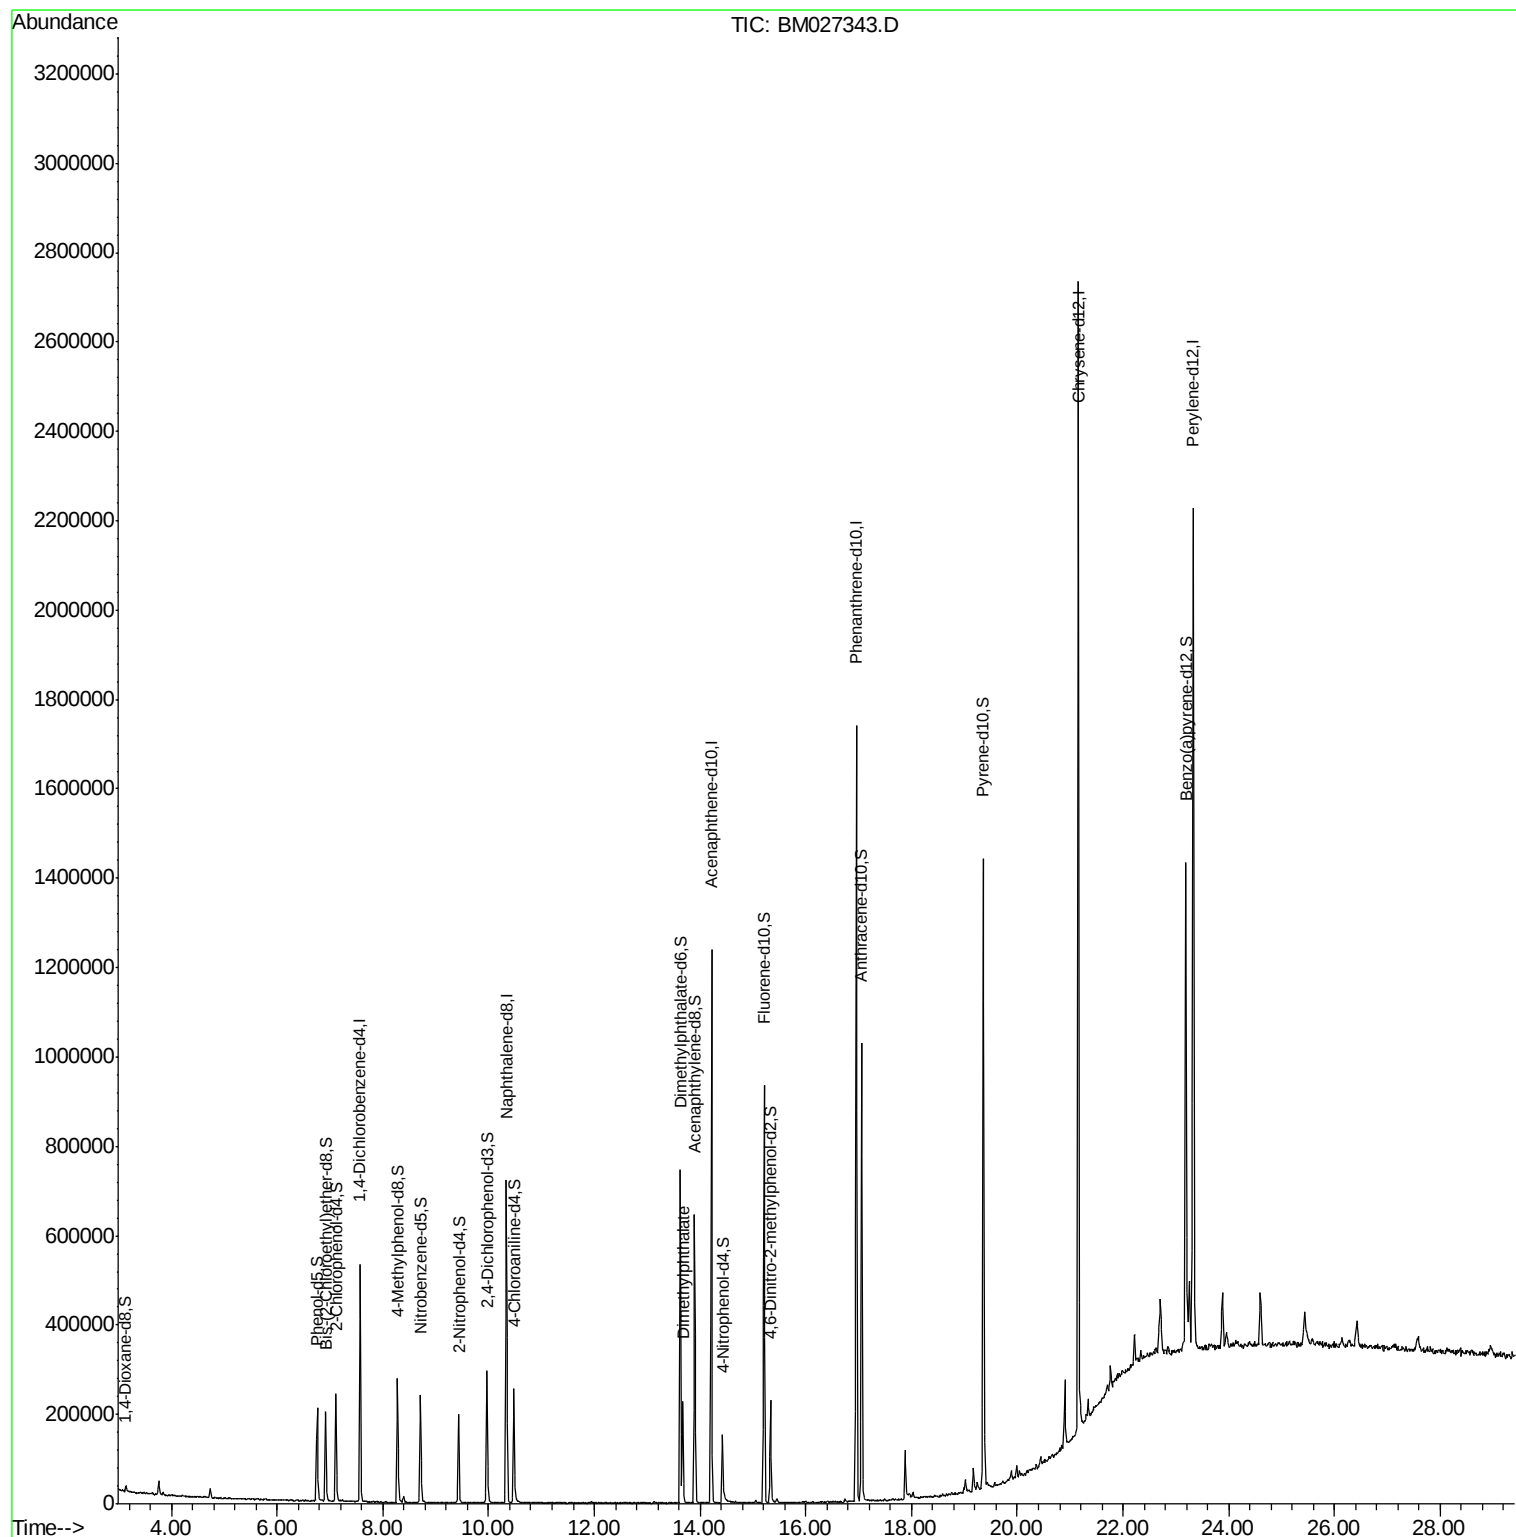

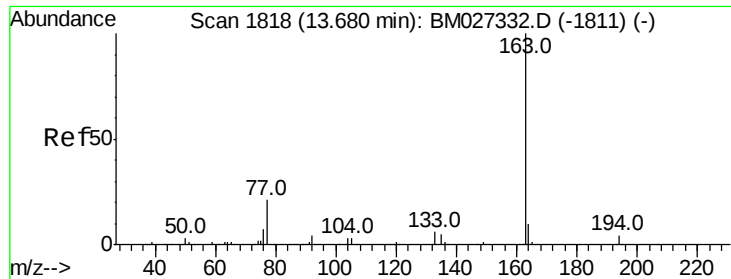

#45

Dimethylphthalate

Concen: 3.836 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM027343.D

Acq: 04 Sep 2020 22:59

Instrument :

BNA_M

ClientSampleId :

C0AE1


Tot Ion:163 Resp: 129103

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.7 8.1 12.1

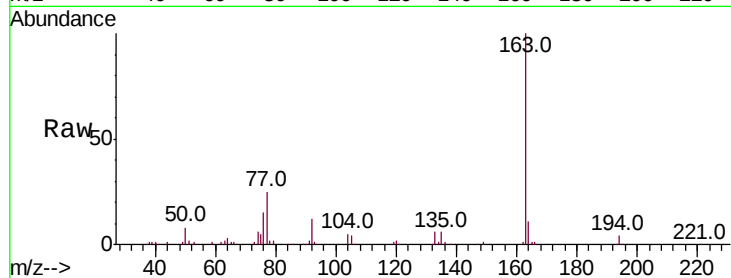

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

