

(QT Reviewed)


```
Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\  
Data File : BM027329.D  
Acq On    : 04 Sep 2020   14:06  
Operator  : JU/CG  
Sample    : SSTD16001  
Misc      :  
ALS Vial  : 8      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
SSTD16001

Manual Integrations

mohammad
9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:45:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 04 12:49:01 2020
Response via : Initial Calibration

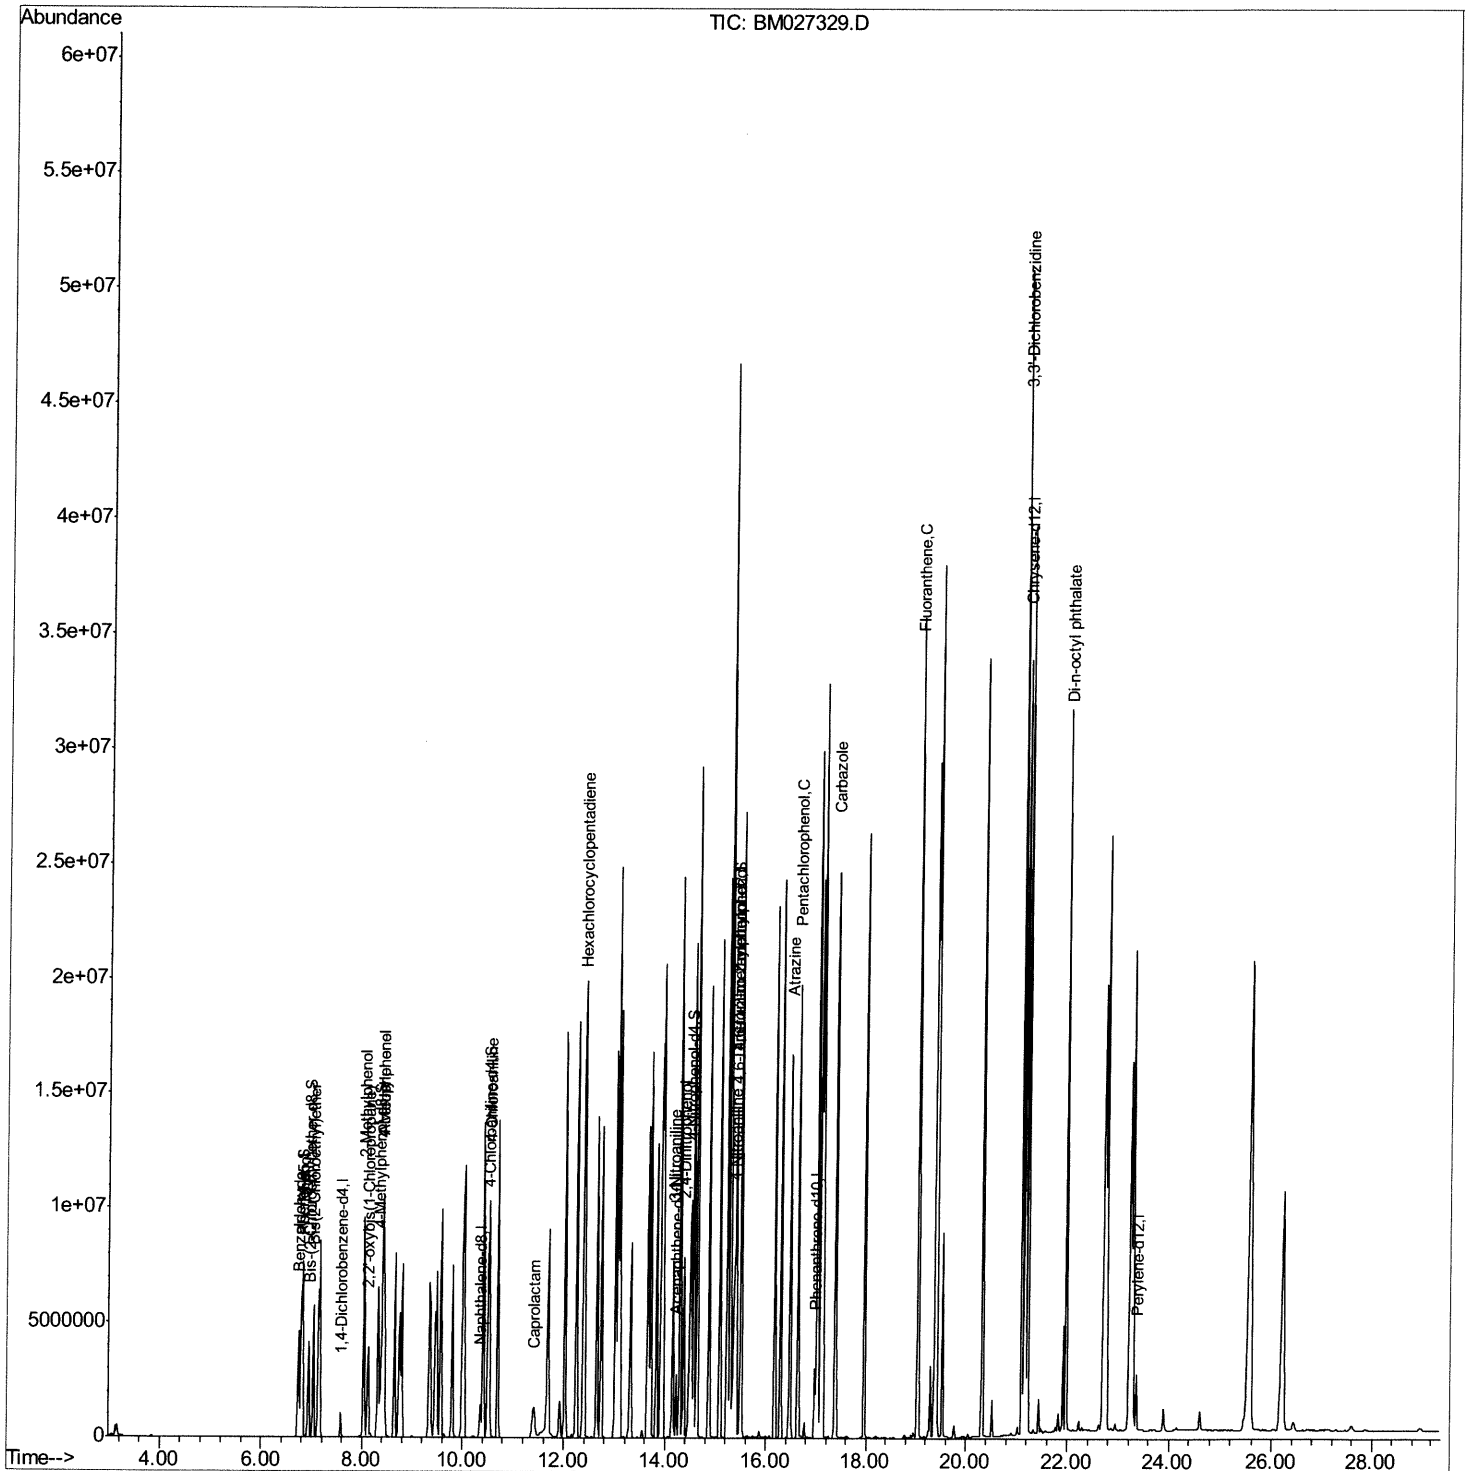

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
 Data File : BM027329.D
 Acq On : 04 Sep 2020 14:06
 Operator : JU/CG
 Sample : SSTD16001
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16001

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:36:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 12:49:01 2020
 Response via : Initial Calibration

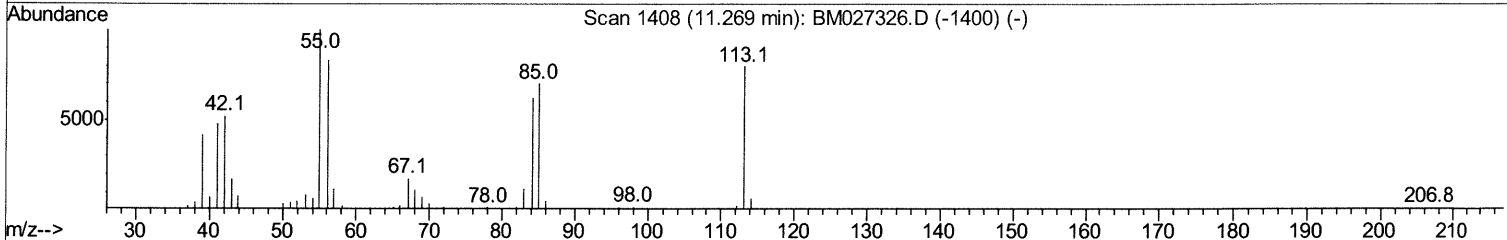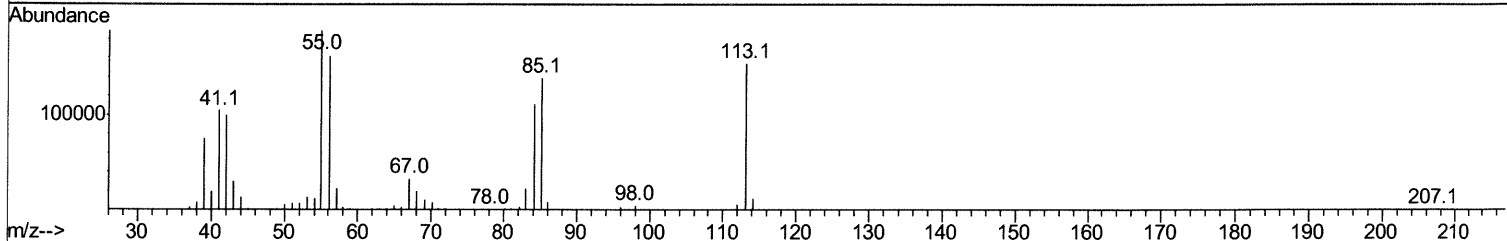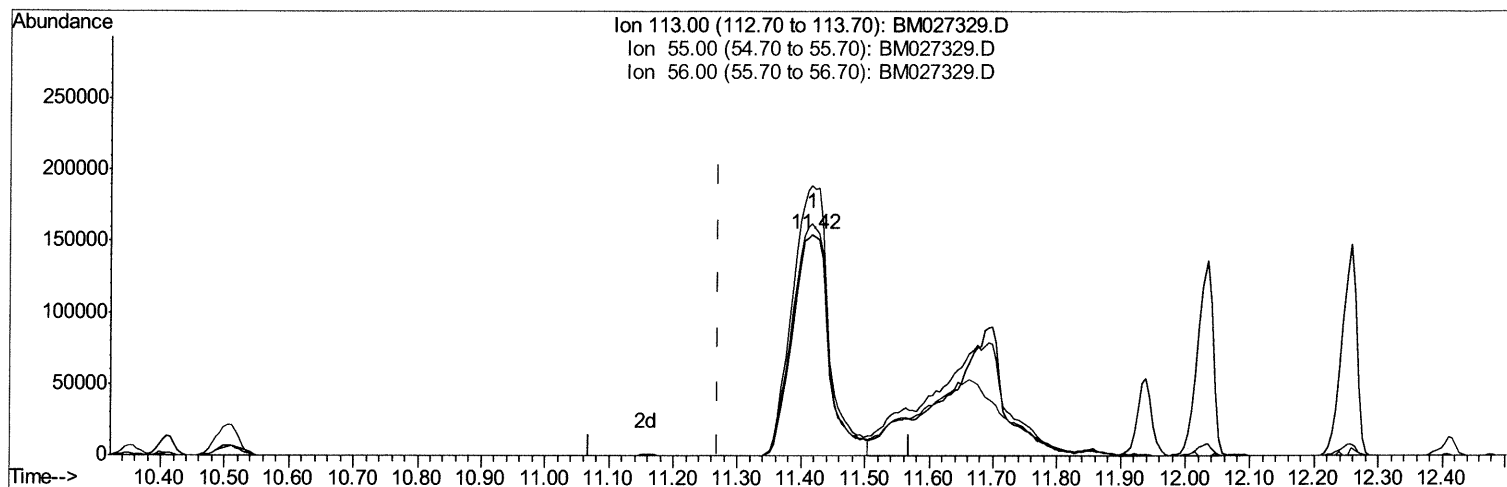

TIC: BM027329.D

(32) Caprolactam

11.416min (+0.147) 97.33ng/ul

response 625183

Ion	Exp%	Act%
113.00	100	100
55.00	125.60	122.13
56.00	104.60	104.92
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
 Data File : BM027329.D
 Acq On : 04 Sep 2020 14:06
 Operator : JU/CG
 Sample : SSTD16001
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16001

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:36:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 12:49:01 2020
 Response via : Initial Calibration

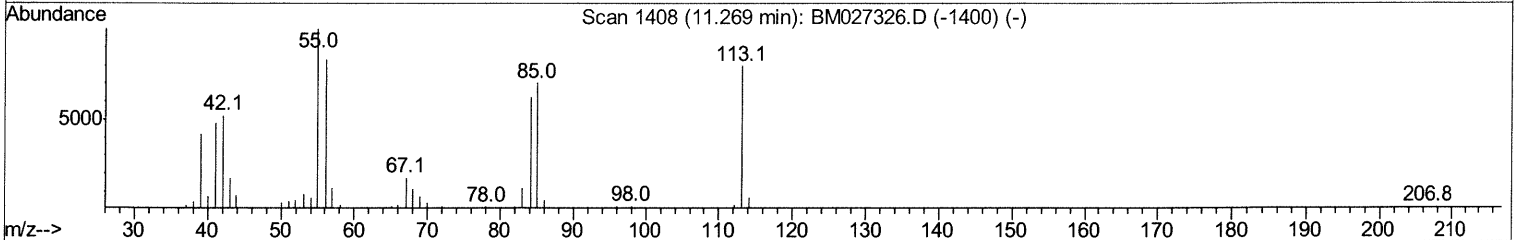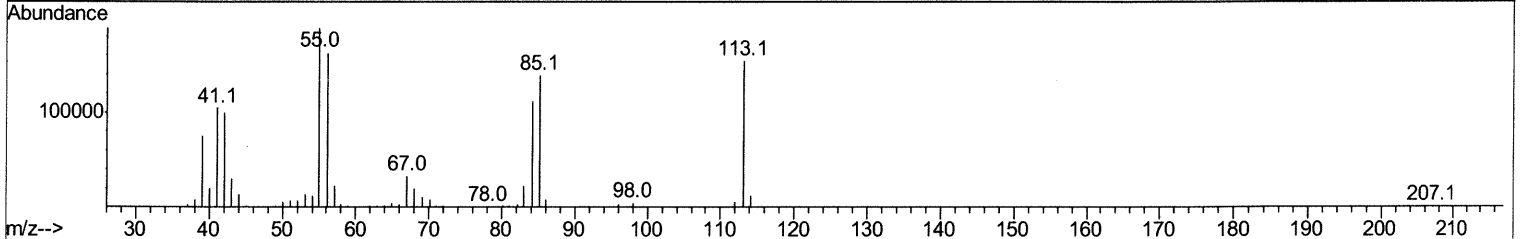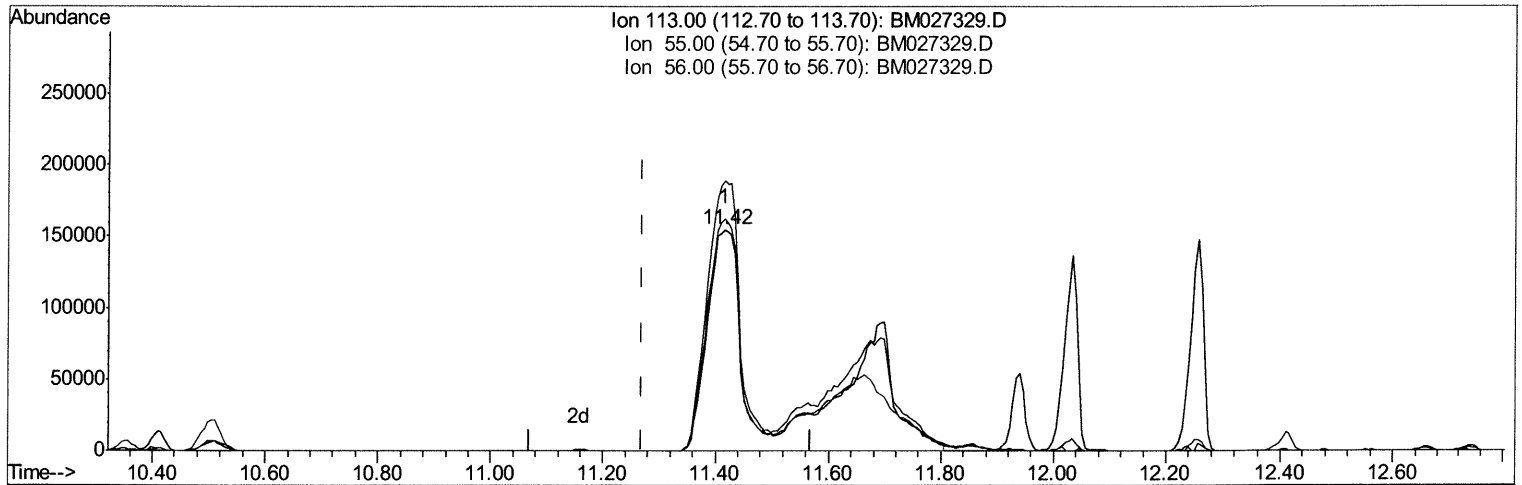

TIC: BM027329.D

(32) Caprolactam

11.416min (+0.147) 192.21ng/ul m 09/09/20 JU

response 1234651

Ion	Exp%	Act%
113.00	100	100
55.00	125.60	122.13
56.00	104.60	104.92
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
Data File : BM027329.D
Acq On : 04 Sep 2020 14:06
Operator : JU/CG
Sample : SSTD16001
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD16001

Manual Integrations
APPROVED

mohammad
9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:36:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 04 12:49:01 2020
Response via : Initial Calibration

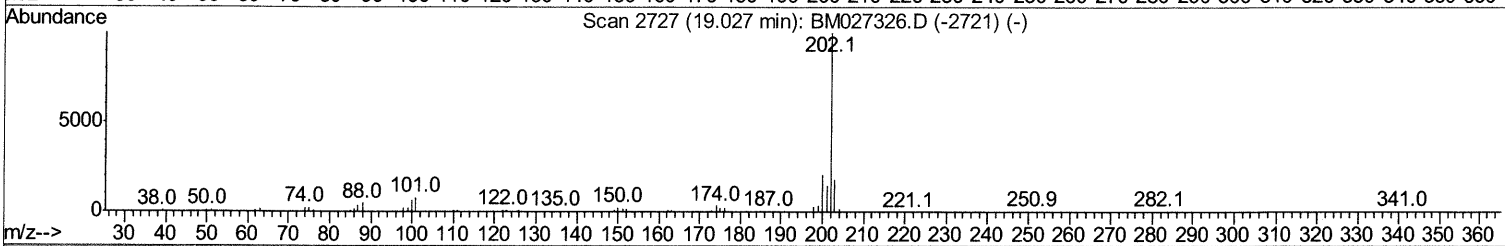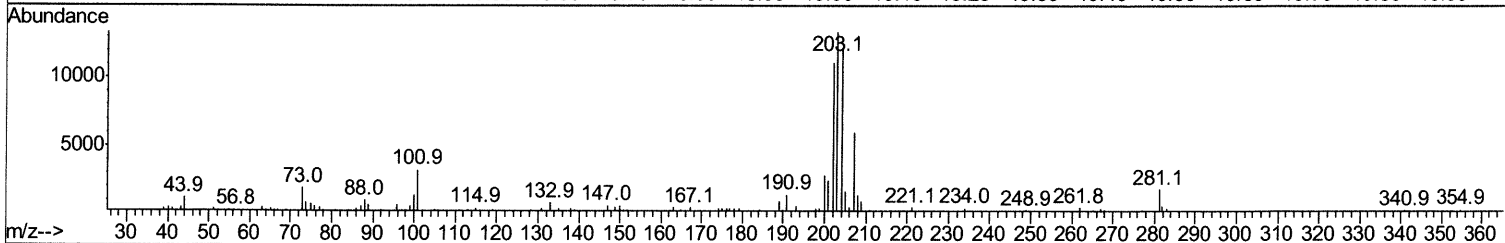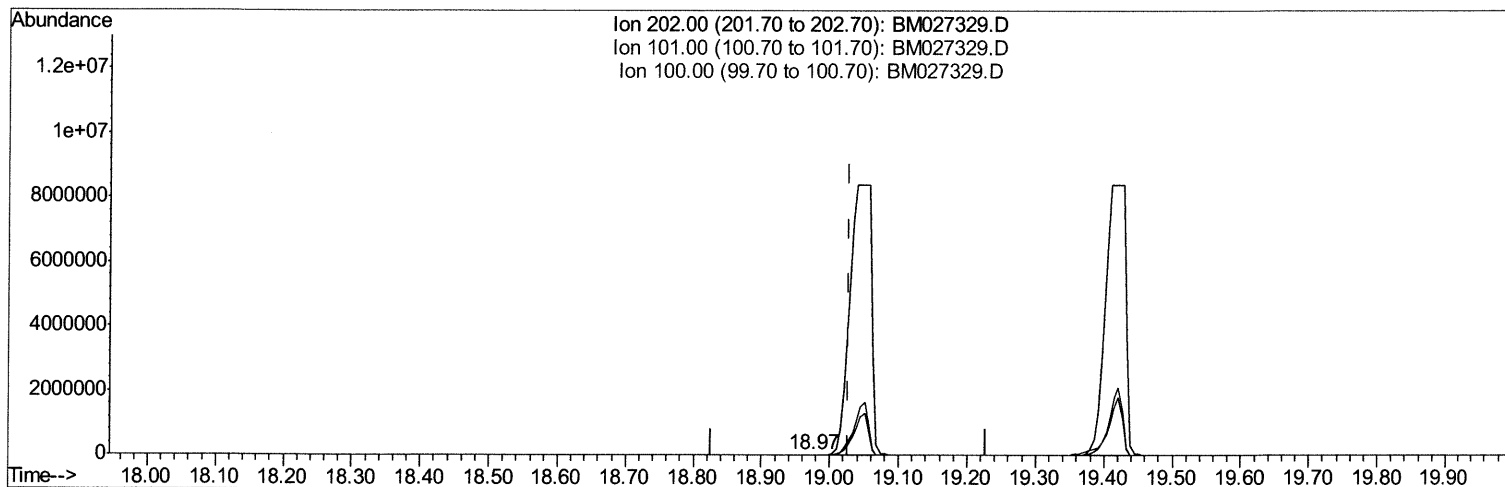

TIC: BM027329.D

(77) Fluoranthene (C)

18.974min (-0.053) 0.09ng/ul

response 13890

Ion	Exp%	Act%
202.00	100	100
101.00	7.70	28.73#
100.00	6.30	11.87#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
Data File : BM027329.D
Acq On : 04 Sep 2020 14:06
Operator : JU/CG
Sample : SSTD16001
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD16001

Manual Integrations
APPROVED

mohammad
9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:36:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 04 12:49:01 2020
Response via : Initial Calibration

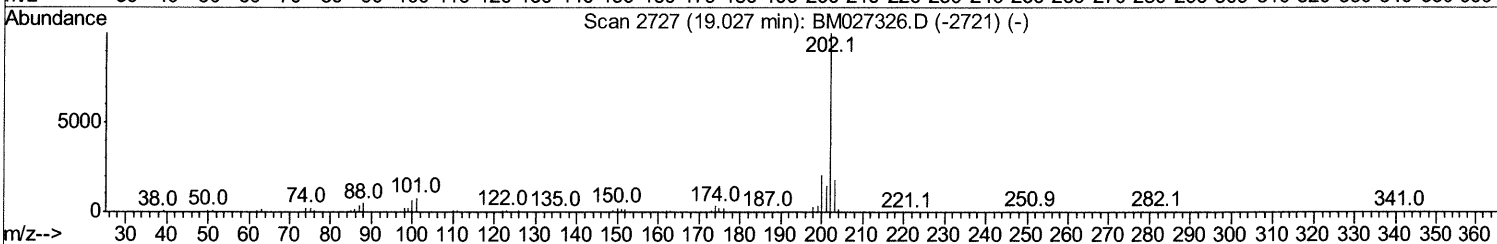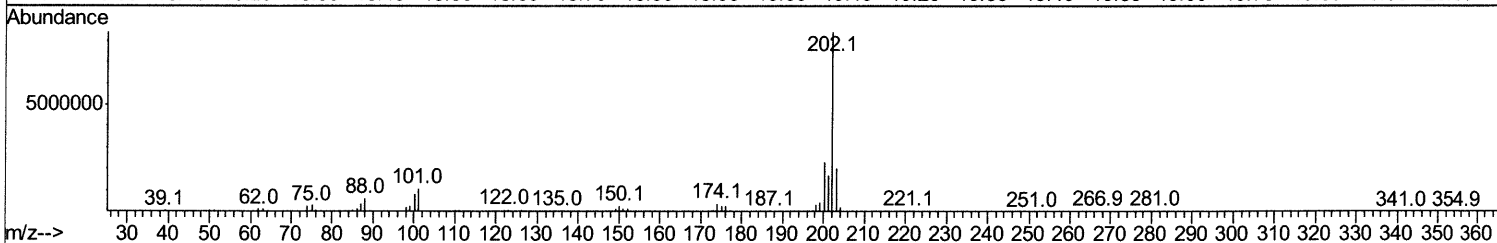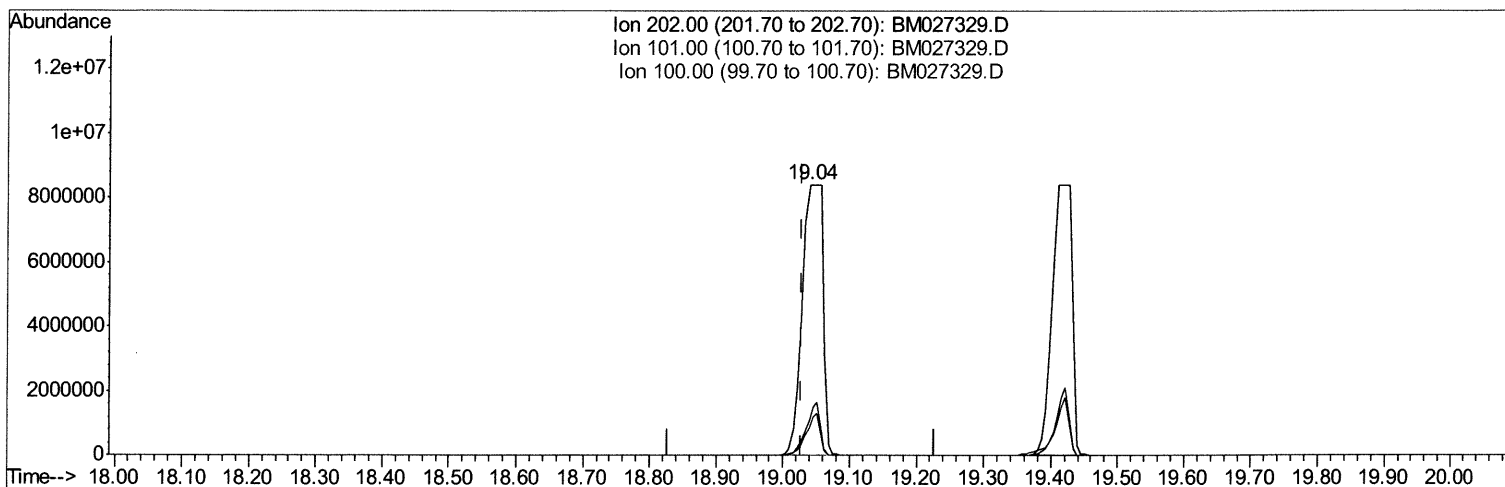

TIC: BM027329.D

(77) Fluoranthene (C)

19.039min (+0.011) 122.28ng/ul m 09/09/20 JU

response 18256519

Ion	Exp%	Act%
202.00	100	100
101.00	7.70	12.64#
100.00	6.30	9.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
 Data File : BM027329.D
 Acq On : 04 Sep 2020 14:06
 Operator : JU/CG
 Sample : SSTD16001
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SSTD16001

Manual Integrations
APPROVED

mohammad
 9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:36:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 12:49:01 2020
 Response via : Initial Calibration

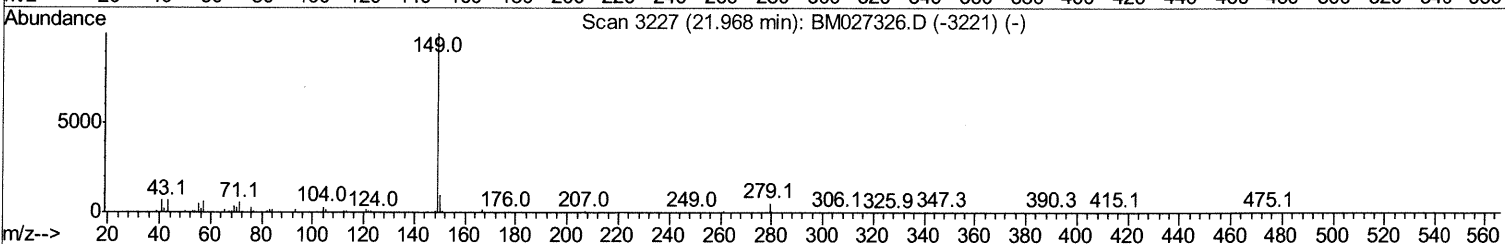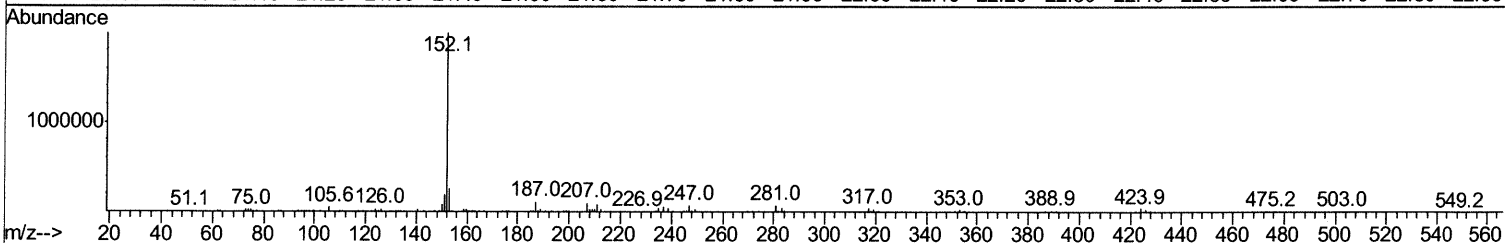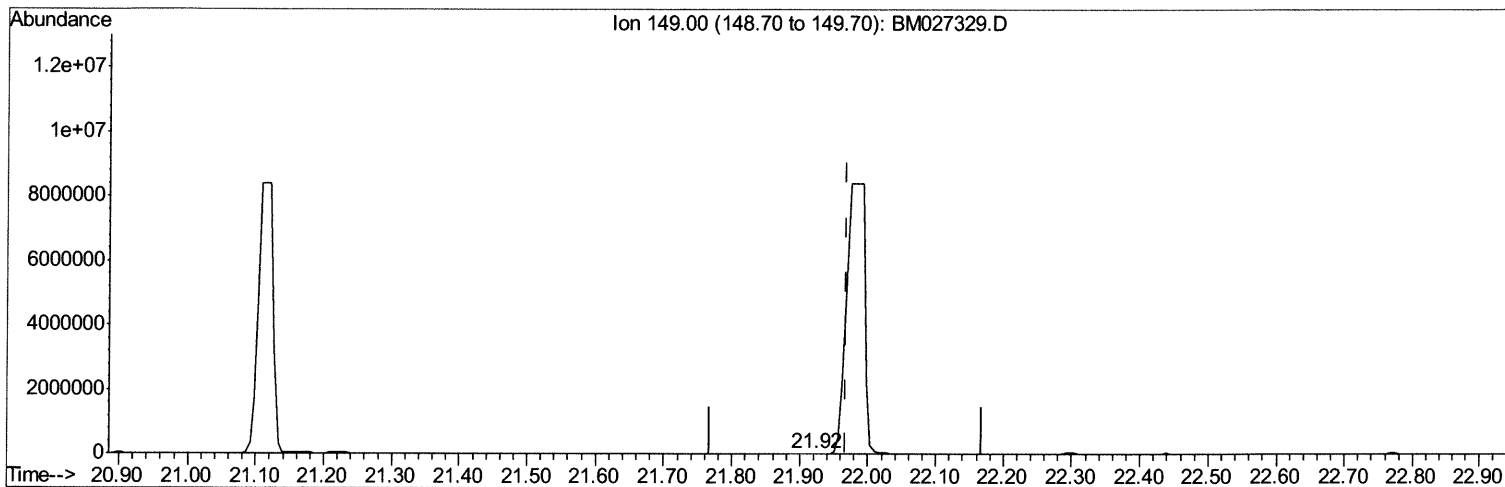

TIC: BM027329.D

(87) Di-n-octyl phthalate

21.921min (-0.047) 0.12ng/ul

response 13795

Ion	Exp%	Act%
149.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
 Data File : BM027329.D
 Acq On : 04 Sep 2020 14:06
 Operator : JU/CG
 Sample : SSTD16001
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16001

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:36:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 12:49:01 2020
 Response via : Initial Calibration

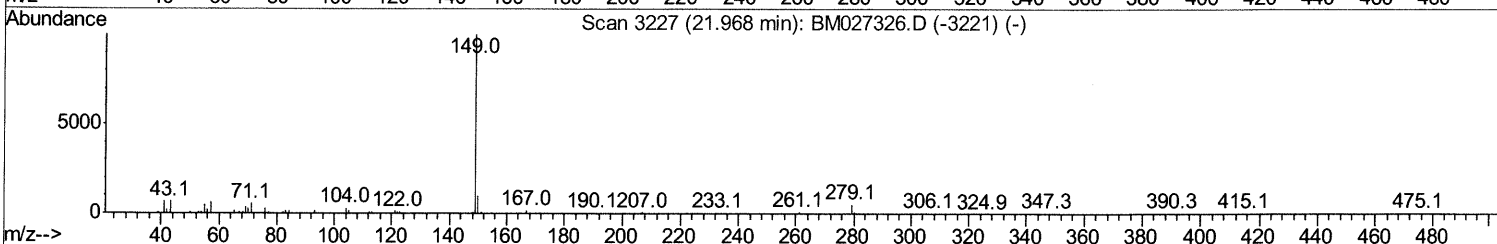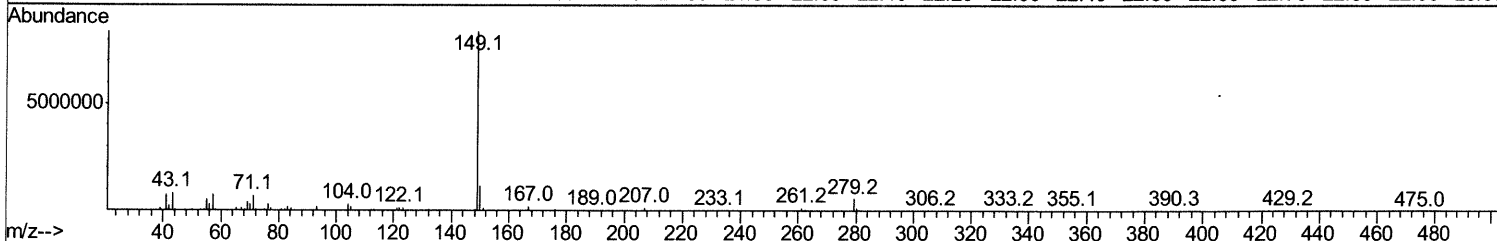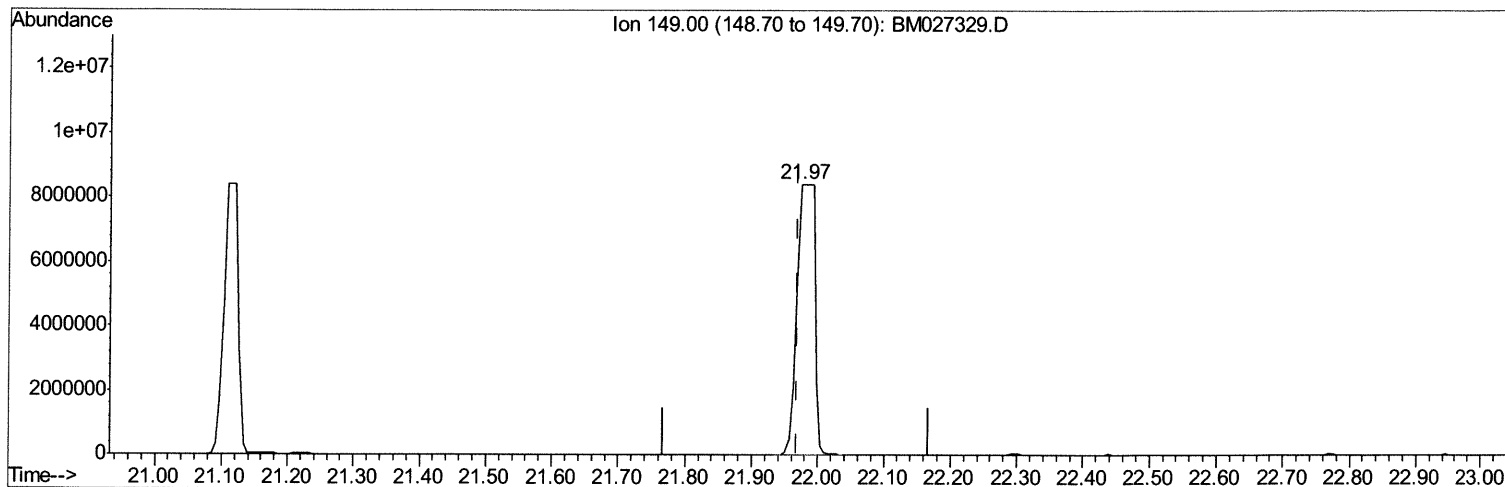

TIC: BM027329.D

(87) Di-n-octyl phthalate

21.974min (+0.006) 135.07ng/ul m 09/09/20 JU

response 15740841

Ion	Exp%	Act%
149.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
 Data File : BM027329.D
 Acq On : 04 Sep 2020 14:06
 Operator : JU/CG
 Sample : SSTD16001
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SSTD16001

Manual Integrations
APPROVED

mohammad
 9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:43:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 12:49:01 2020
 Response via : Initial Calibration

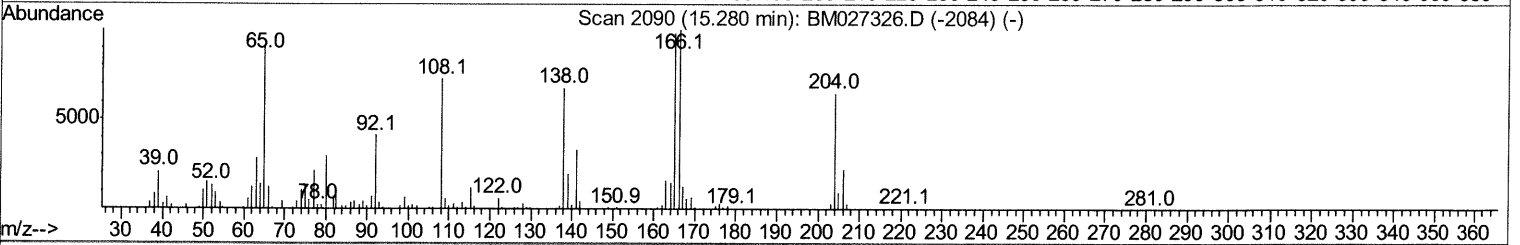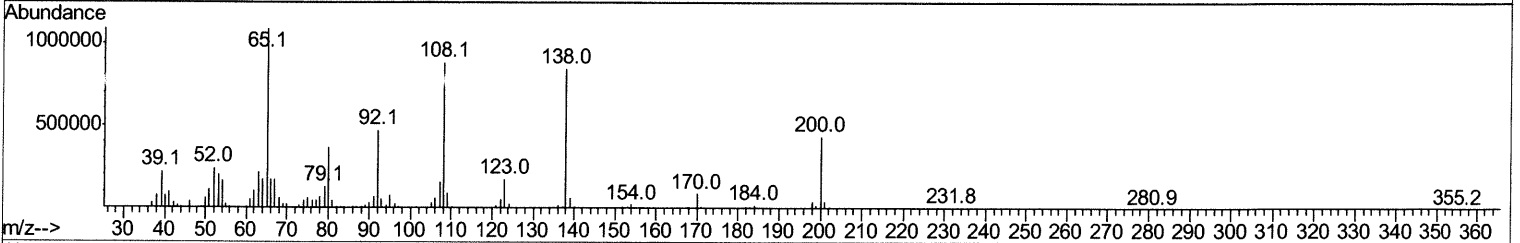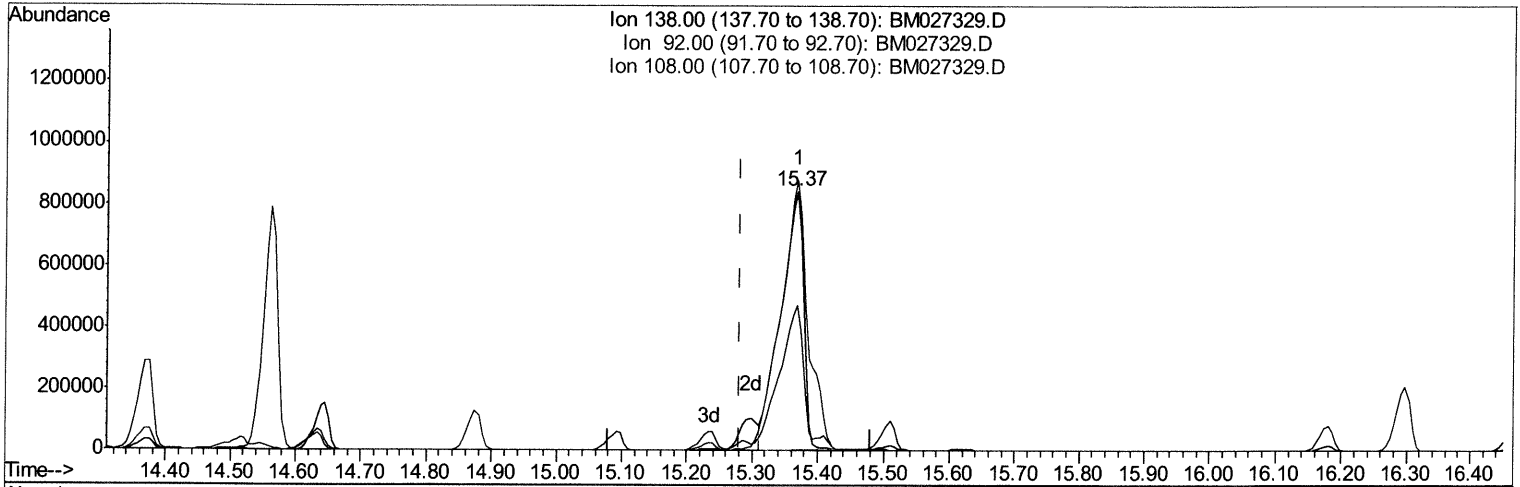

TIC: BM027329.D

(61) 4-Nitroaniline

15.368min (+0.088) 137.99ng/ul

response 2030229

Ion	Exp%	Act%
138.00	100	100
92.00	60.80	55.90
108.00	107.90	104.25
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090420\
Data File : BM027329.D
Acq On : 04 Sep 2020 14:06
Operator : JU/CG
Sample : SSTD16001
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD16001

Manual Integrations
APPROVED

mohammad
9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:43:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 04 12:49:01 2020
Response via : Initial Calibration

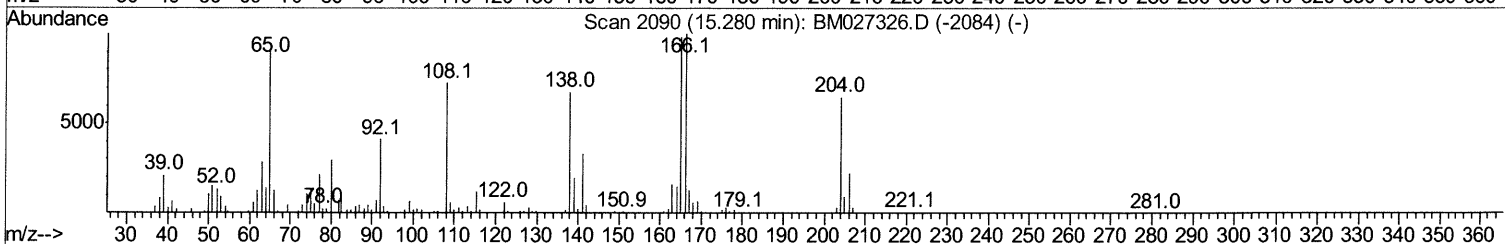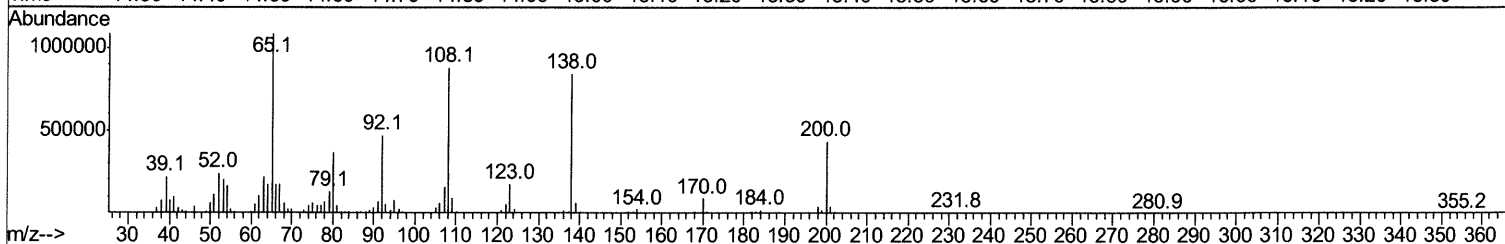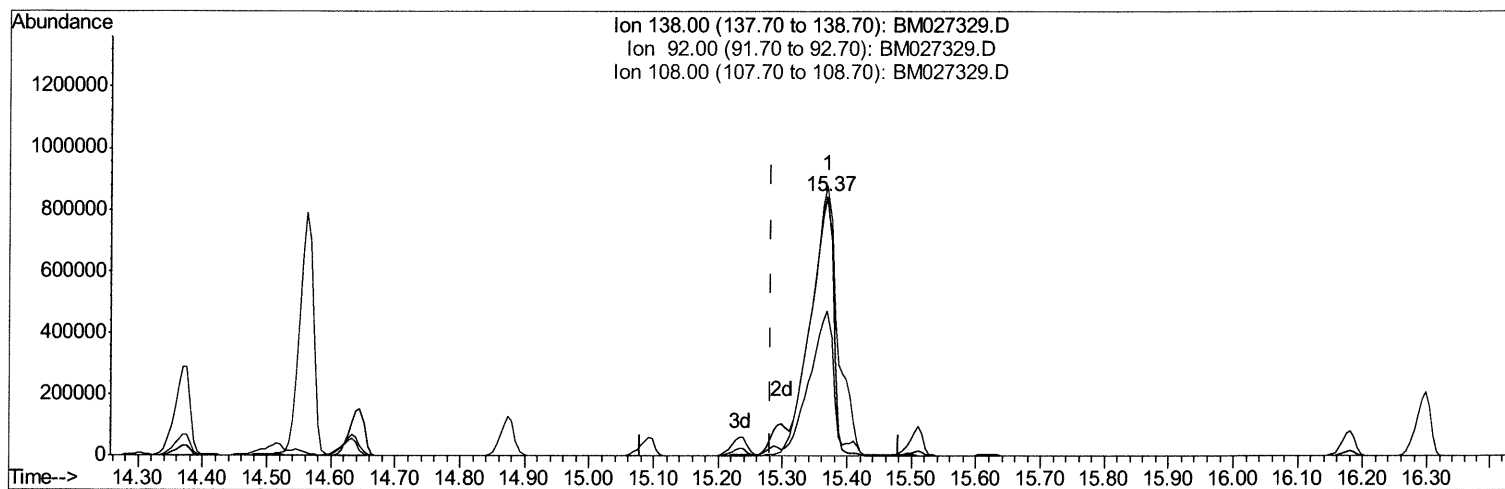

TIC: BM027329.D

(61) 4-Nitroaniline

15.368min (+0.088) 152.39ng/ul m 09/09/20 JU

response 2242132

Ion	Exp%	Act%
138.00	100	100
92.00	60.80	55.90
108.00	107.90	104.25
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027329.D
 Acq On : 04 Sep 2020 14:06
 Operator : JU/CG
 Sample : SSTD16001
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16001

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:45:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 12:49:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	255341	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1170712	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	919242	20.00	ng/ul	0.01
62) Phenanthrene-d10	16.97	188	2183370	20.00	ng/ul	0.01
78) Chrysene-d12	21.18	240	2250828	20.00	ng/ul	0.02
86) Perylene-d12	23.36	264	1495921	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	6.79	99	3852471	186.07	ng/ul	0.04
7) Bis-(2-Chloroethyl)ether-d	6.94	67	2381065	177.74	ng/ul	0.02
9) 2-Chlorophenol-d4	0.00	132	0d	0.00	ng/ul	
13) 4-Methylphenol-d8	8.32	113	3129123	188.25	ng/ul	0.04
19) Nitrobenzene-d5	0.00	128	0d	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.50	131	4151539	174.61	ng/ul	0.02
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul	
52) 4-Nitrophenol-d4	14.50	143	2198380	178.68	ng/ul	0.08
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul	
63) 4,6-Dinitro-2-methylphenol	15.39	200	2839731	199.38	ng/ul	0.05
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul	
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	

Target Compounds

						Ovalue
4) Benzaldehyde	6.73	77	1983242	135.981	ng/ul	96
6) Phenol	6.82	94	4070252	188.019	ng/ul	93
8) Bis(2-Chloroethyl)ether	7.03	93	3120468	179.286	ng/ul	96
11) 2-Methylphenol	8.04	108	3077209	191.160	ng/ul	97
12) 2,2'-oxybis(1-Chloropropan	8.12	45	2336634	173.395	ng/ul	97
14) Acetophenone	8.42	105	5112755	191.985	ng/ul	92
16) 4-Methylphenol	8.40	108	3282569	190.172	ng/ul	97
30) 4-Chloroaniline	10.53	127	4239806	177.985	ng/ul	100
32) Caprolactam	11.42	113	1234651m>	192.212	ng/ul	> 09/09/2024
38) Hexachlorocyclopentadiene	12.39	237	4004811	180.145	ng/ul	98
49) 3-Nitroaniline	14.16	138	2168758	163.070	ng/ul	96
51) 2,4-Dinitrophenol	14.37	184	1952396	217.947	ng/ul#	83
53) 4-Nitrophenol	14.52	109	2050151	175.789	ng/ul	92
61) 4-Nitroaniline	15.37	138	2242132m>	152.392	ng/ul	> 09/09/2024
64) 4,6-Dinitro-2-methylphenol	15.41	198	3020513	195.374	ng/ul#	89
68) Atrazine	16.49	200	4587344	170.009	ng/ul	98
69) Pentachlorophenol	16.64	266	3697220	201.483	ng/ul	98
75) Carbazole	17.39	167	16203500	154.844	ng/ul#	91
77) Fluoranthene	19.04	202	18256519m>	122.285	ng/ul	> 09/09/2024
82) 3,3'-Dichlorobenzidine	21.11	252	7436840	141.827	ng/ul#	99
87) Di-n-octyl phthalate	21.97	149	15740841m>	135.066	ng/ul	> 09/09/2024

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027329.D
Acq On : 04 Sep 2020 14:06
Operator : JU/CG
Sample : SSTD16001
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD16001

Manual Integrations
APPROVED

mohammad
9/8/2020 1:45:44 PM

Quant Time: Sep 04 14:45:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 04 12:49:01 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed