

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027333.D
 Acq On : 04 Sep 2020 16:54
 Operator : JU/CG
 Sample : L3840-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2

Quant Time: Sep 04 17:25:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 14:46:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	94822	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	368487	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	265460	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	642814	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	830417	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1038117	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	7860	3.69	ng/uL	0.00
5) Phenol-d5	6.76	99	99470	12.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	102022	19.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	84569	14.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	87934	13.80	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	50962	18.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	52964	17.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	85843	13.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	114273	14.77	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	481398	22.79	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	353557	14.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	31748	8.54	ng/ul	0.00
58) Fluorene-d10	15.21	176	311663	16.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	52894	12.86	ng/ul	0.00
71) Anthracene-d10	17.06	188	447723	14.73	ng/ul	0.00
79) Pyrene-d10	19.36	212	518367	14.01	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	682713	12.26	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	171331	7.697	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027333.D
Acq On : 04 Sep 2020 16:54
Operator : JU/CG
Sample : L3840-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB2

Quant Time: Sep 04 17:25:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 04 14:46:56 2020
Response via : Initial Calibration

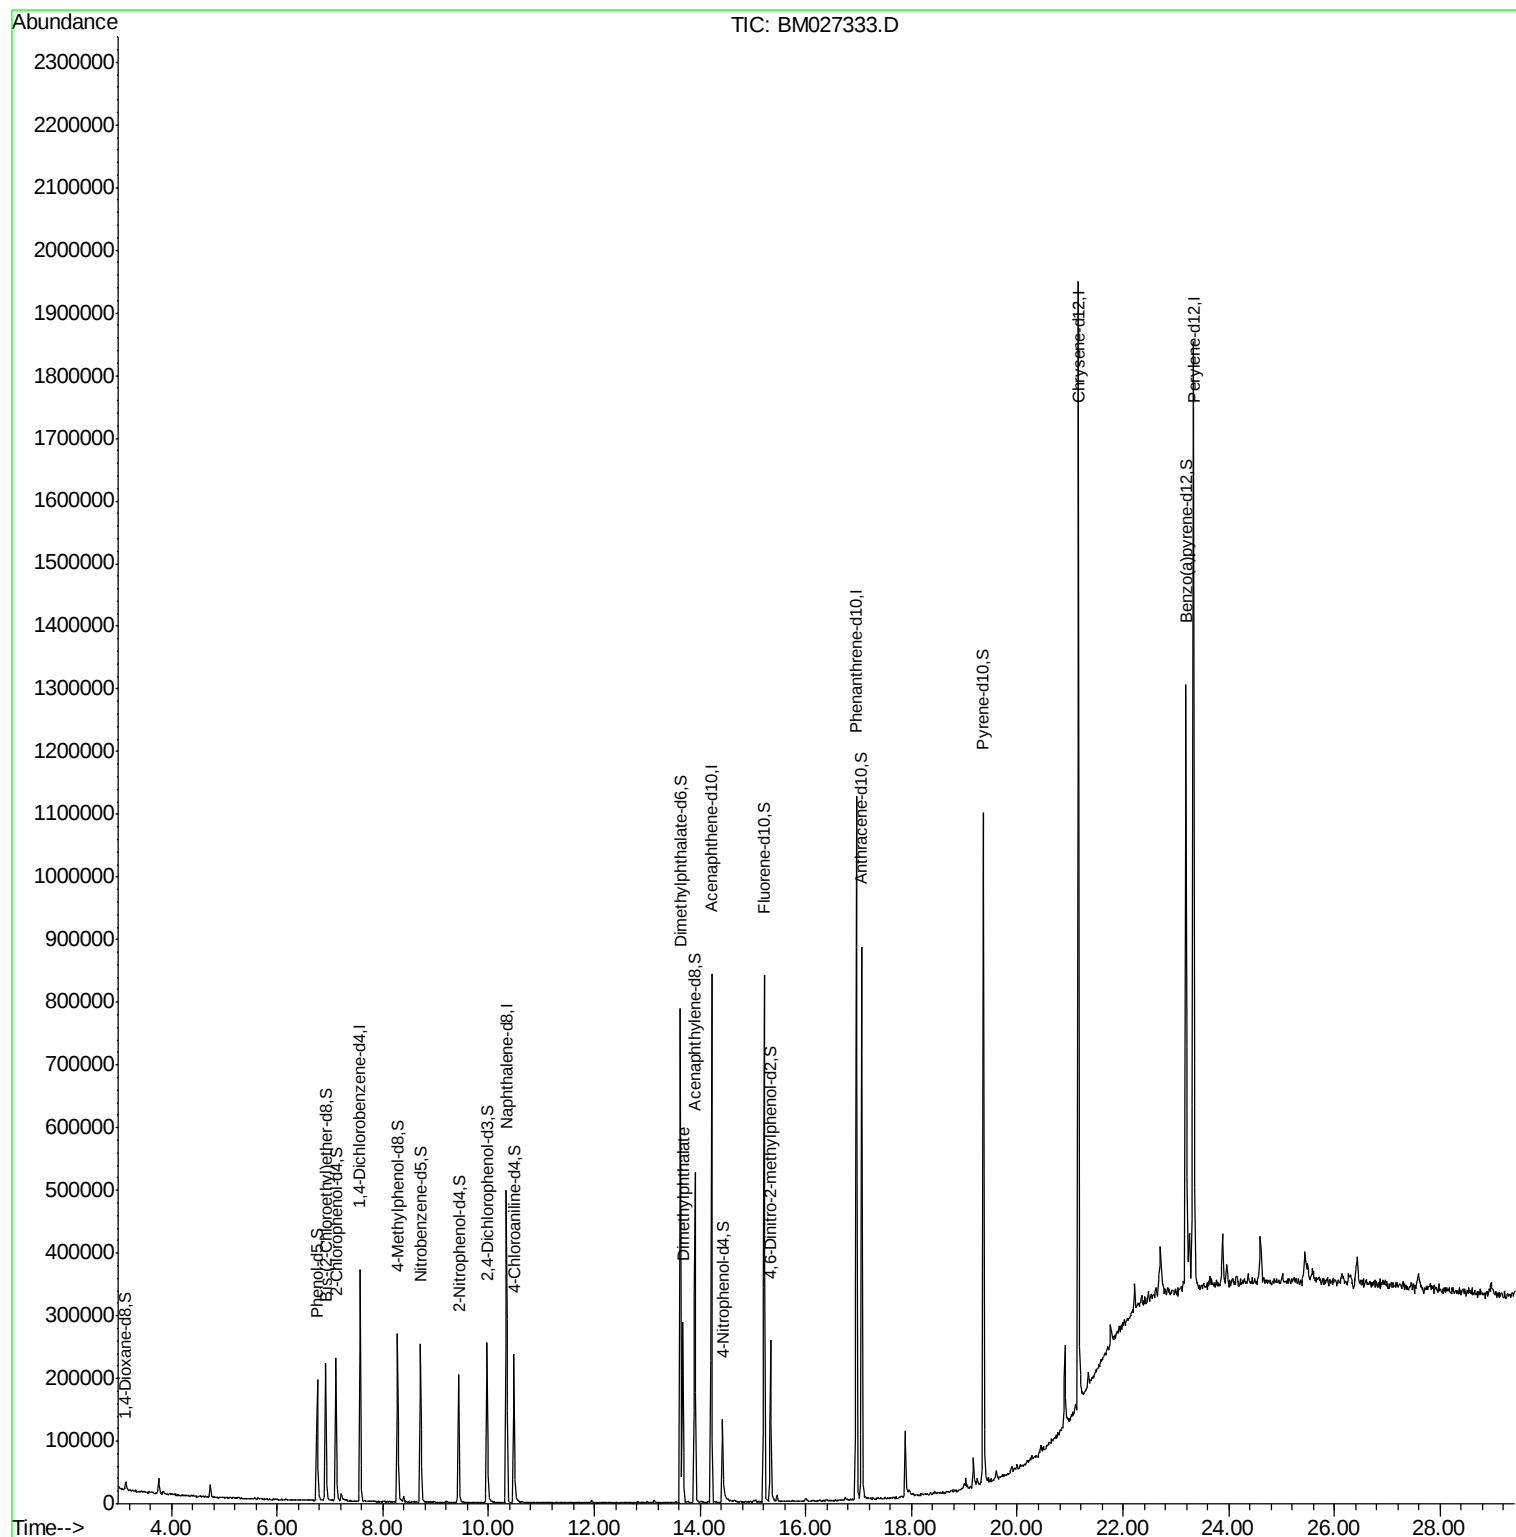

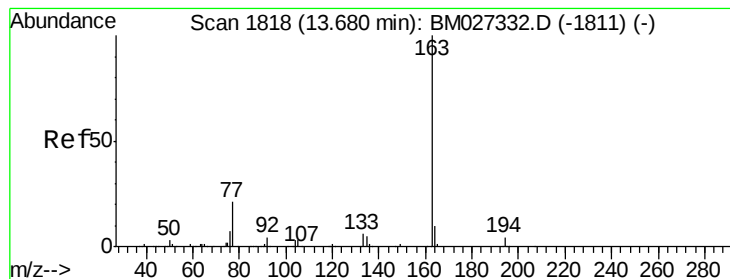

#45

Dimethylphthalate

Concen: 7.697 ng/ul

RT: 13.68 min Scan# 1818

Delta R.T. -0.00 min

Lab File: BM027333.D

Acq: 04 Sep 2020 16:54

Instrument :

BNA_M

ClientSampleId :

C0AB2


Tot Ion:163 Resp: 171331

Ion Ratio Lower Upper

163 100

194 4.5 3.3 4.9

164 10.8 8.1 12.1

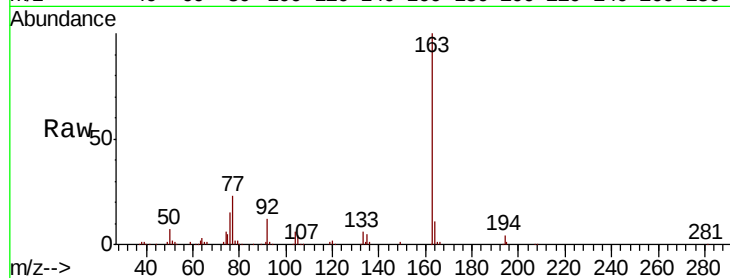

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

