

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027334.D
 Acq On : 04 Sep 2020 17:30
 Operator : JU/CG
 Sample : L3840-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB5

Quant Time: Sep 04 18:03:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 04 14:46:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	94908	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	377636	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	278725	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	671352	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	862300	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1053765	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	18035	8.45	ng/uL	0.00
5) Phenol-d5	6.76	99	301310	38.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	209599	40.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	238639	41.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	246827	38.69	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	120803	42.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	139385	44.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	267936	39.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	336569	42.43	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	952246	42.94	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1107000	44.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	116511	29.83	ng/ul	0.00
58) Fluorene-d10	15.21	176	814563	41.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	126259	29.39	ng/ul	0.00
71) Anthracene-d10	17.06	188	1337470	42.13	ng/ul	0.00
79) Pyrene-d10	19.36	212	1689918	43.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	2317173	41.00	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	335488	14.354	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027334.D
Acq On : 04 Sep 2020 17:30
Operator : JU/CG
Sample : L3840-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB5

Quant Time: Sep 04 18:03:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 04 14:46:56 2020
Response via : Initial Calibration

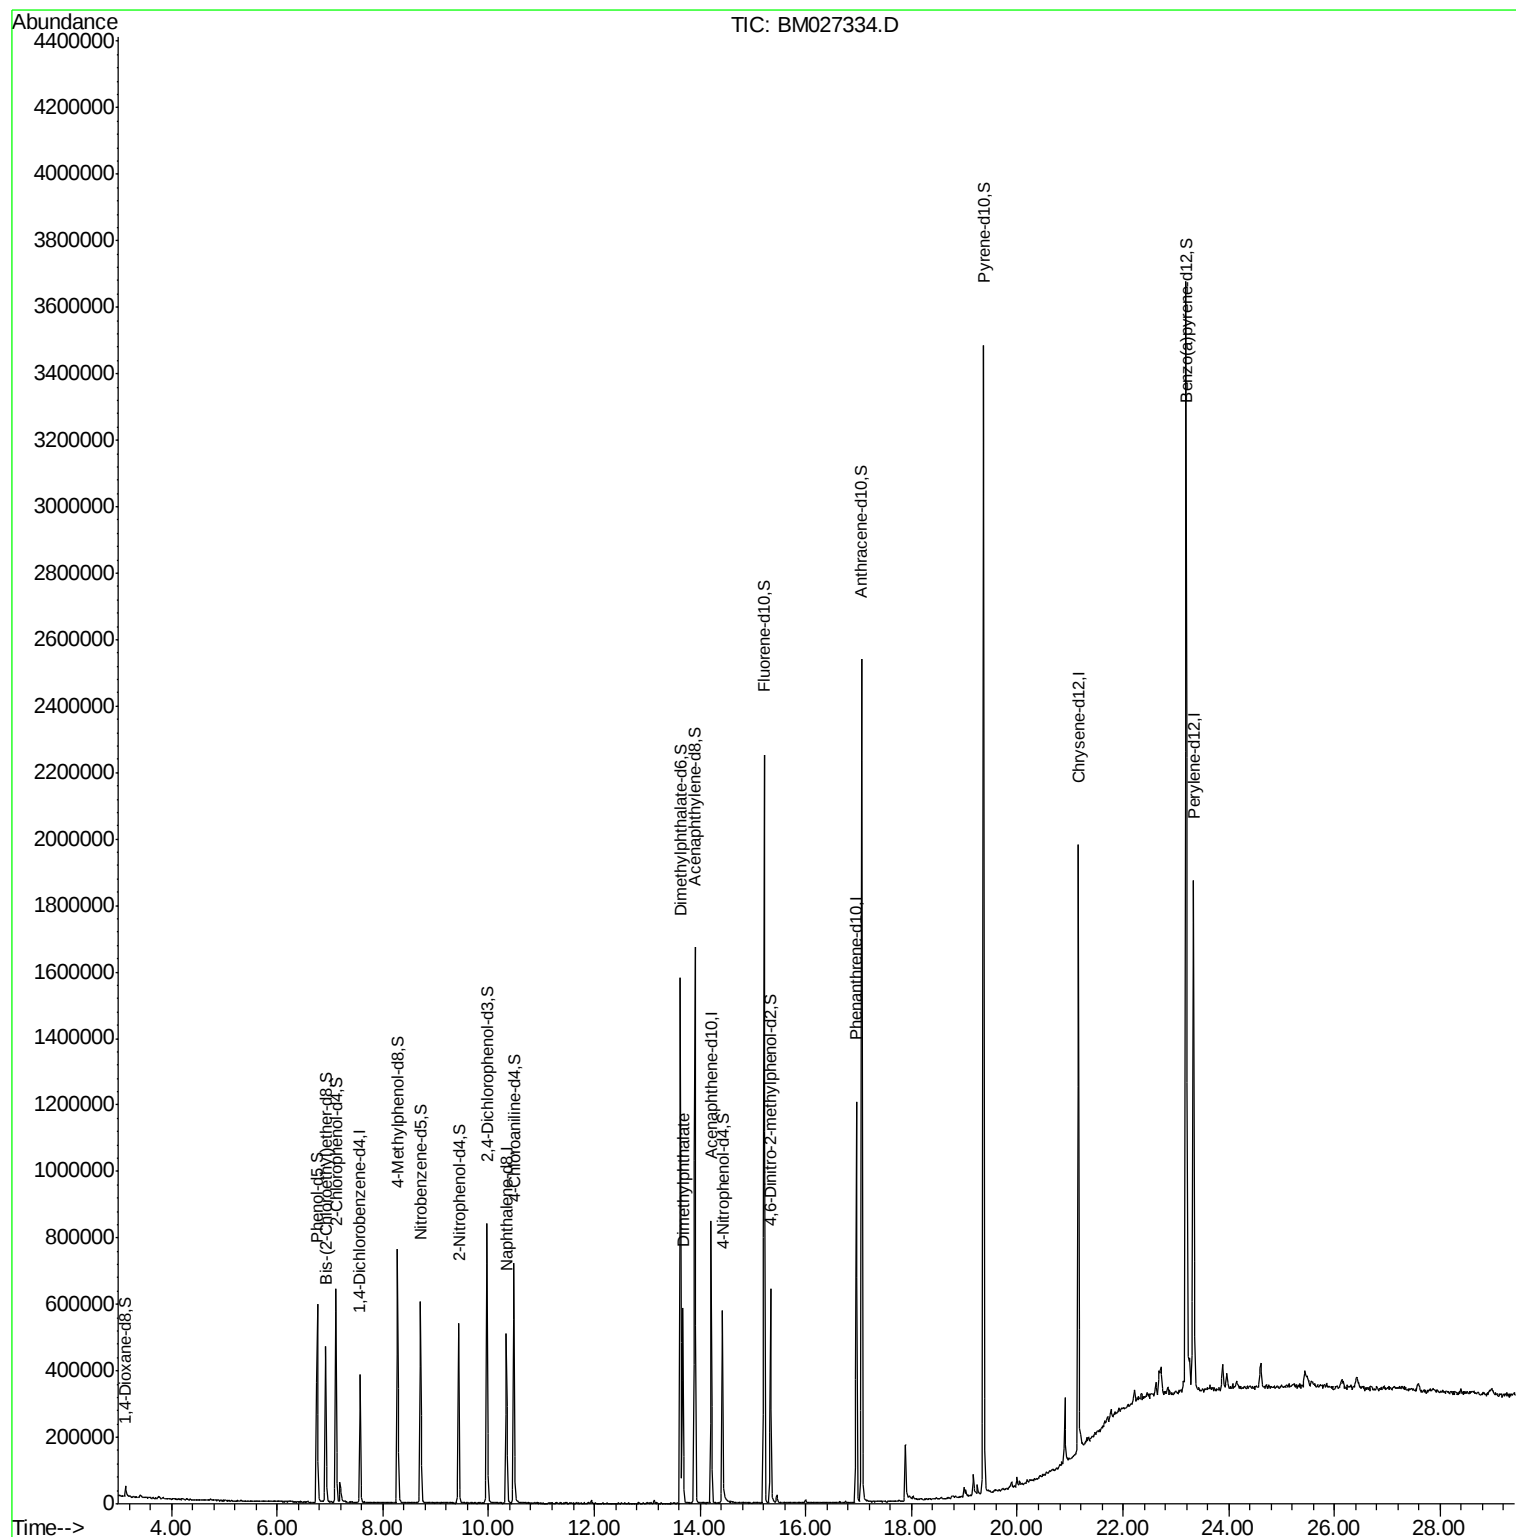

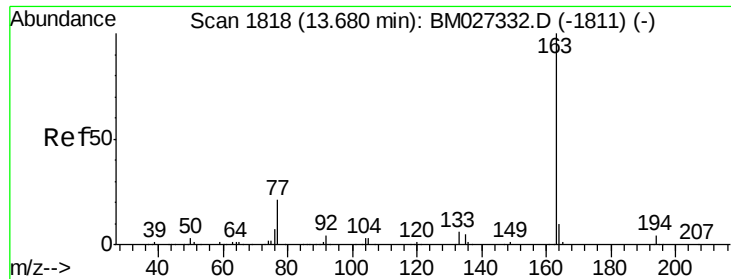

#45

Dimethylphthalate

Concen: 14.354 ng/ul

RT: 13.68 min Scan# 1818

Delta R.T. -0.00 min

Lab File: BM027334.D

Acq: 04 Sep 2020 17:30

Instrument :

BNA_M

ClientSampleId :

C0AB5


Tot Ion:163 Resp: 335488

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.3 8.1 12.1

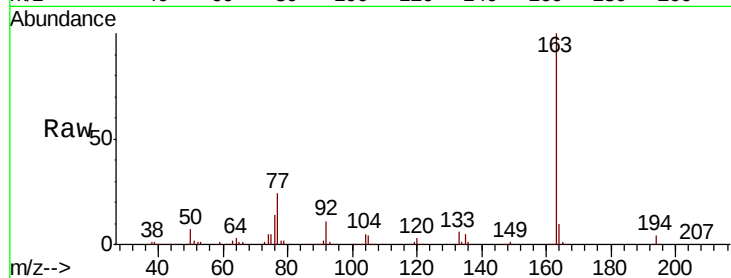

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

