

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027337.D
 Acq On : 04 Sep 2020 19:20
 Operator : JU/CG
 Sample : L3840-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB1

Quant Time: Sep 05 01:25:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 05 00:52:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	148841	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	602272	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	447093	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1068200	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1352825	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1527509	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	10355	3.10	ng/uL	0.00
5) Phenol-d5	6.75	99	152357	12.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	150246	18.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	127824	14.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	136105	13.60	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	75547	16.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	82349	16.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	139206	13.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	180043	14.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	765685	21.52	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	575957	14.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	66328	10.59	ng/ul	0.00
58) Fluorene-d10	15.21	176	500214	15.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	83023	12.14	ng/ul	0.00
71) Anthracene-d10	17.06	188	749546	14.84	ng/ul	0.00
79) Pyrene-d10	19.36	212	885560	14.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	1072428	13.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.67	163	258933	6.906	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027337.D
Acq On : 04 Sep 2020 19:20
Operator : JU/CG
Sample : L3840-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB1

Quant Time: Sep 05 01:25:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 05 00:52:50 2020
Response via : Initial Calibration

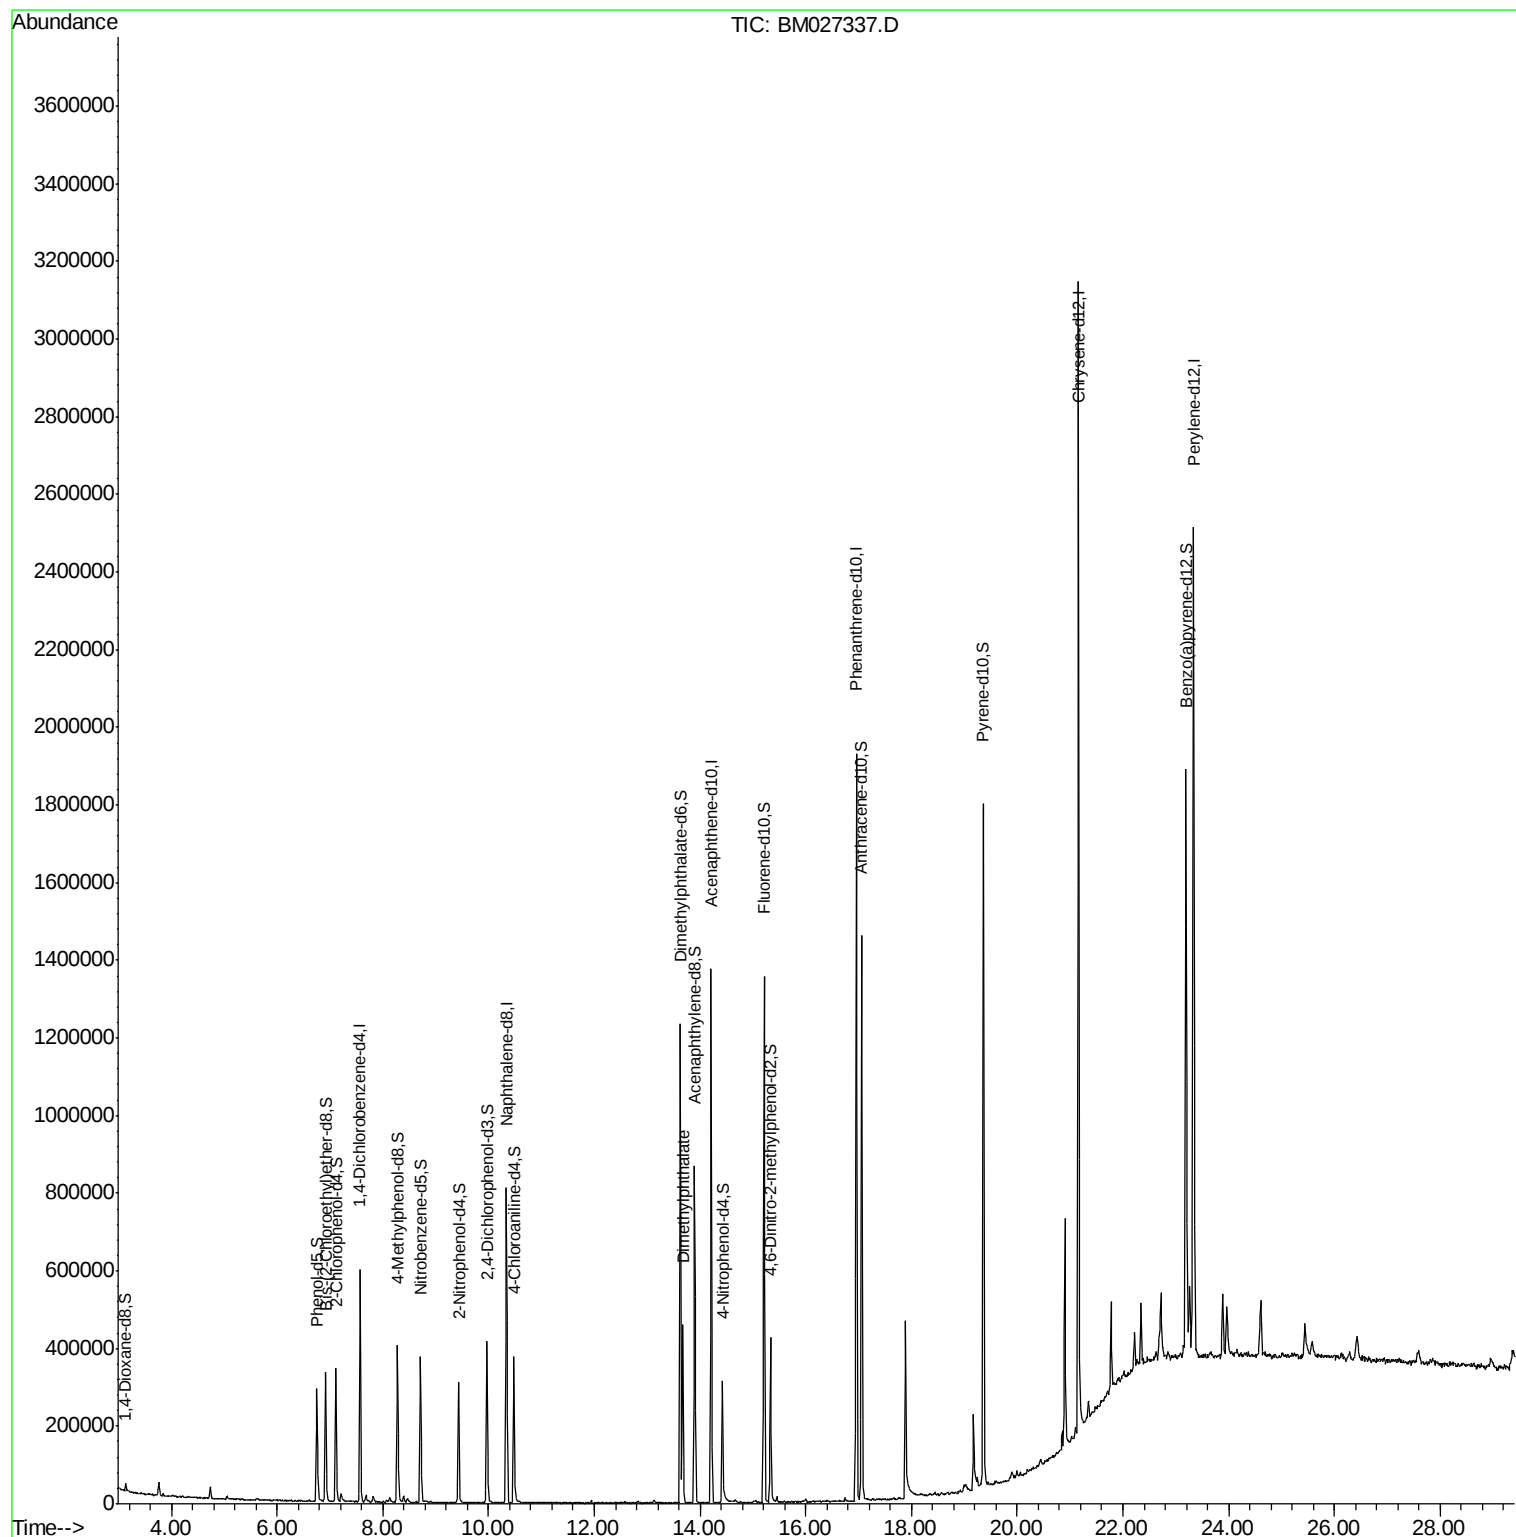

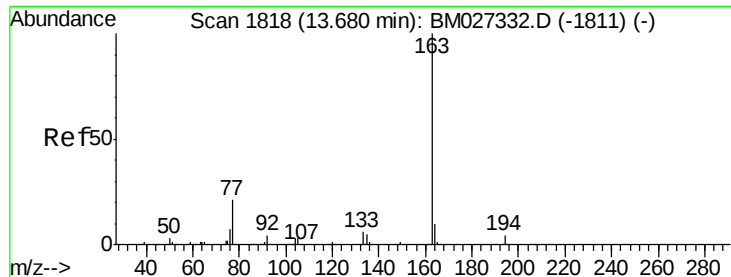

#45

Dimethylphthalate

Concen: 6.906 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM027337.D

Acq: 04 Sep 2020 19:20

Instrument :

BNA_M

ClientSampleId :

C0AB1


Tot Ion:163 Resp: 258933

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.5 8.1 12.1

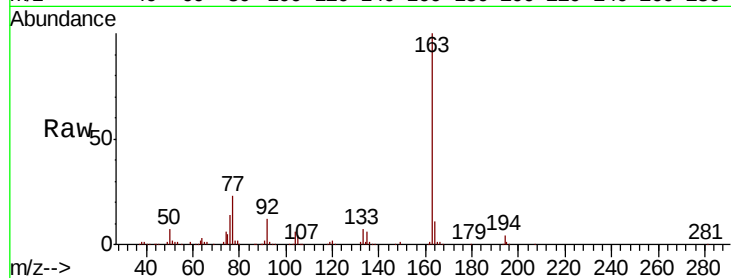

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

