

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027338.D
 Acq On : 04 Sep 2020 19:56
 Operator : JU/CG
 Sample : L3840-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:45:49 PM

Quant Time: Sep 05 01:37:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 05 00:52:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	132646	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	532761	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	400538	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	958088	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1263515	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1355630	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	9896	3.32	ng/uL	0.00
5) Phenol-d5	6.76	99	162548	14.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	124296	17.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	131795	16.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	138661	15.55	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	68859	17.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	77349	17.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	148153	15.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	182110	16.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	612622	19.22	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	646913	17.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	62059	11.06	ng/ul	0.00
58) Fluorene-d10	15.21	176	501256	17.56	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	76492	12.47	ng/ul	0.00
71) Anthracene-d10	17.06	188	808495	17.84	ng/ul	0.00
79) Pyrene-d10	19.36	212	1092958	19.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1392569	19.15	ng/ul	0.00

Target Compounds

					Ovalue
45) Dimethylphthalate	13.67	163	253537	7.549 ng/ul	99
77) Fluoranthene	19.02	202	229713	3.398 ng/ul	99
80) Pyrene	19.39	202	294384	3.851 ng/ul	99
83) Benzo(a)anthracene	21.14	228	380852	4.652 ng/ul	98
85) Chrysene	21.20	228	592393	7.323 ng/ul	99
88) Benzo(b)fluoranthene	22.69	252	567057m	6.336 ng/ul	
89) Benzo(k)fluoranthene	22.73	252	182973	2.039 ng/ul	99
91) Benzo(a)pyrene	23.24	252	322231	3.859 ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.49	276	140683	1.283 ng/ul	95
94) Benzo(g,h,i)perylene	26.14	276	113996	1.244 ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027338.D
Acq On : 04 Sep 2020 19:56
Operator : JU/CG
Sample : L3840-20
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AB8

Manual Integrations
APPROVED

mohammad
9/8/2020 1:45:49 PM

Quant Time: Sep 05 01:37:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 05 00:52:50 2020
Response via : Initial Calibration

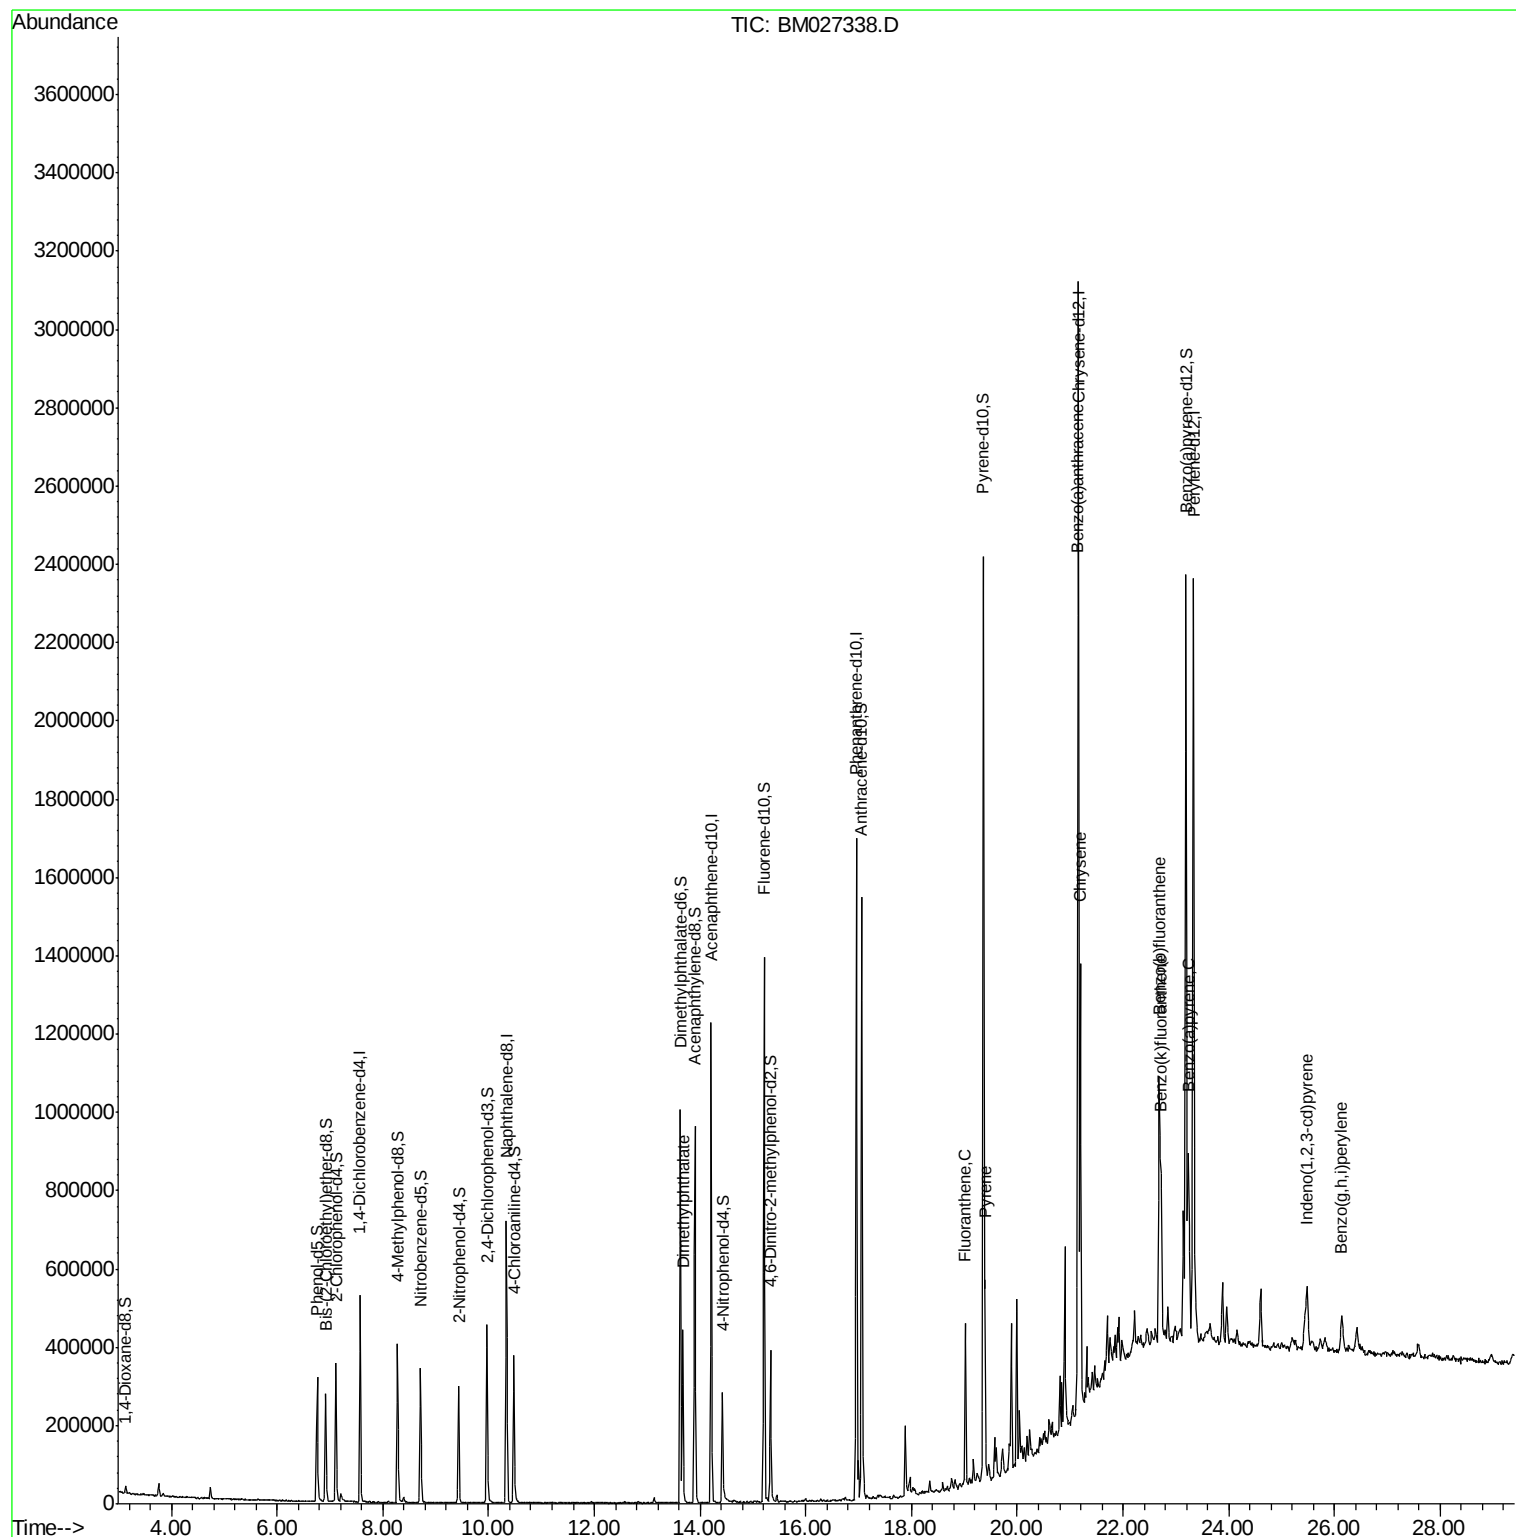

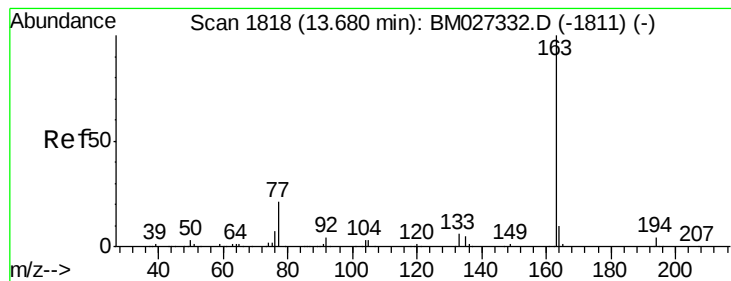

#45

Dimethylphthalate

Concen: 7.549 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56

Instrument :

BNA_M





ClientSampled :

C0AB8

Tot Ion:	163	Resp:	253537
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.3	4.9
164	9.8	8.1	12.1

Manual Integrations
APPROVED

mohammad
9/8/2020 1:45:49 PM

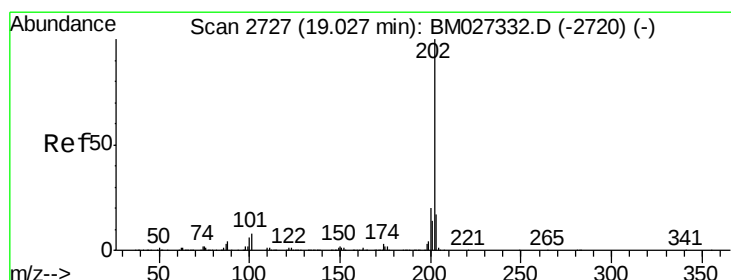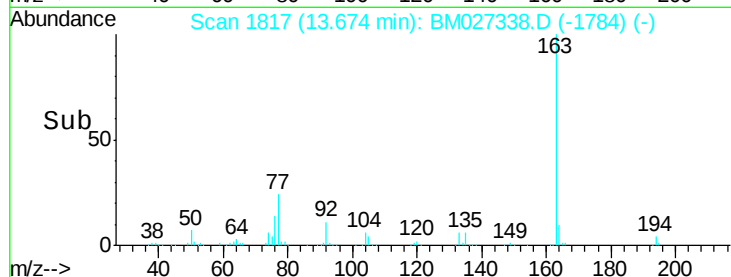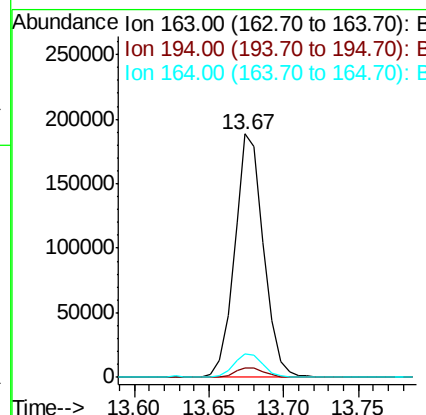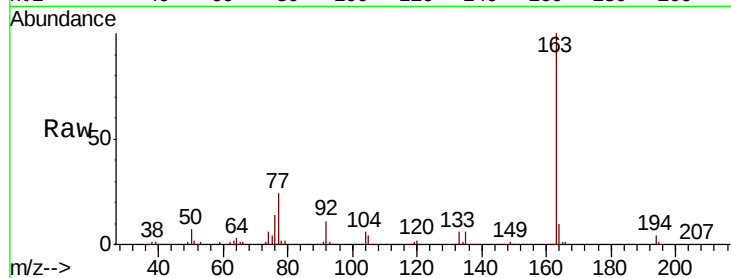

#77

Fluoranthene

Concen: 3.398 ng/ul




RT: 19.02 min Scan# 2726


Delta R.T. -0.01 min

Lab File: BM027338.D

Acq: 04 Sep 2020 19:56

Tgt Ion:	202	Resp:	229713
Ion Ratio	Lower	Upper	
202	100		
101	7.4	6.2	9.2
100	6.2	5.0	7.6

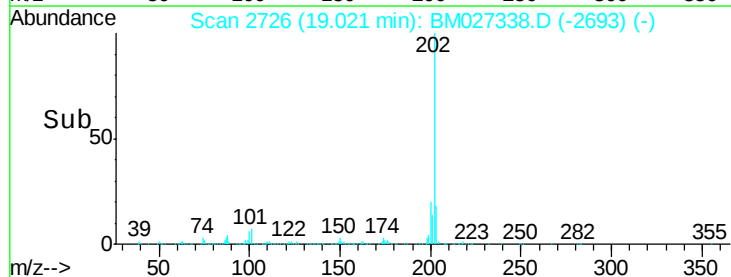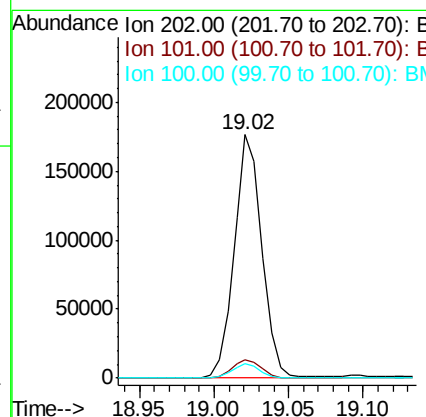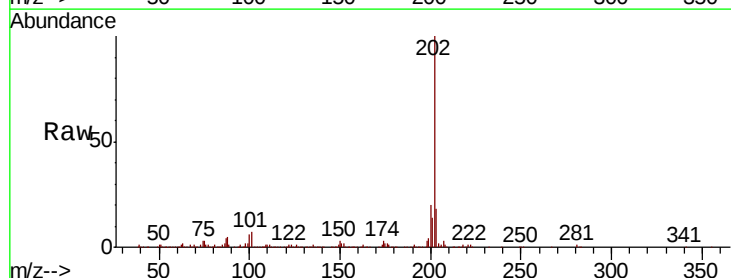

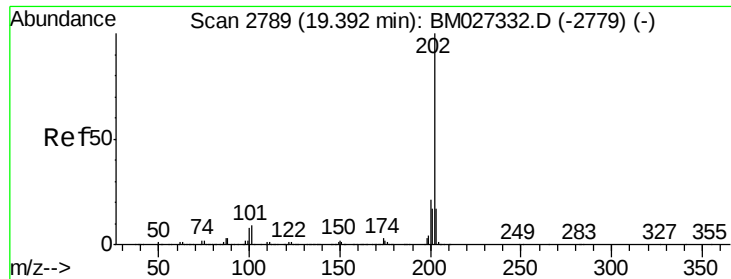





#80
Pvrene
Concen: 3.851 ng/ul
RT: 19.39 min Scan# 2788
Delta R.T. -0.01 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56

Instrument :
BNA_M
ClientSampleId :
C0AB8

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	8.7	7.1	10.7
100	8.4	6.1	9.1




Manual Integrations
APPROVED


mohammad
9/8/2020 1:45:49 PM

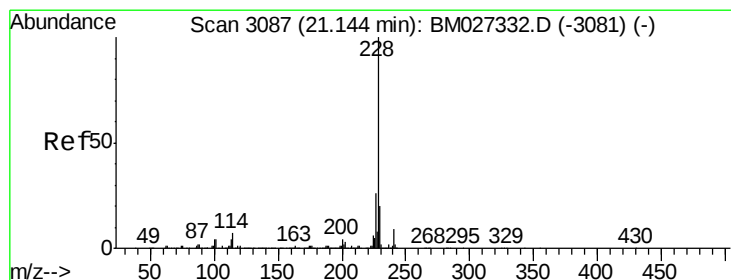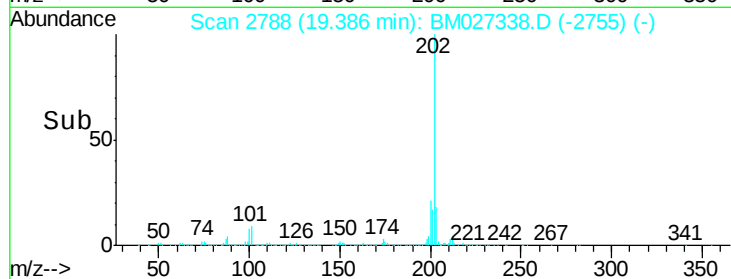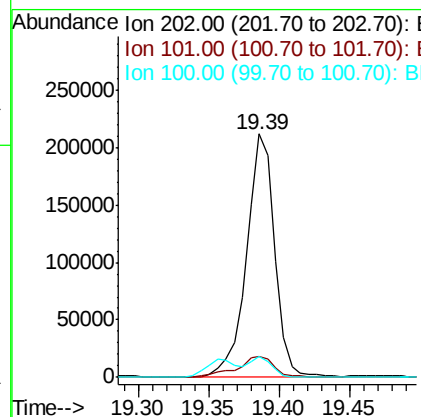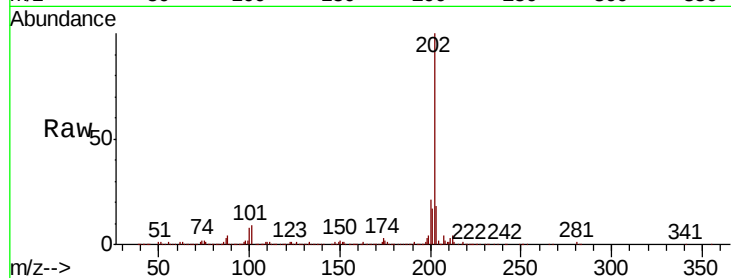

#83
Benzo(a)anthracene
Concen: 4.652 ng/ul
RT: 21.14 min Scan# 3087
Delta R.T. -0.01 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56

Tgt Ion	Ratio	Resp Lower	Upper
228	100		
229	20.5	15.8	23.6
226	26.1	21.5	32.3

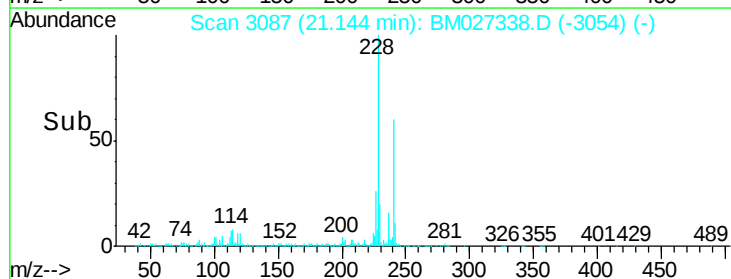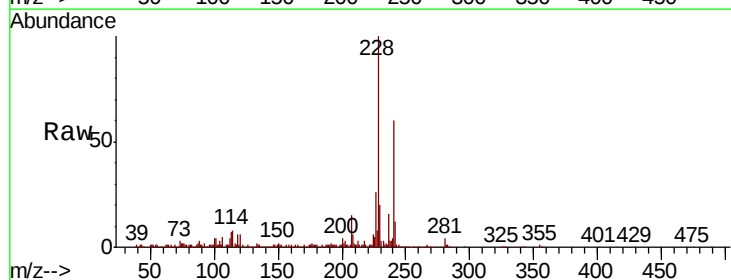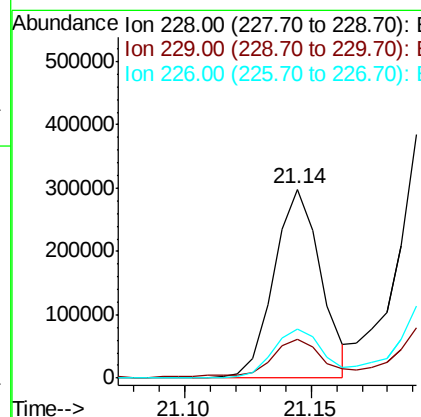

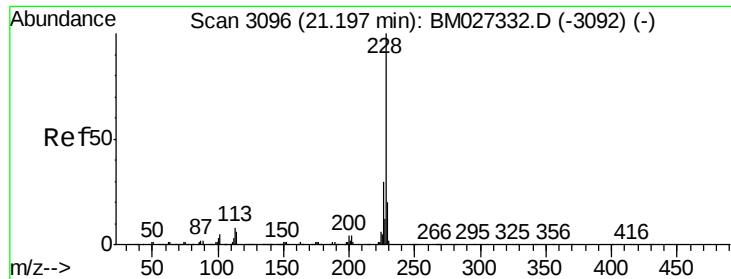





#85
 Chrysene
 Concen: 7.323 ng/ul
 RT: 21.20 min Scan# 3096
 Delta R.T. -0.00 min
 Lab File: BM027338.D
 Acq: 04 Sep 2020 19:56

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Tot Ion:	228	Resp:	592393
Ion Ratio	Lower	Upper	
228	100		
226	29.0	23.4	35.2
229	20.3	15.8	23.8




Manual Integrations
 APPROVED


mohammad
 9/8/2020 1:45:49 PM

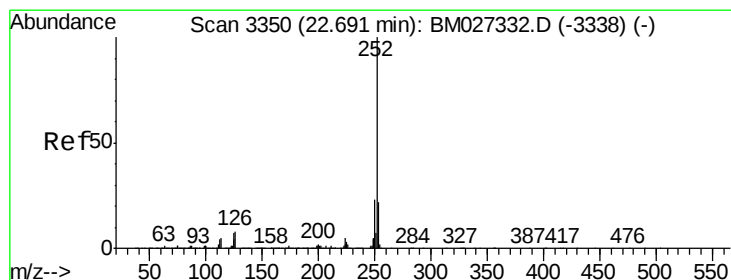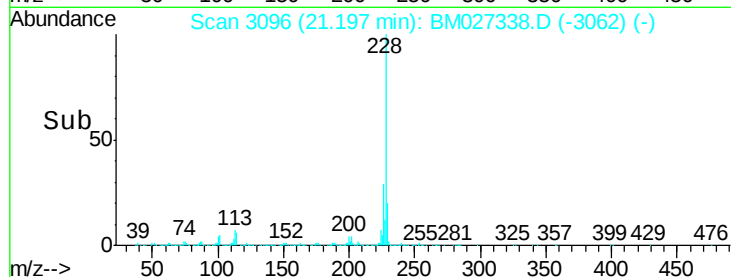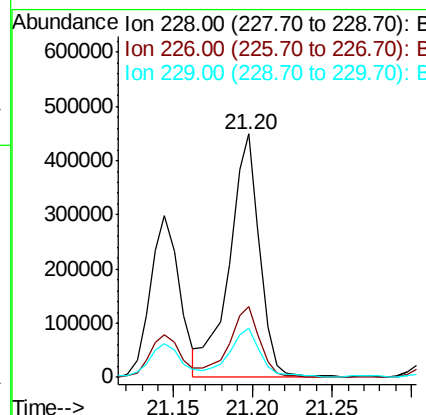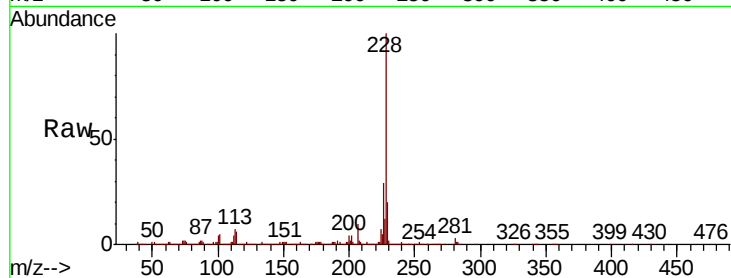

#88
 Benzo(b)fluoranthene
 Concen: 6.336 ng/ul m
 RT: 22.69 min Scan# 3349
 Delta R.T. -0.01 min
 Lab File: BM027338.D
 Acq: 04 Sep 2020 19:56

Tgt Ion:	252	Resp:	567057
Ion Ratio	Lower	Upper	
252	100		
253	23.3	17.7	26.5
125	7.9	5.1	7.7#

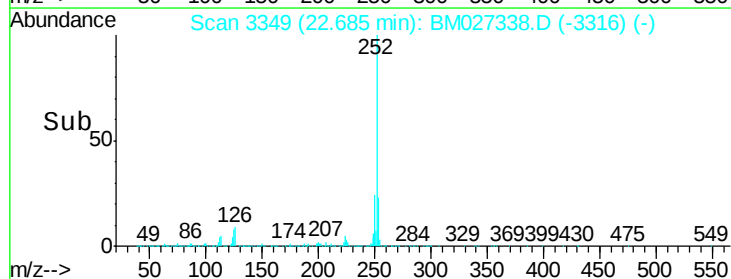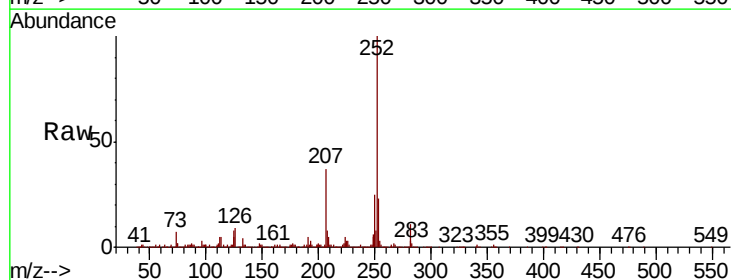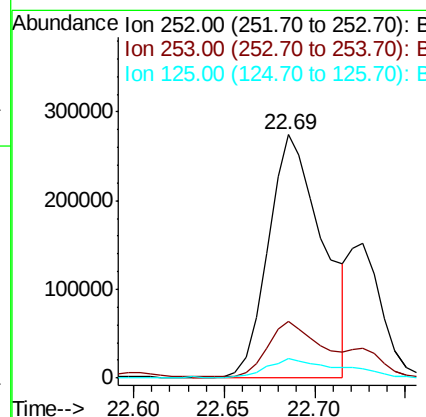

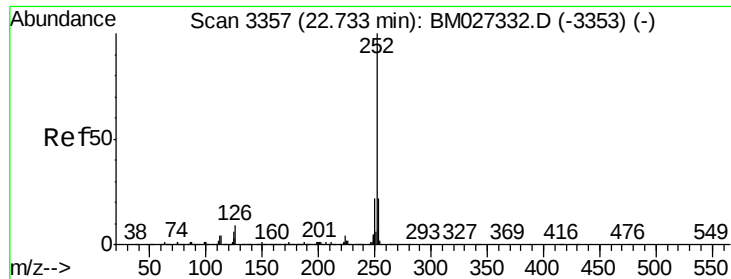





#89
Benzo(k)fluoranthene
Concen: 2.039 ng/ul
RT: 22.73 min Scan# 3356
Delta R.T. -0.01 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56

Instrument :
BNA_M
ClientSampleId :
C0AB8

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.5	17.4	26.0
125	7.2	5.6	8.4




Manual Integrations
APPROVED


mohammad
9/8/2020 1:45:49 PM

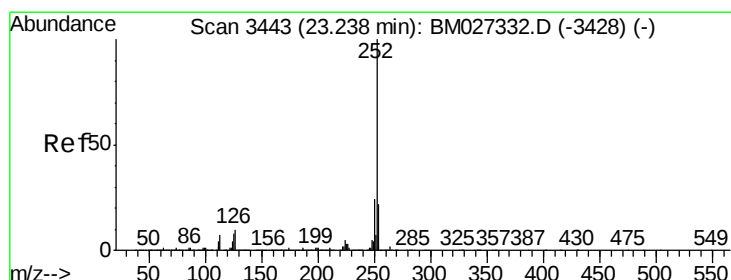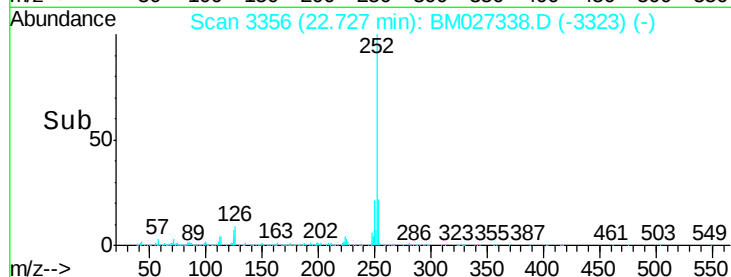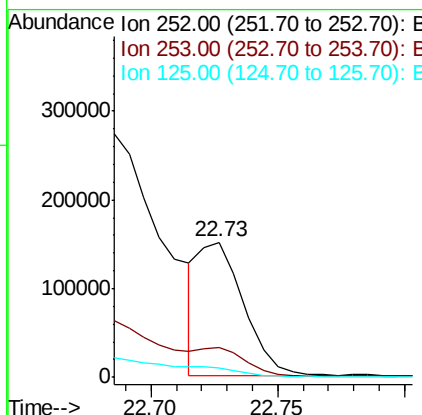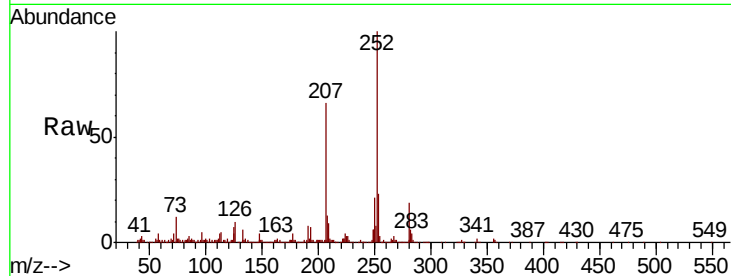

#91
Benzo(a)pyrene
Concen: 3.859 ng/ul
RT: 23.24 min Scan# 3443
Delta R.T. -0.00 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.4	17.5	26.3
125	8.7	6.6	10.0

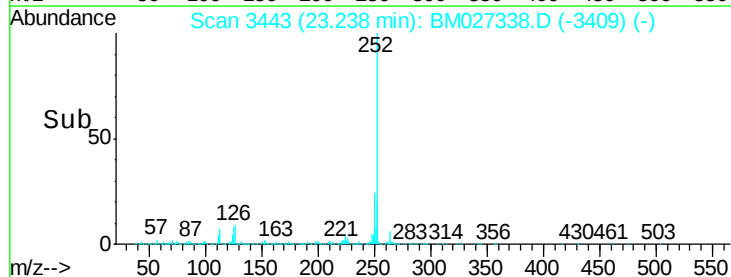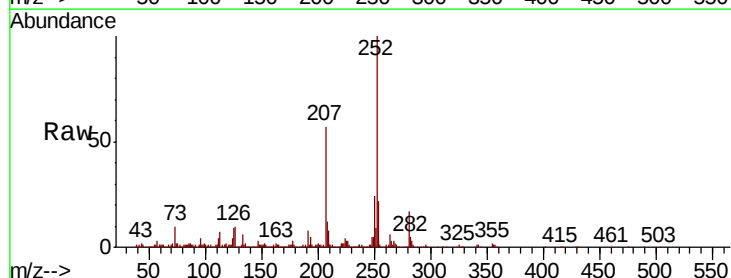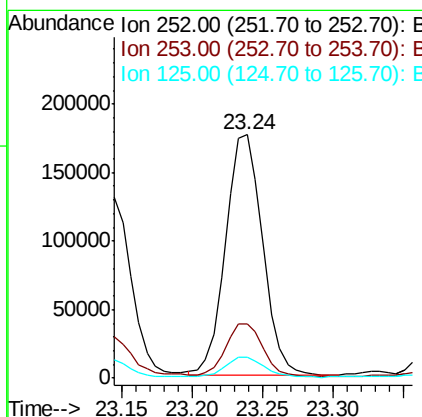

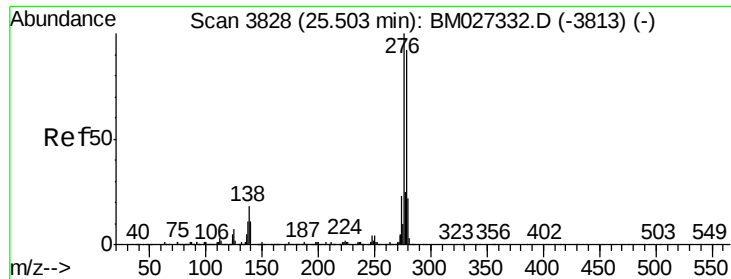

#92





Indeno(1,2,3-cd)pyrene
Concen: 1.283 ng/ul
RT: 25.49 min Scan# 3825
Delta R.T. -0.01 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56

Instrument :
BNA_M
ClientSampleId :
C0AB8

Tot Ion	Ratio	Lower	Upper
276	100		
138	15.0	14.0	21.0
277	27.0	20.1	30.1

Manual Integrations
APPROVED

mohammad
9/8/2020 1:45:49 PM

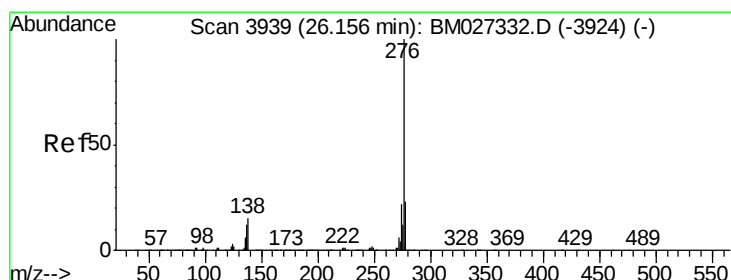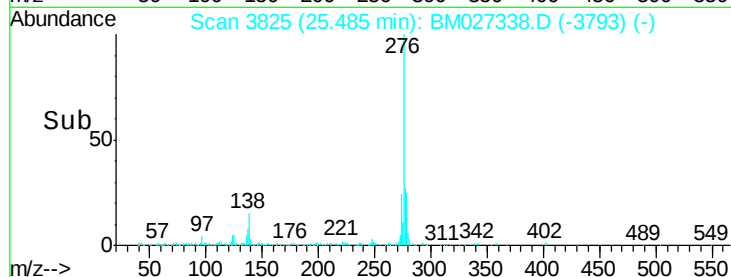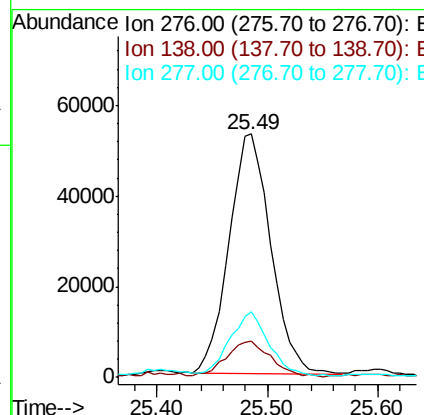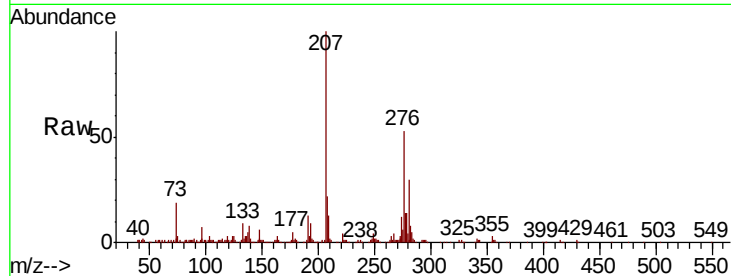

#94

Benzo(g,h,i)perylene
Concen: 1.244 ng/ul
RT: 26.14 min Scan# 3936
Delta R.T. -0.02 min
Lab File: BM027338.D
Acq: 04 Sep 2020 19:56

Tgt Ion	Ratio	Lower	Upper
276	100		
138	13.6	12.2	18.2
277	25.7	18.6	28.0

