

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027340.D
 Acq On : 04 Sep 2020 21:09
 Operator : JU/CG
 Sample : L3840-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA9

Quant Time: Sep 05 01:45:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 05 01:38:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	148178	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	598347	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	442120	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1061592	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1234414	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1315589	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	13998	4.20	ng/uL	0.00
5) Phenol-d5	6.76	99	204693	16.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	183918	22.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	173509	19.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	181960	18.27	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	98284	21.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	109325	22.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	188550	17.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	242719	19.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	891341	25.34	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	797792	20.08	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	77974	12.59	ng/ul	0.00
58) Fluorene-d10	15.21	176	645833	20.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	95934	14.12	ng/ul	0.00
71) Anthracene-d10	17.06	188	968364	19.29	ng/ul	0.00
79) Pyrene-d10	19.36	212	1112551	20.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1226895	17.39	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	295150	7.961	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027340.D
Acq On : 04 Sep 2020 21:09
Operator : JU/CG
Sample : L3840-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA9

Quant Time: Sep 05 01:45:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 05 01:38:08 2020
Response via : Initial Calibration

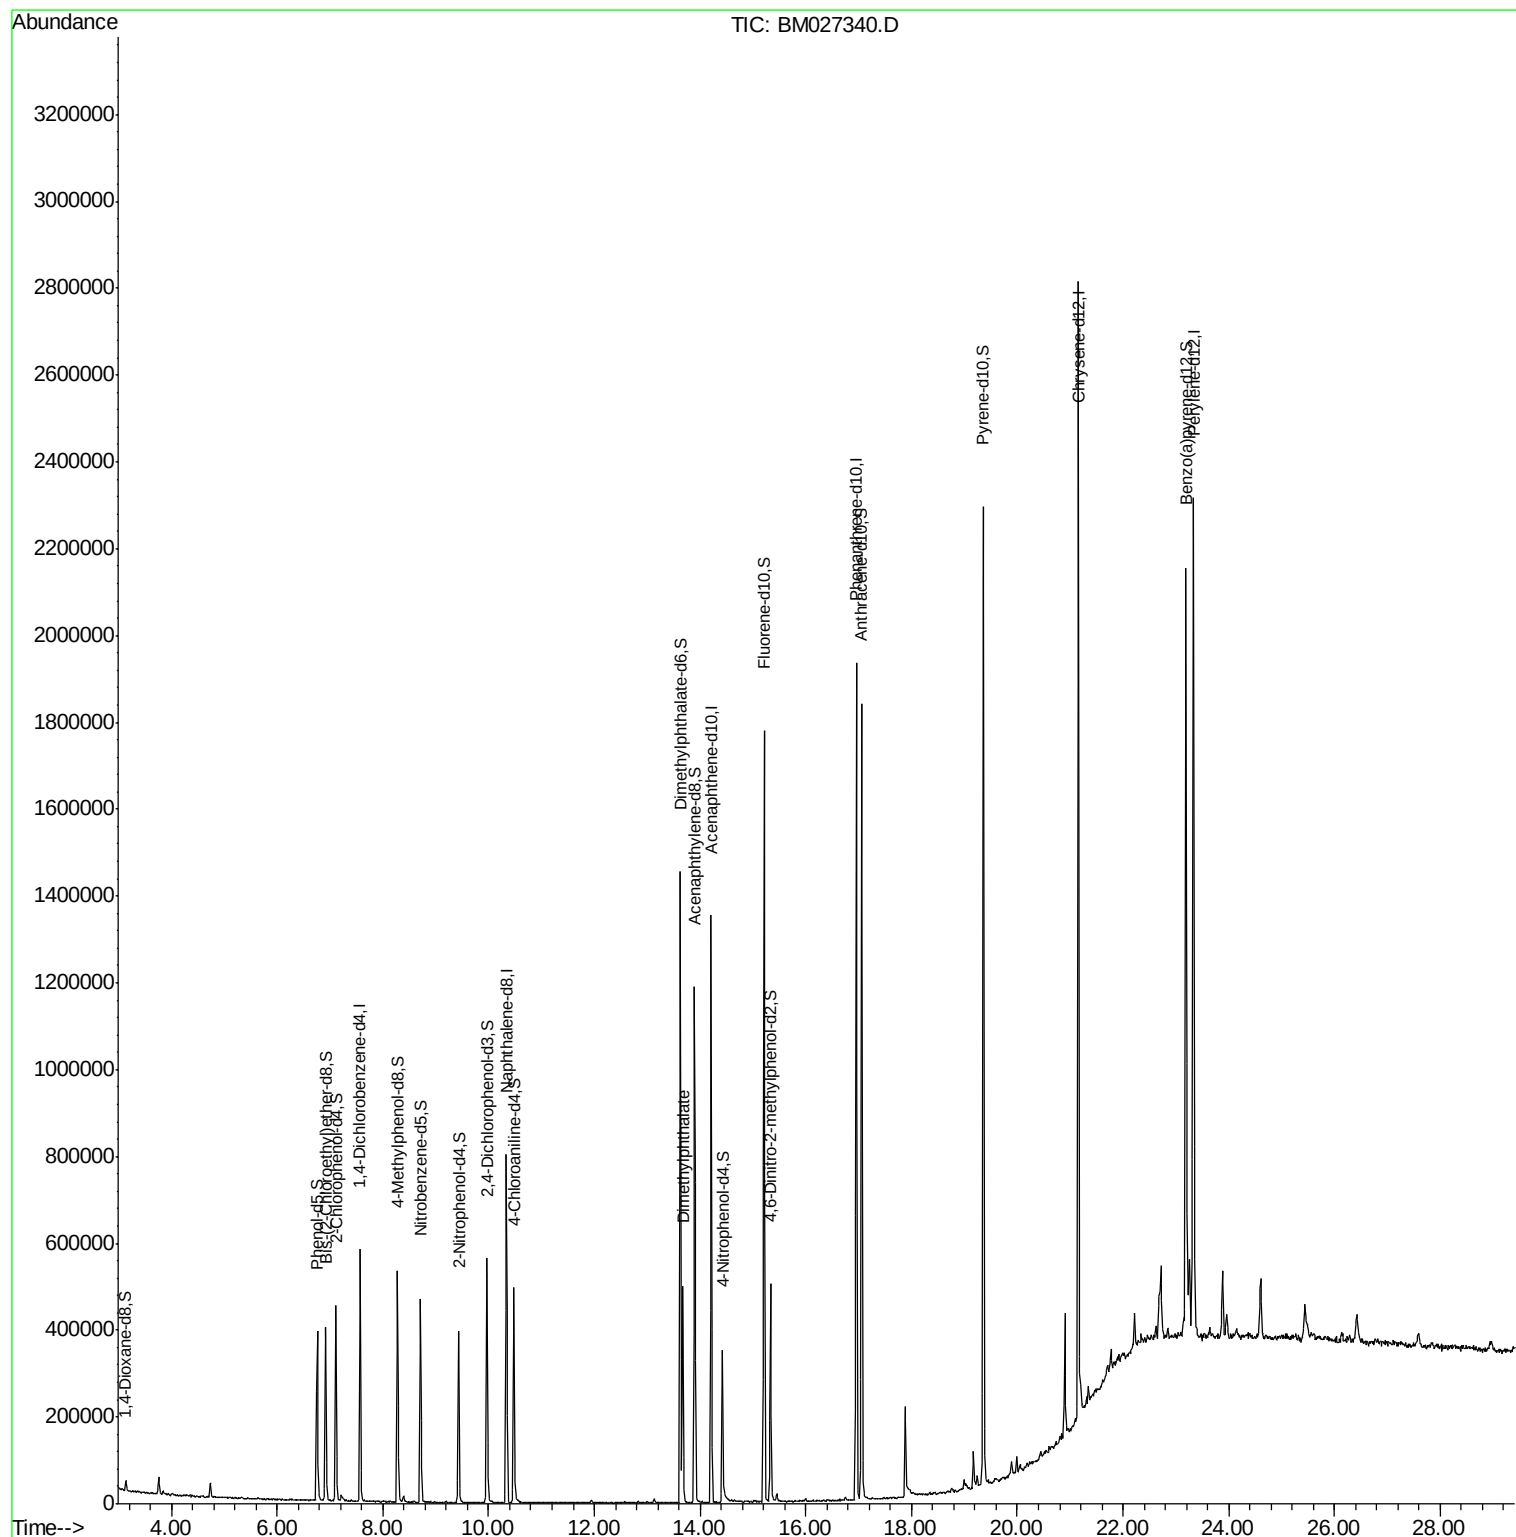

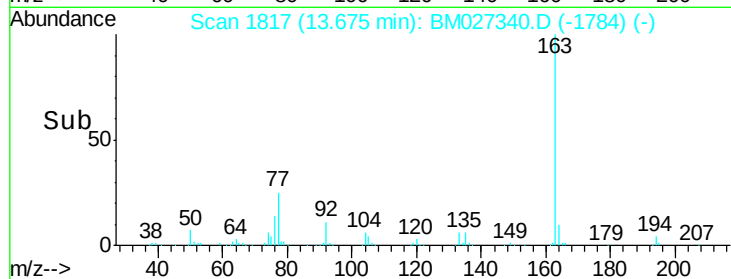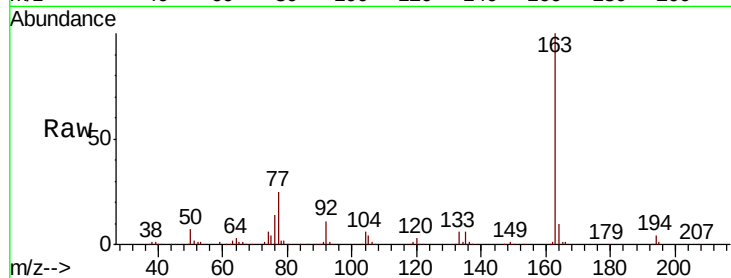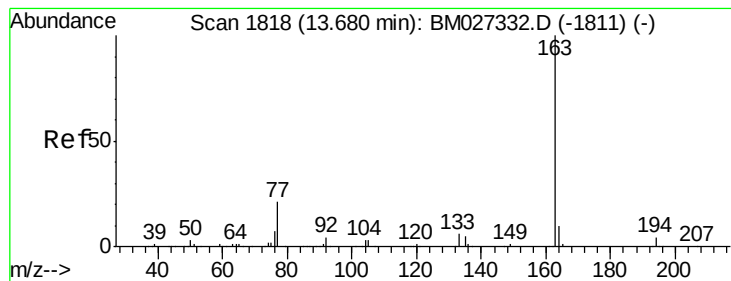

#45

Dimethylphthalate

Concen: 7.961 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM027340.D

Acq: 04 Sep 2020 21:09

Instrument :

BNA_M

ClientSampleId :

C0AA9

Tot Ion:163 Resp: 295150

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.4 8.1 12.1

