

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027343.D
 Acq On : 04 Sep 2020 22:59
 Operator : JU/CG
 Sample : L3843-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	32	rBV3	13709	23700	0.72%	0.091%
2	3.634	108	110	113	rBV4	4303	4168	0.13%	0.016%
3	3.763	126	132	139	rVB	30901	51922	1.58%	0.198%
4	4.281	218	220	223	rBV2	3228	3662	0.11%	0.014%
5	4.734	292	297	305	rVB	22046	36238	1.10%	0.138%
6	6.757	634	641	654	rBV	208175	353655	10.76%	1.351%
7	6.916	662	668	680	rVB	198425	315431	9.59%	1.205%
8	7.110	694	701	712	rBV	241758	387057	11.77%	1.479%
9	7.569	773	779	791	rVB	531311	842102	25.61%	3.217%
10	8.281	893	900	913	rBV	276076	459274	13.97%	1.755%
11	8.392	913	919	925	rVV	13124	21876	0.67%	0.084%
12	8.710	967	973	983	rBV	239605	402802	12.25%	1.539%
13	9.434	1090	1096	1108	rBV	197310	331719	10.09%	1.267%
14	9.969	1181	1187	1200	rBV	296934	494943	15.05%	1.891%
15	10.339	1241	1250	1267	rBV	722811	1171989	35.64%	4.478%
16	10.475	1267	1273	1284	rBV	254438	462526	14.07%	1.767%
17	11.945	1518	1523	1530	rVB4	3718	6452	0.20%	0.025%
18	12.827	1670	1673	1678	rVB4	2322	3296	0.10%	0.013%
19	13.127	1718	1724	1729	rBV3	5340	8292	0.25%	0.032%
20	13.627	1803	1809	1814	rBV	745659	1031157	31.36%	3.940%
21	13.674	1814	1817	1826	rVB	227702	300348	9.13%	1.148%
22	13.898	1849	1855	1865	rBV	645011	931544	28.33%	3.559%
23	14.216	1902	1909	1918	rBV	1238580	1826629	55.55%	6.979%
24	14.421	1937	1944	1959	rBV	152839	299056	9.10%	1.143%
25	15.051	2046	2051	2056	rVB2	6432	8331	0.25%	0.032%
26	15.210	2071	2078	2086	rBV	933777	1303318	39.64%	4.980%
27	15.333	2094	2099	2110	rBV	227855	335956	10.22%	1.284%
28	15.451	2114	2119	2123	rBV2	9117	12831	0.39%	0.049%
29	15.998	2207	2212	2216	rVB4	3724	5777	0.18%	0.022%
30	16.745	2336	2339	2346	rVB3	6676	10682	0.32%	0.041%
31	16.957	2369	2375	2385	rBV	1736722	2380972	72.41%	9.097%
32	17.057	2385	2392	2404	rVV	1024153	1432341	43.56%	5.473%
33	17.274	2425	2429	2433	rBV6	2378	3937	0.12%	0.015%
34	17.880	2525	2532	2537	rBV2	112037	160505	4.88%	0.613%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
 Data File : BM027343.D
 Acq On : 04 Sep 2020 22:59
 Operator : JU/CG
 Sample : L3843-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Title : SVOA CALIBRATION

35	18.027	2554	2557	2562	rVB3	11047	15565	0.47%	0.059%
36	18.174	2578	2582	2583	rBV4	4166	4118	0.13%	0.016%
37	18.415	2619	2623	2625	rBV5	4457	6381	0.19%	0.024%
38	18.439	2625	2627	2629	rBV3	4564	4357	0.13%	0.017%
39	18.592	2651	2653	2656	rVB4	6092	6680	0.20%	0.026%
40	18.668	2664	2666	2668	rBV3	4809	3880	0.12%	0.015%
41	18.915	2706	2708	2713	rBV6	4621	7339	0.22%	0.028%
42	18.992	2717	2721	2723	rBV	14599	21711	0.66%	0.083%
43	19.021	2723	2726	2732	rVB	26916	36449	1.11%	0.139%
44	19.168	2746	2751	2758	rBV	54804	91076	2.77%	0.348%
45	19.245	2760	2764	2769	rVV3	15868	24727	0.75%	0.094%
46	19.356	2777	2783	2793	rBV	1406862	1953182	59.40%	7.463%
47	19.892	2871	2874	2880	rVB2	19657	25501	0.78%	0.097%
48	19.992	2888	2891	2896	rVB3	27738	34597	1.05%	0.132%
49	20.897	3041	3045	3053	rBV4	149303	228981	6.96%	0.875%
50	21.156	3084	3089	3094	rBV	2565684	3182815	96.80%	12.161%
51	23.191	3429	3435	3441	rBV	1061071	1813356	55.15%	6.928%
52	23.327	3452	3458	3471	rVB	1875721	3287973	100.00%	12.562%


Sum of corrected areas: 26173176

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090420\
Data File : BM027343.D
Acq On : 04 Sep 2020 22:59
Operator : JU/CG
Sample : L3843-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

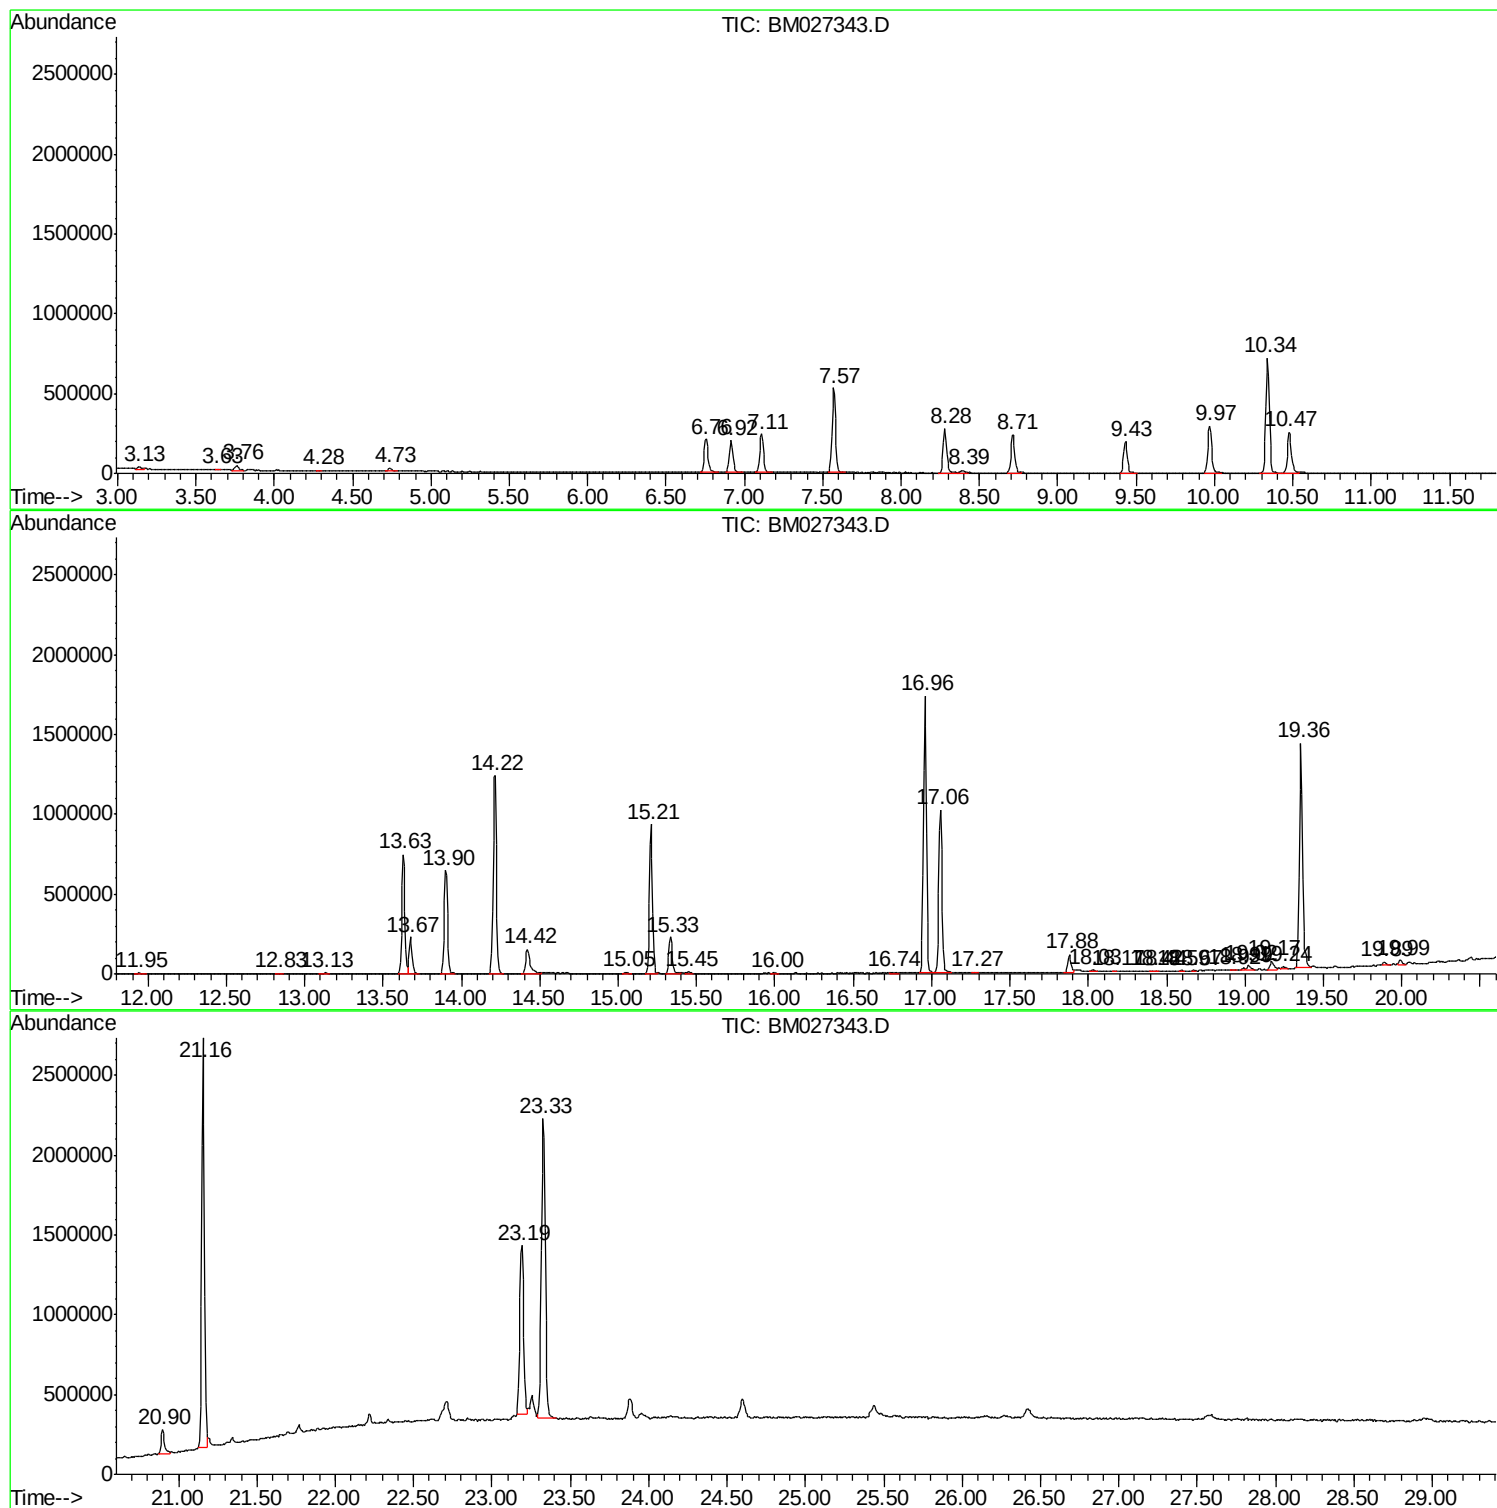

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090420\
Data File : BM027343.D
Acq On : 04 Sep 2020 22:59
Operator : JU/CG
Sample : L3843-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090420\
Data File : BM027343.D
Acq On : 04 Sep 2020 22:59
Operator : JU/CG
Sample : L3843-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc