


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090424\
Data File : BM047431.D
Acq On : 04 Sep 2024 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

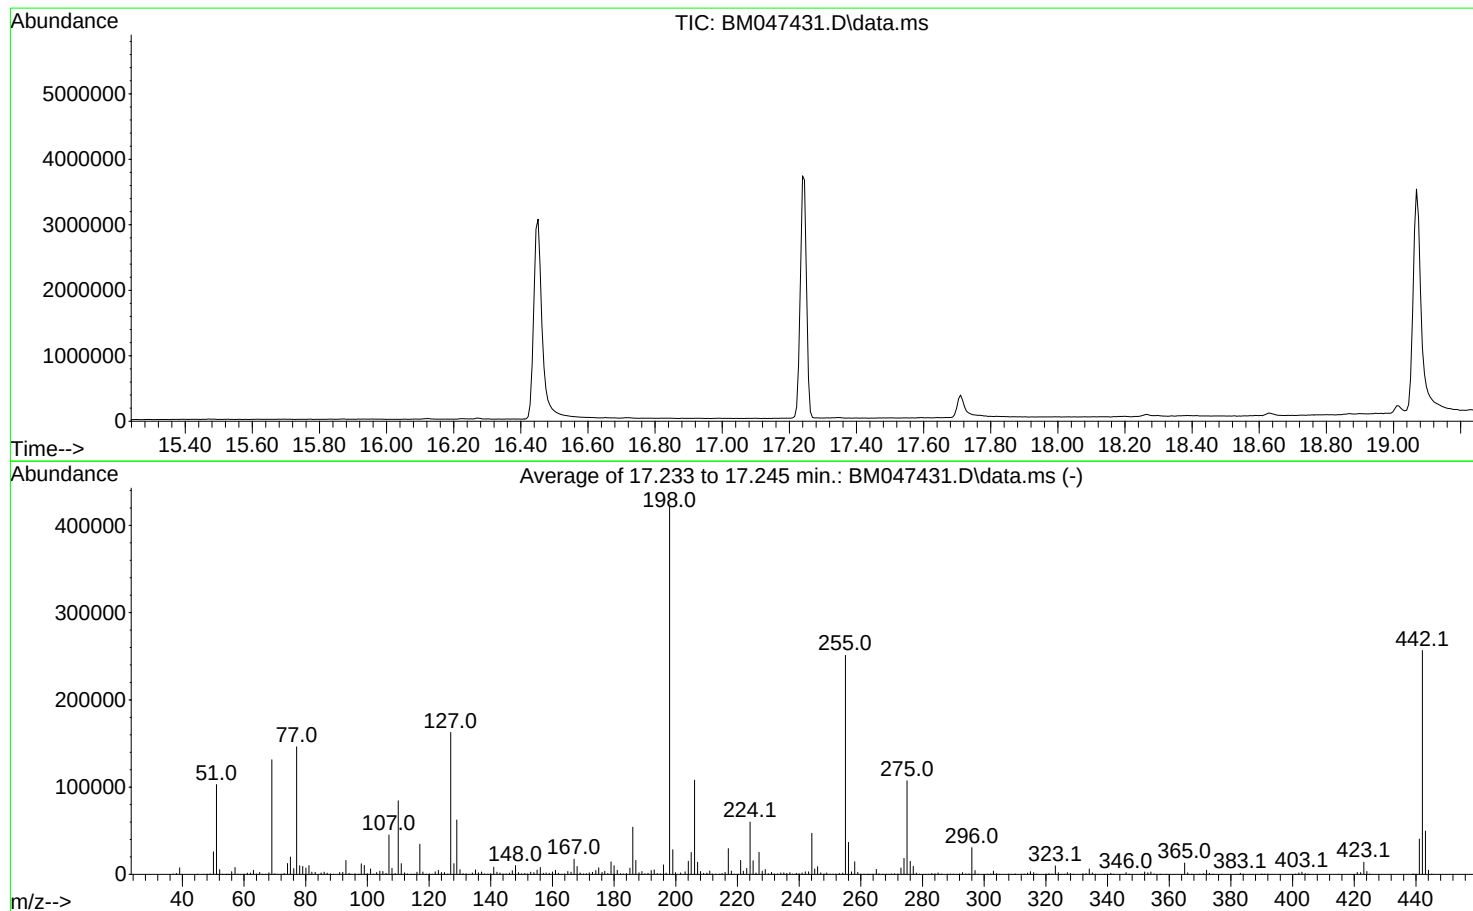




AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	102857	PASS
68	69	0.00	2	1.4	1845	PASS
69	198	0.00	100	31.1	131324	PASS
70	69	0.00	2	0.5	665	PASS
127	198	10	80	38.6	162619	PASS
197	198	0.00	2	0.3	1465	PASS
198	198	100	100	100.0	421675	PASS
199	198	5	9	6.7	28304	PASS
275	198	10	60	25.4	107248	PASS
365	198	1	100	3.1	13074	PASS
441	198	0.01	100	9.6	40573	PASS
442	442	50	100	100.0	256597	PASS
443	442	15	24	19.4	49683	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090424\
Data File : BM047431.D
Acq On : 04 Sep 2024 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 04 11:08:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

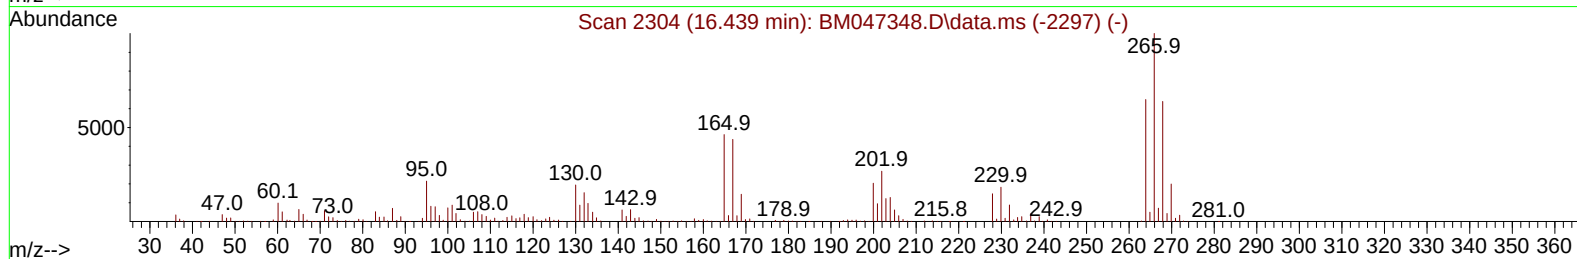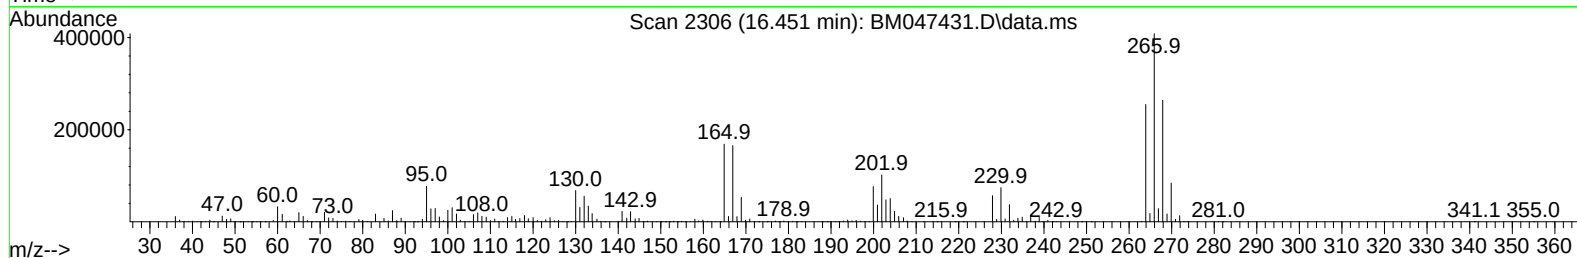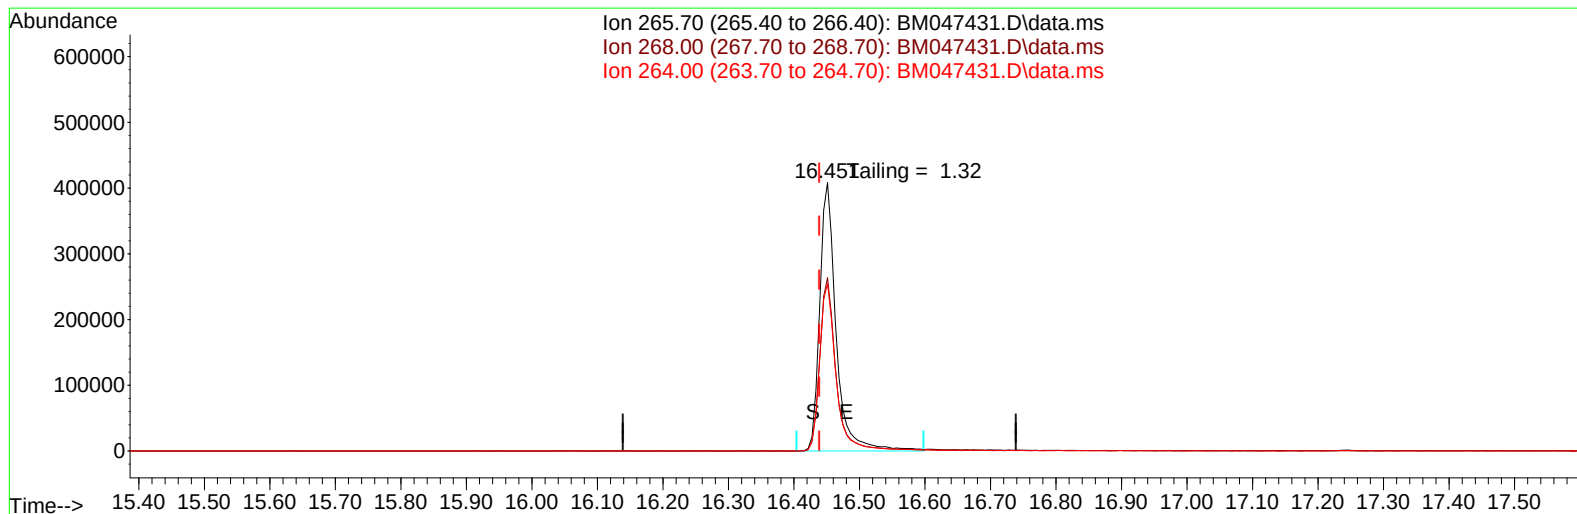

TIC: BM047431.D\data.ms

(70) Pentachlorophenol (C)

16.451min (+ 0.012) 119709.78 ng




response 714824

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.58
264.00	64.90	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090424\
Data File : BM047431.D
Acq On : 04 Sep 2024 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 04 11:08:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

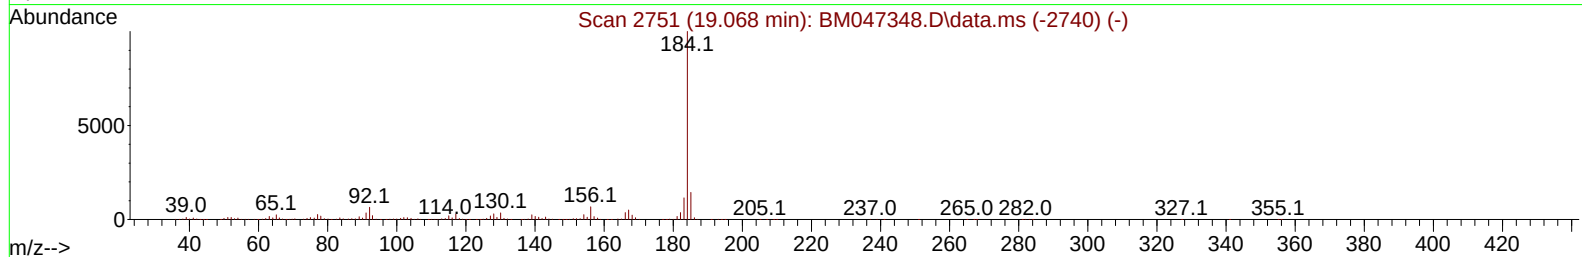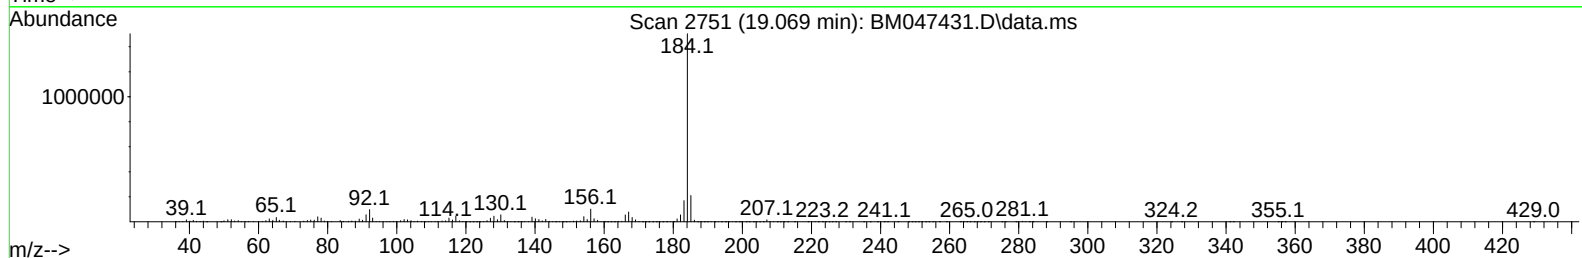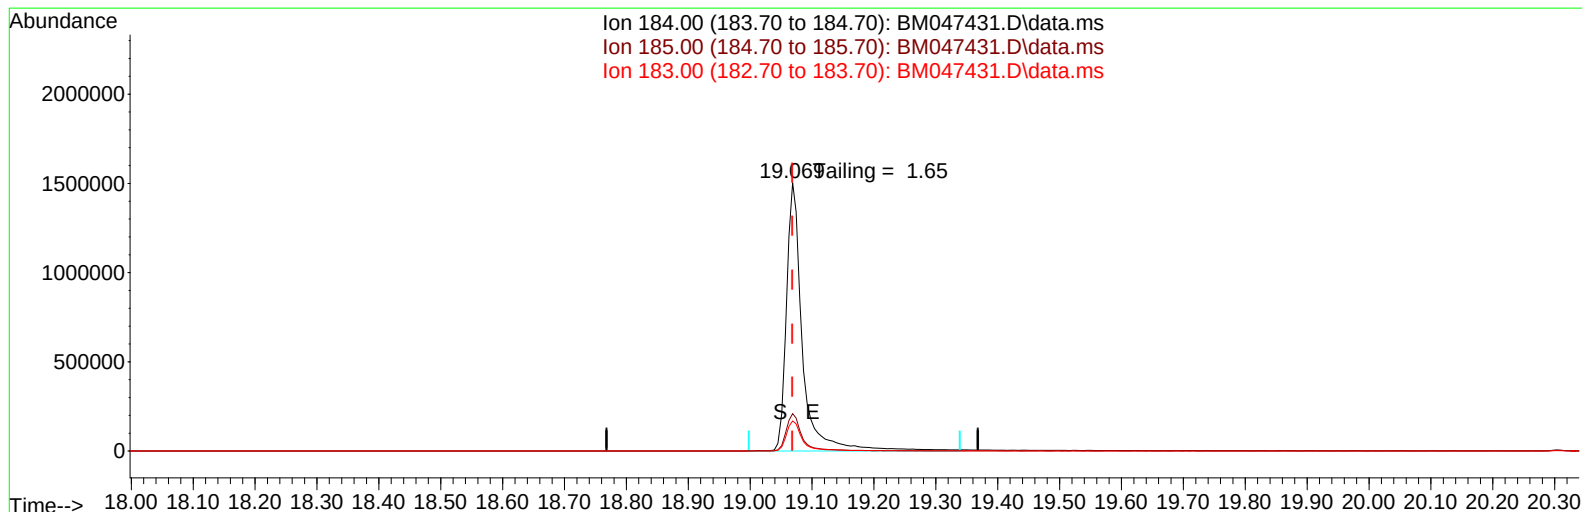

TIC: BM047431.D\data.ms

(77) Benzidine

19.069min (+ 0.001) 49134.61 ng

response 2723784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	11.50	11.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2024	BNA_M	<u>BM047431.D</u>
Compound Name	Response	Retention Time
DDT	1376846	20.304
DDD	91340	19.869
DDE	5706	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
97046	1473892	6.58

Instrument :
BNA_M
ClientSampleId :
DFTPP