

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\
 Data File : BM011443.D
 Acq On : 05 Sep 2017 21:50
 Operator : SJ/JU
 Sample : I5084-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP9-WC1

Quant Time: Sep 06 07:51:04 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 18:39:59 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	394295	20.00	ng	-0.01
21) Naphthalene-d8	10.79	136	1583044	20.00	ng	-0.02
38) Acenaphthene-d10	14.61	164	806173	20.00	ng	-0.02
63) Phenanthrene-d10	17.35	188	1877672	20.00	ng	-0.01
75) Chrysene-d12	21.51	240	2108226	20.00	ng	-0.02
86) Perylene-d12	23.89	264	1226868	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	3387272	144.61	ng	0.00
7) Phenol-d6	7.13	99	4045547	124.55	ng	0.00
23) Nitrobenzene-d5	9.15	82	2611917	108.73	ng	-0.01
41) 2,4,6-Tribromophenol	16.10	330	1456587	156.17	ng	-0.01
44) 2-Fluorobiphenyl	13.24	172	6215216	111.13	ng	-0.01
78) Terphenyl-d14	19.96	244	9318642	109.67	ng	-0.01
Target Compounds						
32) Benzoic acid	10.06	122	366	6.559	ng	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\
Data File : BM011443.D
Acq On : 05 Sep 2017 21:50
Operator : SJ/JU
Sample : I5084-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP9-WC1

Quant Time: Sep 06 07:51:04 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

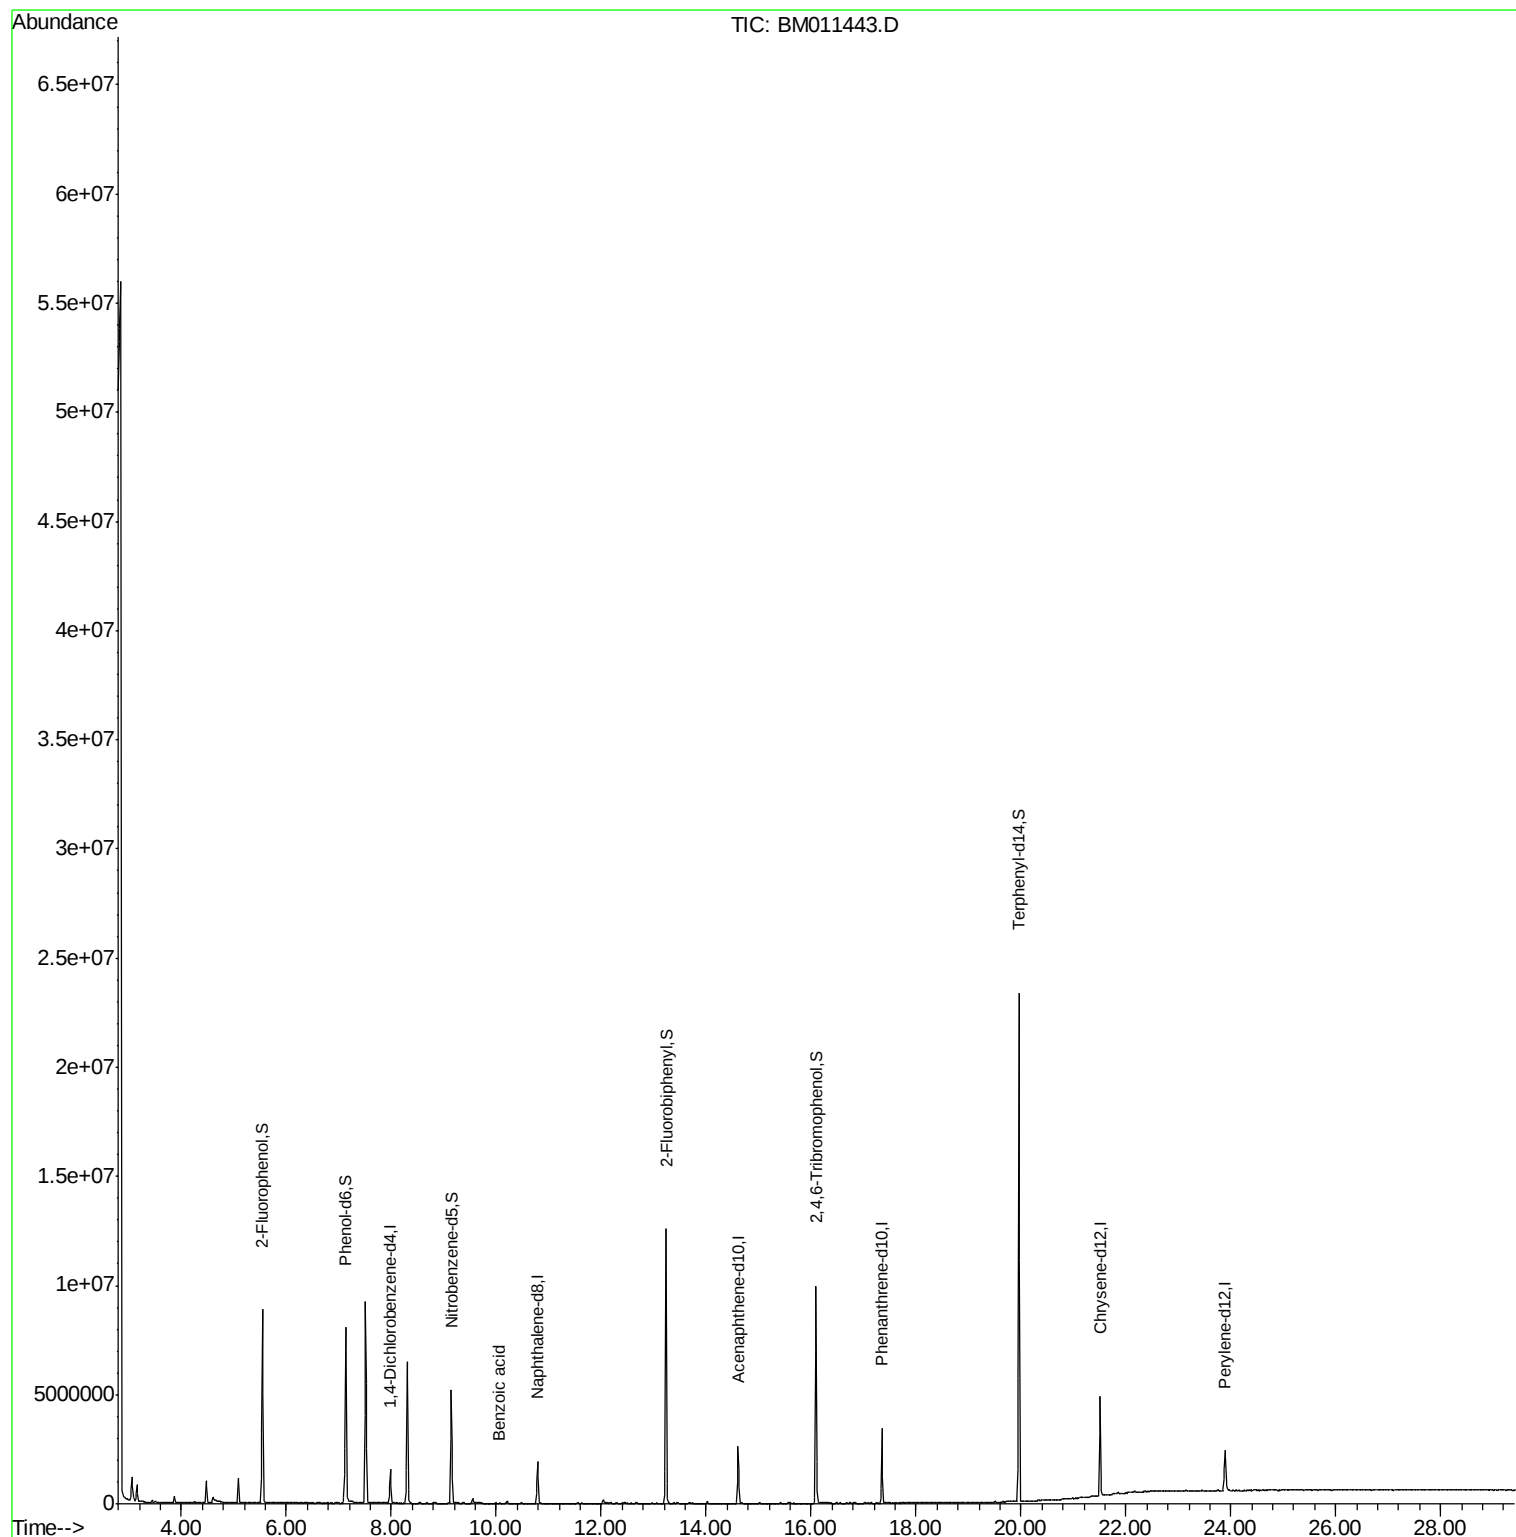







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.98 min Scan# 883
Delta R.T. -0.01 min
Lab File: BM011443.D
Acq: 05 Sep 2017 21:50

Instrument :
BNA_M
ClientSampled :
TP9-WC1




Tot Ion:152 Resp: 394295
Ion Ratio Lower Upper
152 100
150 157.7 119.5 179.3
115 56.4 43.0 64.4

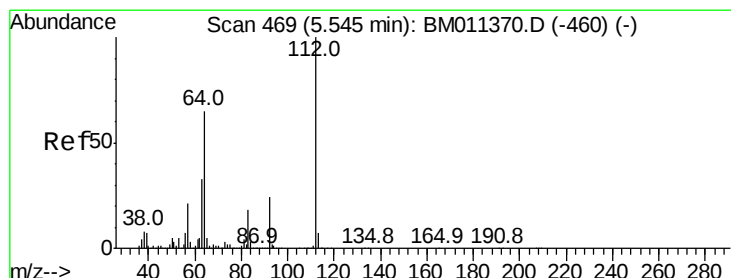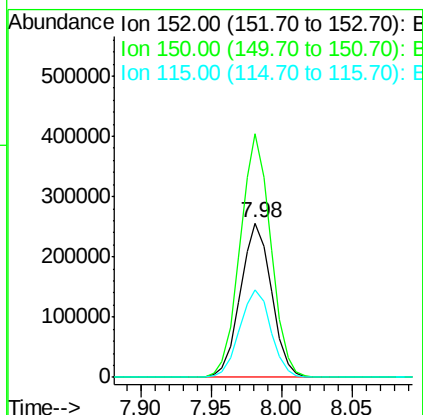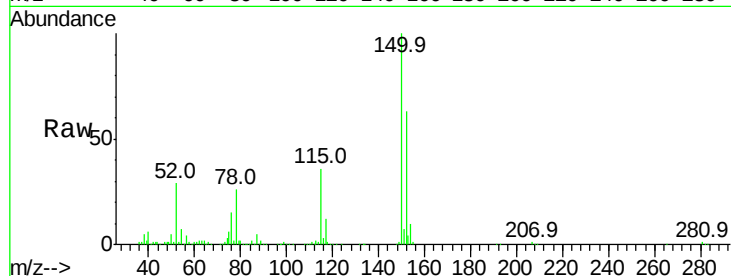


#5

2-Fluorophenol
Concen: 144.605 ng
RT: 5.54 min Scan# 468
Delta R.T. -0.00 min
Lab File: BM011443.D
Acq: 05 Sep 2017 21:50

Tgt Ion:112 Resp: 3387272
Ion Ratio Lower Upper
112 100
64 68.9 38.6 57.8#
63 35.5 19.3 28.9#

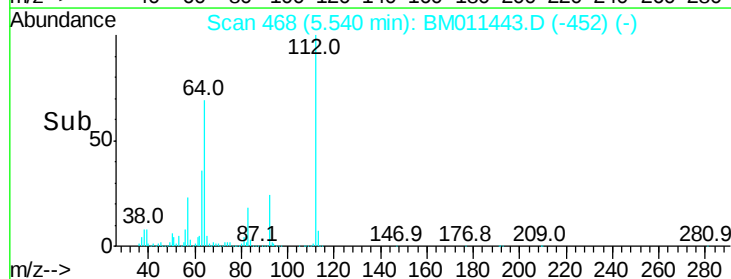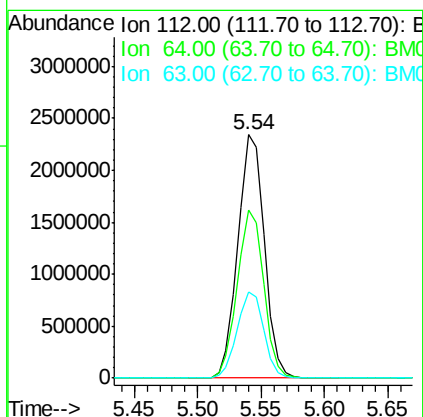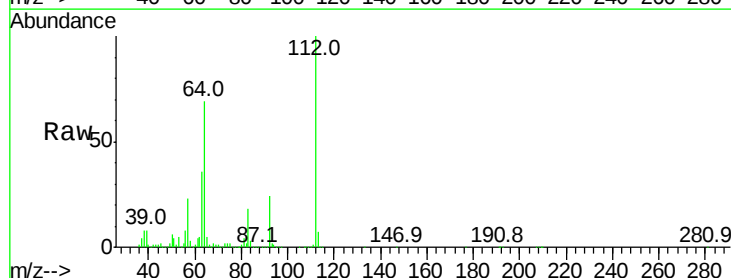



#7

Phenol-d6

Concen: 124.553 ng

RT: 7.13 min Scan# 739

Delta R.T. -0.01 min

Lab File: BM011443.D

Acq: 05 Sep 2017 21:50

Instrument :





BNA_M

ClientSampleId :

TP9-WC1

Tot Ion: 99 Resp: 4045547

Ion	Ratio	Lower	Upper
99	100		
42	24.6	11.0	16.4#
71	29.9	23.4	35.2

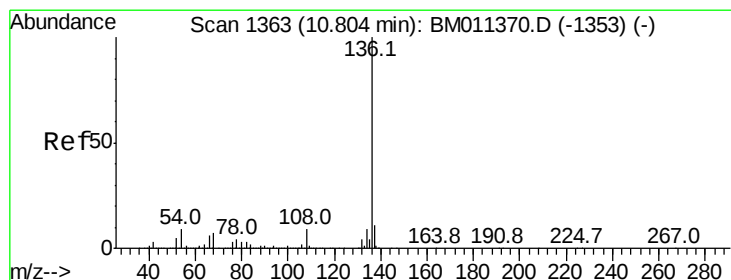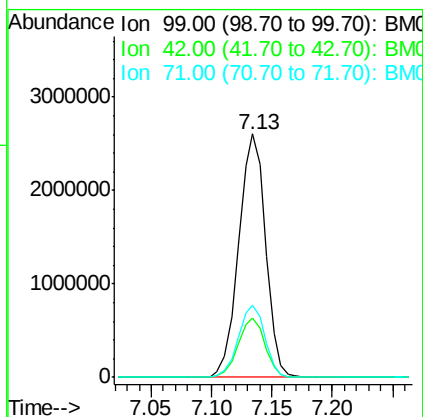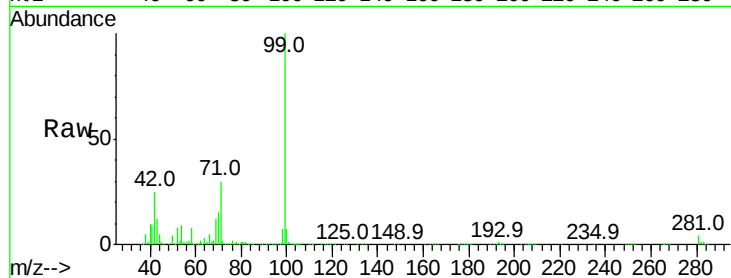

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.79 min Scan# 1360




Delta R.T. -0.02 min


Lab File: BM011443.D

Acq: 05 Sep 2017 21:50

Tgt Ion: 136 Resp: 1583044

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	10.1	4.6	6.8#
68	7.0	3.7	5.5#

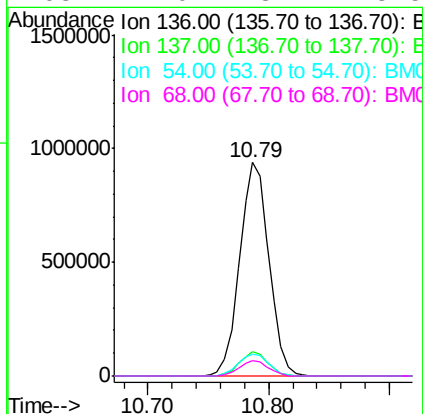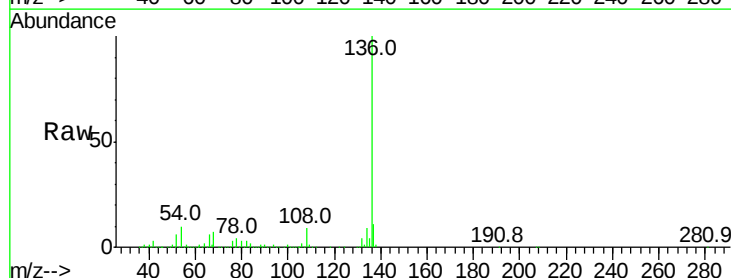



#23

Nitrobenzene-d5

Concen: 108.728 ng

RT: 9.15 min Scan# 1081

Delta R.T. -0.01 min

Lab File: BM011443.D

Acq: 05 Sep 2017 21:50

Instrument :

BNA_M

ClientSampled :

TP9-WC1


Tot Ion: 82 Resp: 2611917

Ion Ratio Lower Upper

82 100

128 42.7 32.8 49.2




54 65.0 40.6 60.8#

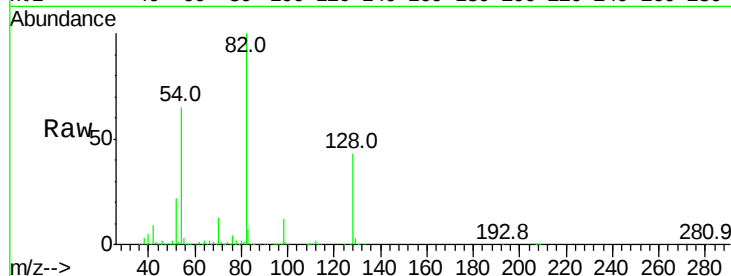

Abundance Ion 82.00 (81.70 to 82.70): BM011370.D (-1076) (-)

Ion 128.00 (127.70 to 128.70): BM011370.D (-1076) (-)

Ion 54.00 (53.70 to 54.70): BM011370.D (-1076) (-)

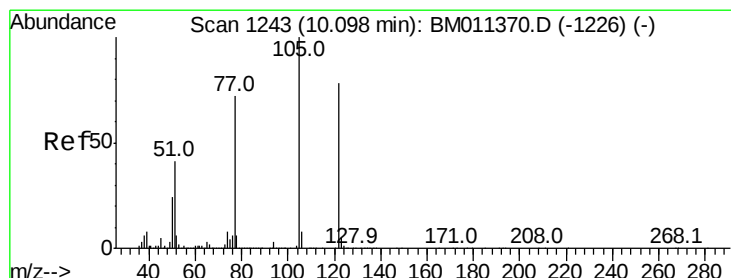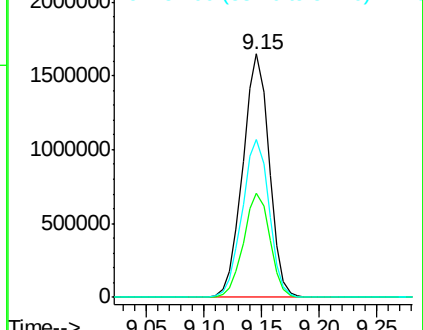

#32

Benzoic acid

Concen: 6.559 ng

RT: 10.06 min Scan# 1236

Delta R.T. -0.04 min

Lab File: BM011443.D

Acq: 05 Sep 2017 21:50


Tgt Ion: 122 Resp: 366

Ion Ratio Lower Upper

122 100

105 137.8 99.9 139.9



77 338.0 73.7 113.7#

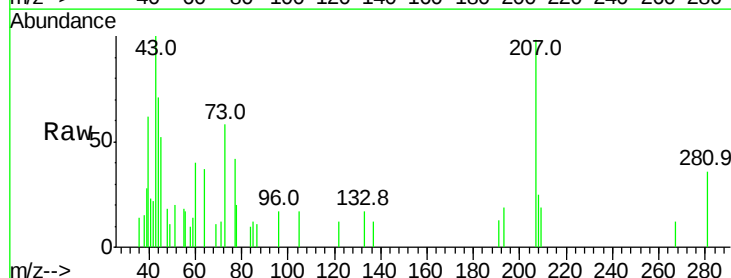


Abundance Ion 122.00 (121.70 to 122.70): BM011370.D (-1226) (-)

Ion 105.00 (104.70 to 105.70): BM011370.D (-1226) (-)

Ion 77.00 (76.70 to 77.70): BM011370.D (-1226) (-)




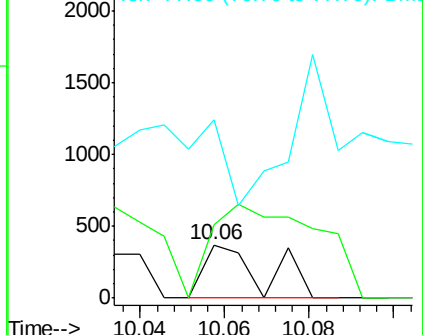


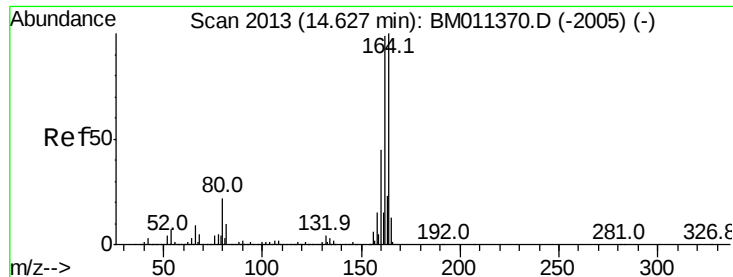

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.61 min Scan# 2010
Delta R.T. -0.02 min
Lab File: BM011443.D
Acq: 05 Sep 2017 21:50




Instrument :
BNA_M
ClientSampleId :
TP9-WC1


Tot Ion	Ratio	Lower	Upper
164	100		
162	100.4	82.4	123.6
160	46.5	35.8	53.6

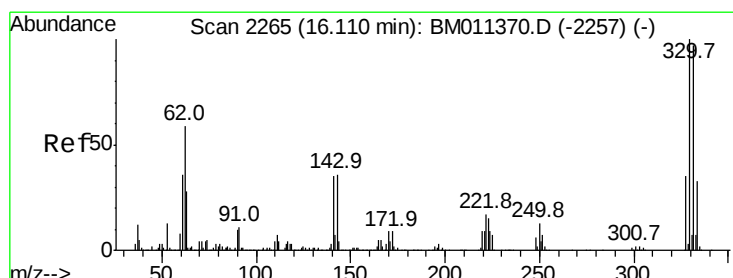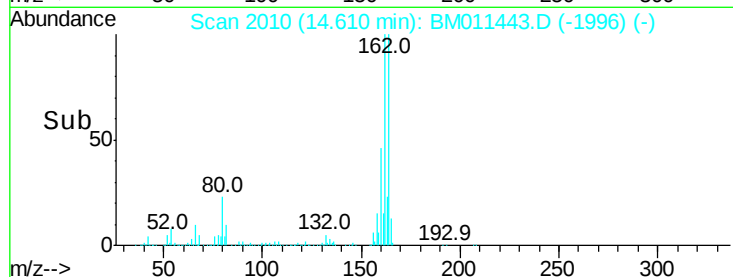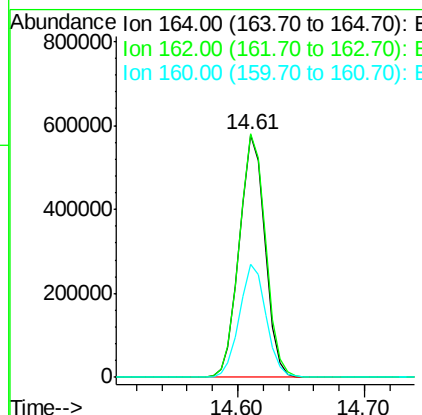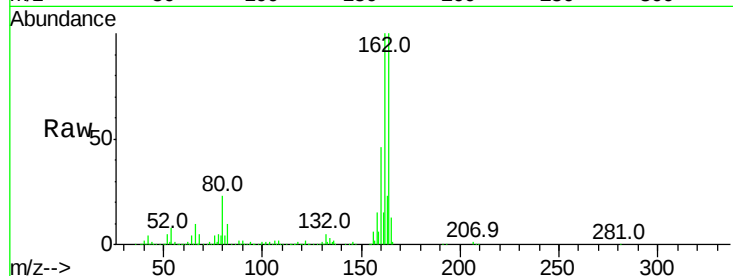

#41
2,4,6-Tribromophenol
Concen: 156.168 ng
RT: 16.10 min Scan# 2263
Delta R.T. -0.01 min
Lab File: BM011443.D
Acq: 05 Sep 2017 21:50

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.7	0.0	0.0#
141	42.2	0.0	0.0#


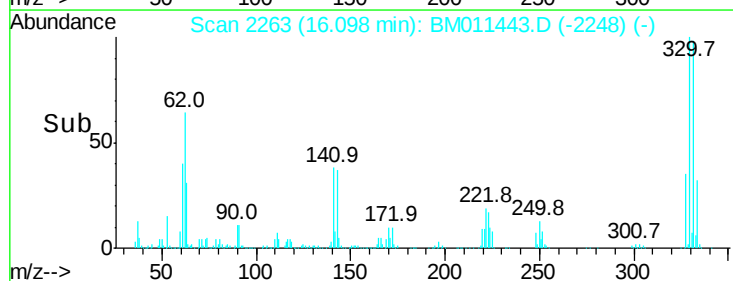
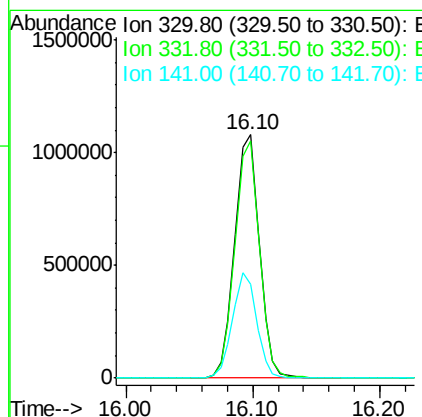
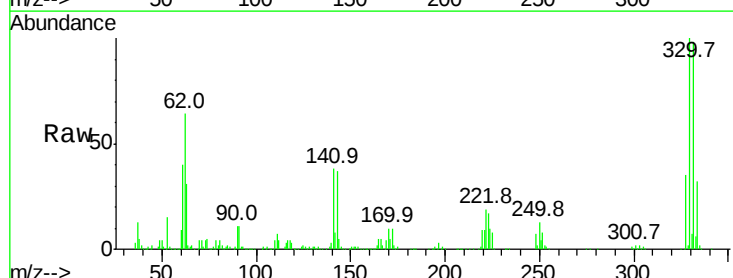




#44
 2-Fluorobiphenyl
 Concen: 111.131 ng
 RT: 13.24 min Scan# 1777
 Delta R.T. -0.01 min
 Lab File: BM011443.D
 Acq: 05 Sep 2017 21:50




Instrument :
 BNA_M
 ClientSampleId :
 TP9-WC1


Tot Ion:172 Resp: 6215216
 Ion Ratio Lower Upper
 172 100
 171 35.4 28.5 42.7
 170 24.0 18.8 28.2

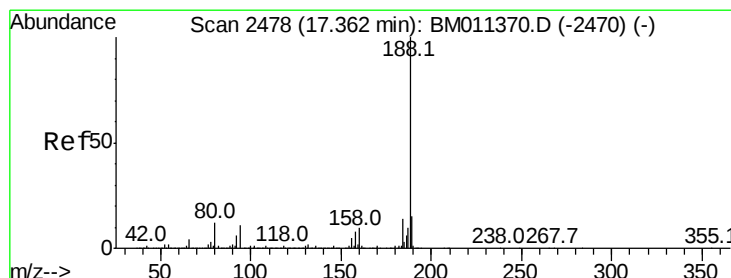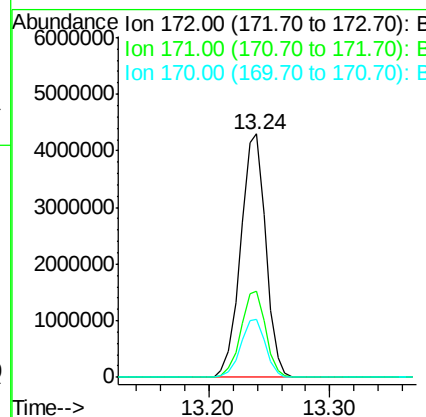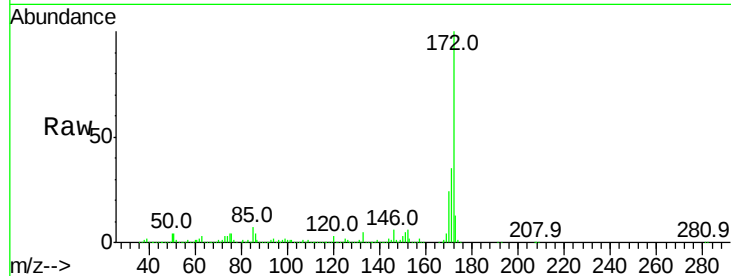

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.35 min Scan# 2476
 Delta R.T. -0.01 min
 Lab File: BM011443.D
 Acq: 05 Sep 2017 21:50

Tgt Ion:188 Resp: 1877672
 Ion Ratio Lower Upper
 188 100
 94 10.4 8.7 13.1
 80 11.4 9.3 13.9

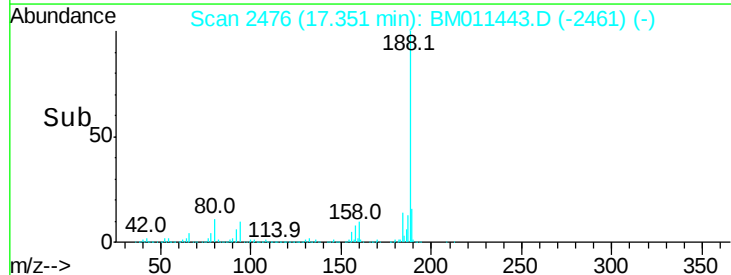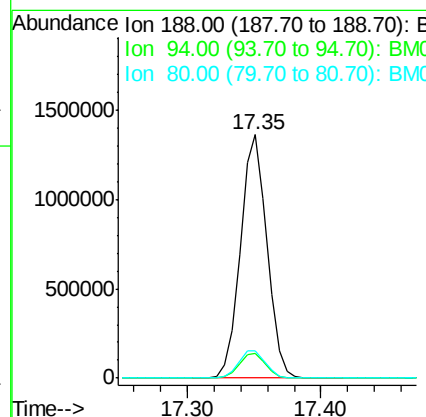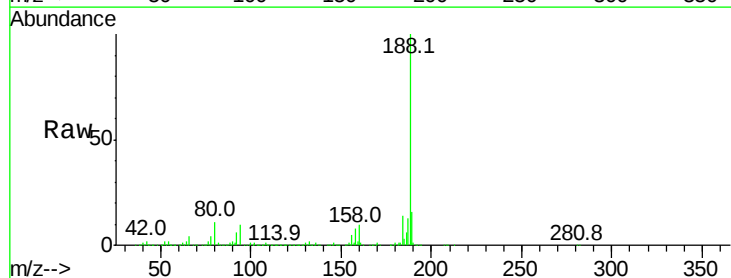

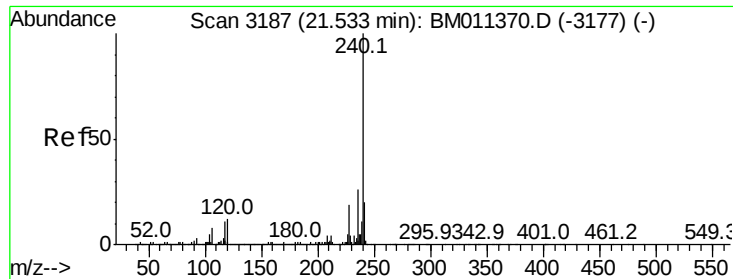

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.51 min Scan# 3183

Delta R.T. -0.02 min

Lab File: BM011443.D

Acq: 05 Sep 2017 21:50

Instrument :

BNA_M

ClientSampleId :

TP9-WC1


Tot Ion:240 Resp: 2108226

Ion Ratio Lower Upper

240 100

120 13.2 8.2 12.2#




236 25.4 20.0 30.0

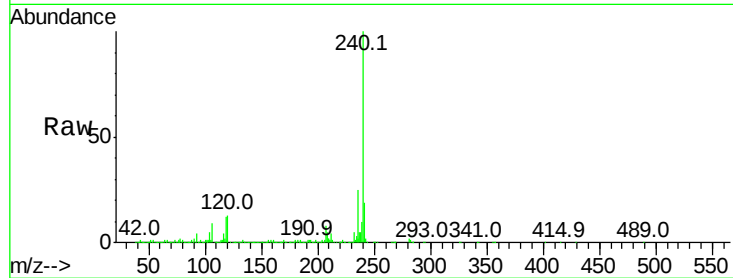

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

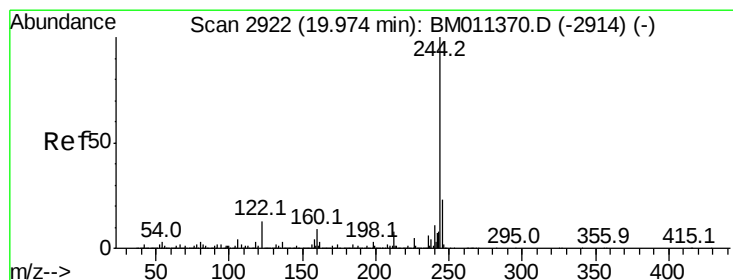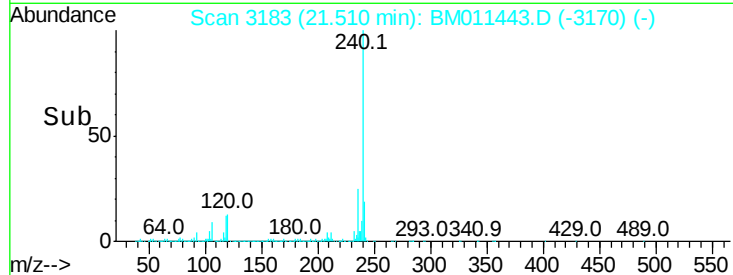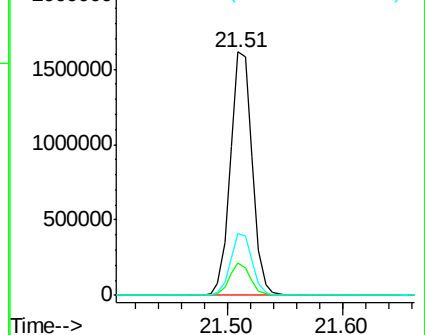

#78

Terphenyl-d14

Concen: 109.673 ng

RT: 19.96 min Scan# 2920

Delta R.T. -0.01 min

Lab File: BM011443.D

Acq: 05 Sep 2017 21:50


Tgt Ion:244 Resp: 9318642

Ion Ratio Lower Upper

244 100

212 7.7 4.9 7.3#



122 11.3 6.2 9.4#

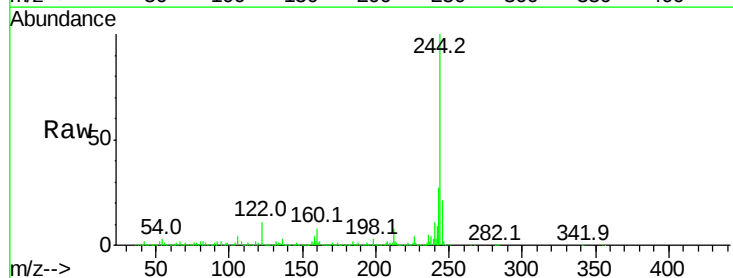


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

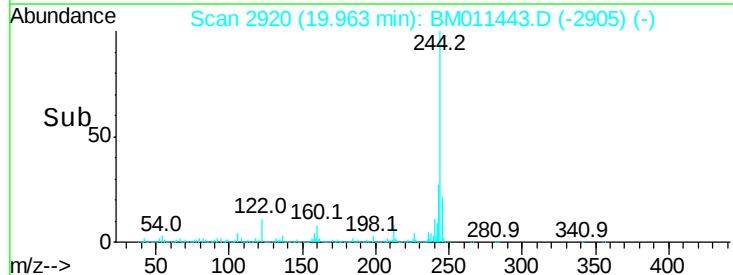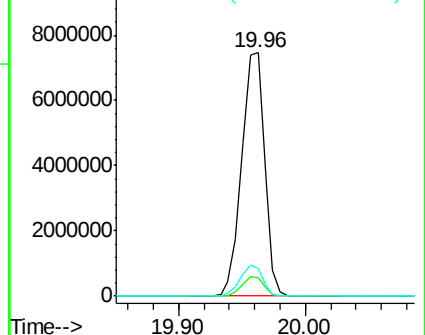

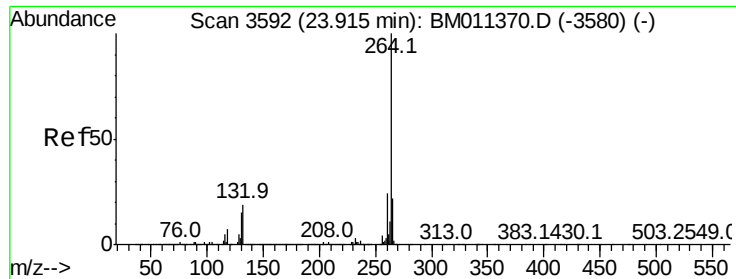

#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.89 min Scan# 3588
Delta R.T. -0.02 min
Lab File: BM011443.D
Acq: 05 Sep 2017 21:50

Instrument :
BNA_M
ClientSampleId :
TP9-WC1

Tot Ion: 264 Resp: 1226868

Ion	Ratio	Lower	Upper
264	100		
260	24.9	18.6	27.8
265	22.2	17.3	25.9

