
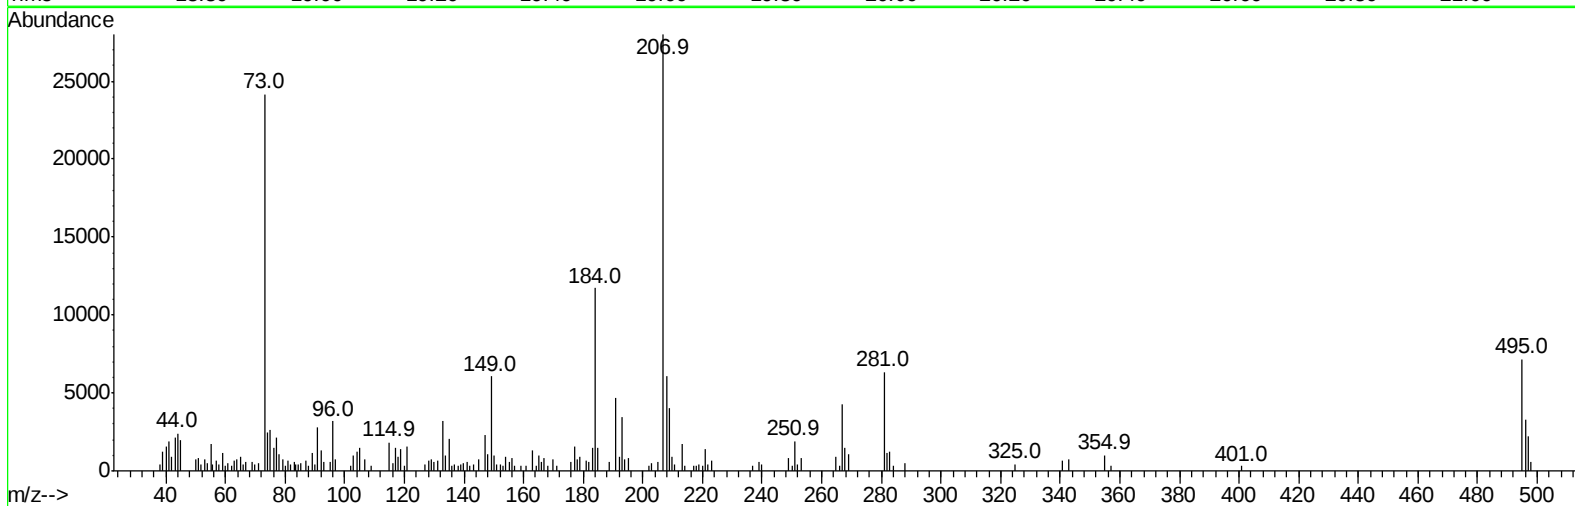


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\
Data File : BM011424.D
Acq On : 05 Sep 2017 09:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:16:49 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

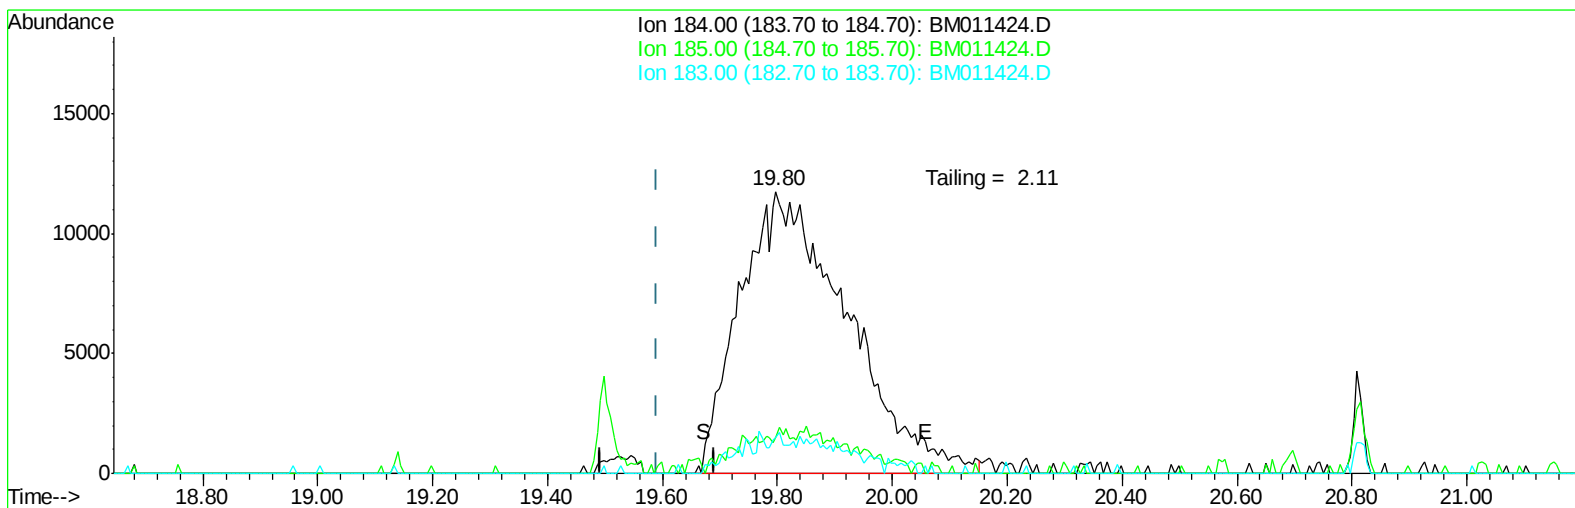

TIC: BM011424.D

(76) Benzidine



19.798min (+0.206) 142.01ng m

response 152788

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	12.75
183.00	11.10	12.72
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\
Data File : BM011424.D
Acq On : 05 Sep 2017 09:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:16:49 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

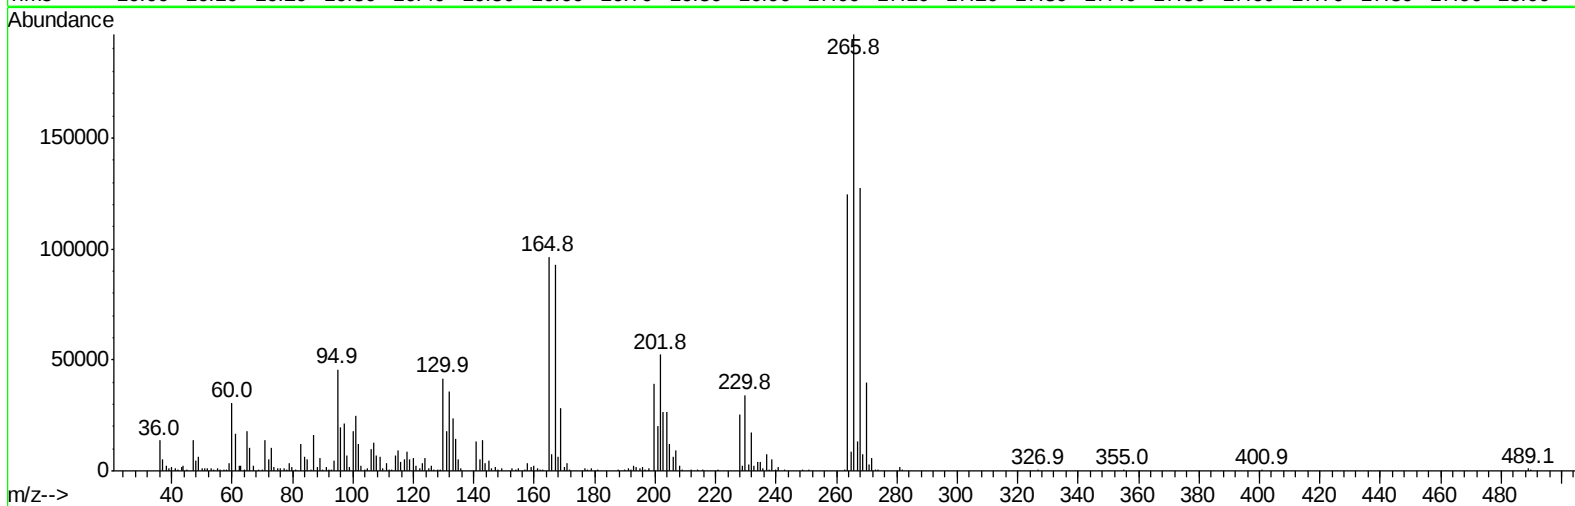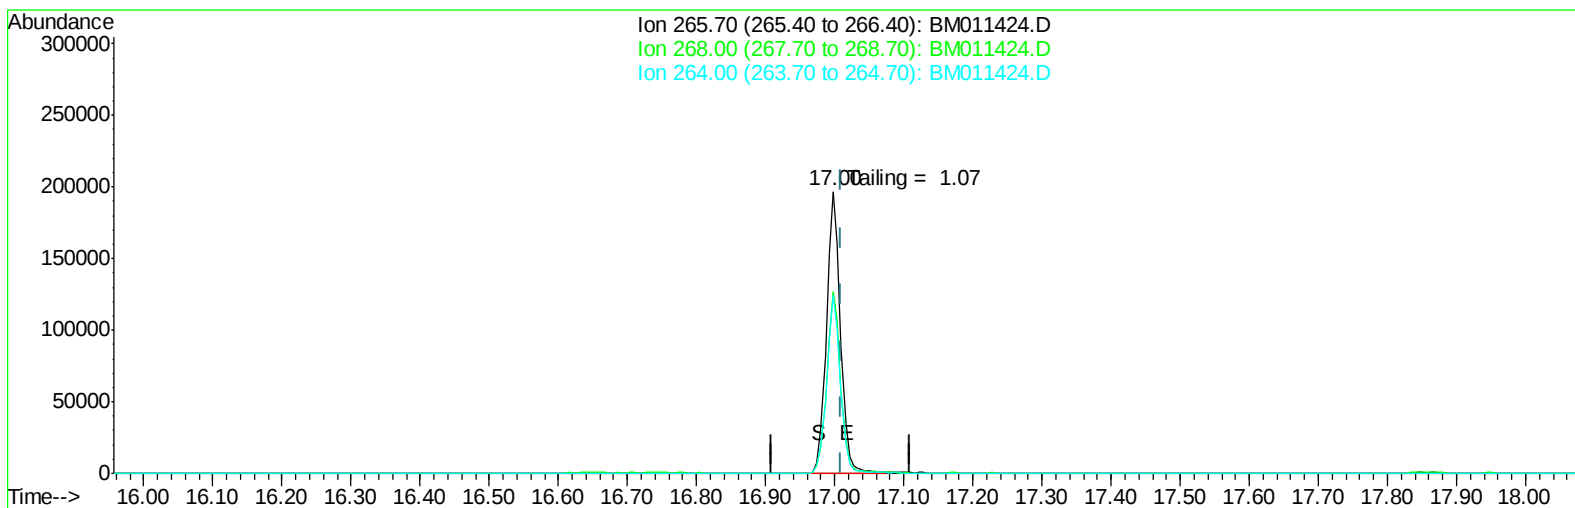

TIC: BM011424.D

(69) Pentachlorophenol (C)

16.998min (-0.012) 62165.11ng

response 276774

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.76
264.00	61.20	63.42
0.00	0.00	0.00