
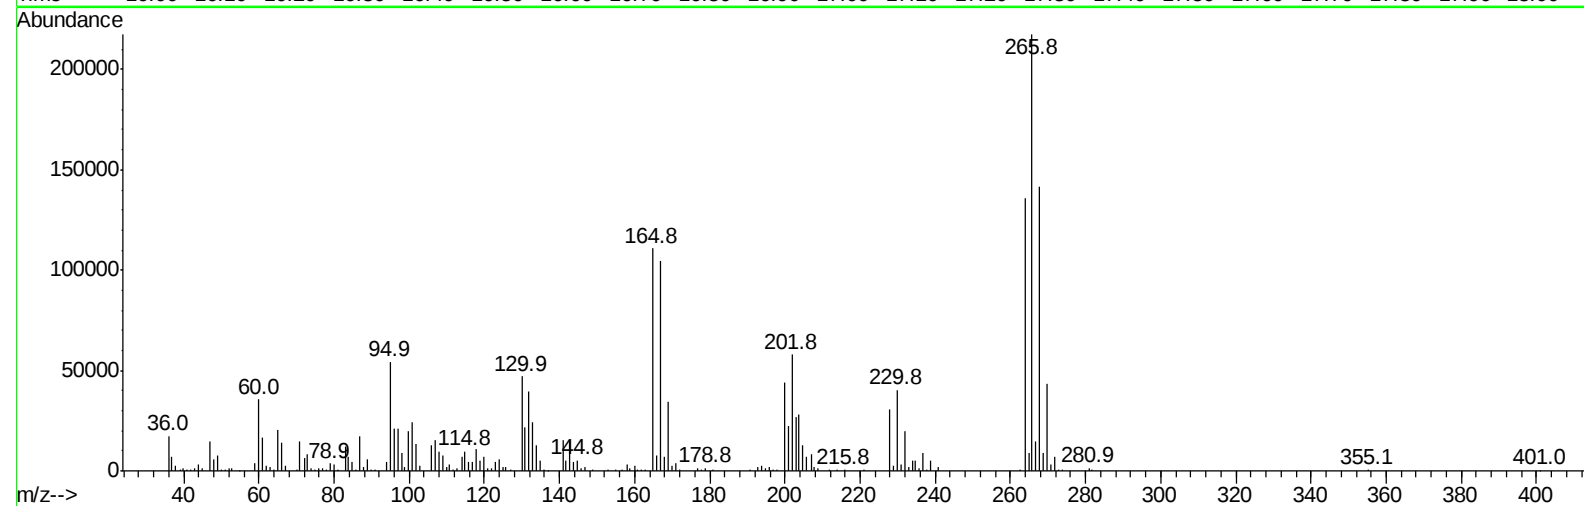


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\
Data File : BM011431.D
Acq On : 05 Sep 2017 14:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:19:17 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

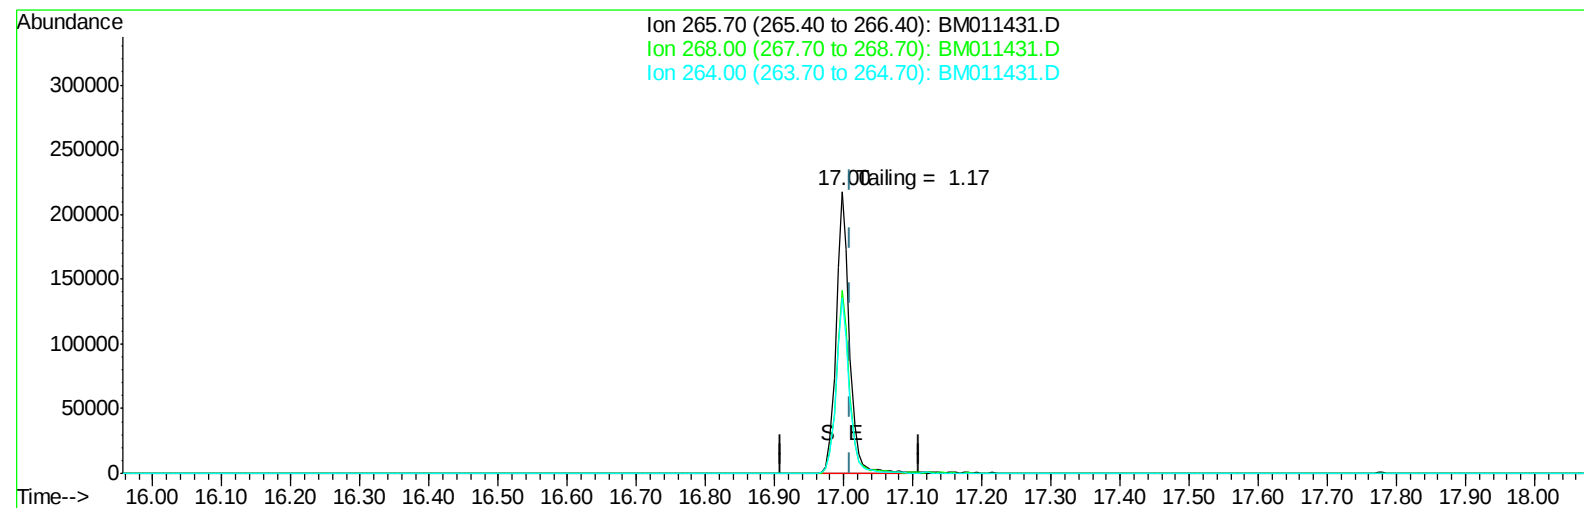

TIC: BM011431.D

(69) Pentachlorophenol (C)



16.998min (-0.012) 48659.39ng

response 289847

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.13
264.00	61.20	62.39
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\
Data File : BM011431.D
Acq On : 05 Sep 2017 14:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:19:17 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

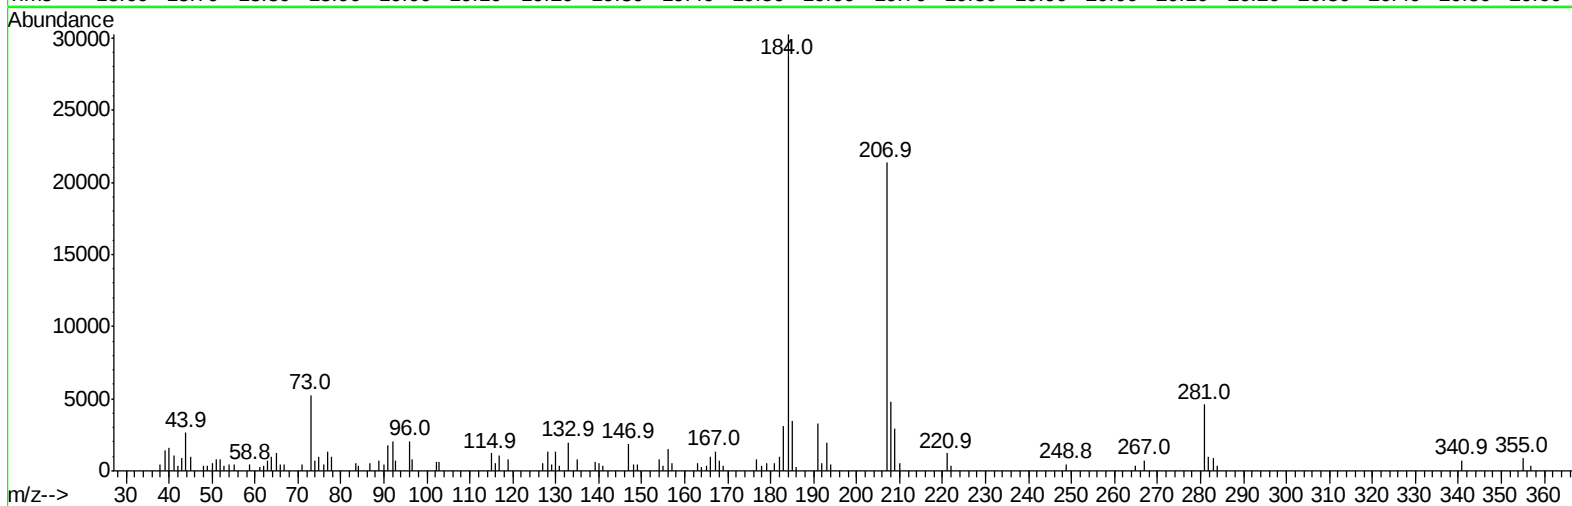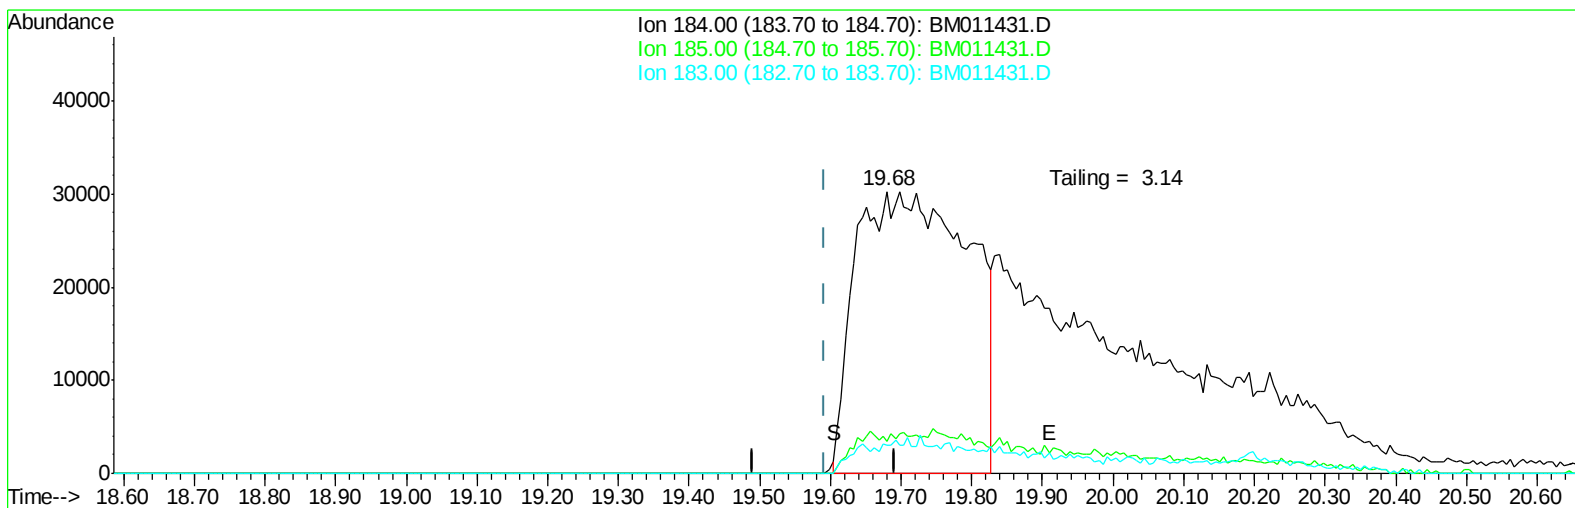

TIC: BM011431.D

(76) Benzidine

19.680min (+0.088) 5748.21ng m

response 336605

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	11.57
183.00	11.10	10.17
0.00	0.00	0.00