


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\
 Data File : BM011424.D
 Acq On : 05 Sep 2017 09:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 31 18:39:59 2017

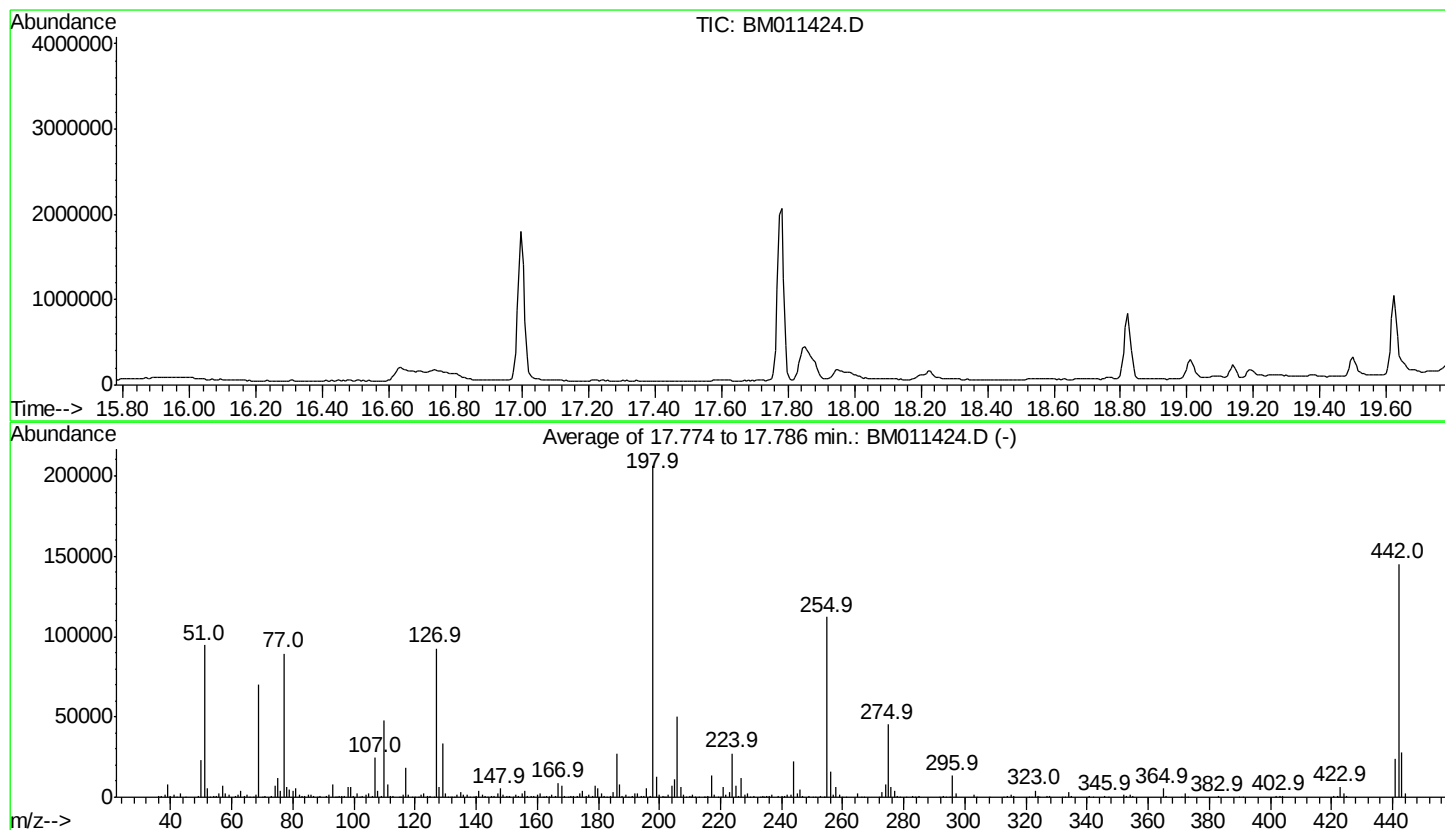

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	94594	PASS
68	69	0.00	2	2.0	1370	PASS
69	198	0.00	100	34.0	70111	PASS
70	69	0.00	2	0.2	173	PASS
127	198	10	80	44.8	92485	PASS
197	198	0.00	2	0.3	658	PASS
198	198	100	100	100.0	206400	PASS
199	198	5	9	6.2	12822	PASS
275	198	10	60	21.9	45138	PASS
365	198	1	100	2.5	5210	PASS
441	443	0.01	100	85.5	24189	PASS
442	198	50	100	70.4	145389	PASS
443	442	15	24	19.5	28280	PASS