


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090517\  
 Data File : BM011431.D  
 Acq On : 05 Sep 2017 14:33  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-BM083117.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Aug 31 18:39:59 2017

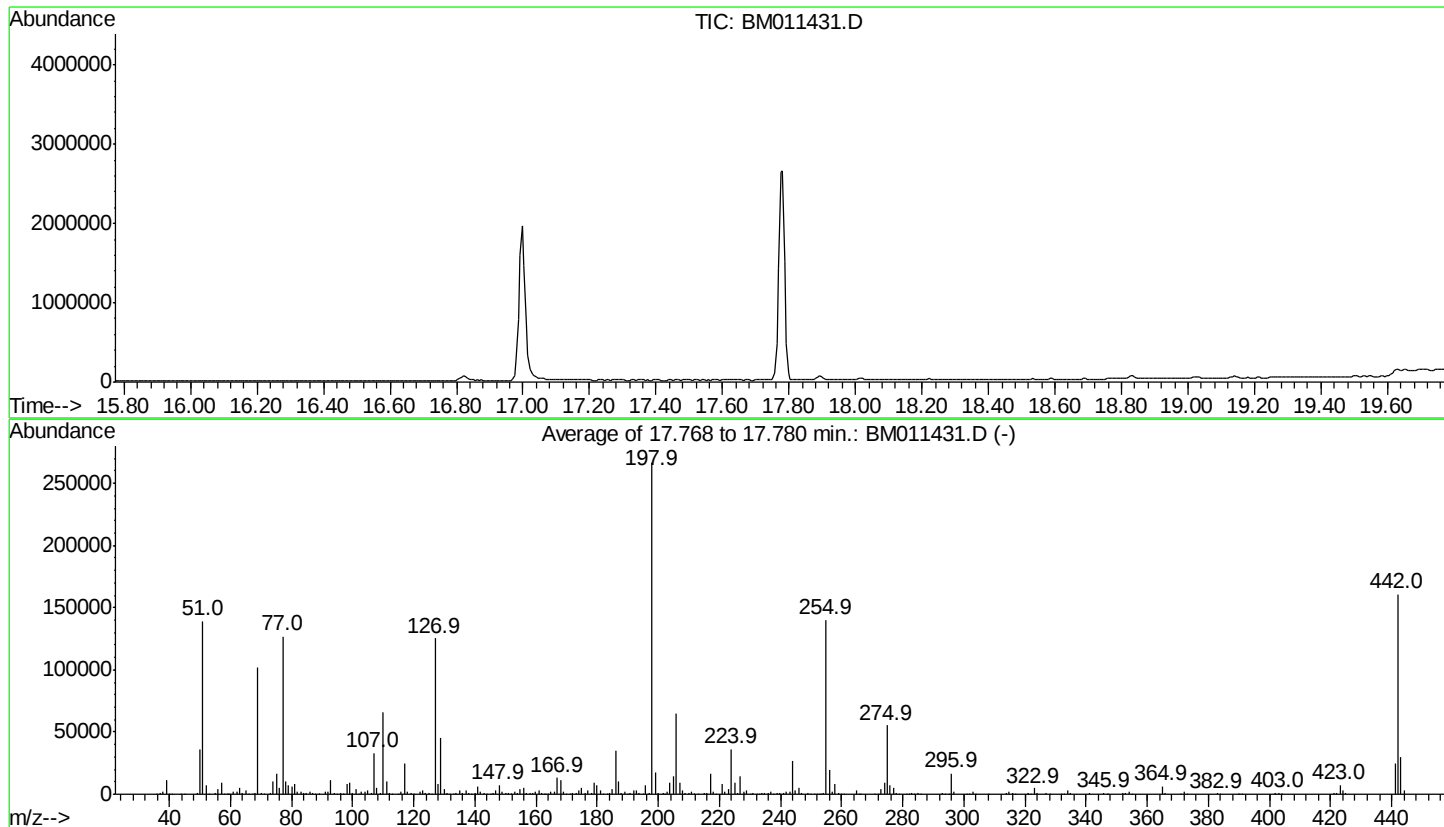

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2541

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 52.3      | 139414  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.5       | 1536    | PASS             |
| 69          | 198          | 0.00         | 100          | 38.2      | 101938  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 724     | PASS             |
| 127         | 198          | 10           | 80           | 46.9      | 125186  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 641     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 266666  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 17393   | PASS             |
| 275         | 198          | 10           | 60           | 20.7      | 55197   | PASS             |
| 365         | 198          | 1            | 100          | 2.5       | 6705    | PASS             |
| 441         | 443          | 0.01         | 100          | 82.4      | 24920   | PASS             |
| 442         | 198          | 50           | 100          | 60.4      | 161061  | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 30231   | PASS             |