
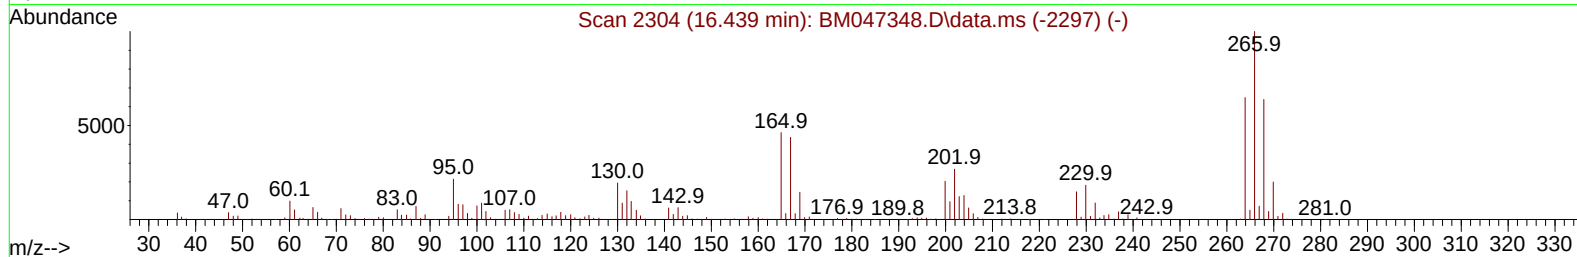
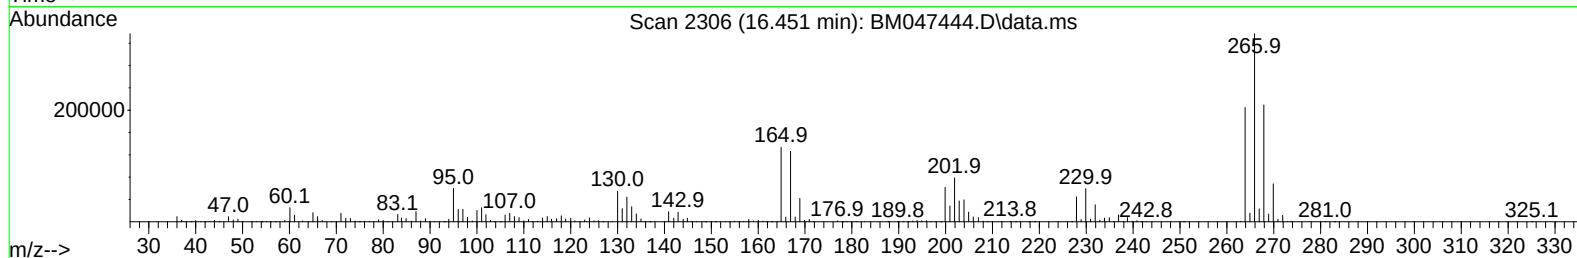


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090524\
Data File : BM047444.D
Acq On : 05 Sep 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 14:13:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

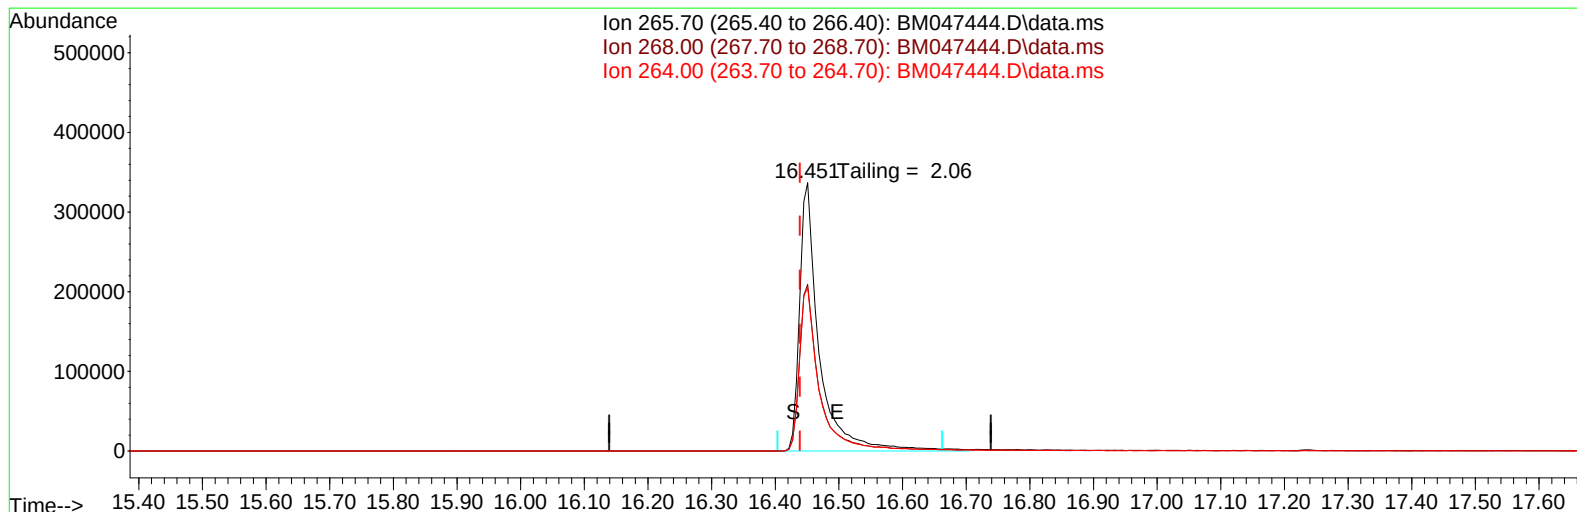

TIC: BM047444.D\data.ms

(70) Pentachlorophenol (C)




16.451min (+ 0.012) 0.00 ng

response 717696

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.11
264.00	64.90	60.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090524\
Data File : BM047444.D
Acq On : 05 Sep 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 14:13:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

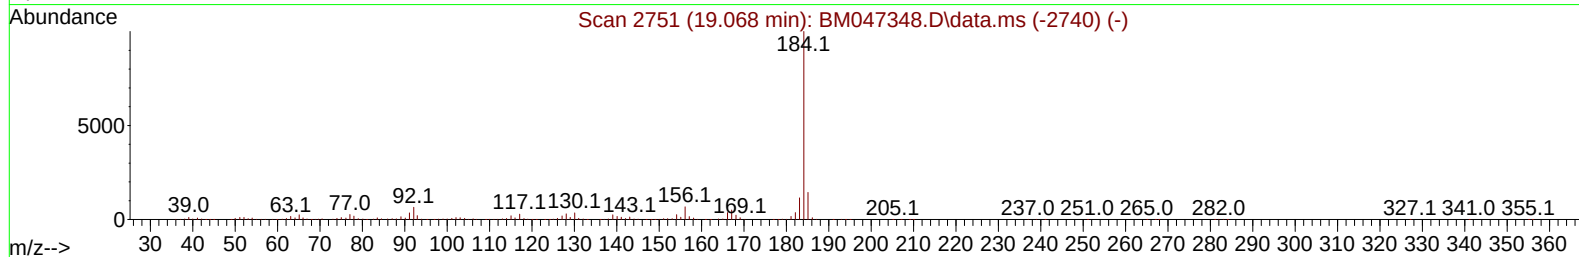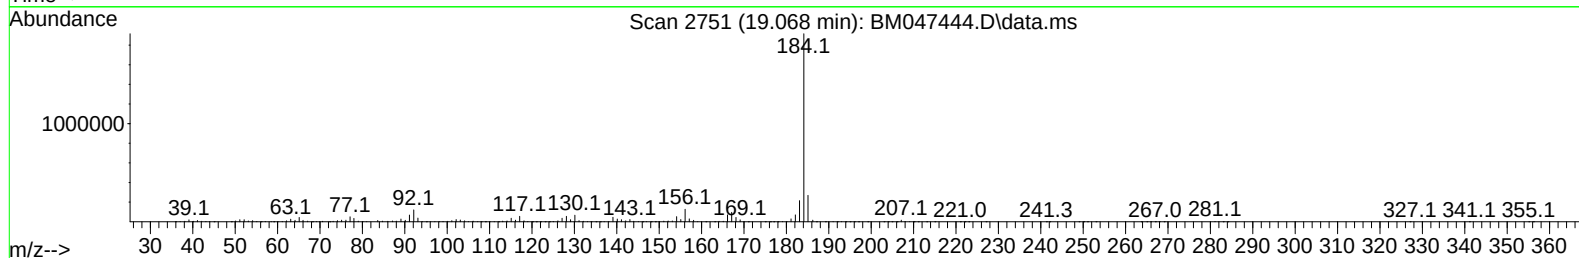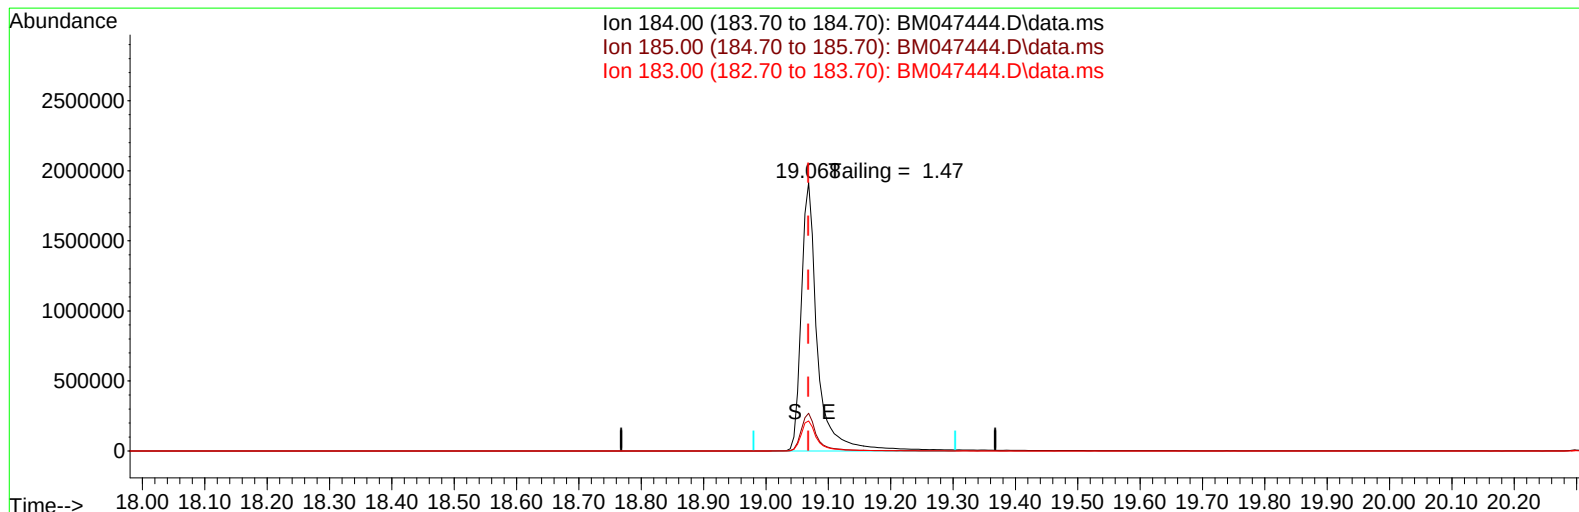

TIC: BM047444.D\data.ms

(77) Benzidine

19.068min (+ 0.000) 95786.93 ng

response 3471222

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.09
183.00	11.50	11.20
0.00	0.00	0.00