


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090524\
Data File : BM047444.D
Acq On : 05 Sep 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

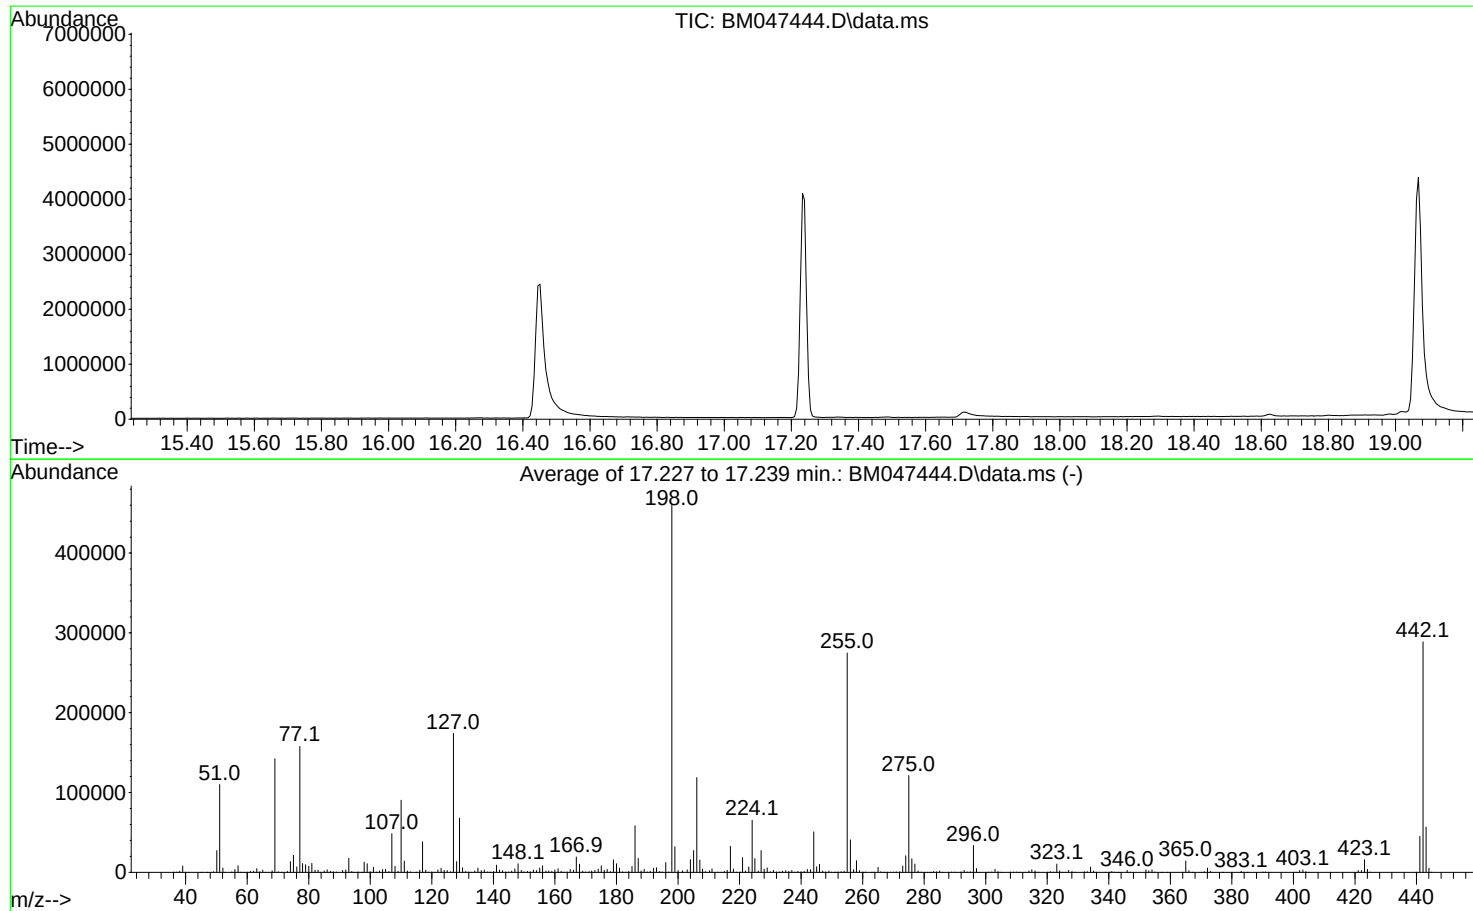

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2431

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	23.9	110058	PASS
68	69	0.00	2	1.5	2094	PASS
69	198	0.00	100	30.9	142243	PASS
70	69	0.00	2	0.6	795	PASS
127	198	10	80	37.8	174187	PASS
197	198	0.00	2	0.1	688	PASS
198	198	100	100	100.0	460821	PASS
199	198	5	9	7.0	32131	PASS
275	198	10	60	26.3	121251	PASS
365	198	1	100	3.1	14175	PASS
441	198	0.01	100	9.8	45189	PASS
442	442	50	100	100.0	288832	PASS
443	442	15	24	19.6	56677	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/5/2024	BNA_M	<u>BM047444.D</u>
Compound Name	Response	Retention Time
DDT	1713290	20.298
DDD	46590	19.862
DDE	8111	19.345
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
54701	1767991	3.09

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090524\
Data File : BM047444.D
Acq On : 05 Sep 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 05 14:13:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

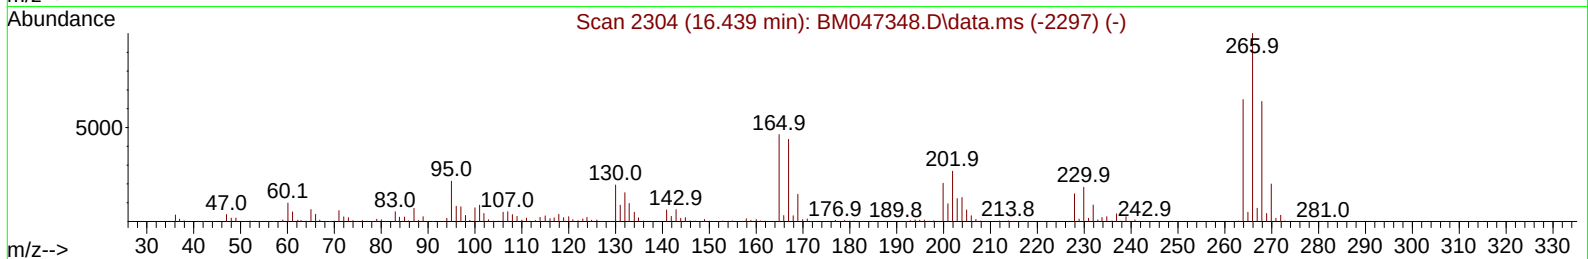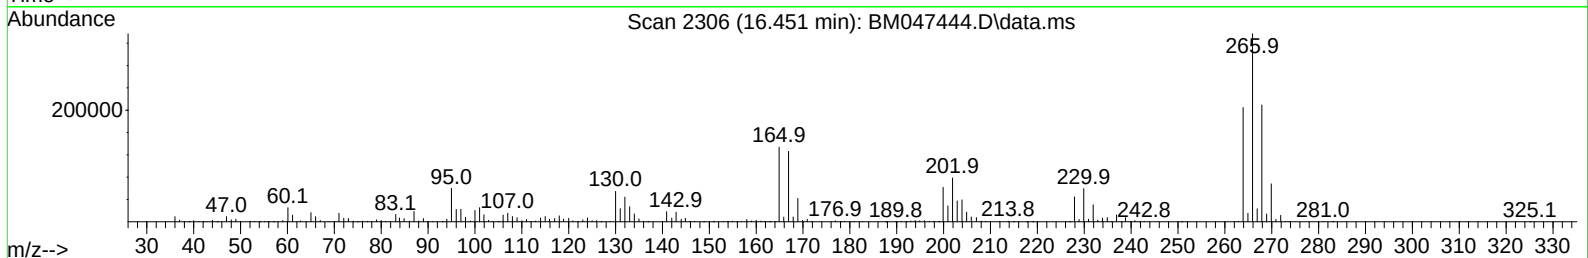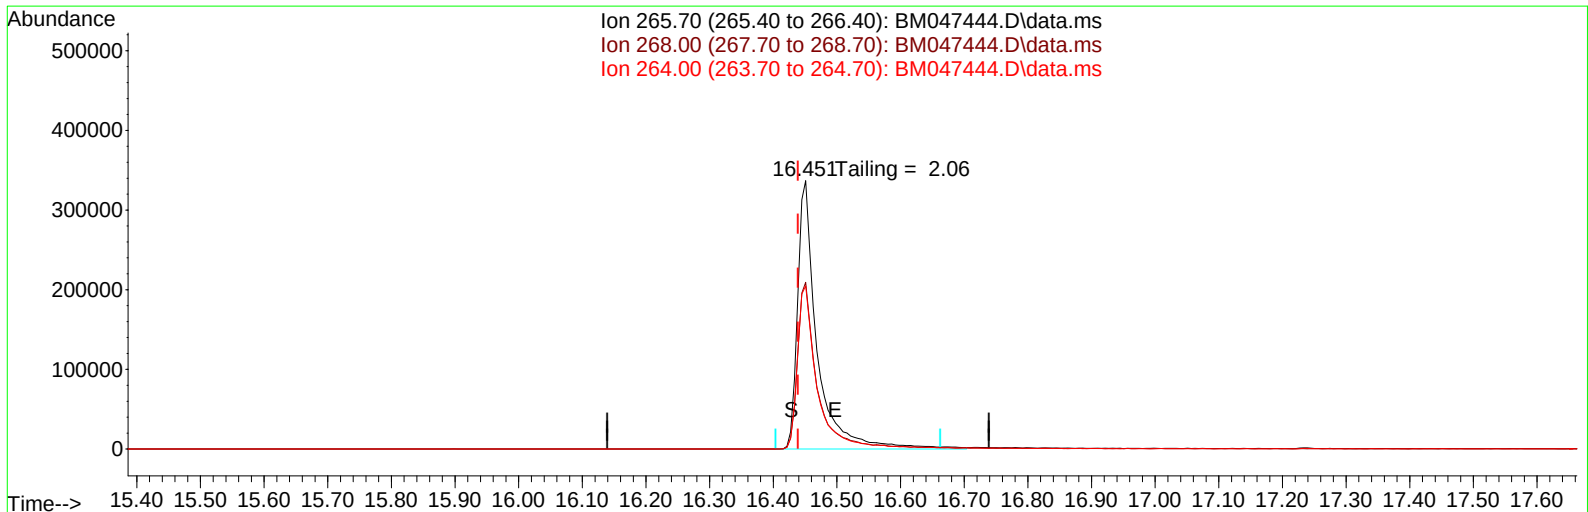

TIC: BM047444.D\data.ms

(70) Pentachlorophenol (C)

16.451min (+ 0.012) 0.00 ng




response 717696

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.11
264.00	64.90	60.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090524\
Data File : BM047444.D
Acq On : 05 Sep 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 05 14:13:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

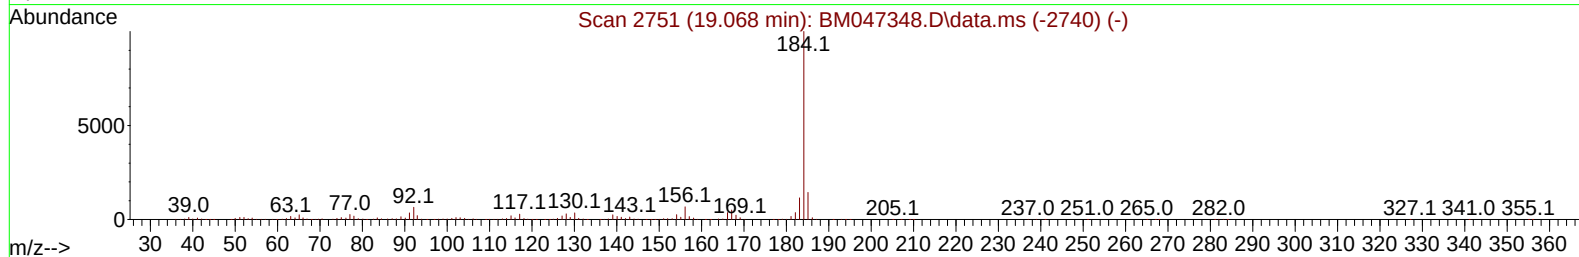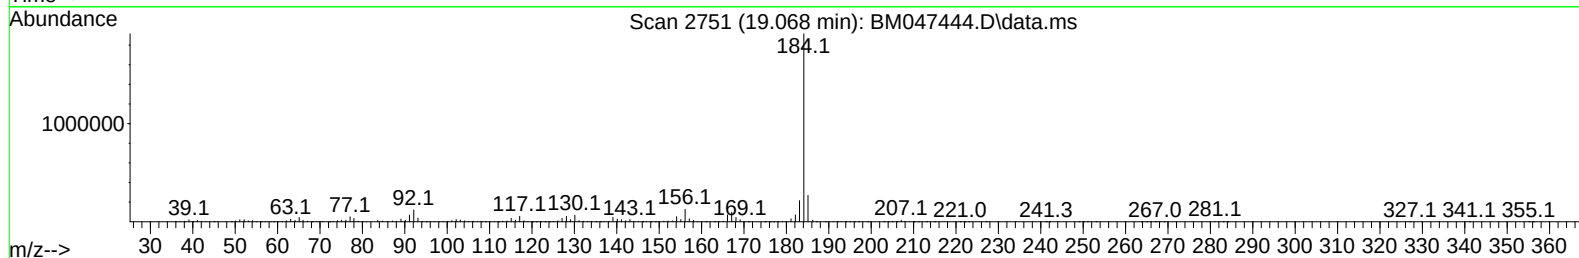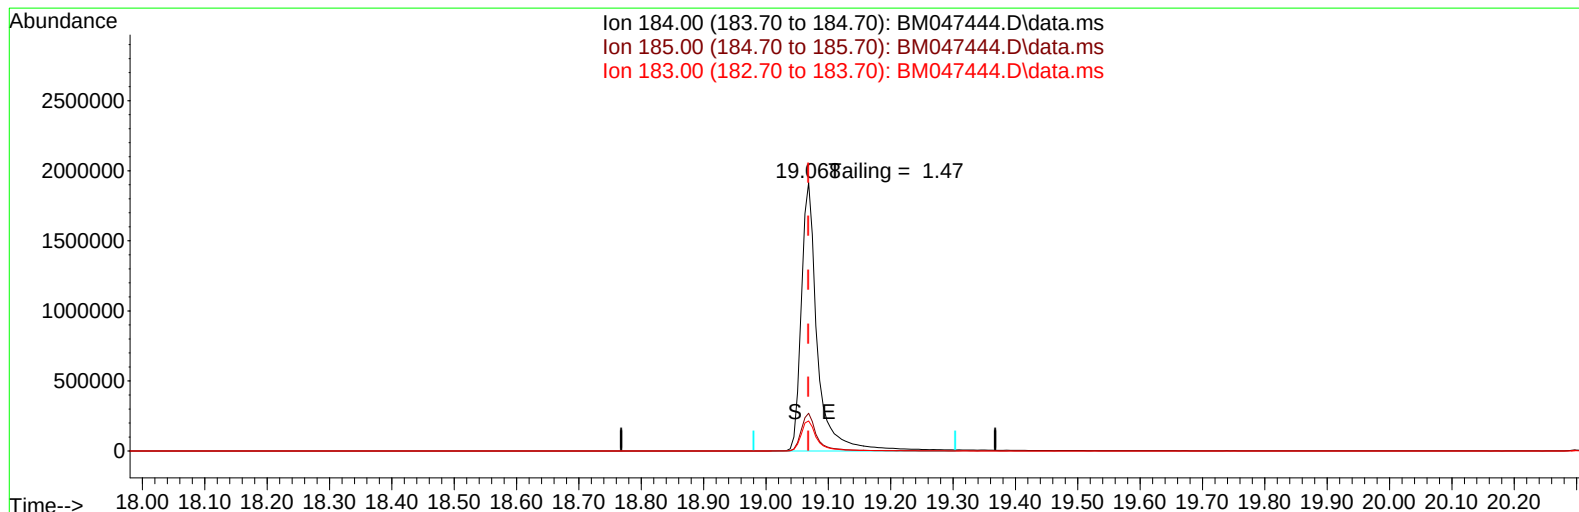

TIC: BM047444.D\data.ms

(77) Benzidine

19.068min (+ 0.000) 95786.93 ng

response 3471222

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.09
183.00	11.50	11.20
0.00	0.00	0.00