

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
 Data File : BM007422.D
 Acq On : 06 Sep 2016 20:06
 Operator : UM/SJ
 Sample : H4674-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0036

Quant Time: Sep 07 01:17:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:17:41 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	225391	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1137026	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	829368	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	2208621	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2911902	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	2733825	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	7875	1.79	ng/uL	0.00
5) Phenol-d5	6.96	99	173773	8.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	230061	20.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	279860	17.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	257514	13.87	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	173059	20.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	206809	21.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	385517	19.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	103448	4.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1623669	22.69	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1784709	21.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	109670	8.12	ng/ul	0.00
57) Fluorene-d10	15.42	176	1405195	22.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	308645	22.22	ng/ul	0.00
70) Anthracene-d10	17.27	188	2531262	24.53	ng/ul	0.00
76) Pyrene-d10	19.56	212	3190936	26.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	3089628	24.54	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.88	163	127745	1.79	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007422.D
Acq On : 06 Sep 2016 20:06
Operator : UM/SJ
Sample : H4674-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0036

Quant Time: Sep 07 01:17:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:17:41 2016
Response via : Initial Calibration

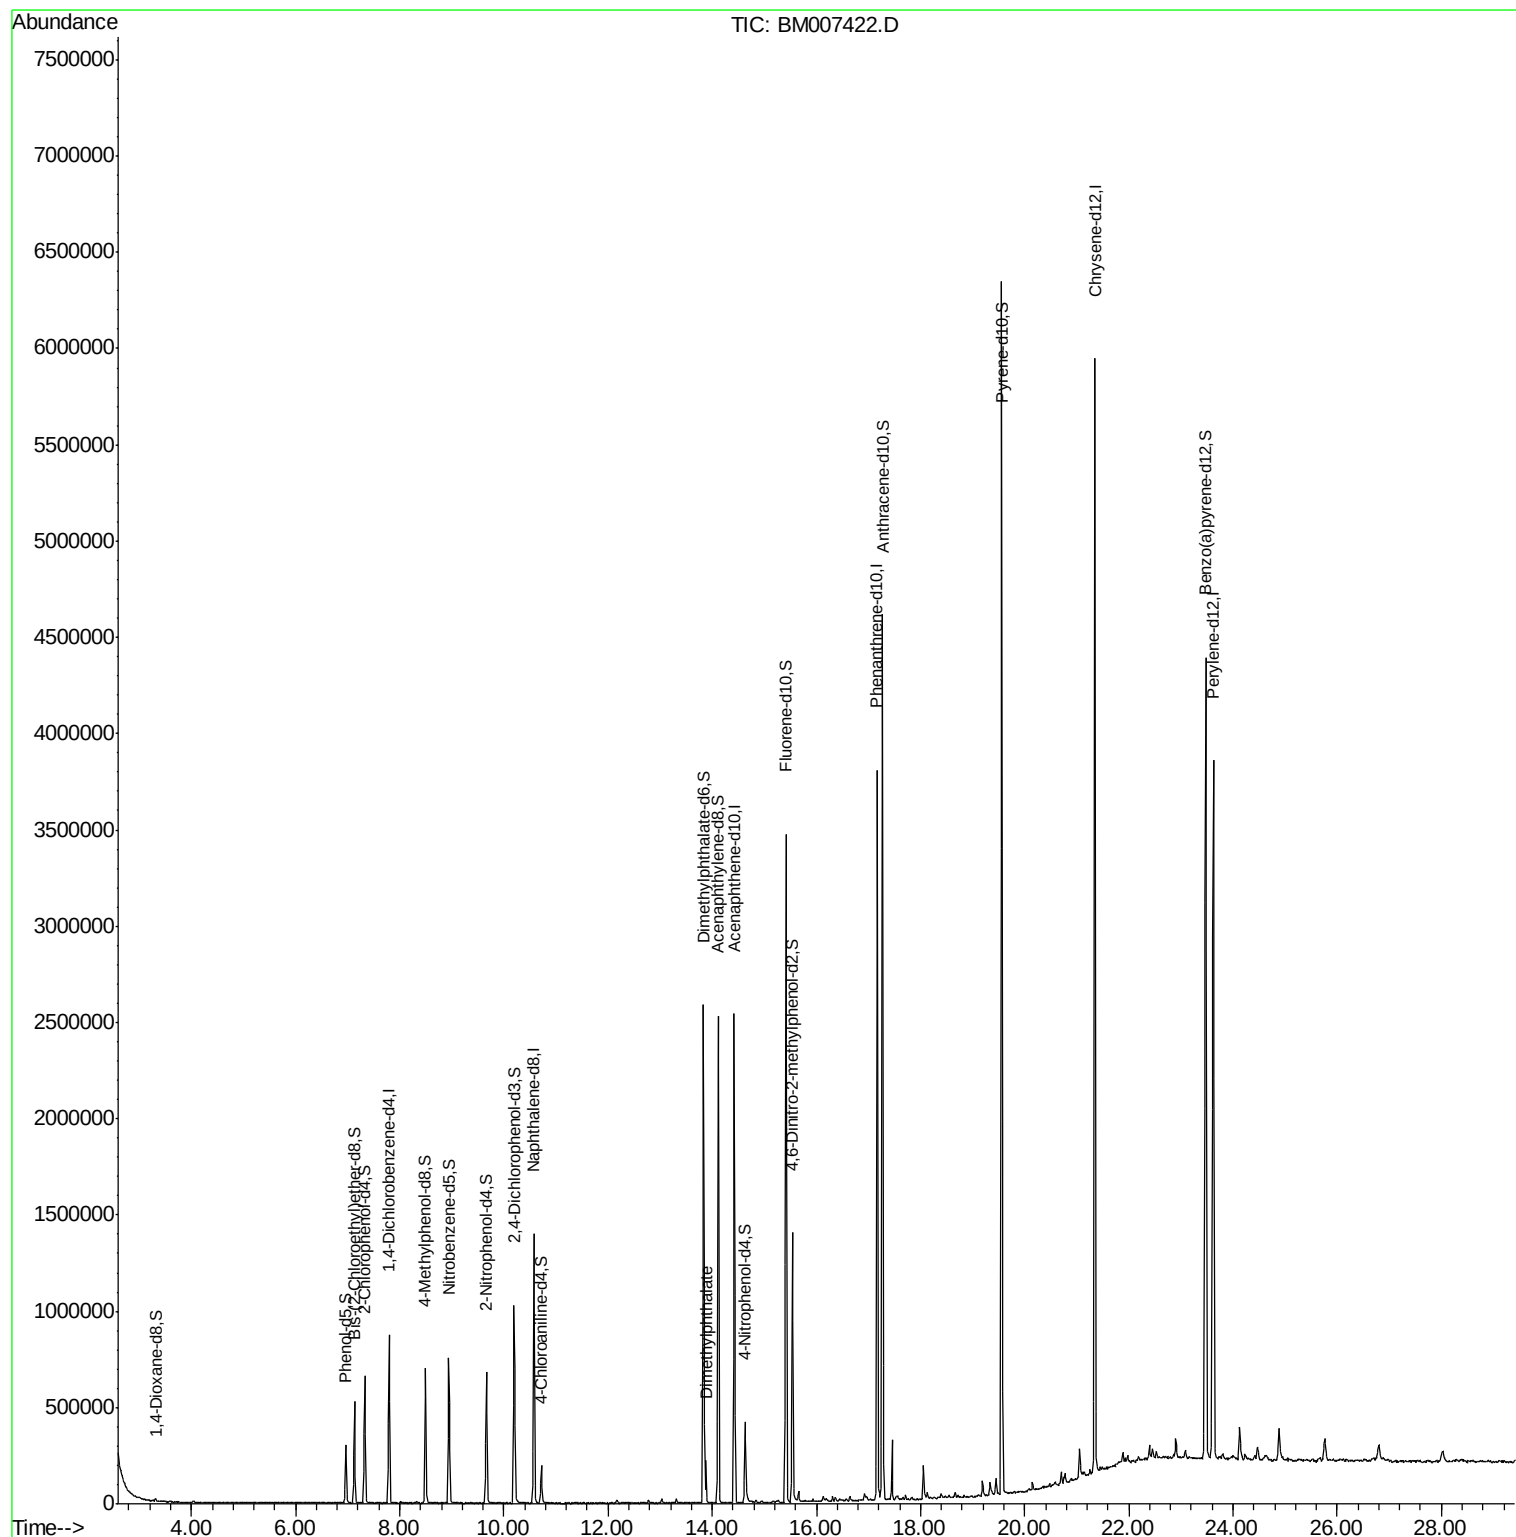

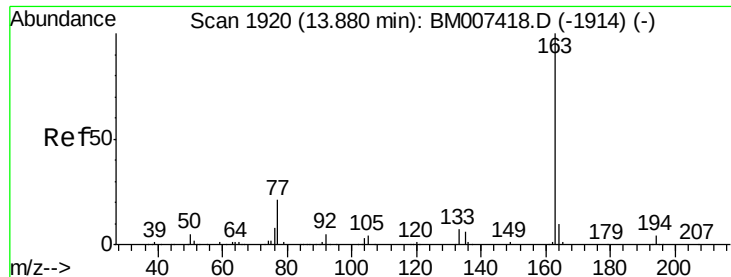

#44

Dimethylphthalate

Concen: 1.79 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. -0.00 min

Lab File: BM007422.D

Acq: 06 Sep 2016 20:06

Instrument :

BNA_M

ClientSampleId :

C0036



Tgt Ion:163 Resp: 127745

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 9.5 7.8 11.8

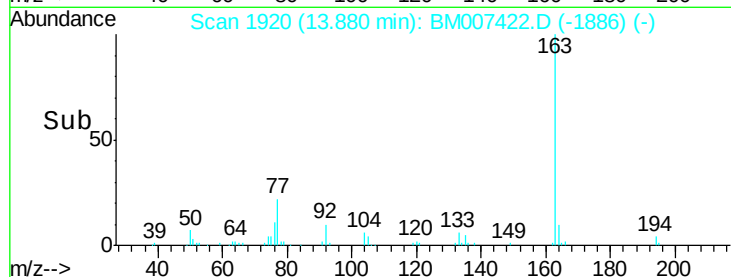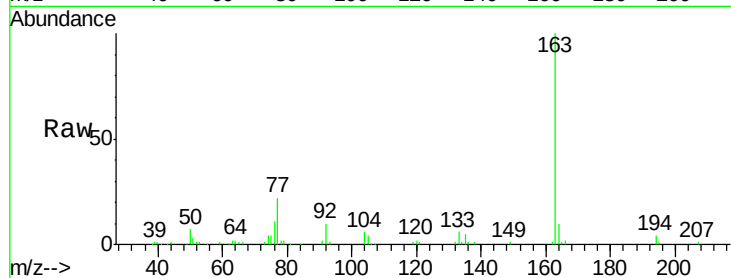

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

