

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
 Data File : BM007417.D
 Acq On : 06 Sep 2016 16:29
 Operator : UM/SJ
 Sample : H4639-23
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3C3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	738	744	755	rBV	695000	1111841	14.71%	1.599%
2	7.128	765	772	782	rBV	541843	833265	11.03%	1.199%
3	7.328	799	806	816	rBV	717262	1148396	15.20%	1.652%
4	7.792	879	885	893	rBV	733335	1189609	15.74%	1.711%
5	8.492	997	1004	1016	rBV	935289	1550510	20.52%	2.231%
6	8.951	1074	1082	1092	rBV	726931	1241034	16.42%	1.785%
7	9.669	1196	1204	1218	rBV	650070	1118516	14.80%	1.609%
8	10.198	1287	1294	1313	rBV	944924	1673234	22.14%	2.407%
9	10.580	1351	1359	1369	rBV	1214136	2040914	27.01%	2.936%
10	10.716	1373	1382	1397	rBV	919689	1632650	21.61%	2.349%
11	13.833	1905	1912	1922	rBV	2340047	3400705	45.01%	4.892%
12	14.115	1953	1960	1970	rBV	2315177	3631165	48.06%	5.224%
13	14.427	2006	2013	2023	rVB2	2193863	3411719	45.15%	4.908%
14	14.627	2040	2047	2066	rBV	984202	1695023	22.43%	2.438%
15	15.421	2174	2182	2192	rBV	3324783	4972523	65.81%	7.153%
16	15.545	2196	2203	2215	rBV	1114336	1646381	21.79%	2.368%
17	17.168	2473	2479	2487	rBV2	3354206	4833405	63.97%	6.953%
18	17.268	2489	2496	2510	rBV2	4153526	5991518	79.29%	8.619%
19	19.450	2862	2867	2871	rBV2	58568	77375	1.02%	0.111%
20	19.562	2879	2886	2897	rBV	5403251	7556219	100.00%	10.870%
21	21.350	3184	3190	3201	rBV	5240949	6555491	86.76%	9.431%
22	23.480	3544	3552	3565	rVB2	3360391	6546860	86.64%	9.418%
23	23.621	3568	3576	3588	rVB	2791749	5655218	74.84%	8.135%


Sum of corrected areas: 69513571

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007417.D
Acq On : 06 Sep 2016 16:29
Operator : UM/SJ
Sample : H4639-23
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

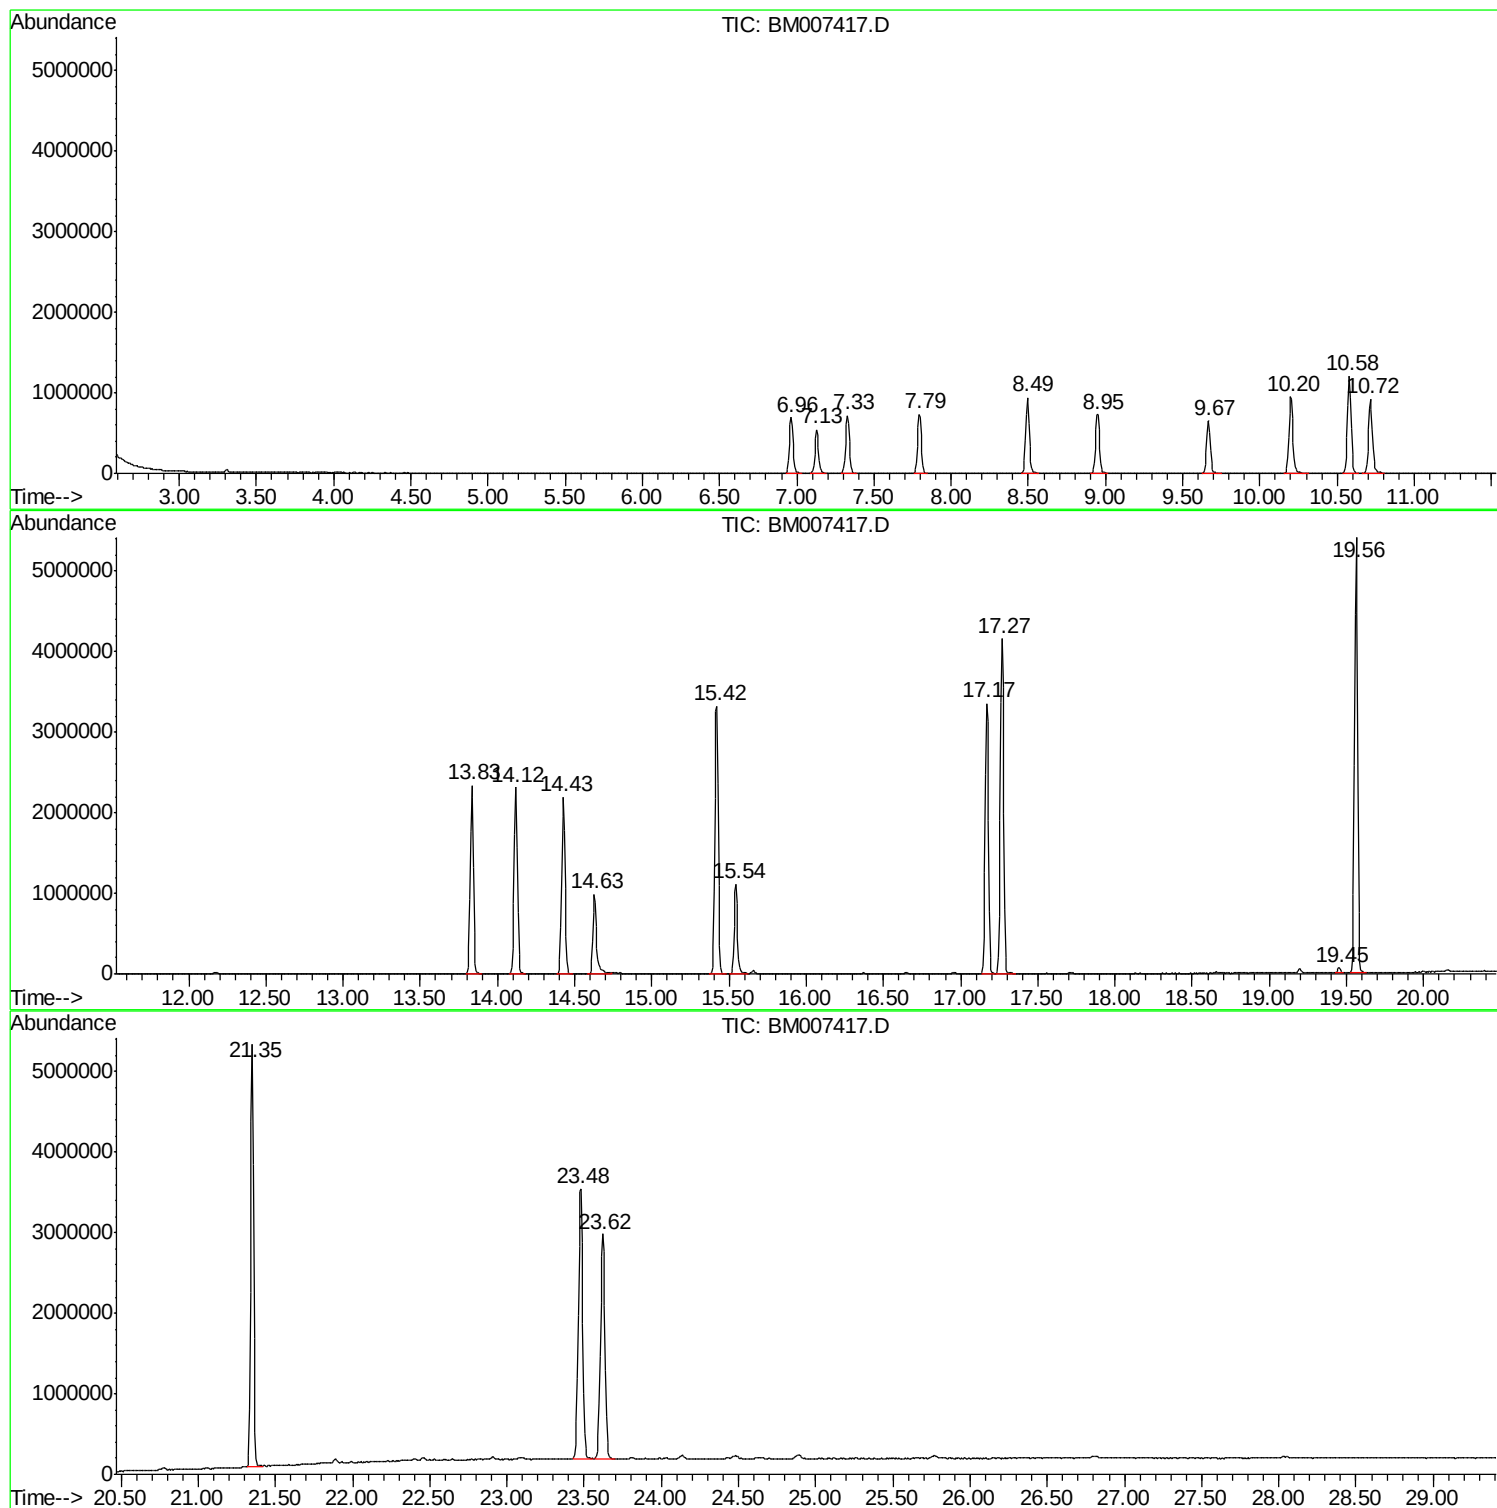

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007417.D
Acq On : 06 Sep 2016 16:29
Operator : UM/SJ
Sample : H4639-23
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007417.D
Acq On : 06 Sep 2016 16:29
Operator : UM/SJ
Sample : H4639-23
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc