

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
 Data File : BM007423.D
 Acq On : 06 Sep 2016 20:42
 Operator : UM/SJ
 Sample : H4674-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0037

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	736	744	752	rBV	316059	512981	5.74%	0.624%
2	7.128	763	772	782	rBV	636858	1001316	11.20%	1.219%
3	7.328	799	806	816	rBV	745197	1206734	13.49%	1.469%
4	7.792	878	885	899	rVB	983954	1604146	17.94%	1.953%
5	8.492	994	1004	1013	rBV	743353	1237189	13.83%	1.506%
6	8.945	1074	1081	1090	rBV	901033	1528549	17.09%	1.861%
7	9.669	1194	1204	1215	rBV	802155	1392698	15.57%	1.695%
8	10.198	1286	1294	1308	rBV	1141879	2048366	22.90%	2.494%
9	10.580	1348	1359	1368	rBV	1578115	2731422	30.54%	3.325%
10	10.716	1375	1382	1394	rBV	186760	344996	3.86%	0.420%
11	13.833	1905	1912	1920	rBV	2867395	3941238	44.07%	4.798%
12	14.116	1953	1960	1971	rBV	2909024	4387866	49.06%	5.341%
13	14.427	2004	2013	2021	rBV2	2934743	4505429	50.38%	5.485%
14	14.633	2040	2048	2073	rBV	377014	731072	8.17%	0.890%
15	15.415	2174	2181	2191	rBV	3932461	5941906	66.44%	7.233%
16	15.545	2196	2203	2214	rVV	1474707	2142031	23.95%	2.608%
17	17.168	2473	2479	2488	rVB2	4307803	6232003	69.68%	7.586%
18	17.268	2489	2496	2506	rBV	4988178	7047331	78.80%	8.579%
19	18.056	2625	2630	2639	rBV	169802	255047	2.85%	0.310%
20	19.192	2819	2823	2830	rBV2	70869	106341	1.19%	0.129%
21	19.333	2844	2847	2853	rBV3	71923	103510	1.16%	0.126%
22	19.450	2862	2867	2870	rBV2	84706	115838	1.30%	0.141%
23	19.562	2879	2886	2897	rBV	6394354	8943468	100.00%	10.887%
24	21.350	3184	3190	3200	rBV	6515220	8546737	95.56%	10.404%
25	23.474	3543	3551	3564	rVB2	4126766	8074680	90.29%	9.830%
26	23.621	3568	3576	3589	rVB	3877224	7464340	83.46%	9.087%


Sum of corrected areas: 82147234

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007423.D
Acq On : 06 Sep 2016 20:42
Operator : UM/SJ
Sample : H4674-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0037

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

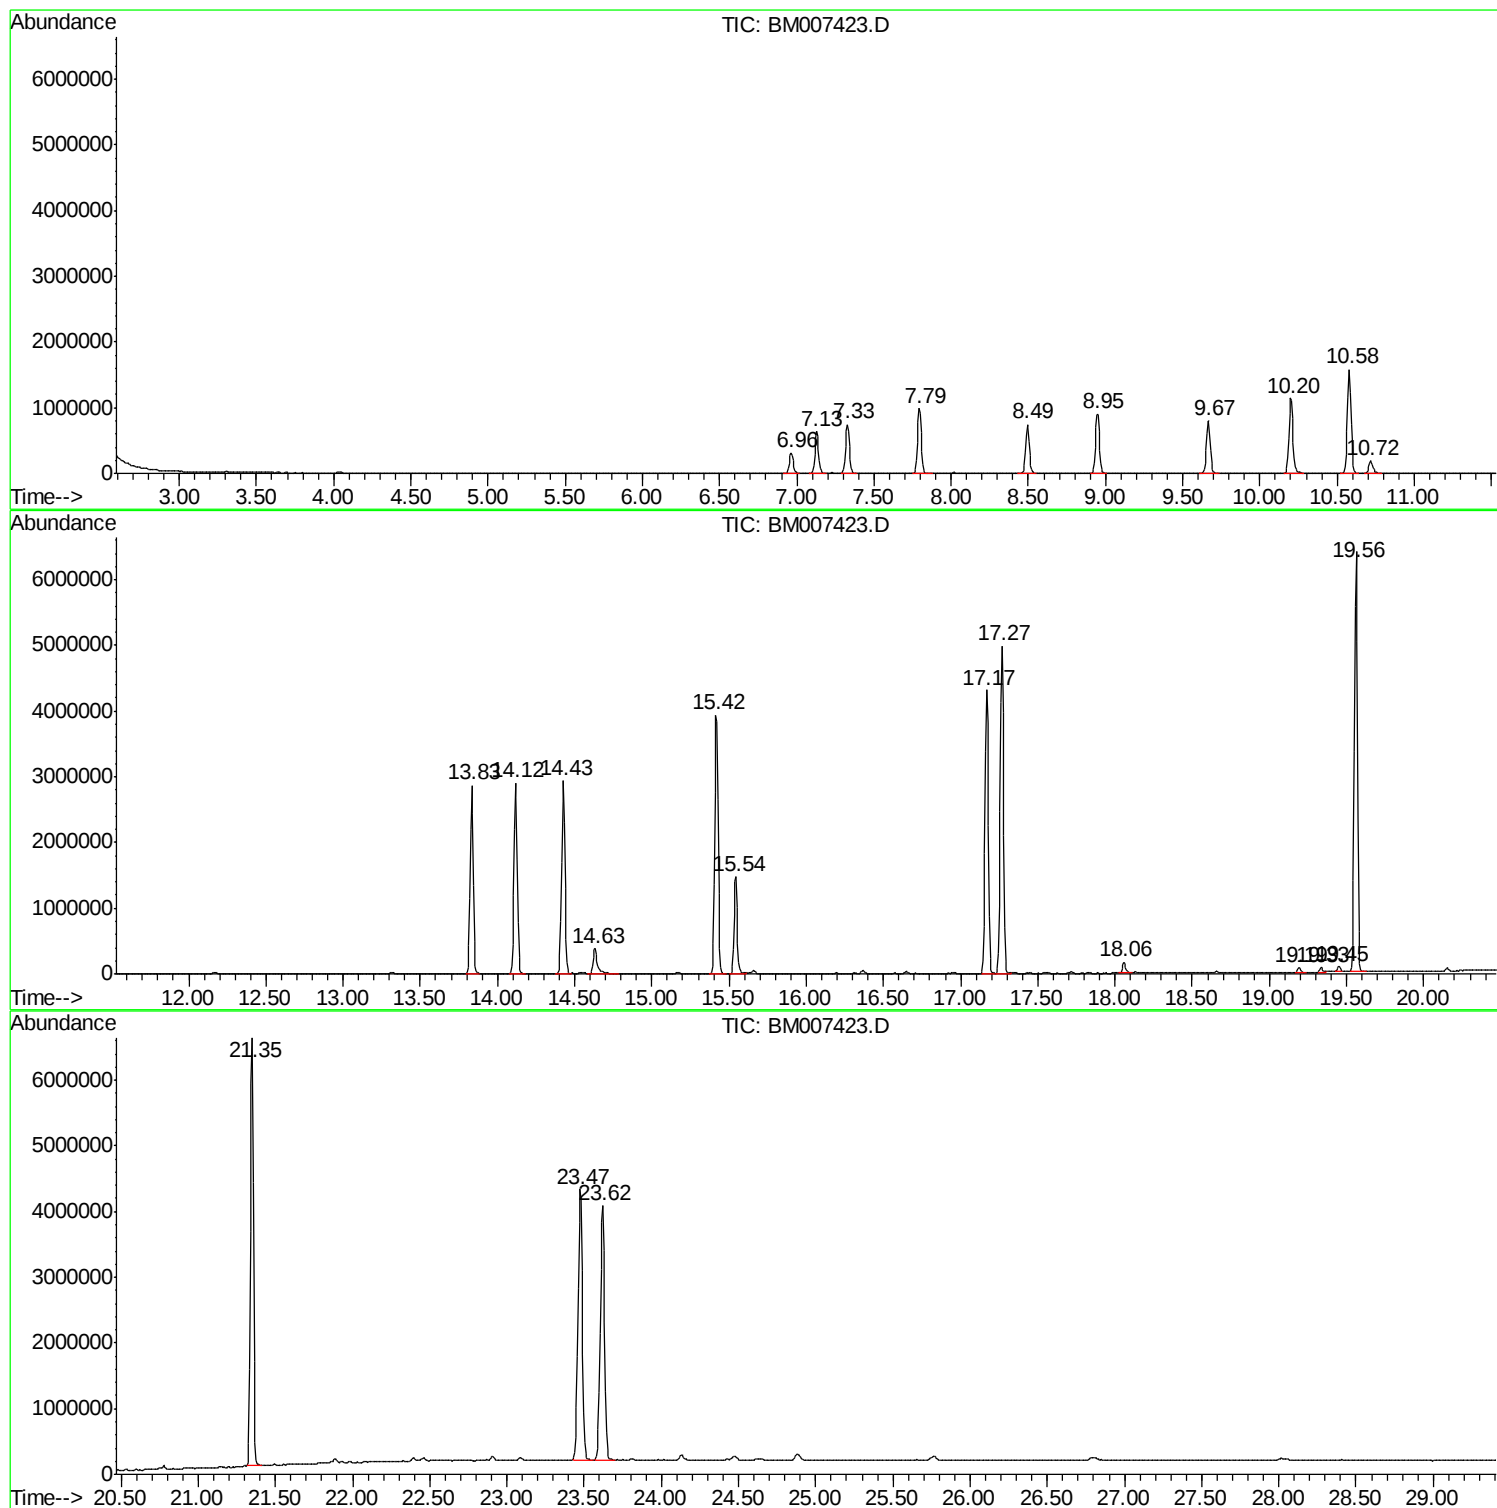

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007423.D
Acq On : 06 Sep 2016 20:42
Operator : UM/SJ
Sample : H4674-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0037

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007423.D
Acq On : 06 Sep 2016 20:42
Operator : UM/SJ
Sample : H4674-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0037

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc