

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
 Data File : BM007427.D
 Acq On : 06 Sep 2016 23:06
 Operator : UM/SJ
 Sample : H4674-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0041

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	737	744	756	rBV	256917	425639	5.11%	0.611%
2	7.128	766	772	785	rBV	498510	783609	9.40%	1.125%
3	7.328	799	806	817	rVB	587021	951049	11.41%	1.365%
4	7.792	877	885	895	rBV	918770	1499182	17.99%	2.152%
5	8.492	995	1004	1013	rBV	559137	938848	11.27%	1.348%
6	8.945	1074	1081	1089	rBV	696466	1182191	14.19%	1.697%
7	9.663	1195	1203	1214	rBV	626539	1079095	12.95%	1.549%
8	10.198	1287	1294	1312	rBV	904564	1607846	19.29%	2.308%
9	10.580	1350	1359	1367	rBV	1477564	2557798	30.69%	3.672%
10	10.716	1376	1382	1395	rBV	192286	360010	4.32%	0.517%
11	13.833	1905	1912	1923	rBV	2235481	3108360	37.30%	4.462%
12	14.115	1953	1960	1974	rBV	2280235	3423932	41.08%	4.916%
13	14.427	2006	2013	2021	rBV2	2706787	4263126	51.15%	6.120%
14	14.633	2042	2048	2065	rBV	286356	554059	6.65%	0.795%
15	15.415	2174	2181	2196	rVB	3184732	4673468	56.08%	6.709%
16	15.545	2196	2203	2217	rBV	1091700	1617137	19.40%	2.322%
17	17.168	2472	2479	2487	rBV	4193330	5997017	71.96%	8.610%
18	17.268	2489	2496	2512	rVB2	3649665	5453678	65.44%	7.829%
19	19.192	2816	2823	2827	rBV	56643	85302	1.02%	0.122%
20	19.450	2862	2867	2871	rBV2	62676	93949	1.13%	0.135%
21	19.556	2879	2885	2892	rBV	4798083	6980761	83.76%	10.022%
22	21.350	3183	3190	3199	rBV	6176988	8333942	100.00%	11.964%
23	23.474	3543	3551	3563	rVB2	3218718	6197574	74.37%	8.897%
24	23.621	3567	3576	3589	rVB	3660392	7295866	87.54%	10.474%
25	24.879	3786	3790	3800	rVB4	86840	192144	2.31%	0.276%


Sum of corrected areas: 69655582

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007427.D
Acq On : 06 Sep 2016 23:06
Operator : UM/SJ
Sample : H4674-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0041

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

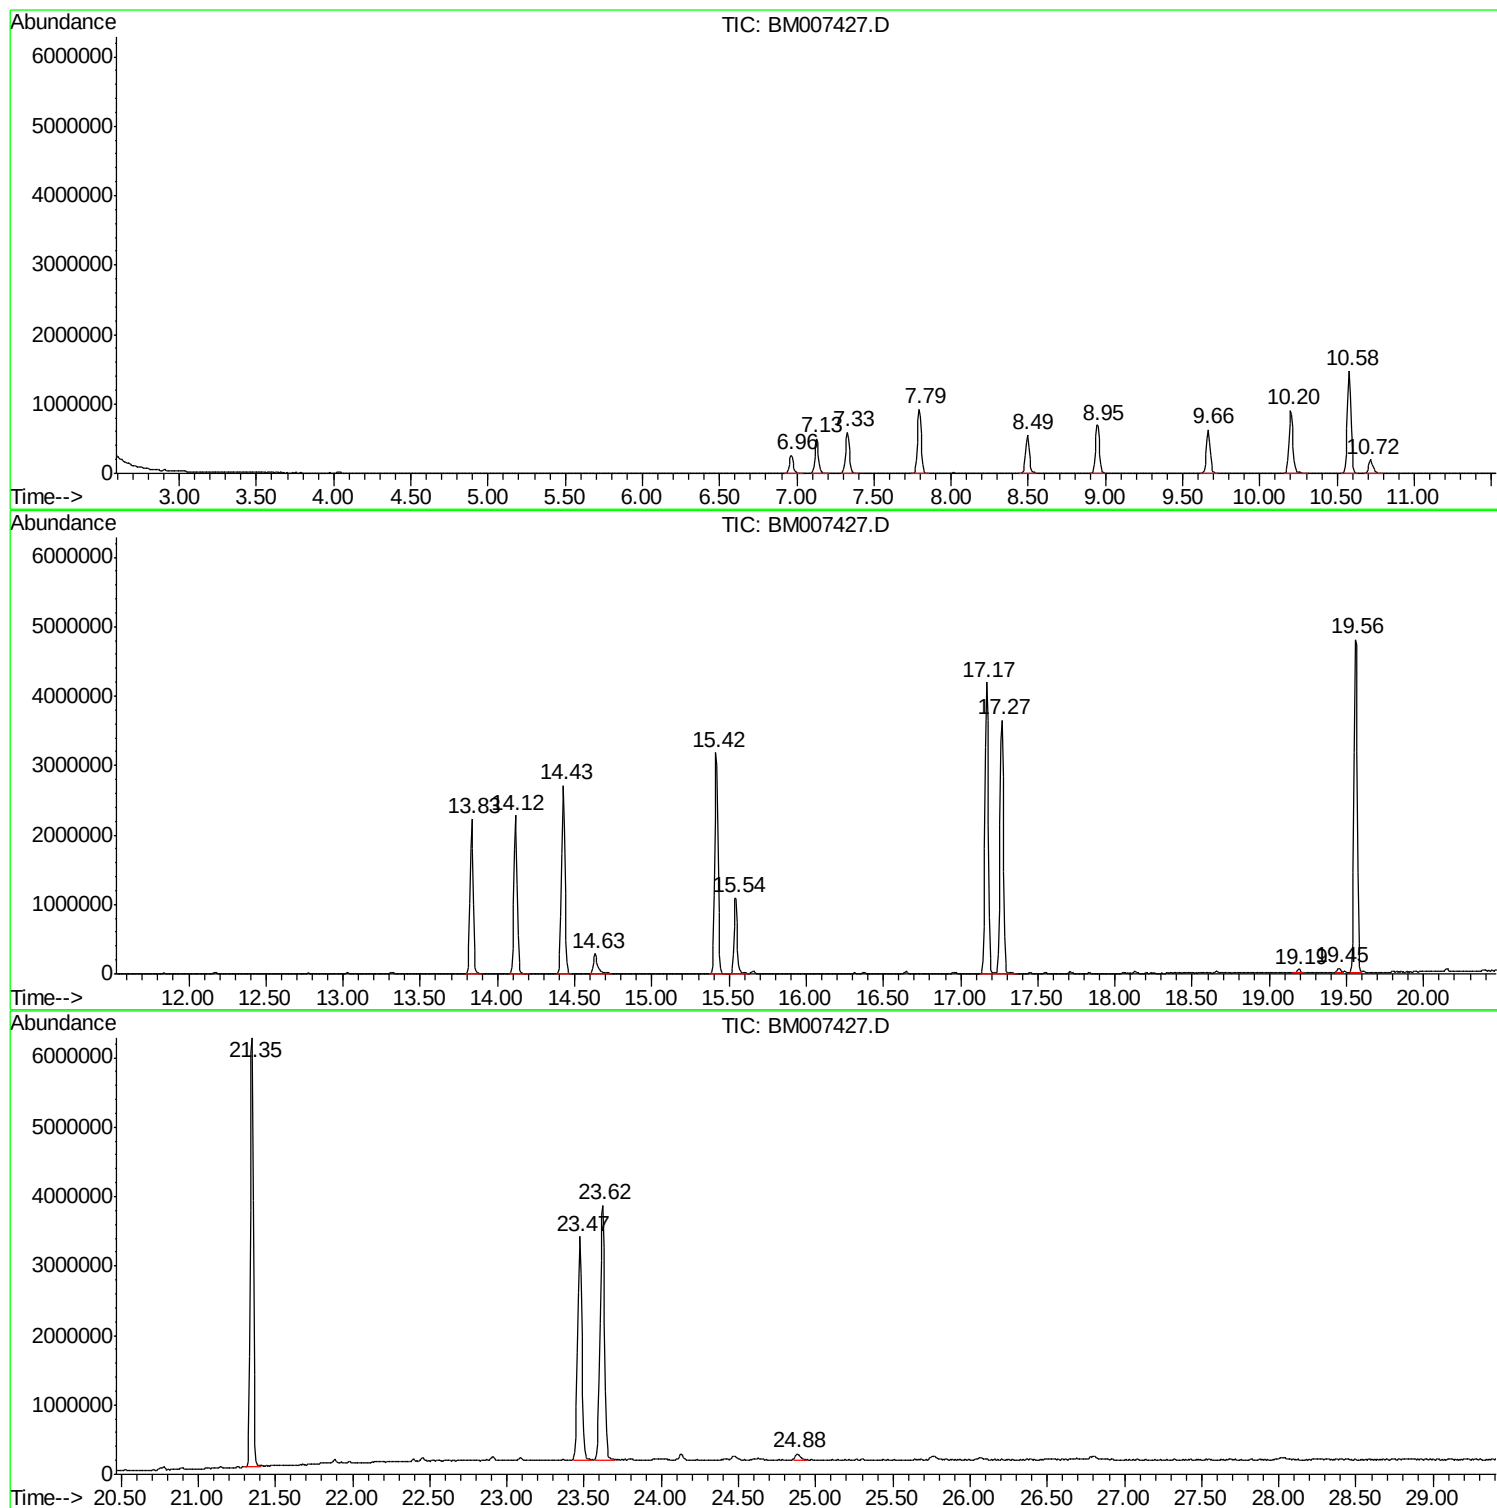

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007427.D
Acq On : 06 Sep 2016 23:06
Operator : UM/SJ
Sample : H4674-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0041

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090616\
Data File : BM007427.D
Acq On : 06 Sep 2016 23:06
Operator : UM/SJ
Sample : H4674-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0041

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc