
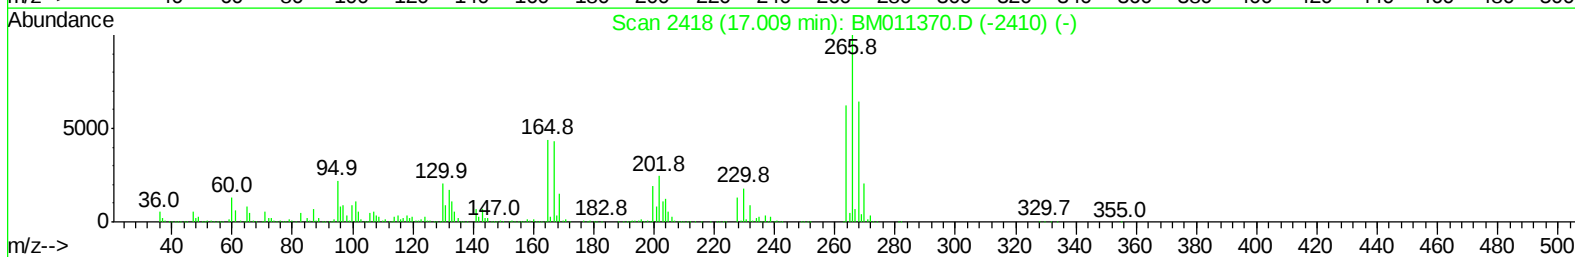
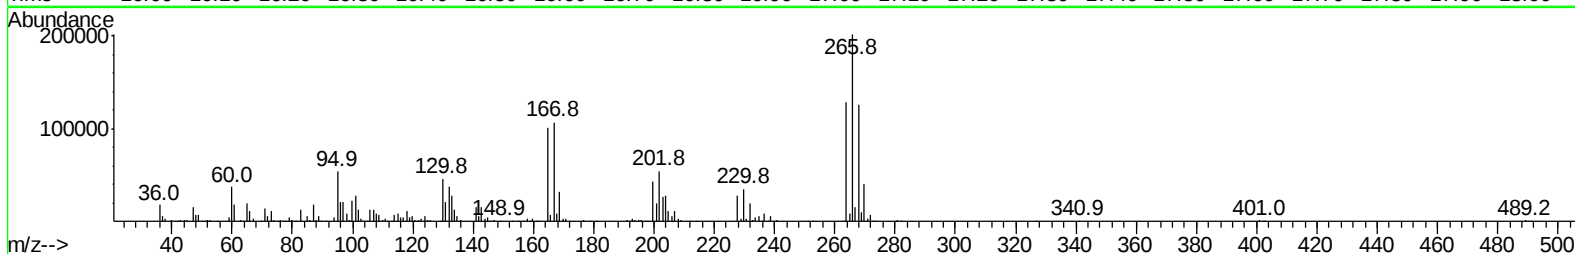


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090617\
Data File : BM011450.D
Acq On : 06 Sep 2017 09:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:57:59 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

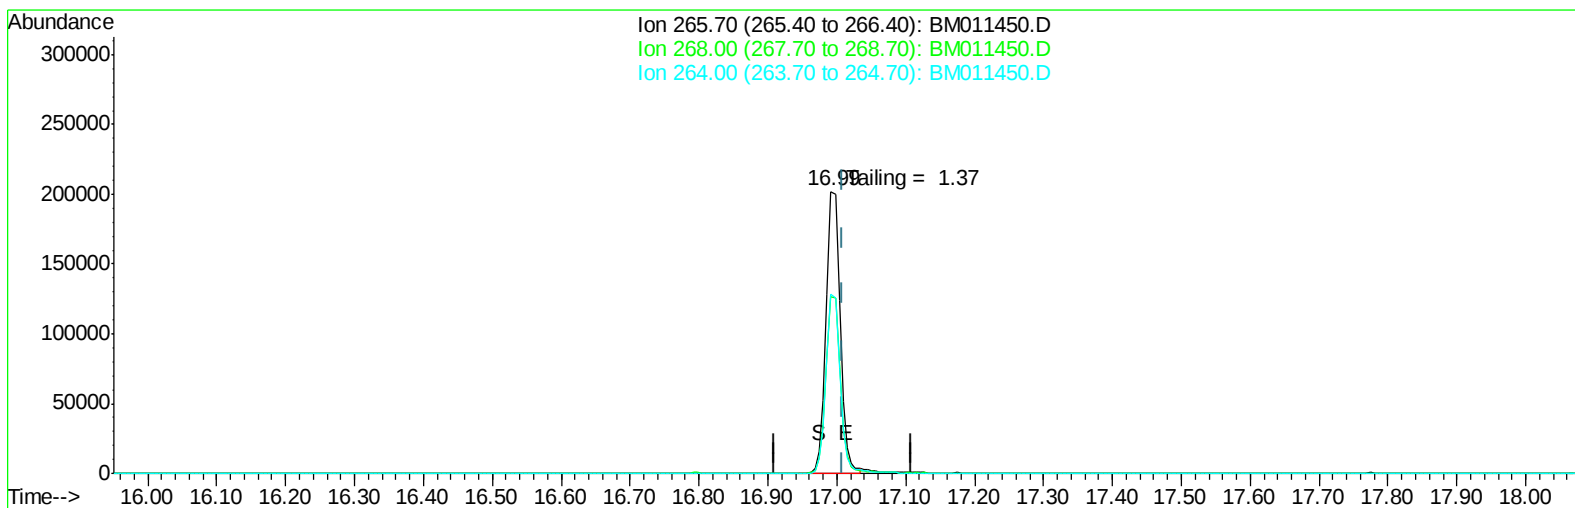

TIC: BM011450.D

(69) Pentachlorophenol (C)




16.992min (-0.018) 30861.06ng

response 290905

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.68
264.00	61.20	63.77
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090617\
Data File : BM011450.D
Acq On : 06 Sep 2017 09:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:57:59 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

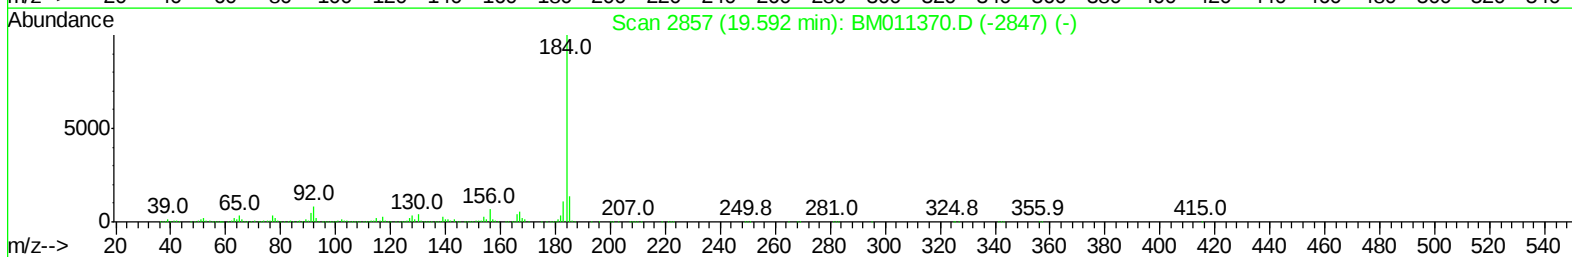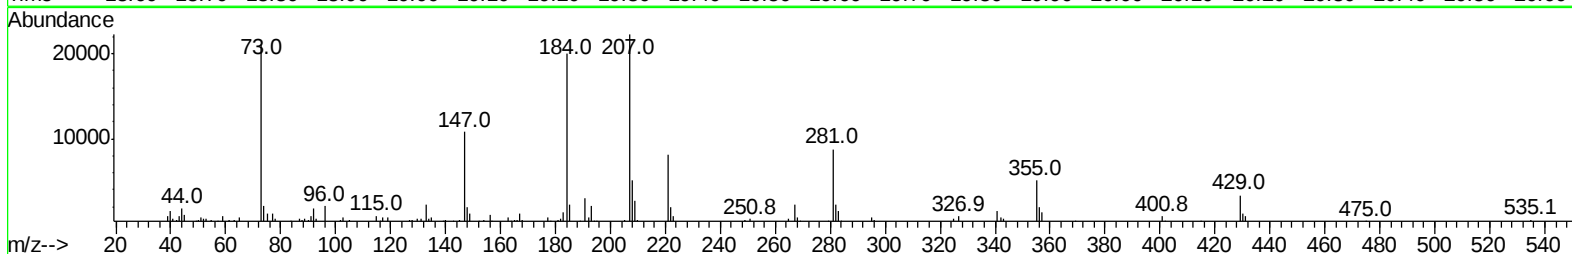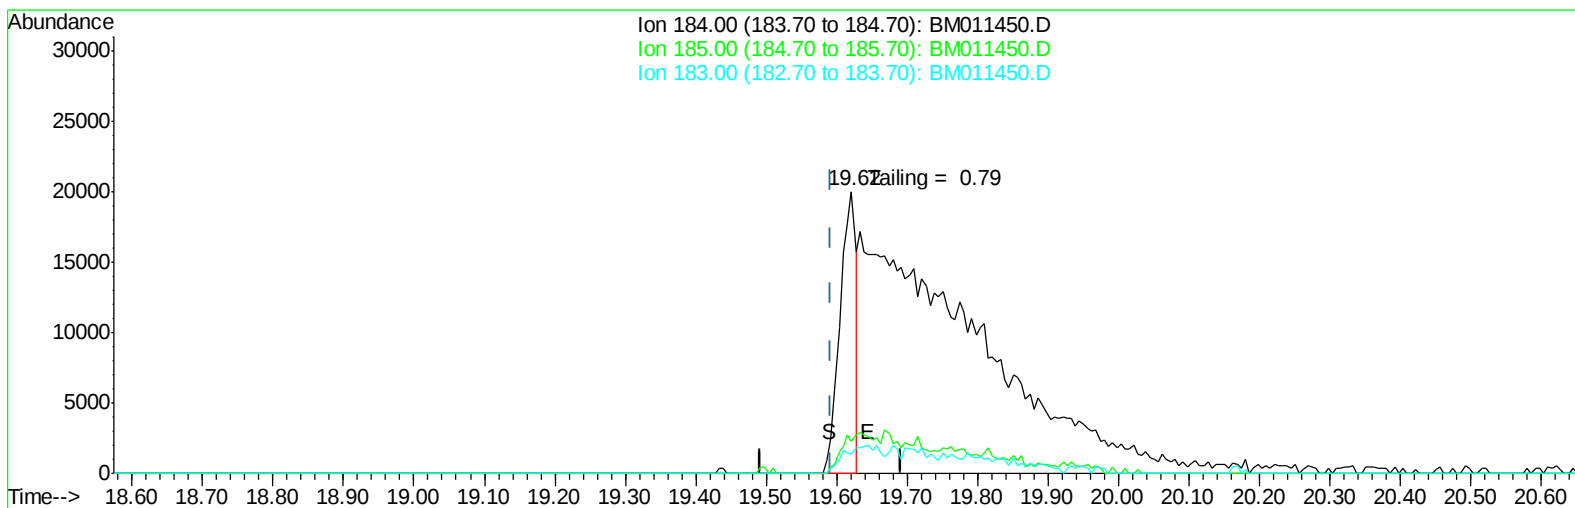

TIC: BM011450.D

(76) Benzidine

19.621min (+0.029) 173.66ng

response 53906

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	11.60
183.00	11.10	6.70#
0.00	0.00	0.00