


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM090617\
 Data File : BM011450.D
 Acq On : 06 Sep 2017 09:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 31 18:39:59 2017

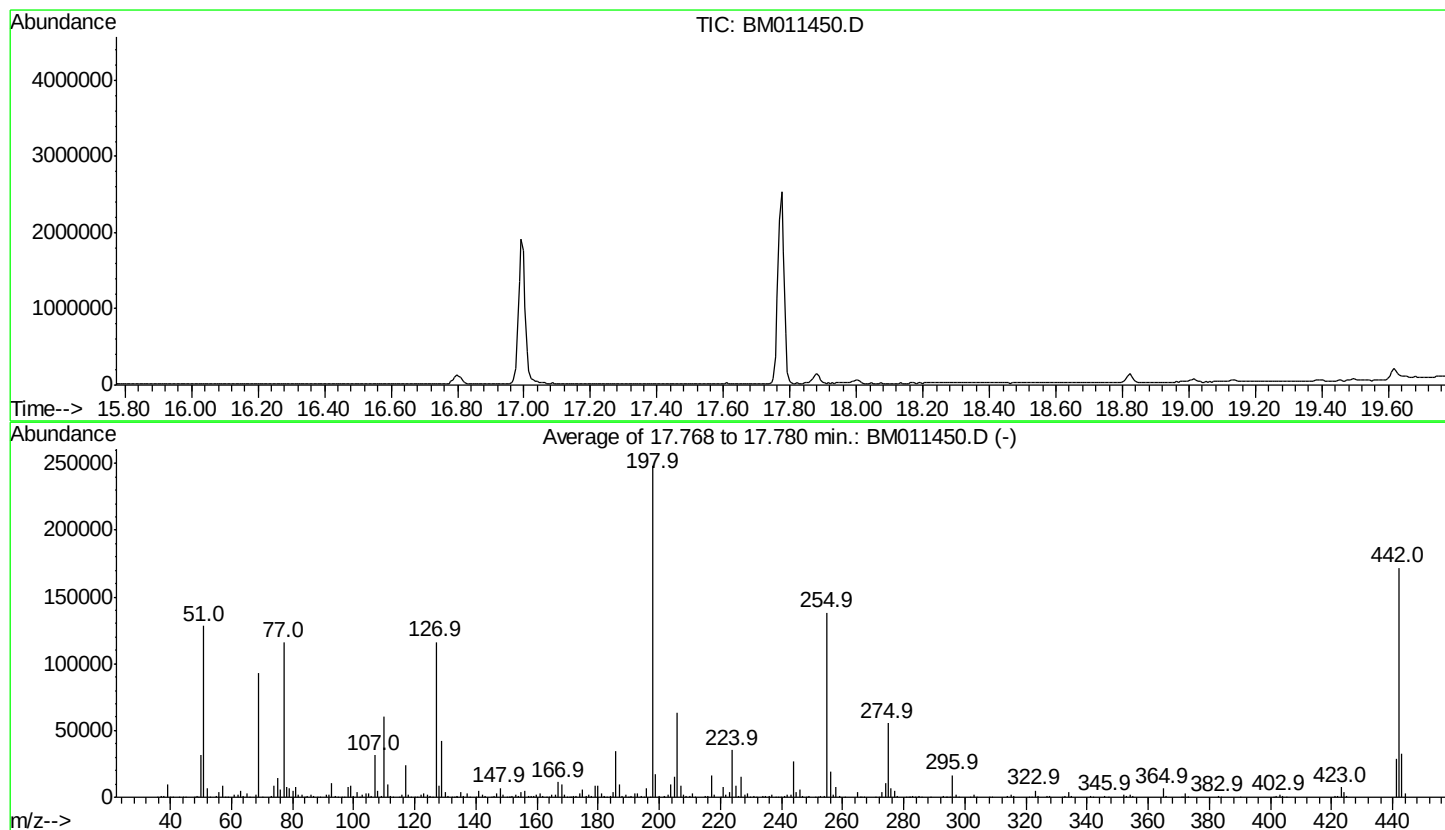

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	128390	PASS
68	69	0.00	2	1.6	1517	PASS
69	198	0.00	100	37.3	92672	PASS
70	69	0.00	2	0.3	322	PASS
127	198	10	80	46.8	116272	PASS
197	198	0.00	2	0.1	340	PASS
198	198	100	100	100.0	248405	PASS
199	198	5	9	7.0	17266	PASS
275	198	10	60	22.4	55525	PASS
365	198	1	100	2.6	6492	PASS
441	443	0.01	100	88.6	28650	PASS
442	198	50	100	69.1	171669	PASS
443	442	15	24	18.8	32328	PASS