
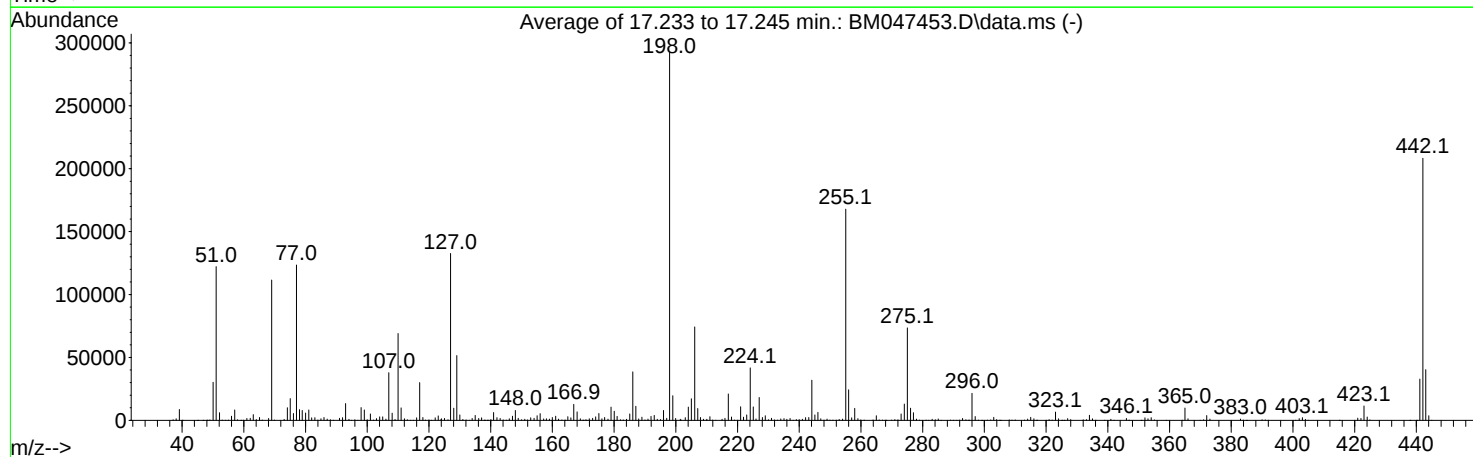


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090624\
Data File : BM047453.D
Acq On : 06 Sep 2024 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 07 01:23:53 2024

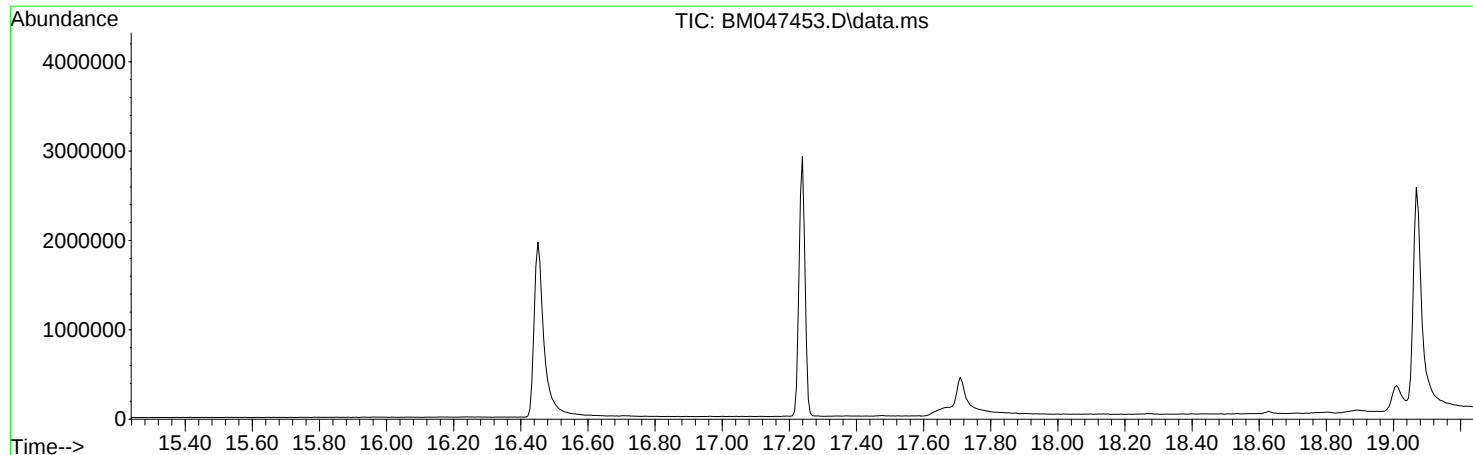

AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	122255	PASS
68	69	0.00	2	1.4	1582	PASS
69	198	0.00	100	38.2	111553	PASS
70	69	0.00	2	0.2	230	PASS
127	198	10	80	45.4	132616	PASS
197	198	0.00	2	0.6	1625	PASS
198	198	100	100	100.0	292331	PASS
199	198	5	9	6.7	19602	PASS
275	198	10	60	25.1	73507	PASS
365	198	1	100	3.4	9826	PASS
441	198	0.01	100	11.2	32840	PASS
442	442	50	100	100.0	208341	PASS
443	442	15	24	19.3	40304	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/6/2024	BNA_M	<u>BM047453.D</u>
Compound Name	Response	Retention Time
DDT	940733	20.303
DDD	19507	19.903
DDE	4071	19.35
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23578	964311	2.45

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090624\
Data File : BM047453.D
Acq On : 06 Sep 2024 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 07 01:34:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 07 01:23:53 2024
Response via : Initial Calibration

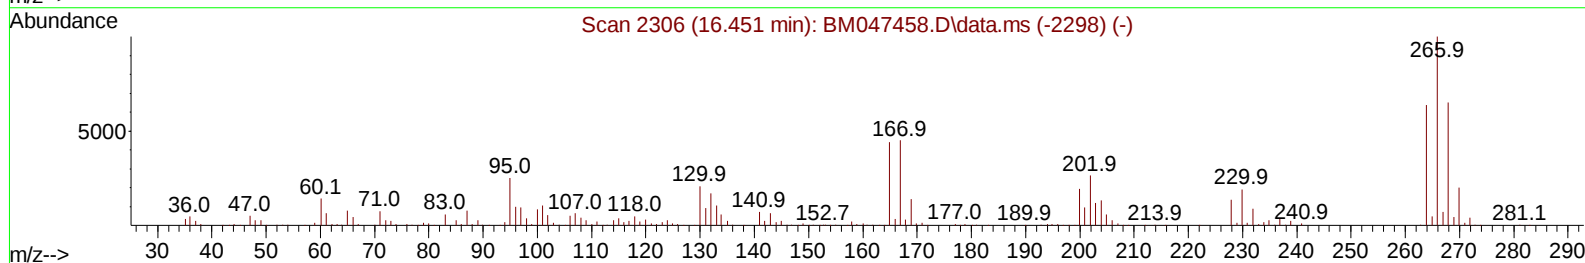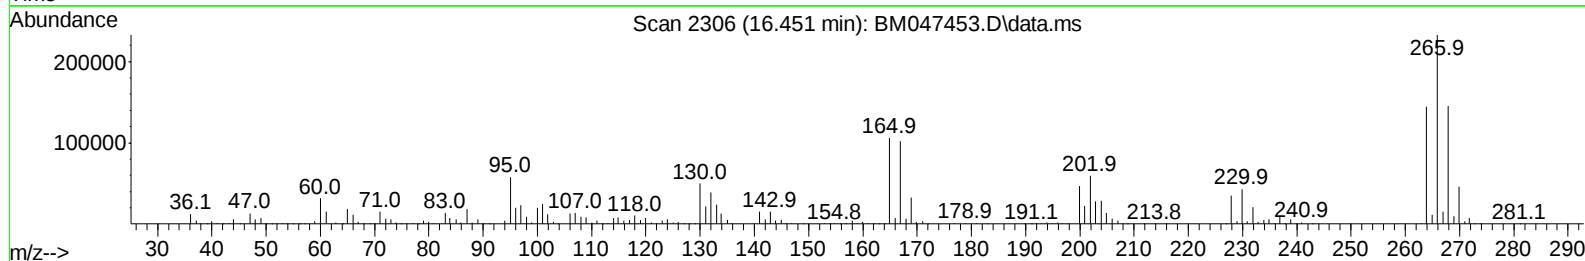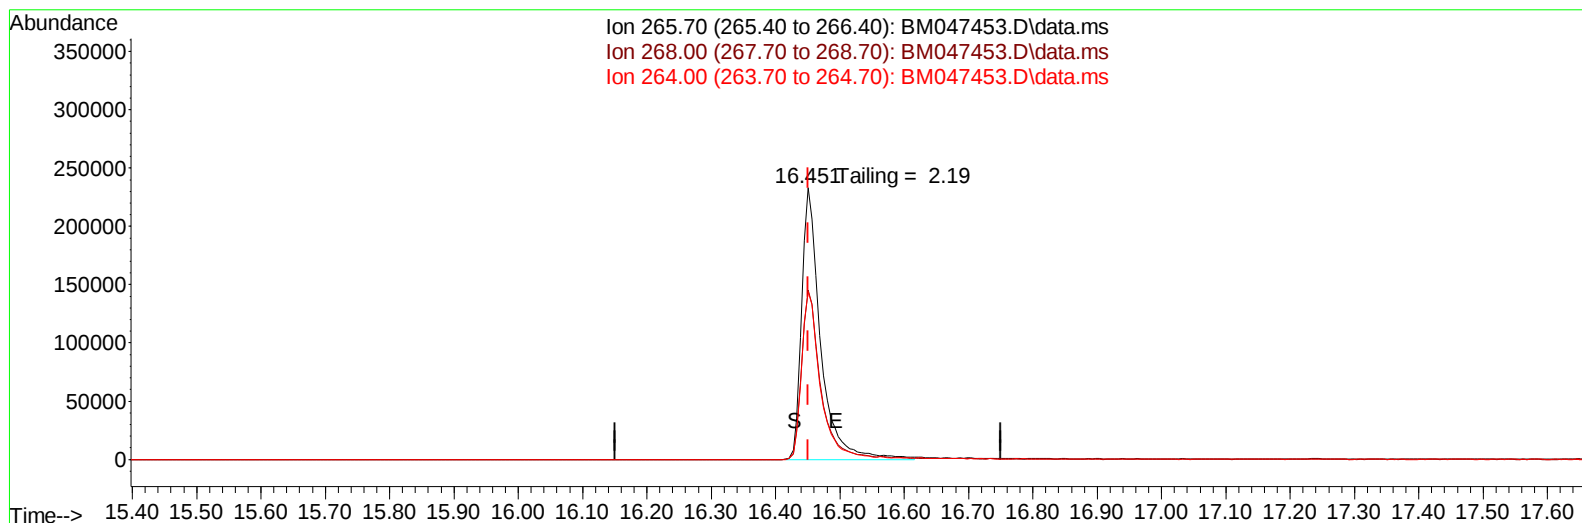

TIC: BM047453.D\data.ms

(70) Pentachlorophenol (C)

16.451min (+ 0.000) 0.00 ng




response 478780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.34
264.00	63.80	61.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090624\
Data File : BM047453.D
Acq On : 06 Sep 2024 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 07 01:34:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 07 01:23:53 2024
Response via : Initial Calibration

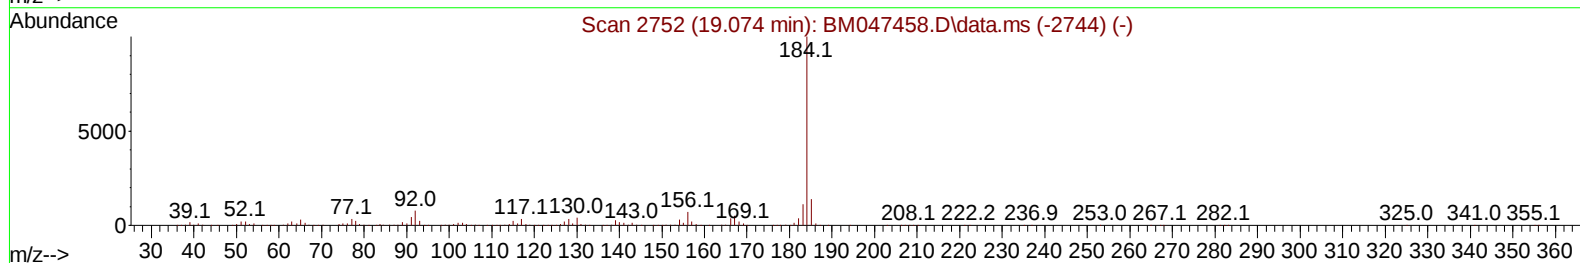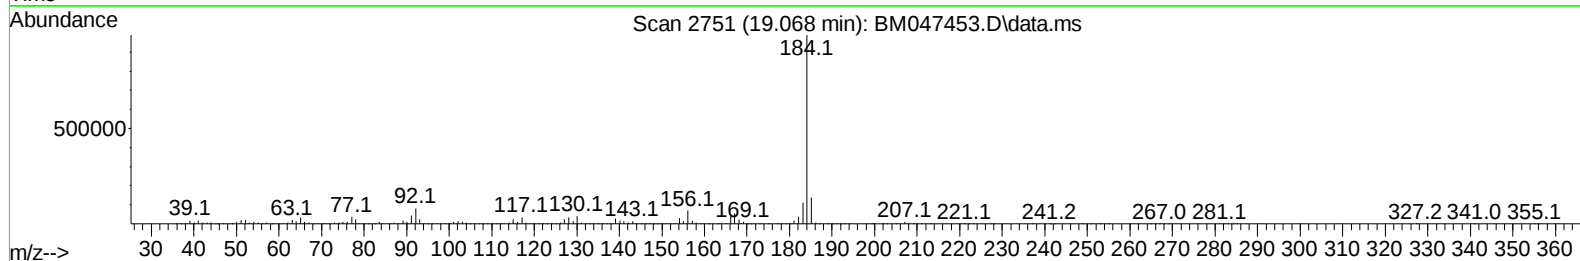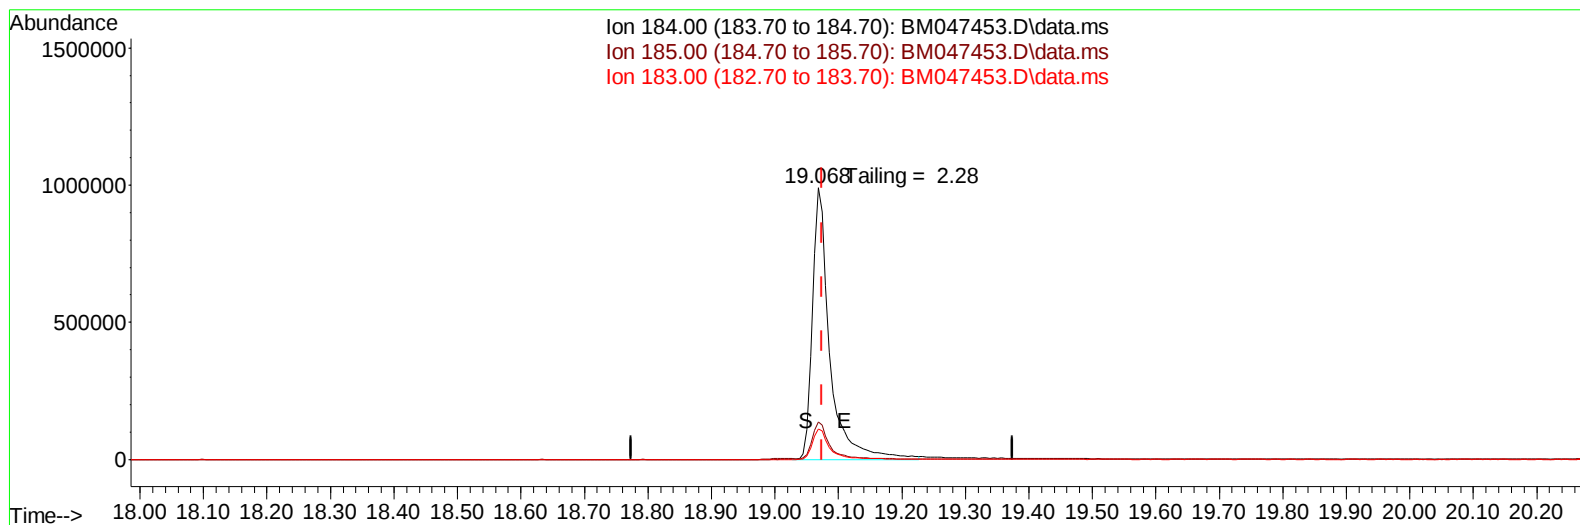

TIC: BM047453.D\data.ms

(77) Benzidine

19.068min (-0.006) 30509.70 ng

response 1910260

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.79
183.00	11.10	11.29
0.00	0.00	0.00