
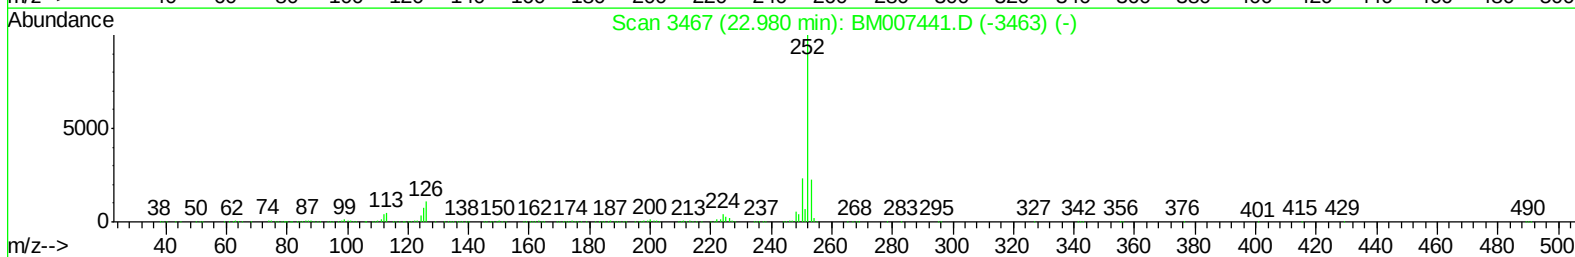
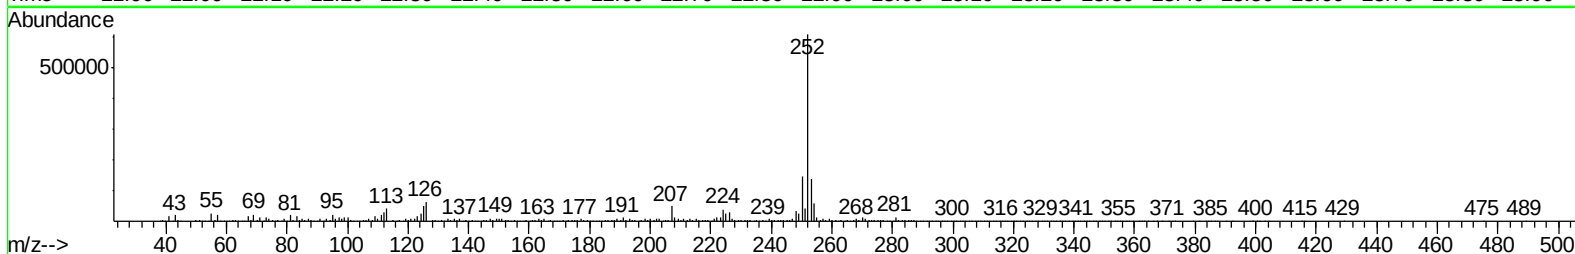


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007449.D
Acq On : 07 Sep 2016 21:18
Operator : UM/SJ
Sample : H4666-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Sep 08 04:43:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

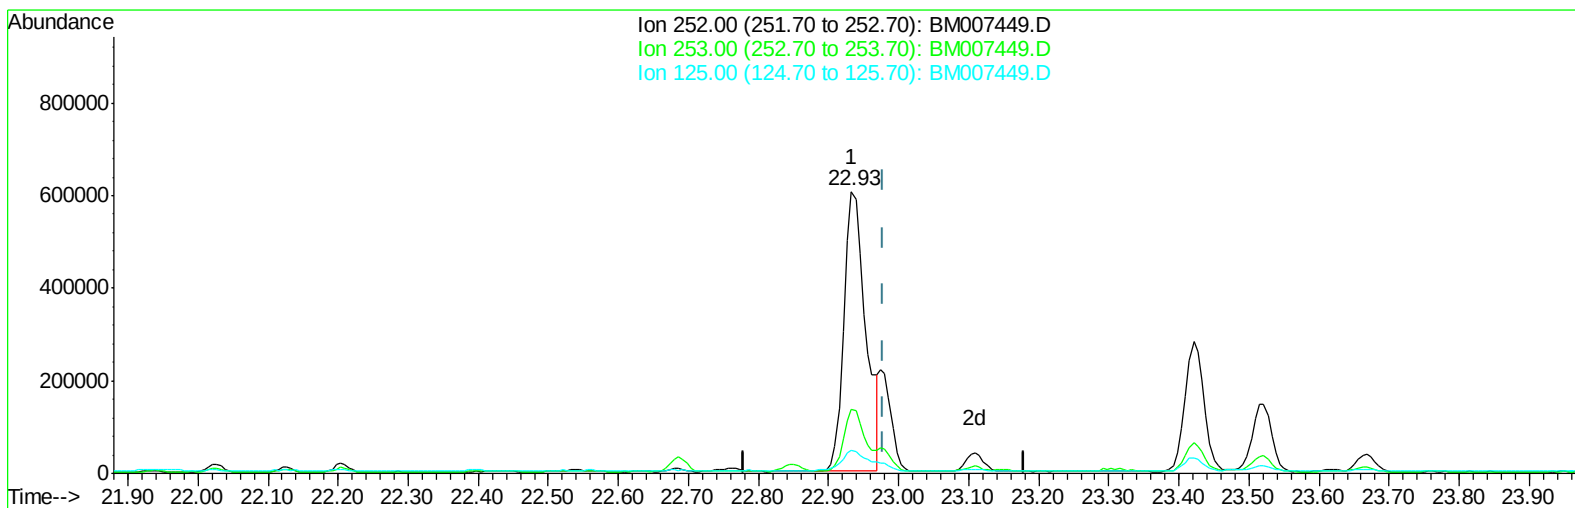

TIC: BM007449.D

(86) Benzo(k)fluoranthene

22.933min (-0.047) 9.29ng/ul

response 1296086

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	22.67
125.00	7.10	8.11
0.00	0.00	0.00