
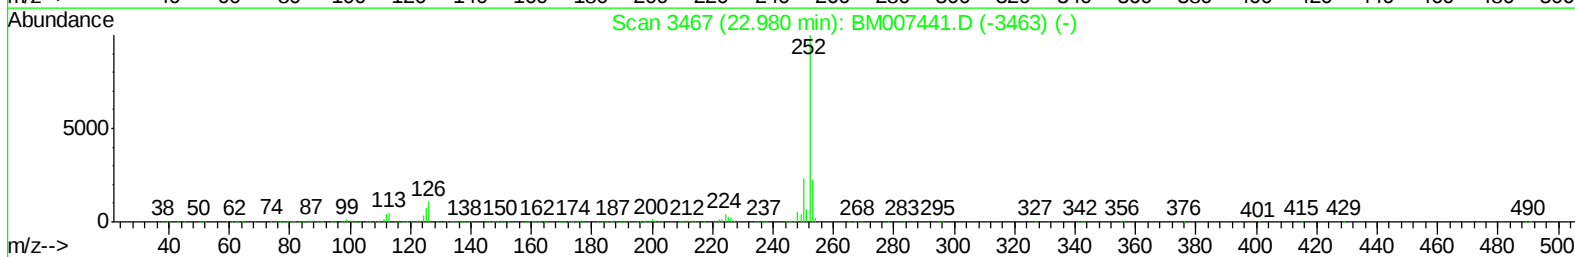
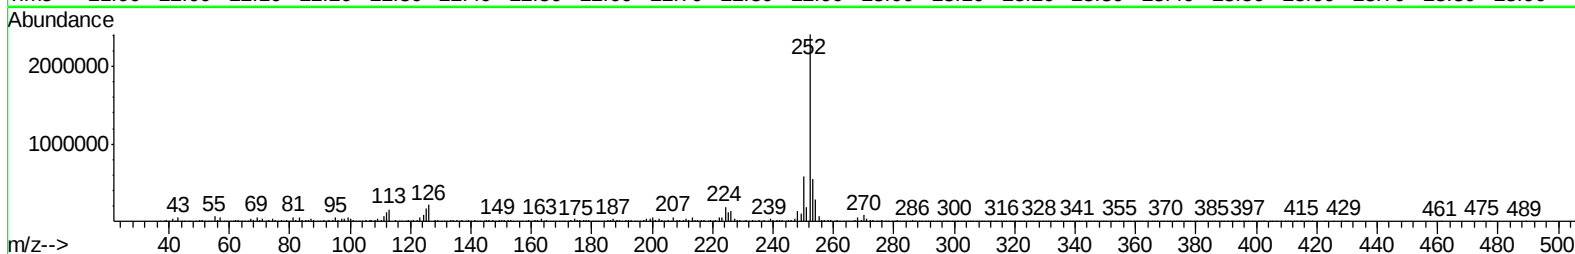


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007451.D
Acq On : 07 Sep 2016 22:30
Operator : UM/SJ
Sample : H4666-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Sep 08 03:13:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

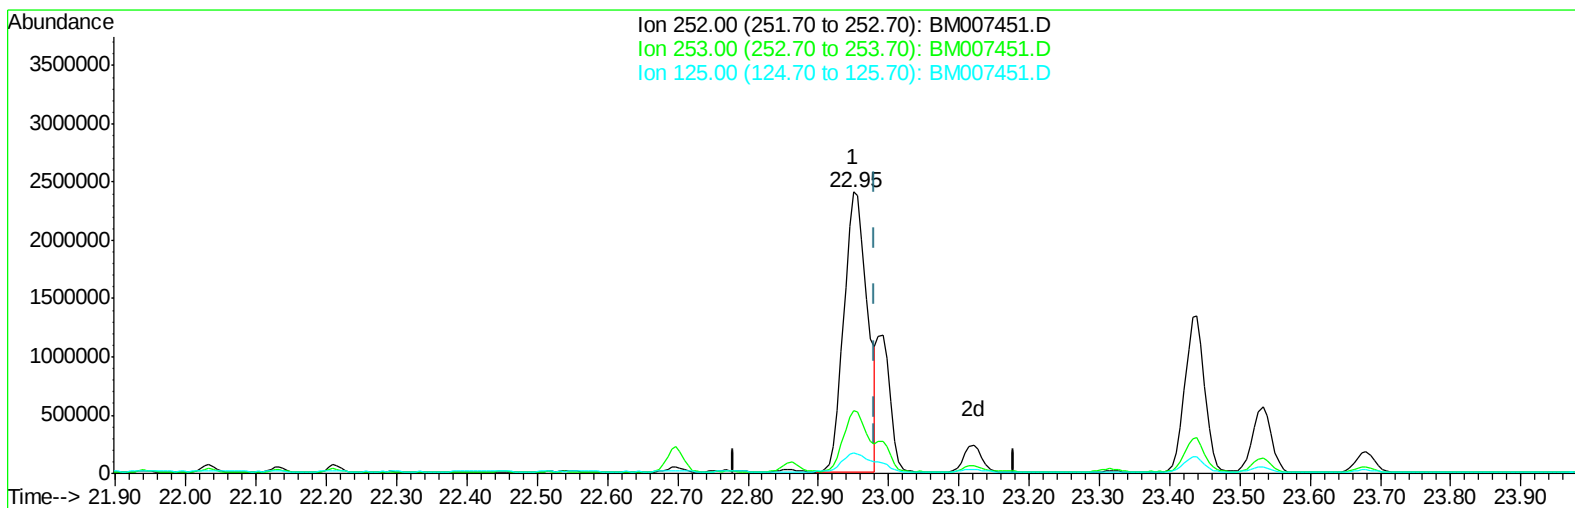

TIC: BM007451.D

(86) Benzo(k)fluoranthene

22.950min (-0.029) 50.87ng/ul

response 5640118

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	22.50
125.00	7.10	7.16
0.00	0.00	0.00