
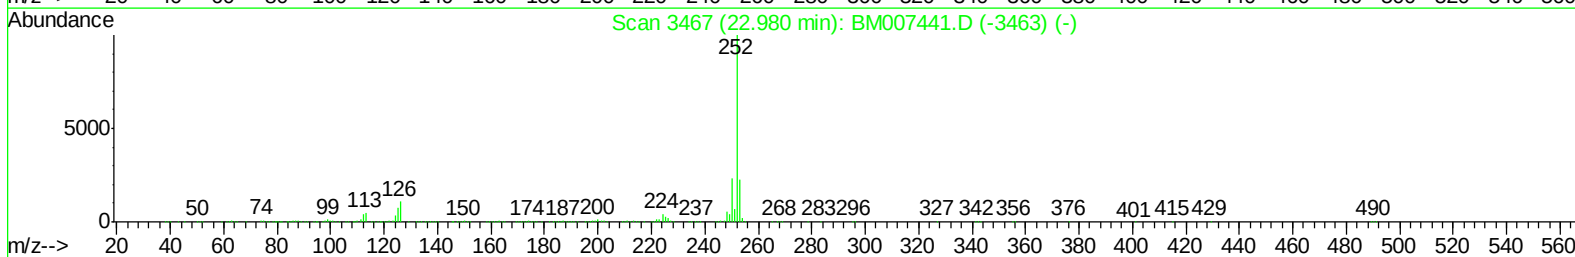
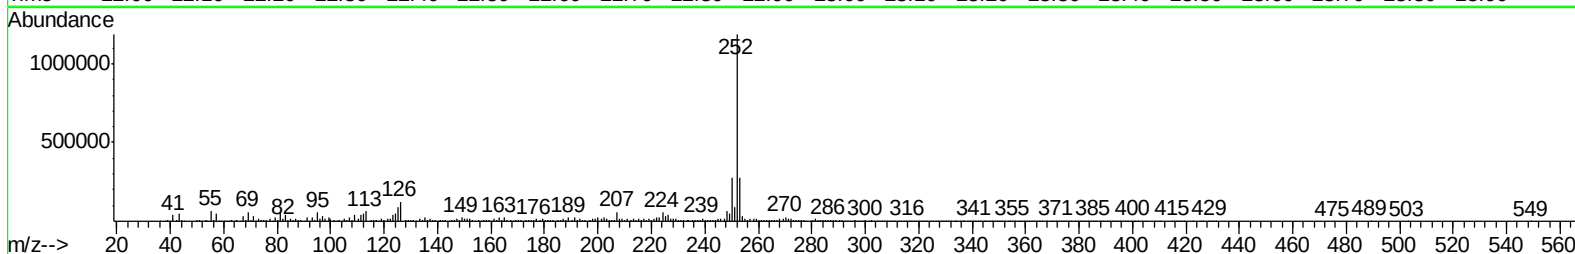


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007451.D
Acq On : 07 Sep 2016 22:30
Operator : UM/SJ
Sample : H4666-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Sep 08 03:13:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

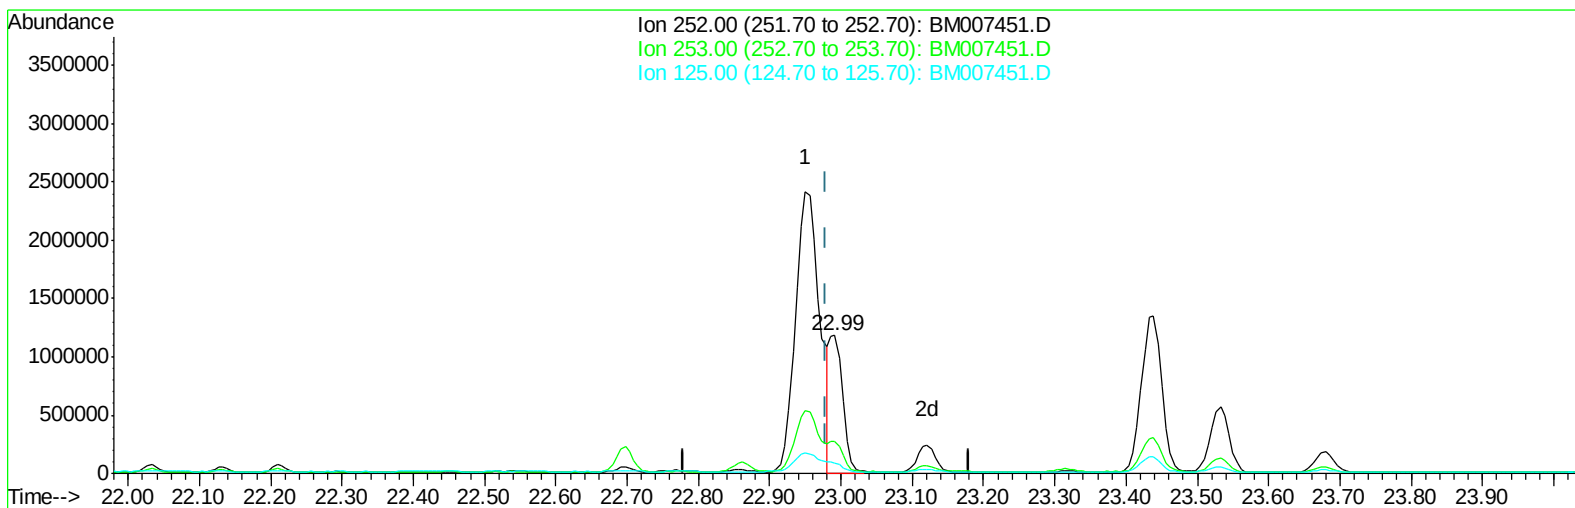

TIC: BM007451.D

(86) Benzo(k)fluoranthene

22.991min (+0.012) 14.10ng/ul m

response 1562640

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	23.37
125.00	7.10	7.90
0.00	0.00	0.00