
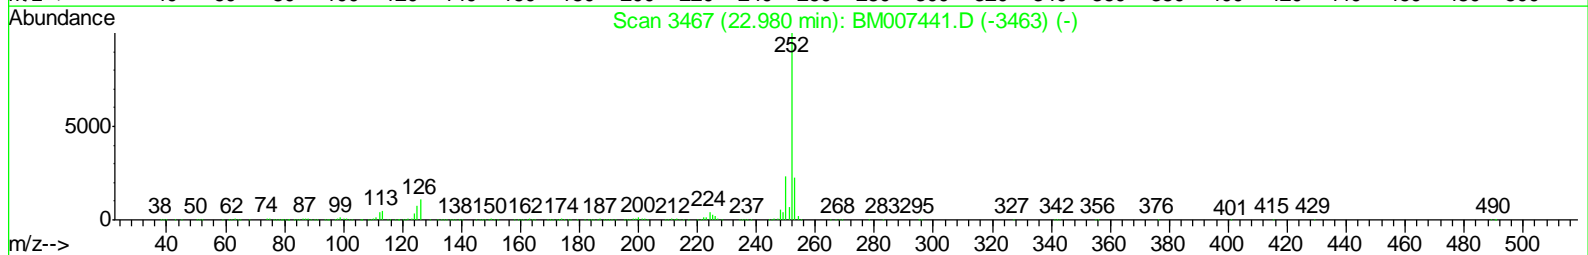
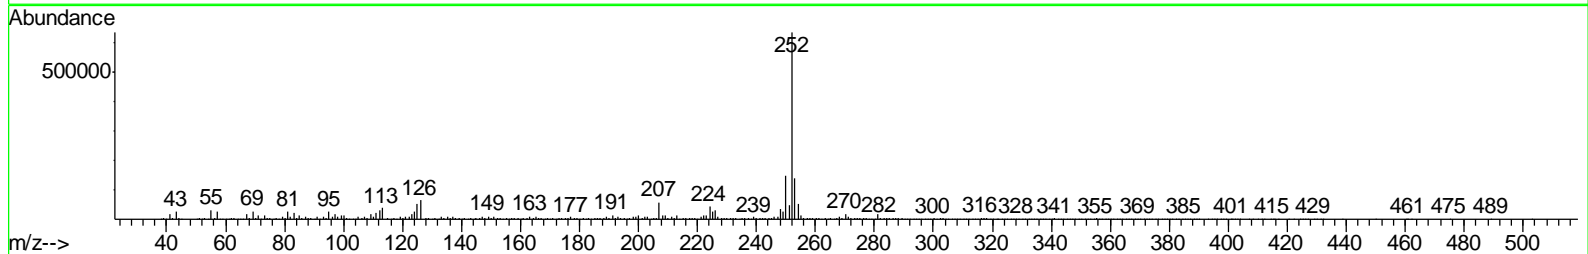


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
 Data File : BM007452.D
 Acq On : 07 Sep 2016 23:06
 Operator : UM/SJ
 Sample : H4666-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 08 03:13:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 08 03:10:54 2016
 Response via : Initial Calibration

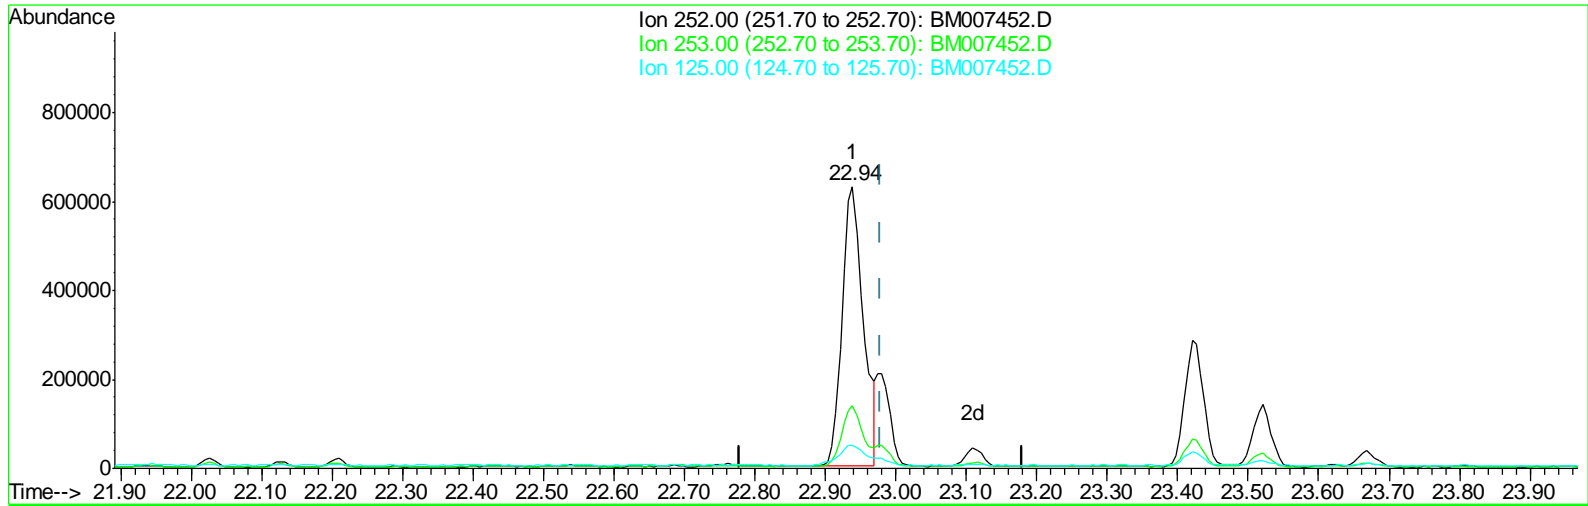

TIC: BM007452.D

(86) Benzo(k)fluoranthene
 22.939min (-0.041) 10.77ng/ul
 response 1297841

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	22.31
125.00	7.10	8.31
0.00	0.00	0.00