
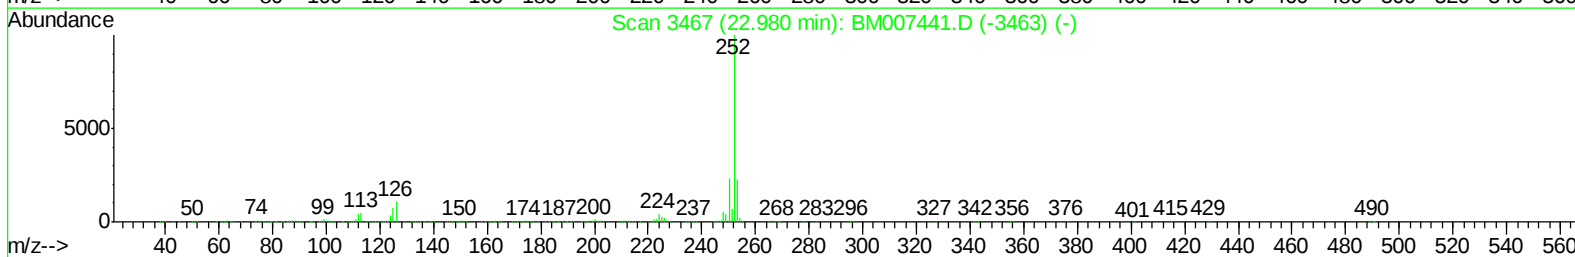
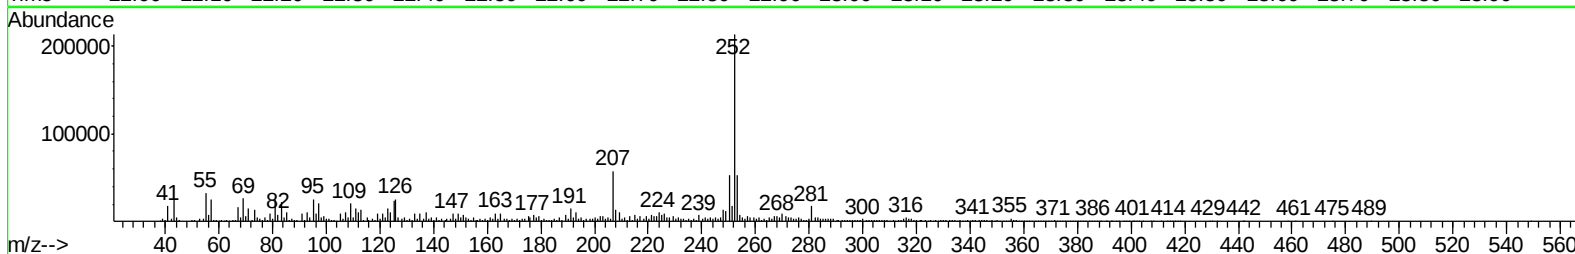


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007452.D
Acq On : 07 Sep 2016 23:06
Operator : UM/SJ
Sample : H4666-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 08 03:13:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

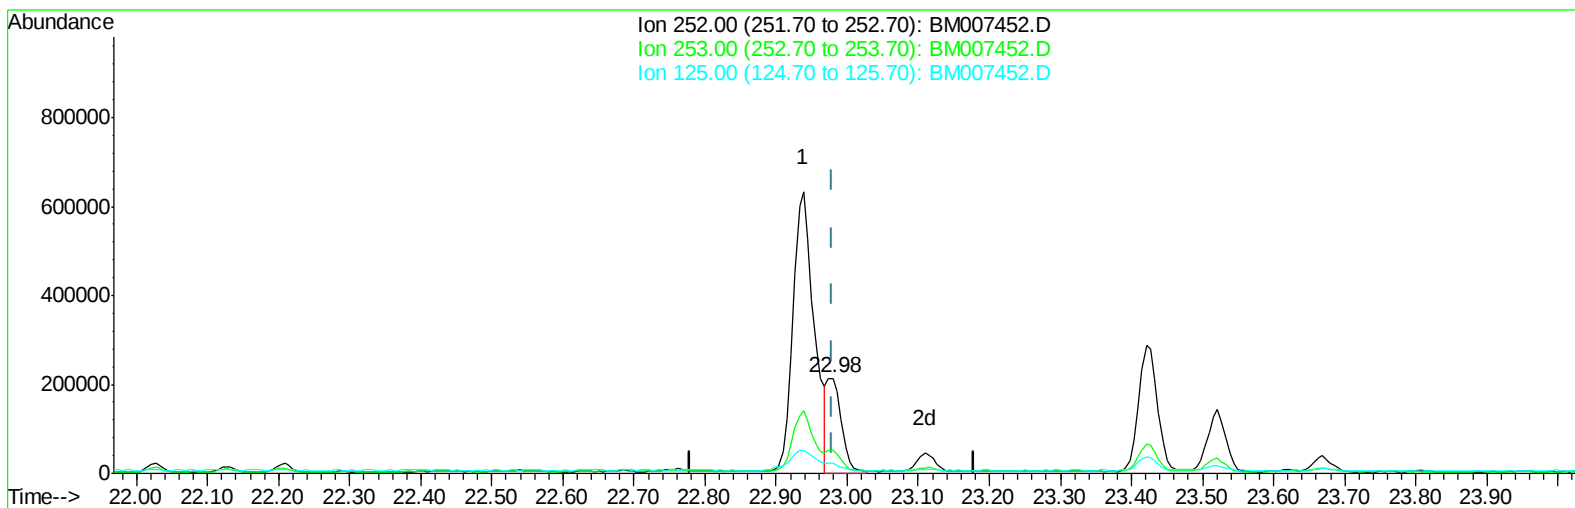

TIC: BM007452.D

(86) Benzo(k)fluoranthene

22.980min (+0.000) 2.47ng/ul m

response 297802

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	24.50
125.00	7.10	10.77#
0.00	0.00	0.00