
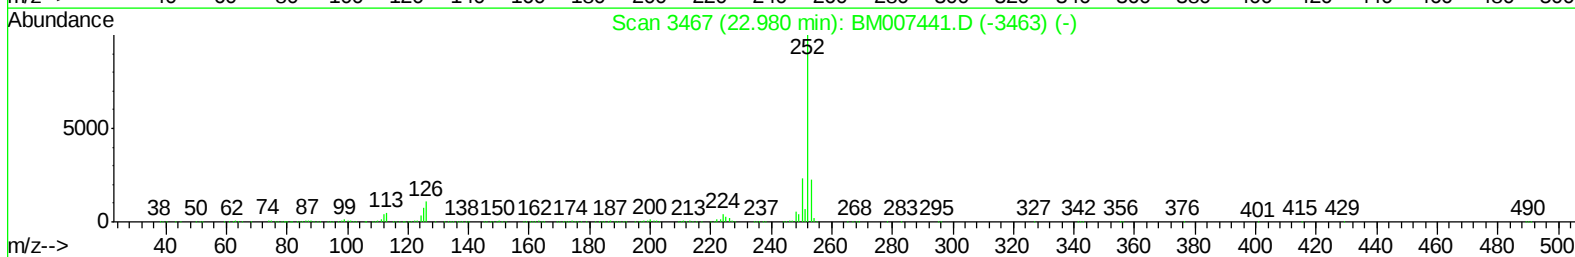
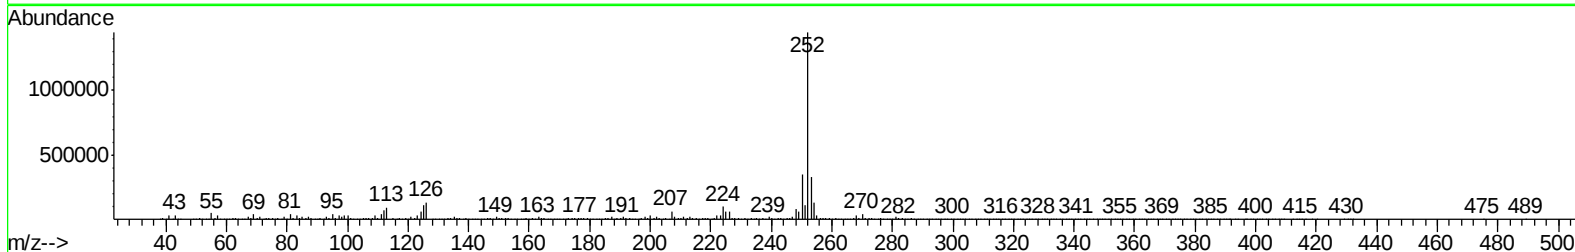


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007455.D
Acq On : 08 Sep 2016 00:54
Operator : UM/SJ
Sample : H4666-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Sep 08 03:14:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

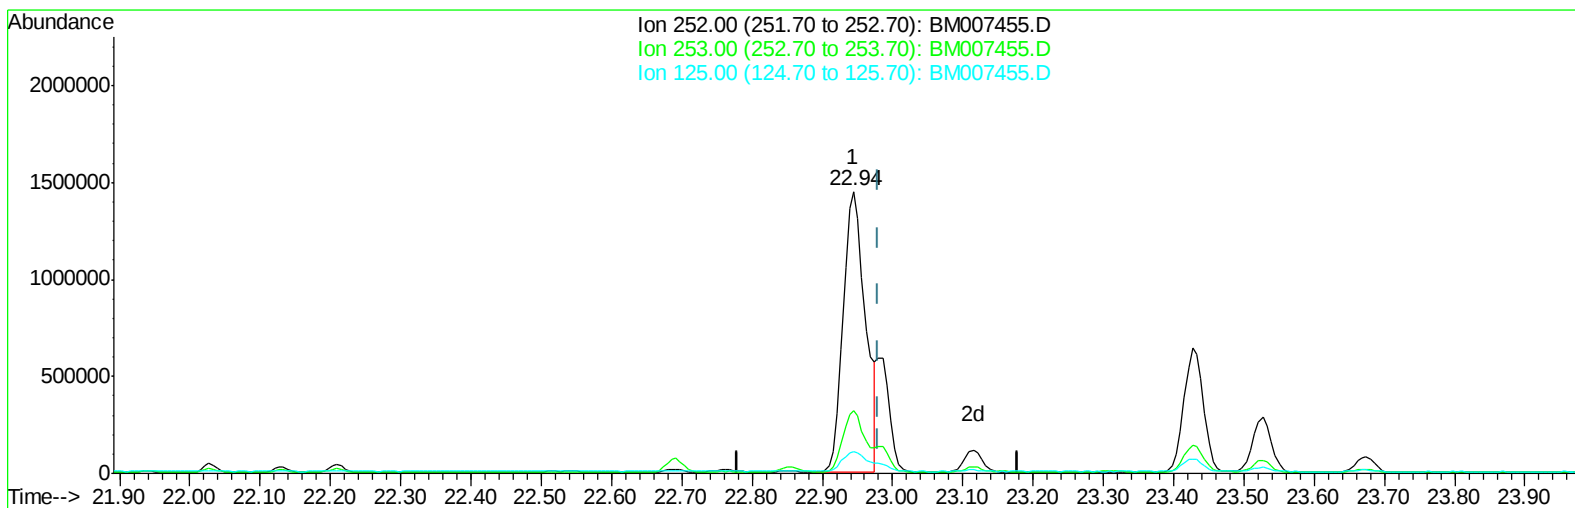

TIC: BM007455.D

(86) Benzo(k)fluoranthene

22.944min (-0.035) 30.35ng/ul

response 3217324

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	22.46
125.00	7.10	7.71
0.00	0.00	0.00