
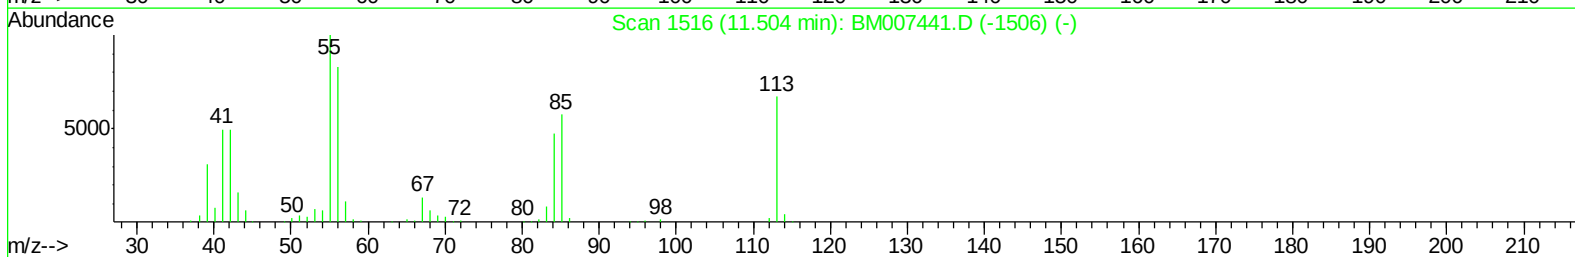
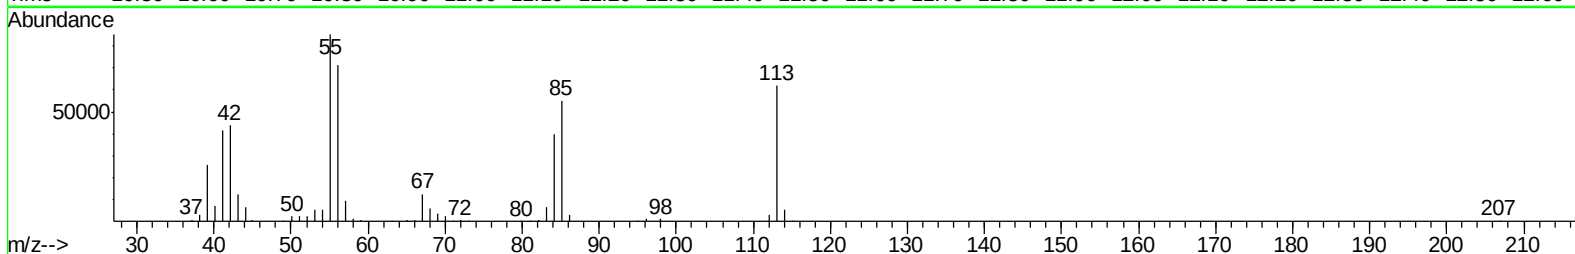


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007456.D
Acq On : 08 Sep 2016 01:31
Operator : UM/SJ
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 08 06:40:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

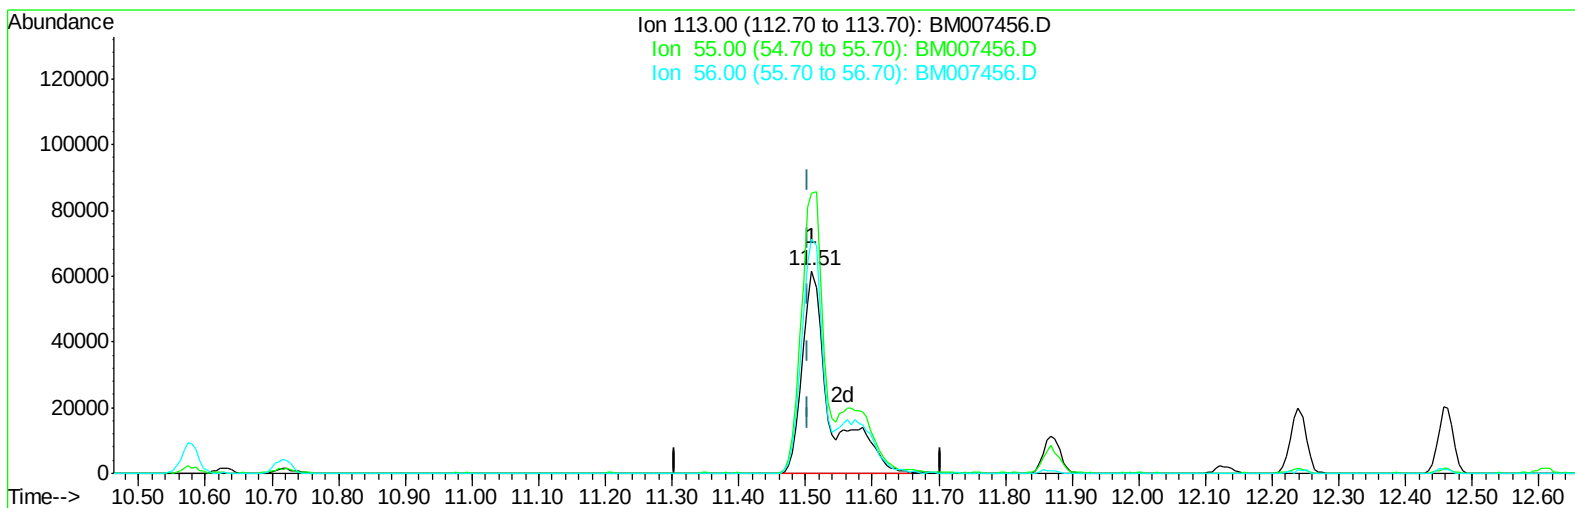

TIC: BM007456.D

(32) Caprolactam

11.510min (+0.006) 18.81ng/ul m

response 179060

Ion	Exp%	Act%
113.00	100	100
55.00	152.40	138.13
56.00	121.70	115.63
0.00	0.00	0.00