

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
 Data File : BM007450.D
 Acq On : 07 Sep 2016 21:54
 Operator : UM/SJ
 Sample : H4666-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD399

Quant Time: Sep 08 03:13:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 08 03:10:54 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	278230	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1369589	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	938394	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	2307174	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2832753	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	2578886	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	16030	2.94	ng/uL	0.00
5) Phenol-d5	6.96	99	419689	15.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	230933	16.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	320940	16.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	362796	15.83	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	173370	17.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	204684	17.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	398039	17.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	170515	5.85	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1378604	17.03	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1684114	17.95	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	175540	11.49	ng/ul	0.00
57) Fluorene-d10	15.42	176	1233896	17.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	220612	15.21	ng/ul	0.00
70) Anthracene-d10	17.26	188	1998635	18.54	ng/ul	0.00
76) Pyrene-d10	19.56	212	2406375	20.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	2145622	18.06	ng/ul	0.00

Target Compounds


					Qvalue
6) Phenol	6.99	94	38844	1.42 ng/ul	91
28) Naphthalene	10.63	128	192964	2.83 ng/ul	98
34) 2-Methylnaphthalene	12.24	142	174639	3.13 ng/ul	97
44) Dimethylphthalate	13.88	163	906253	11.24 ng/ul	100
53) Dibenzofuran	14.82	168	173916	1.85 ng/ul	94
69) Phenanthrene	17.21	178	904426	7.30 ng/ul	99
71) Anthracene	17.30	178	144964	1.13 ng/ul	99
74) Fluoranthene	19.22	202	1205256	7.75 ng/ul	98
77) Pyrene	19.59	202	949705	6.25 ng/ul	99
80) Benzo(a)anthracene	21.39	228	885352	5.30 ng/ul	95
82) Chrysene	21.39	228	883062	5.84 ng/ul	97
85) Benzo(b)fluoranthene	22.93	252	1306266	8.57 ng/ul	98
86) Benzo(k)fluoranthene	22.93	252	1306266	9.27 ng/ul	98
88) Benzo(a)pyrene	23.52	252	322507	2.21 ng/ul#	97
89) Indeno(1,2,3-cd)pyrene	25.90	276	244591	1.37 ng/ul	99
91) Benzo(g,h,i)perylene	26.60	276	196807	1.29 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007450.D
Acq On : 07 Sep 2016 21:54
Operator : UM/SJ
Sample : H4666-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD399

Quant Time: Sep 08 03:13:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

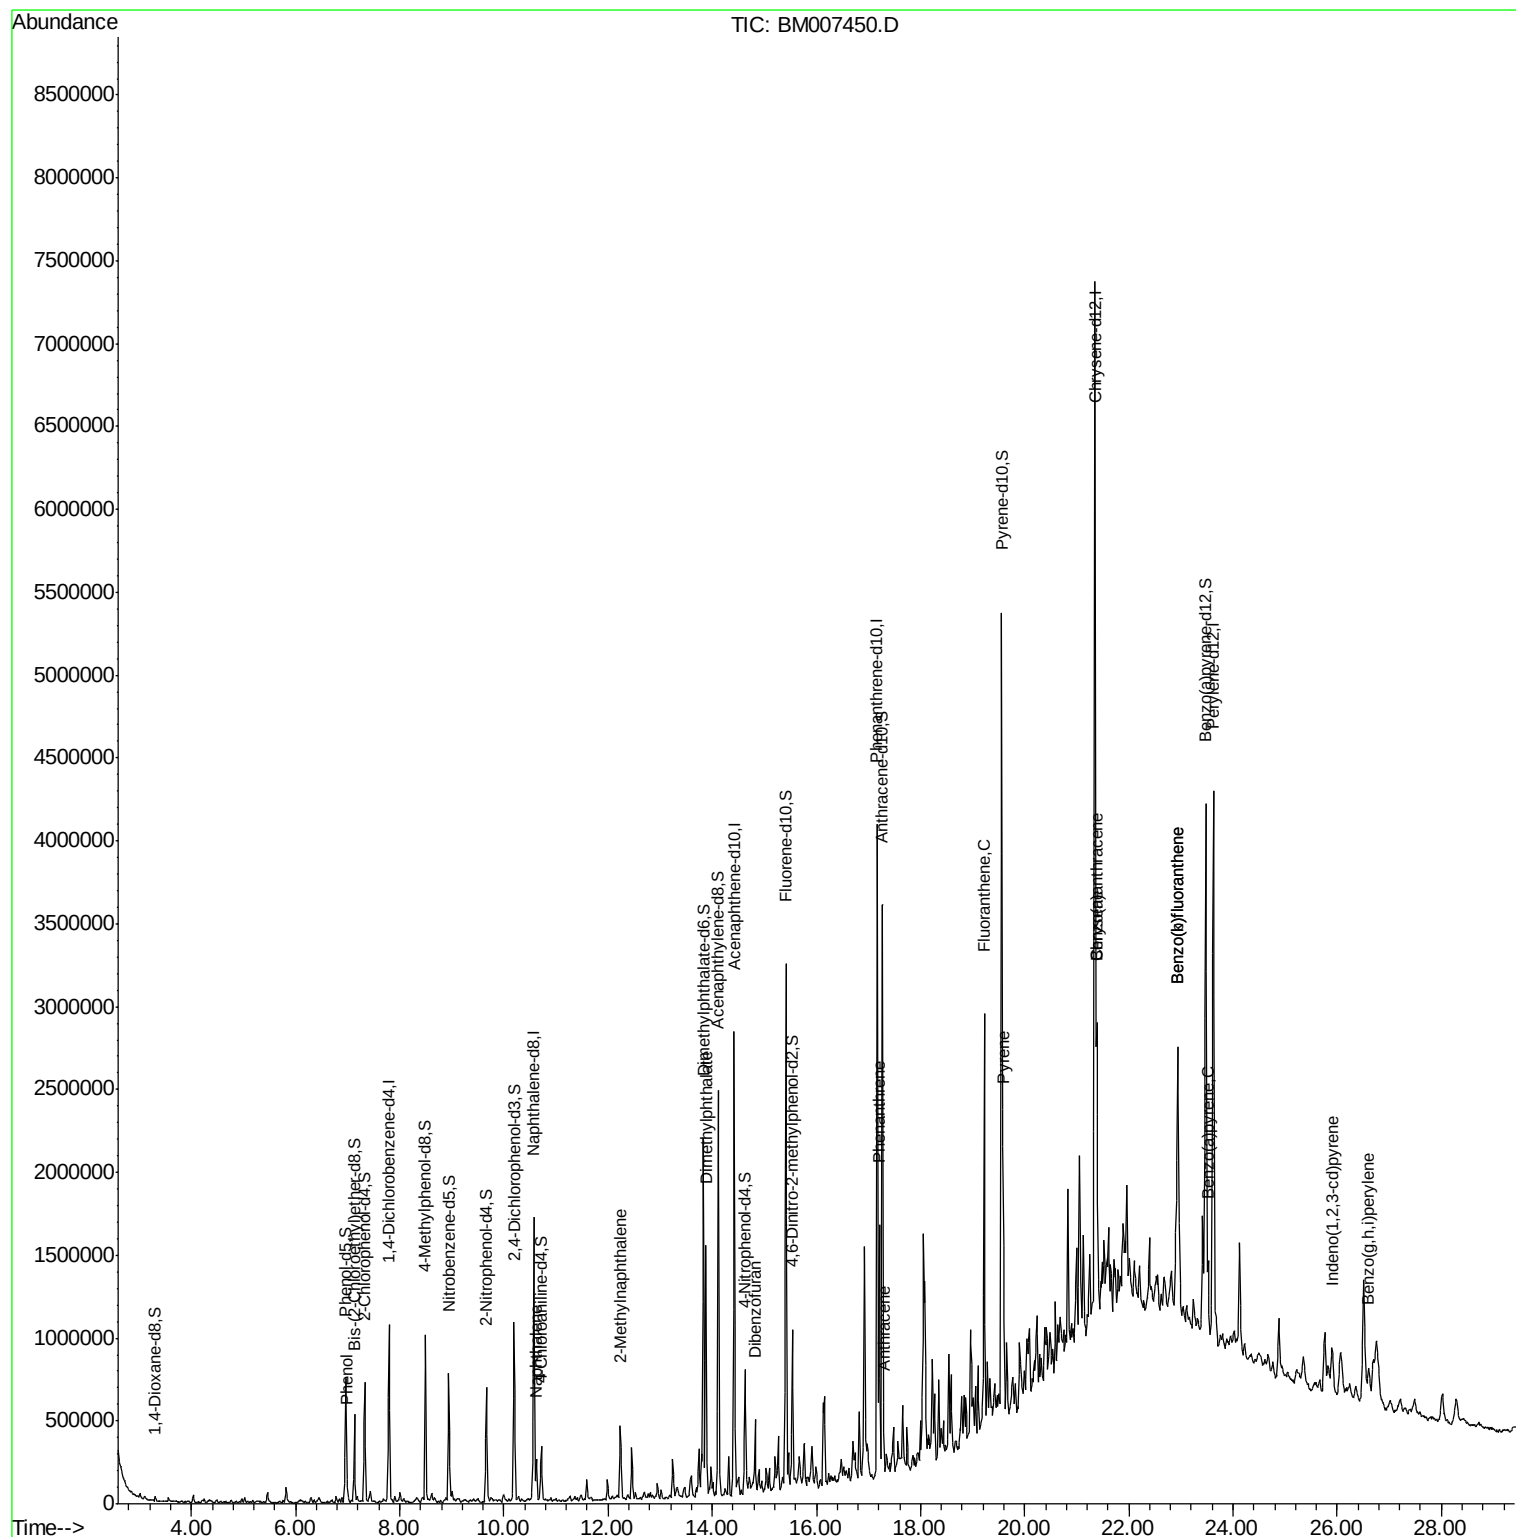

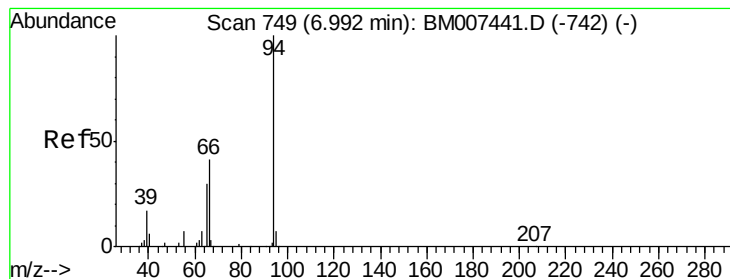

#6

Phenol

Concen: 1.42 ng/ul

RT: 6.99 min Scan# 748

Delta R.T. -0.01 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54

Instrument :

BNA_M

ClientSampleId :

BD399





Tgt Ion: 94 Resp: 38844

Ion Ratio Lower Upper

94 100

65 32.7 23.9 35.9

66 49.1 33.5 50.3

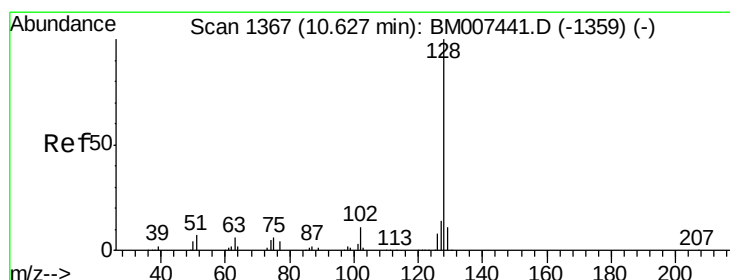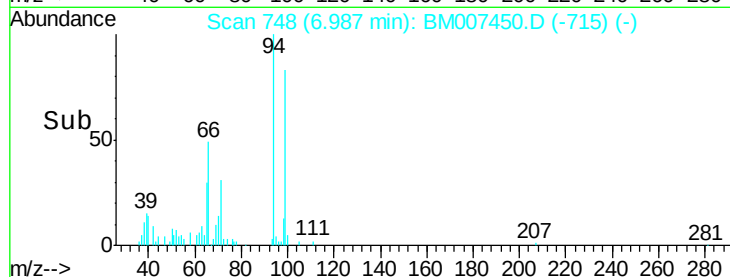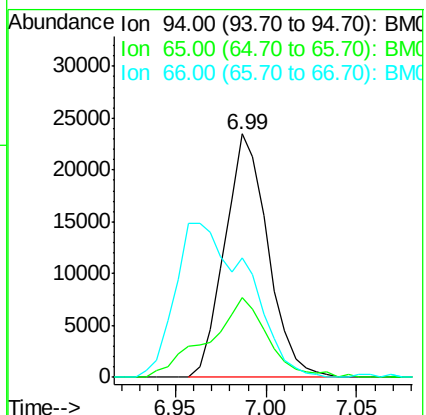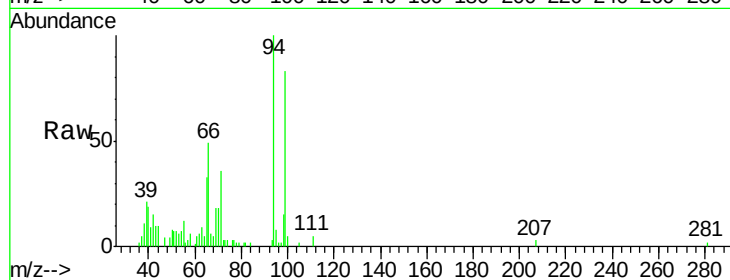

#28

Naphthalene

Concen: 2.83 ng/ul

RT: 10.63 min Scan# 1367

Delta R.T. 0.00 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54




Tgt Ion: 128 Resp: 192964


Ion Ratio Lower Upper

128 100

129 10.9 8.6 12.8

127 14.5 10.6 15.8

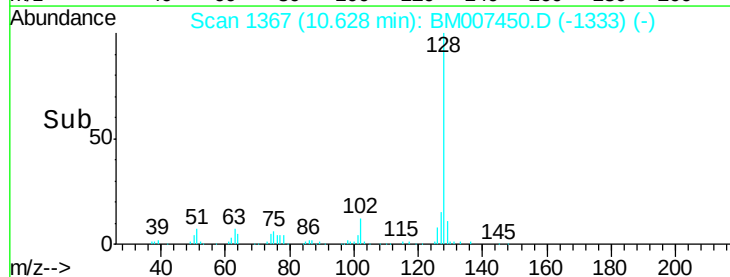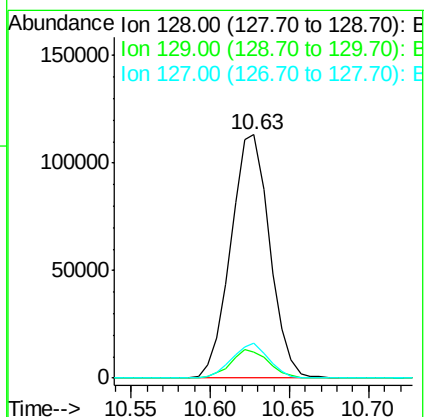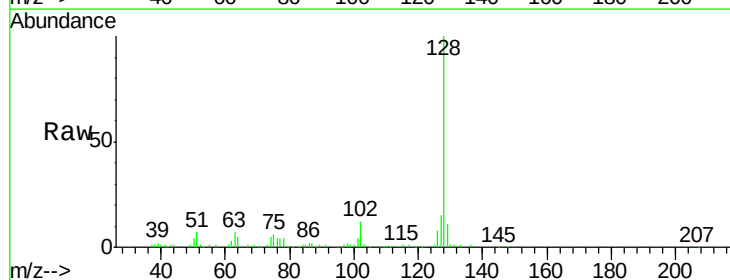


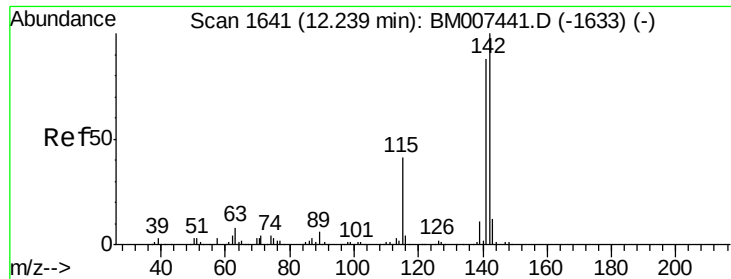




#34
 2-Methylnaphthalene
 Concen: 3.13 ng/ul
 RT: 12.24 min Scan# 1641
 Delta R.T. 0.00 min
 Lab File: BM007450.D
 Acq: 07 Sep 2016 21:54

Instrument :
 BNA_M
 ClientSampleId :
 BD399

Tgt Ion:142 Resp: 174639
 Ion Ratio Lower Upper
 142 100
 141 91.5 71.3 106.9




Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E

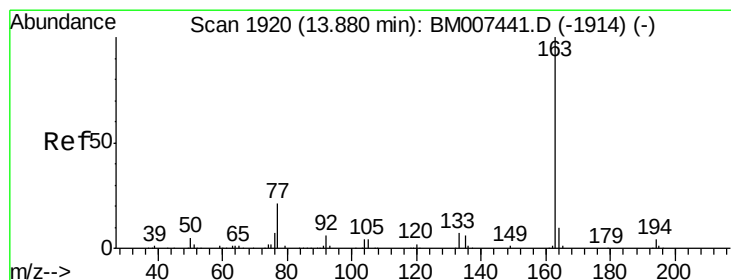
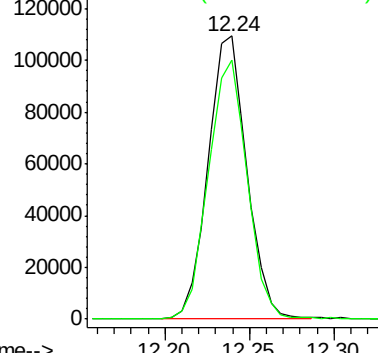



#44
 Dimethylphthalate
 Concen: 11.24 ng/ul
 RT: 13.88 min Scan# 1920
 Delta R.T. 0.00 min
 Lab File: BM007450.D
 Acq: 07 Sep 2016 21:54

Tgt Ion:163 Resp: 906253
 Ion Ratio Lower Upper
 163 100
 194 4.2 3.4 5.2
 164 9.7 7.8 11.8



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E




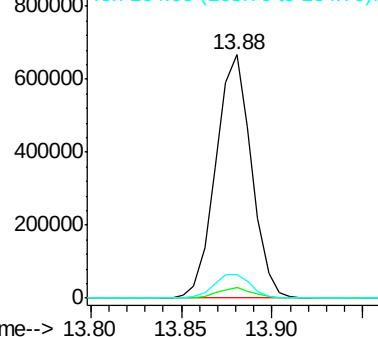


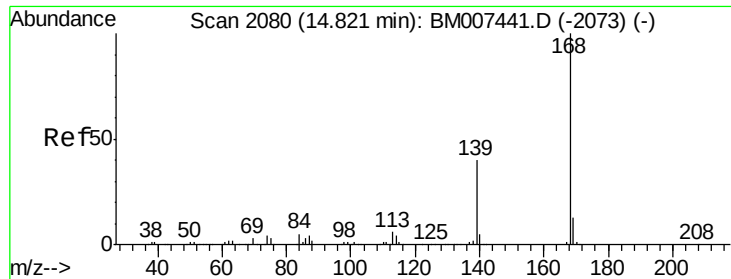

#53
Dibenzenofuran
Concen: 1.85 ng/ul
RT: 14.82 min Scan# 2080
Delta R.T. 0.00 min
Lab File: BM007450.D
Acq: 07 Sep 2016 21:54




Instrument :
BNA_M
ClientSampled :
BD399


Tgt Ion:168 Resp: 173916
Ion Ratio Lower Upper
168 100
139 41.4 30.1 45.1

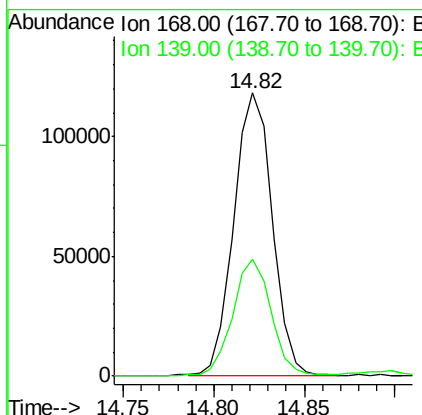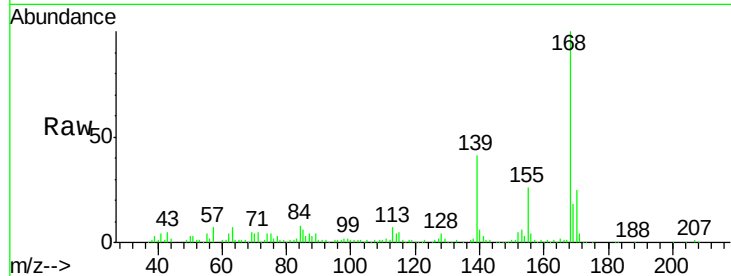

#69
Phenanthrene
Concen: 7.30 ng/ul
RT: 17.21 min Scan# 2486
Delta R.T. 0.00 min
Lab File: BM007450.D
Acq: 07 Sep 2016 21:54

Tgt Ion:178 Resp: 904426
Ion Ratio Lower Upper
178 100
179 15.1 12.2 18.2
176 18.3 15.1 22.7

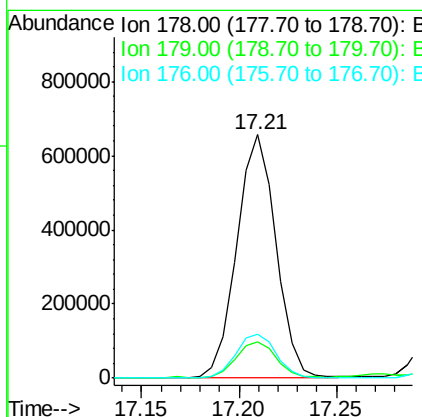


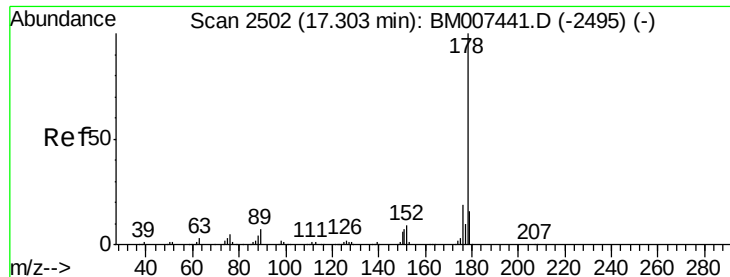




#71
 Anthracene
 Concen: 1.13 ng/ul
 RT: 17.30 min Scan# 2501
 Delta R.T. -0.01 min
 Lab File: BM007450.D
 Acq: 07 Sep 2016 21:54

Instrument :
 BNA_M
 ClientSampleId :
 BD399

Tgt Ion:178 Resp: 144964
 Ion Ratio Lower Upper
 178 100
 179 15.1 12.1 18.1
 176 17.1 14.5 21.7

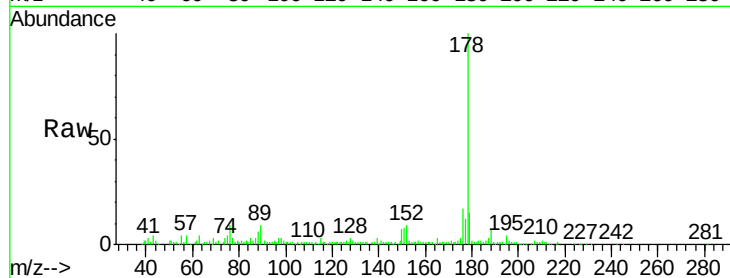


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

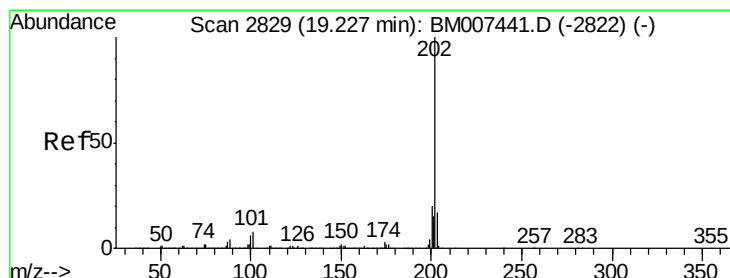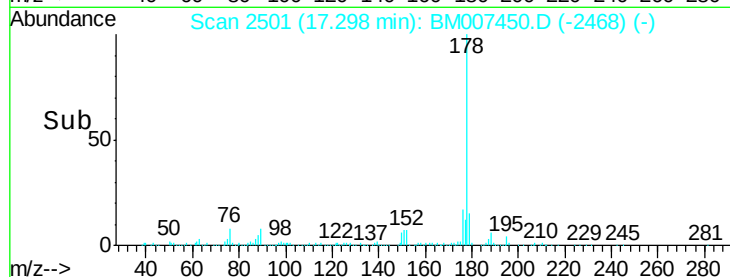
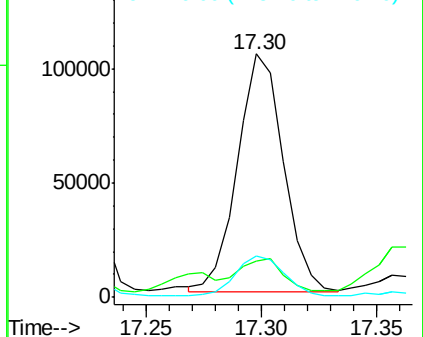



#74
 Fluoranthene
 Concen: 7.75 ng/ul
 RT: 19.22 min Scan# 2828
 Delta R.T. -0.01 min
 Lab File: BM007450.D
 Acq: 07 Sep 2016 21:54

Tgt Ion:202 Resp: 1205256
 Ion Ratio Lower Upper
 202 100
 101 9.6 6.9 10.3
 100 6.4 5.4 8.0

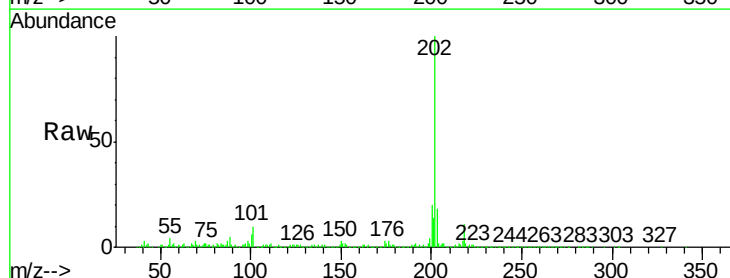

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

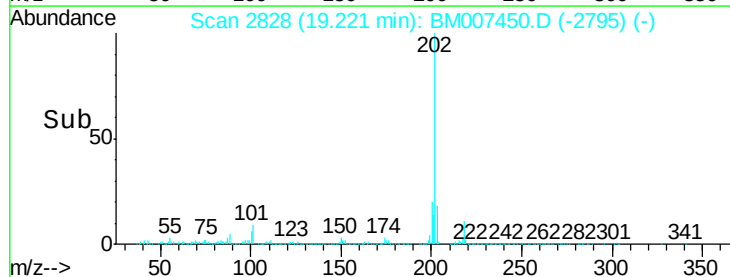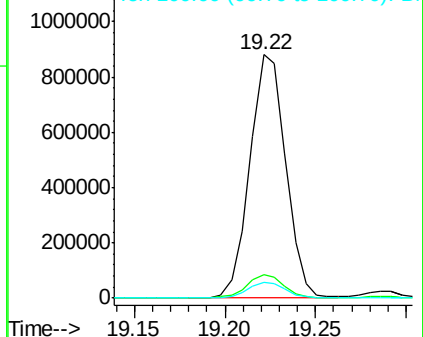

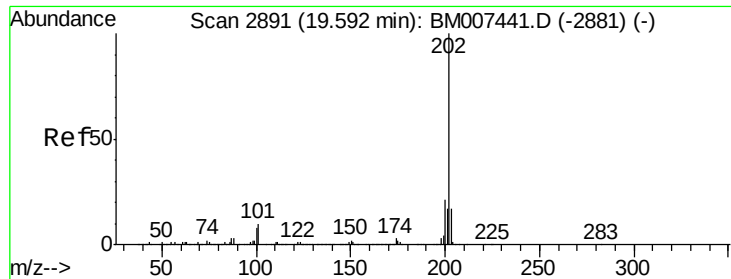

#77

Pyrene

Concen: 6.25 ng/ul

RT: 19.59 min Scan# 2890

Delta R.T. -0.01 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54

Instrument :

BNA_M

ClientSampleId :

BD399


Tgt Ion:202 Resp: 949705

Ion Ratio Lower Upper

202 100

101 11.1 8.4 12.6




100 8.7 6.9 10.3

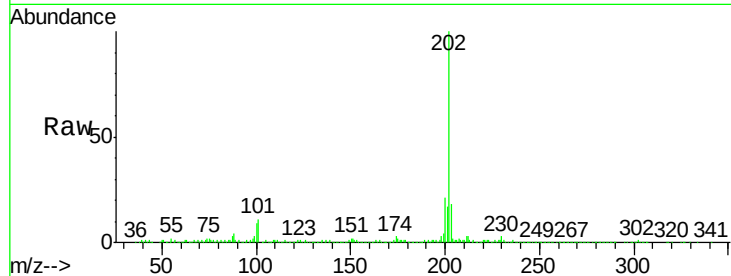

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

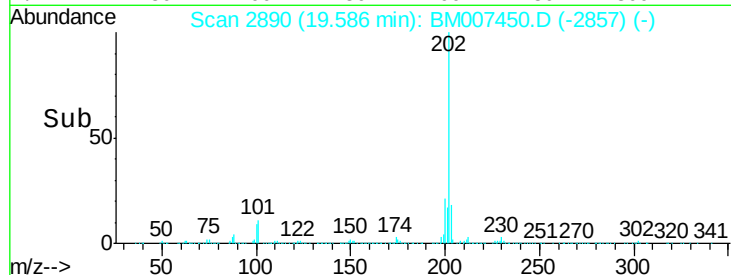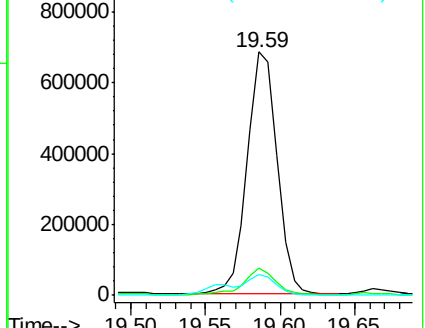

#80

Benzo(a)anthracene

Concen: 5.30 ng/ul

RT: 21.39 min Scan# 3196

Delta R.T. 0.05 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54


Tgt Ion:228 Resp: 885352

Ion Ratio Lower Upper

228 100

229 21.7 15.6 23.4



226 30.2 21.8 32.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

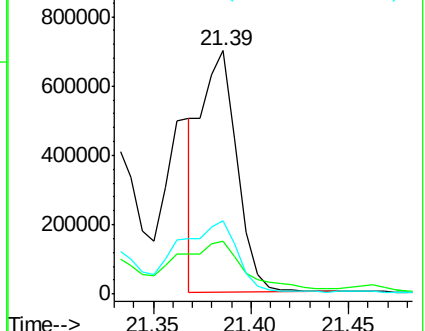

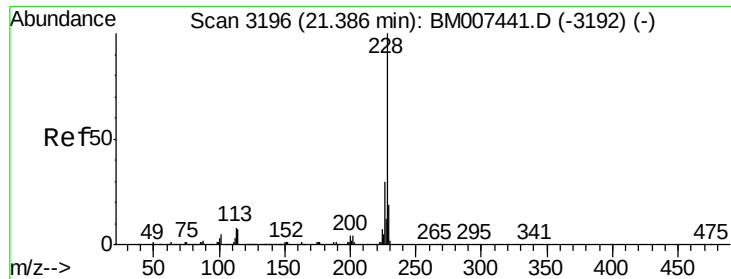

#82

Chrysene

Concen: 5.84 ng/ul

RT: 21.39 min Scan# 3196

Delta R.T. 0.00 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54

Instrument :

BNA_M

ClientSampleId :

BD399


Tgt Ion:228 Resp: 883062

Ion Ratio Lower Upper

228 100

226 30.2 23.4 35.2




229 21.7 15.5 23.3

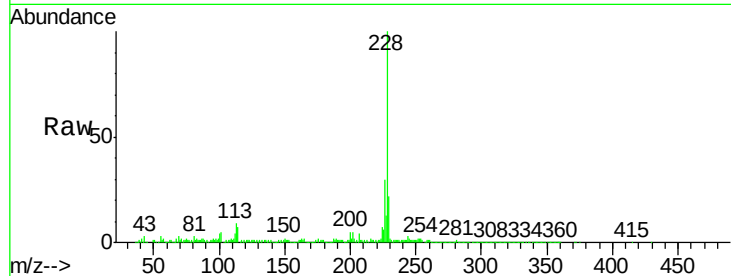

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

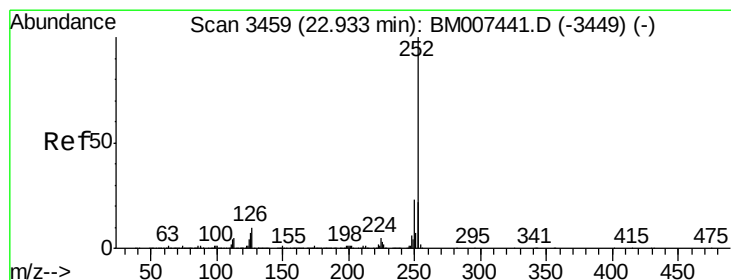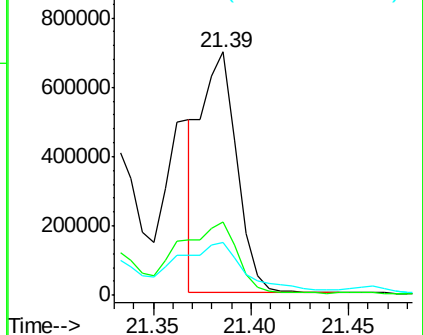

#85

Benzo(b)fluoranthene

Concen: 8.57 ng/ul

RT: 22.93 min Scan# 3459

Delta R.T. 0.00 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54


Tgt Ion:252 Resp: 1306266

Ion Ratio Lower Upper

252 100

253 22.5 17.1 25.7



125 8.2 5.8 8.8




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

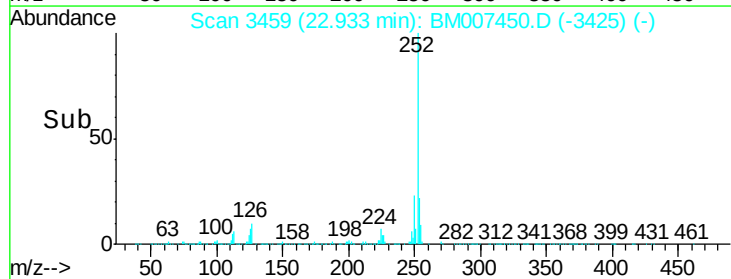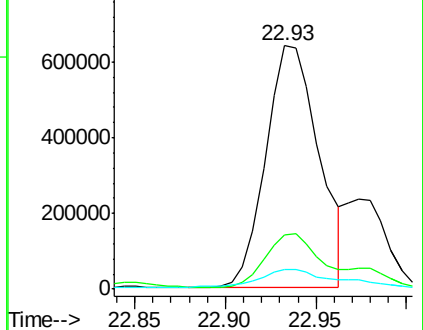



#86

Benzo(k)fluoranthene

Concen: 9.27 ng/ul

RT: 22.93 min Scan# 3459

Delta R.T. -0.05 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54

Instrument :

BNA_M

ClientSampleId :

BD399


Tgt Ion:252 Resp: 1306266

Ion Ratio Lower Upper

252 100

253 22.5 17.6 26.4




125 8.2 5.7 8.5

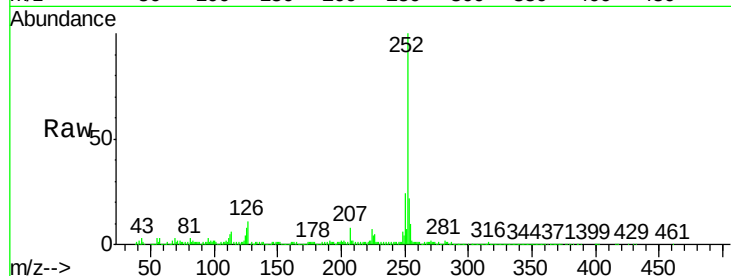

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

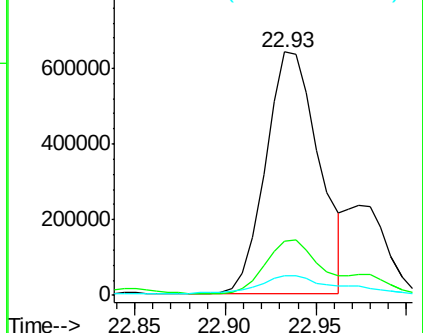

#88

Benzo(a)pyrene

Concen: 2.21 ng/ul

RT: 23.52 min Scan# 3559

Delta R.T. 0.00 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54


Tgt Ion:252 Resp: 322507

Ion Ratio Lower Upper

252 100

253 23.4 17.7 26.5



125 9.9 6.6 9.8#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

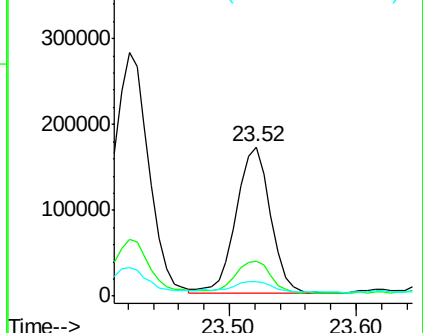



#89

Indeno(1,2,3-cd)pyrene

Concen: 1.37 ng/ul

RT: 25.90 min Scan# 3964

Delta R.T. -0.01 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54





Instrument :

BNA_M

ClientSampleId :

BD399

Tgt Ion:	276	Resp:	244591
Ion	Ratio	Lower	Upper
276	100		
138	18.3	13.9	20.9
277	24.7	20.1	30.1

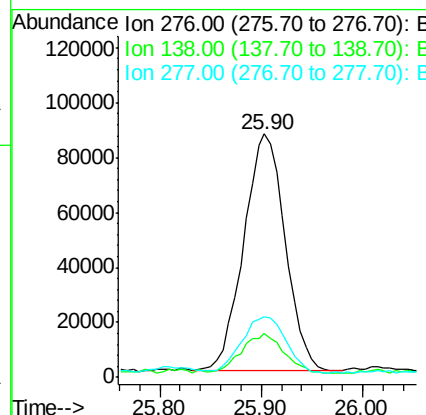

#91

Benzo(g,h,i)perylene

Concen: 1.29 ng/ul

RT: 26.60 min Scan# 4083

Delta R.T. -0.01 min

Lab File: BM007450.D

Acq: 07 Sep 2016 21:54

Tgt Ion:	276	Resp:	196807
Ion	Ratio	Lower	Upper
276	100		
138	17.3	13.5	20.3
277	25.3	19.3	28.9

