

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
 Data File : BM007453.D
 Acq On : 07 Sep 2016 23:42
 Operator : UM/SJ
 Sample : H4666-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3A9

Quant Time: Sep 08 03:13:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 08 03:10:54 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	276095	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1336448	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	882027	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	2133469	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2366331	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	1998123	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	18191	3.37	ng/uL	0.00
5) Phenol-d5	6.96	99	488549	18.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	255235	18.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	374456	19.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	407717	17.93	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	199471	20.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	236007	20.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	453880	19.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	159863	5.62	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1566575	20.59	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1868434	21.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	213306	14.85	ng/ul	0.00
57) Fluorene-d10	15.42	176	1388054	21.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	250810	18.70	ng/ul	0.00
70) Anthracene-d10	17.27	188	2261260	22.69	ng/ul	0.00
76) Pyrene-d10	19.56	212	2669636	26.98	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	2093474	22.75	ng/ul	0.00

Target Compounds

					Qvalue
6) Phenol	6.99	94	33188	1.23 ng/ul	97
28) Naphthalene	10.63	128	360363	5.42 ng/ul	99
30) 4-Chloroaniline	10.63	127	47054	1.61 ng/ul#	5
34) 2-Methylnaphthalene	12.24	142	270242	4.97 ng/ul	100
40) 1,1'-Biphenyl	13.26	154	100482	1.47 ng/ul	97
44) Dimethylphthalate	13.88	163	915989	12.09 ng/ul	99
47) Acenaphthylene	14.15	152	111637	1.23 ng/ul	98
53) Dibenzofuran	14.82	168	424340	4.80 ng/ul	97
69) Phenanthrene	17.21	178	1592715	13.91 ng/ul	99
71) Anthracene	17.30	178	402136	3.40 ng/ul	99
72) Carbazole	17.57	167	157329	1.53 ng/ul	96
74) Fluoranthene	19.23	202	1882460	13.10 ng/ul	100
77) Pyrene	19.59	202	1133376	8.93 ng/ul	99
80) Benzo(a)anthracene	21.37	228	777982	5.58 ng/ul	92
81) Bis(2-ethylhexyl)phthalate	21.26	149	90582	1.18 ng/ul#	95
82) Chrysene	21.37	228	775267	6.14 ng/ul	94
85) Benzo(b)fluoranthene	22.94	252	2433160	20.59 ng/ul	98
86) Benzo(k)fluoranthene	22.94	252	2431821	22.27 ng/ul	99
88) Benzo(a)pyrene	23.52	252	298684	2.64 ng/ul#	89
89) Indeno(1,2,3-cd)pyrene	25.91	276	440941	3.18 ng/ul	98
90) Dibenzo(a,h)anthracene	25.92	278	158977	1.38 ng/ul#	81
91) Benzo(g,h,i)perylene	26.62	276	295008	2.50 ng/ul	99

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007453.D
Acq On : 07 Sep 2016 23:42
Operator : UM/SJ
Sample : H4666-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A9

Quant Time: Sep 08 03:13:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007453.D
Acq On : 07 Sep 2016 23:42
Operator : UM/SJ
Sample : H4666-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A9

Quant Time: Sep 08 03:13:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 08 03:10:54 2016
Response via : Initial Calibration

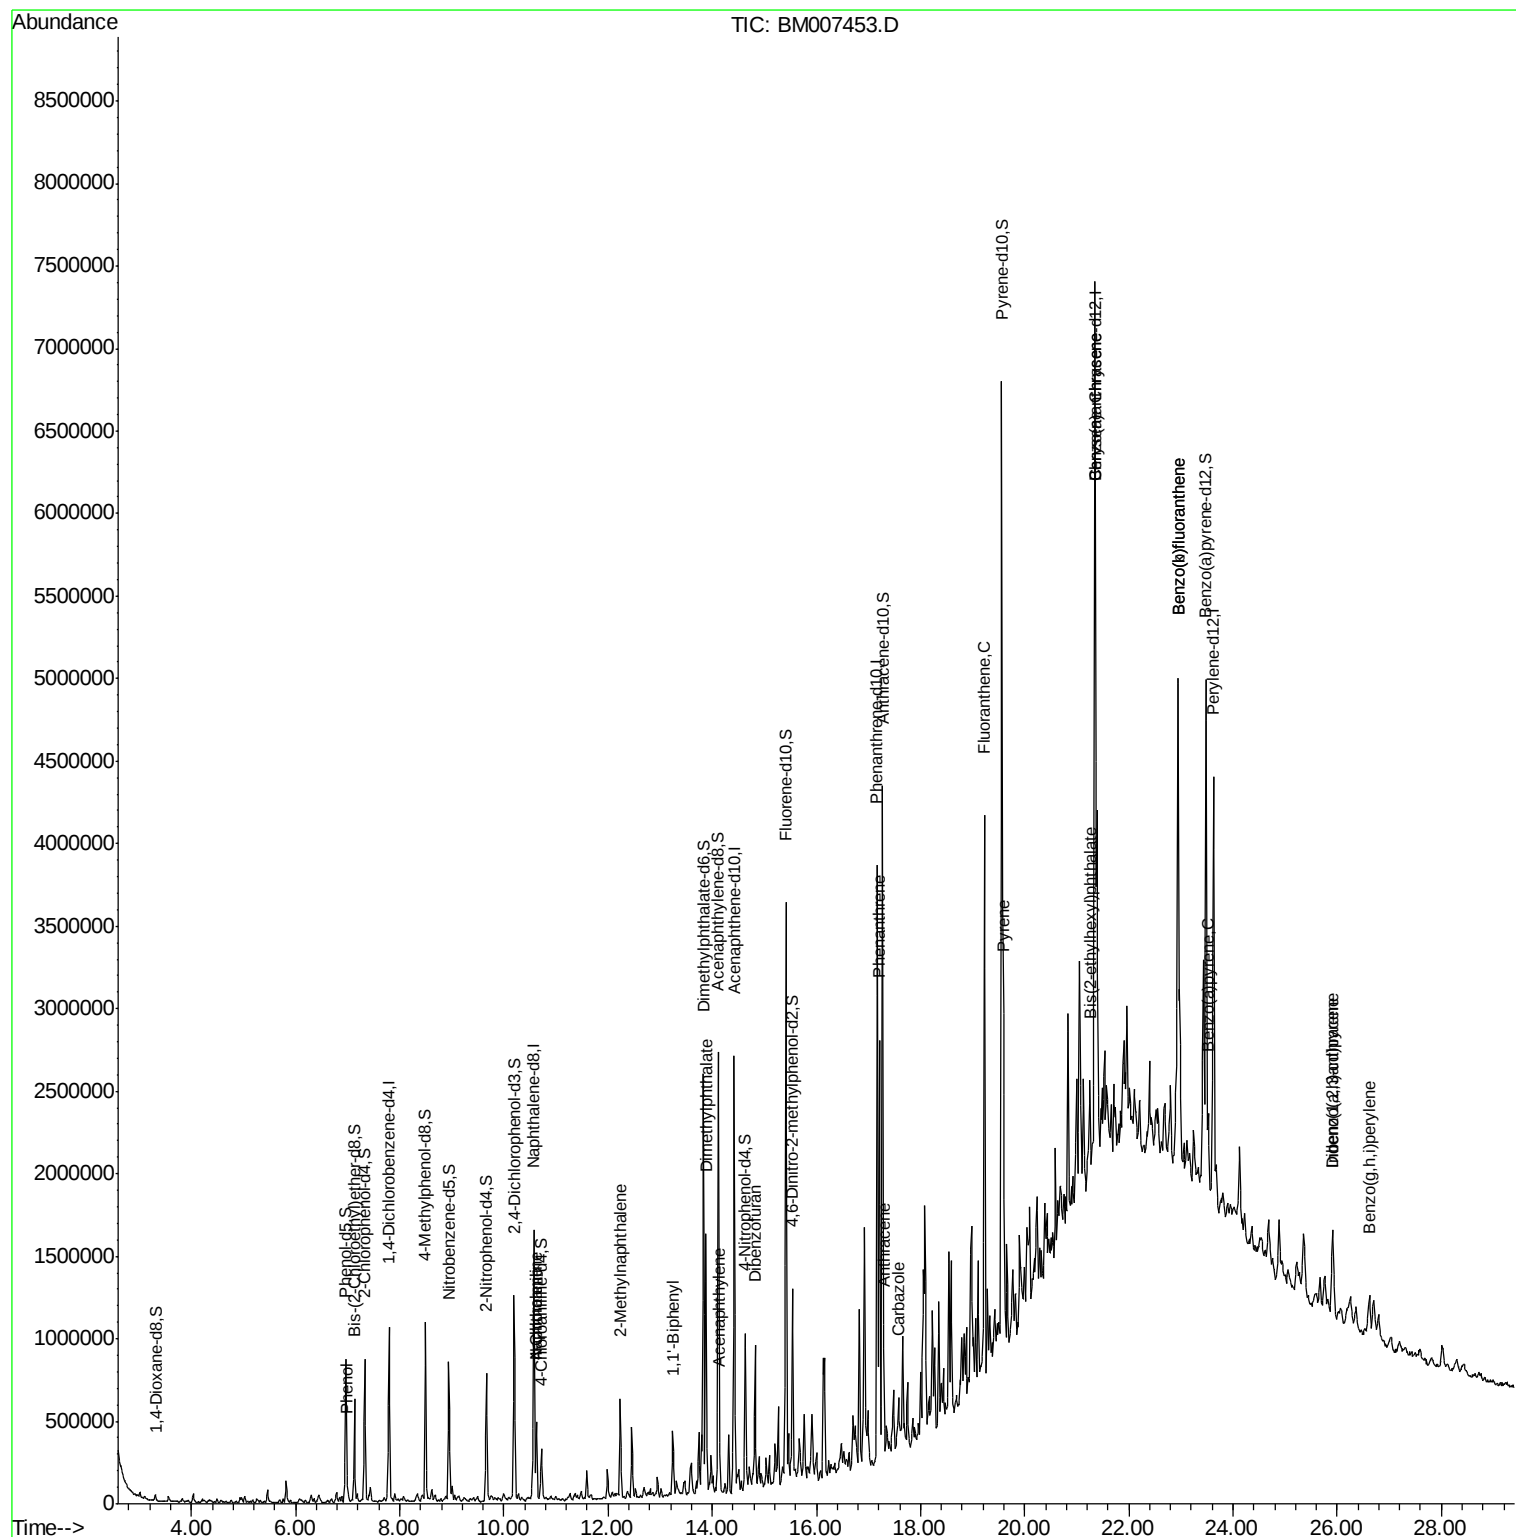

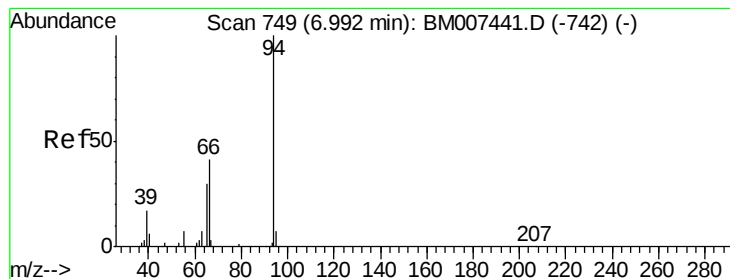

#6

Phenol

Concen: 1.23 ng/ul

RT: 6.99 min Scan# 749

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion: 94 Resp: 33188

Ion Ratio Lower Upper

94 100

65 28.6 23.9 35.9




66 43.7 33.5 50.3



Abundance Ion 94.00 (93.70 to 94.70): BM007441.D (-742) (-)

Ion 65.00 (64.70 to 65.70): BM007441.D (-742) (-)

Ion 66.00 (65.70 to 66.70): BM007441.D (-742) (-)

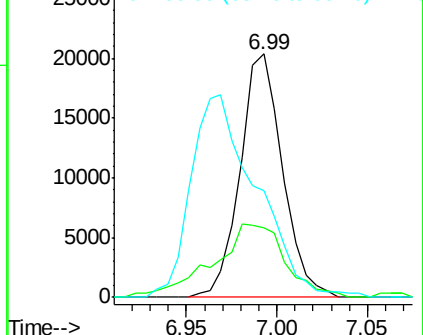

#28

Naphthalene

Concen: 5.42 ng/ul

RT: 10.63 min Scan# 1367

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion: 128 Resp: 360363

Ion Ratio Lower Upper

128 100

129 10.6 8.6 12.8



127 12.9 10.6 15.8




Abundance Ion 128.00 (127.70 to 128.70): BM007441.D (-1359) (-)

Ion 129.00 (128.70 to 129.70): BM007441.D (-1359) (-)

Ion 127.00 (126.70 to 127.70): BM007441.D (-1359) (-)




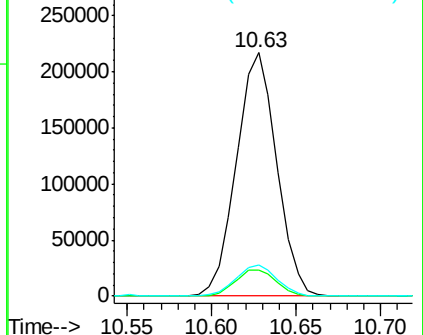




#30
 4-Chloroaniline
 Concen: 1.61 ng/ul
 RT: 10.63 min Scan# 1367
 Delta R.T. -0.11 min
 Lab File: BM007453.D
 Acq: 07 Sep 2016 23:42




Instrument :
 BNA_M
 ClientSampleId :
 BD3A9


Tgt Ion:127 Resp: 47054
 Ion Ratio Lower Upper
 127 100
 129 82.7 24.6 37.0#

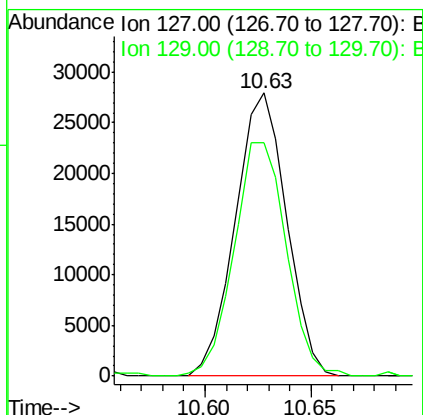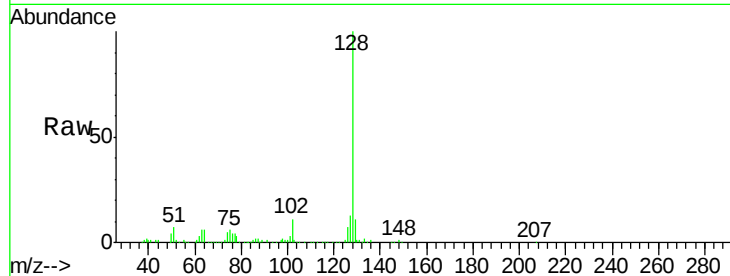

#34
 2-Methylnaphthalene
 Concen: 4.97 ng/ul
 RT: 12.24 min Scan# 1641
 Delta R.T. 0.00 min
 Lab File: BM007453.D
 Acq: 07 Sep 2016 23:42

Tgt Ion:142 Resp: 270242
 Ion Ratio Lower Upper
 142 100
 141 89.4 71.3 106.9

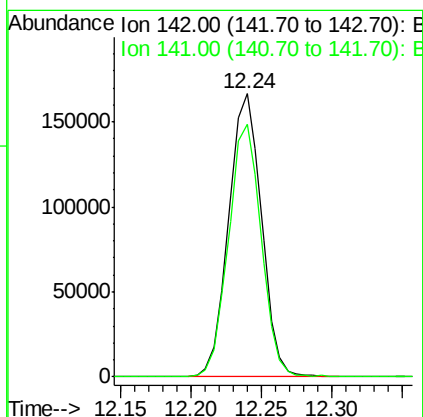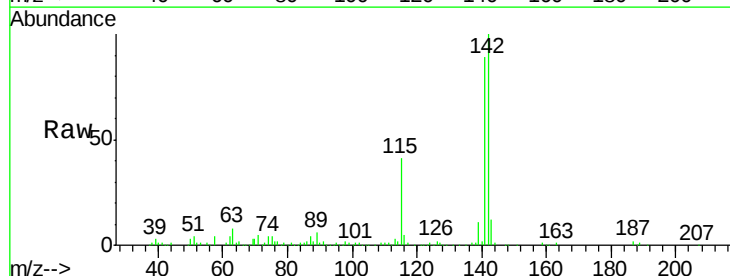

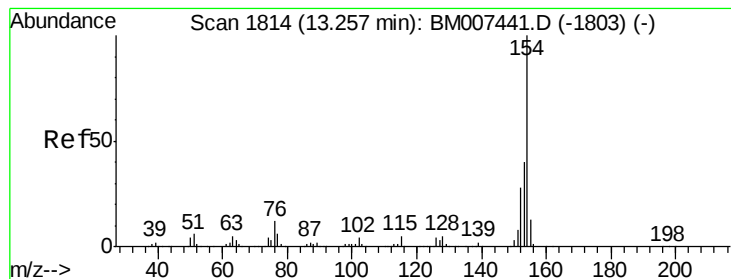

#40

1,1'-Biphenyl

Concen: 1.47 ng/ul

RT: 13.26 min Scan# 1814

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:154 Resp: 100482

Ion Ratio Lower Upper

154 100

153 37.5 31.3 46.9




76 10.1 10.0 15.0



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BM

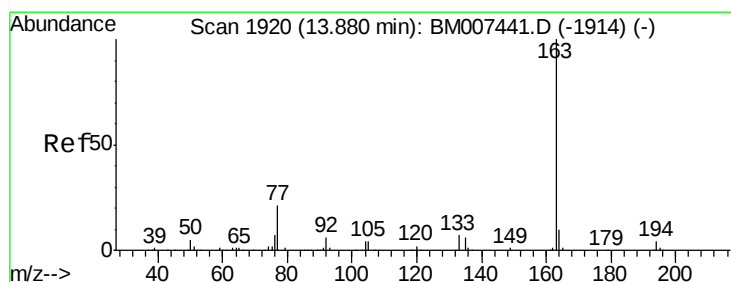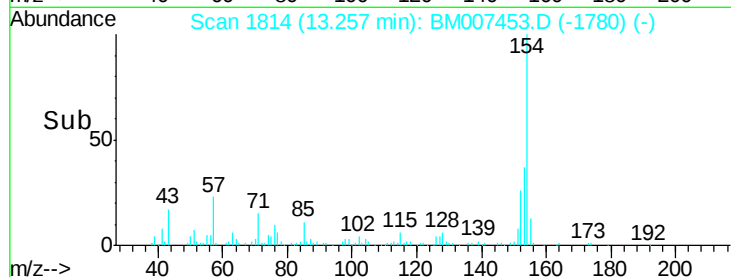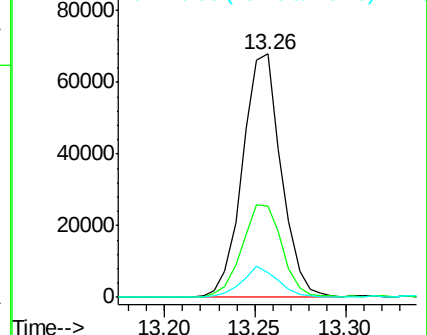

#44

Dimethylphthalate

Concen: 12.09 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:163 Resp: 915989

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2



164 10.3 7.8 11.8




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

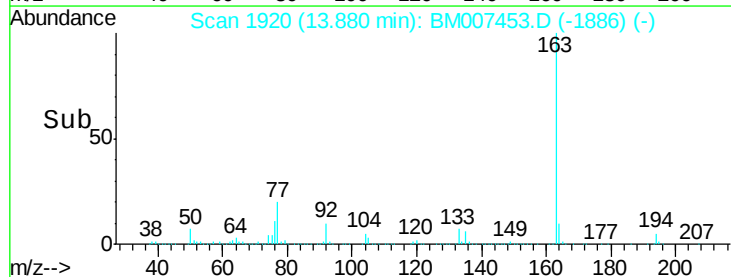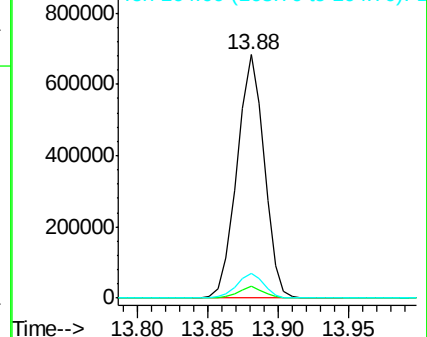

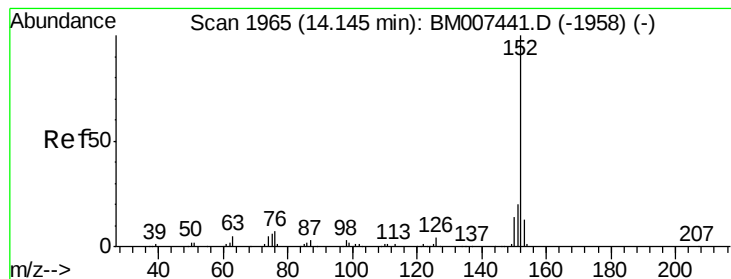

#47

Acenaphthylene

Concen: 1.23 ng/ul

RT: 14.15 min Scan# 1965

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:152 Resp: 111637

Ion Ratio Lower Upper

152 100

151 19.9 16.0 24.0




153 15.6 11.0 16.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

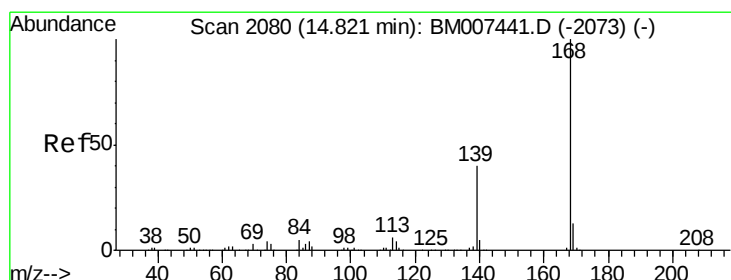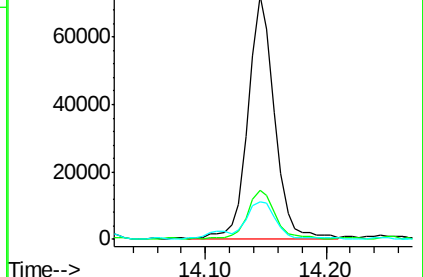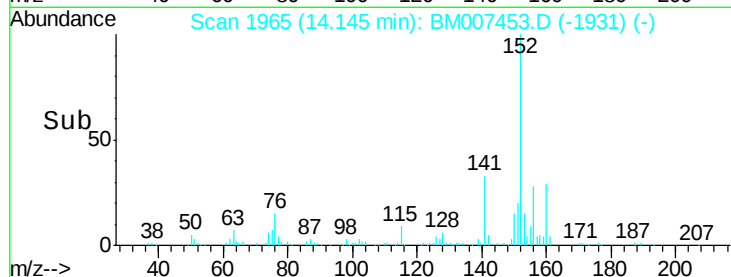

#53

Dibenzofuran

Concen: 4.80 ng/ul

RT: 14.82 min Scan# 2080

Delta R.T. 0.00 min

Lab File: BM007453.D


Acq: 07 Sep 2016 23:42

Tgt Ion:168 Resp: 424340

Ion Ratio Lower Upper



168 100


139 39.6 30.1 45.1



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

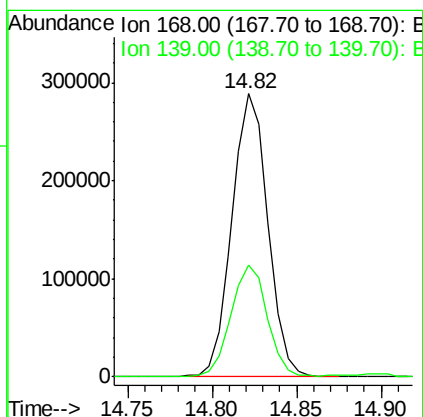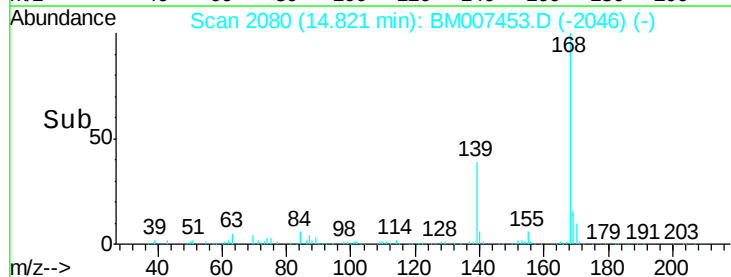

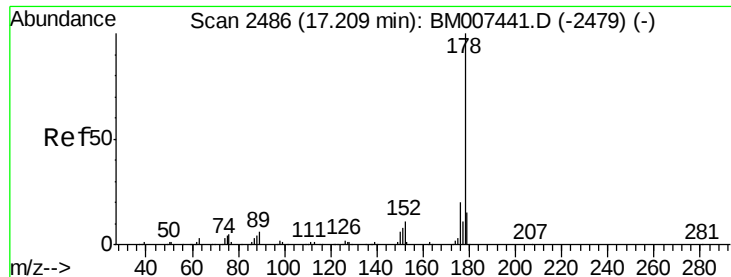

#69

Phenanthrene

Concen: 13.91 ng/ul

RT: 17.21 min Scan# 2486

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:178 Resp: 1592715

Ion Ratio Lower Upper

178 100

179 15.6 12.2 18.2




176 19.5 15.1 22.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

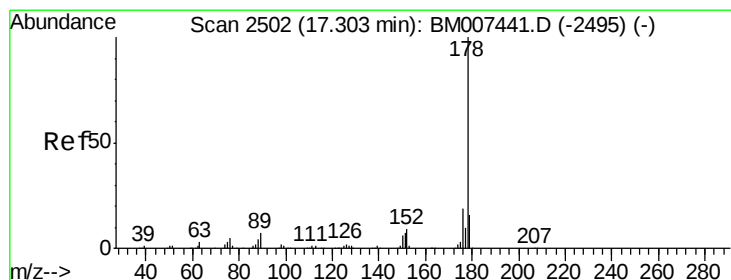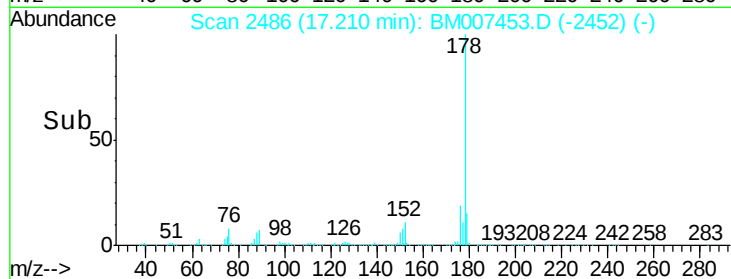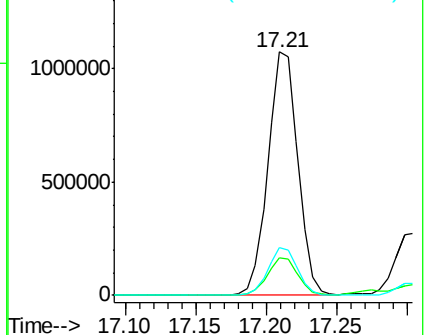

#71

Anthracene

Concen: 3.40 ng/ul

RT: 17.30 min Scan# 2502

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:178 Resp: 402136

Ion Ratio Lower Upper

178 100

179 16.3 12.1 18.1



176 18.3 14.5 21.7




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

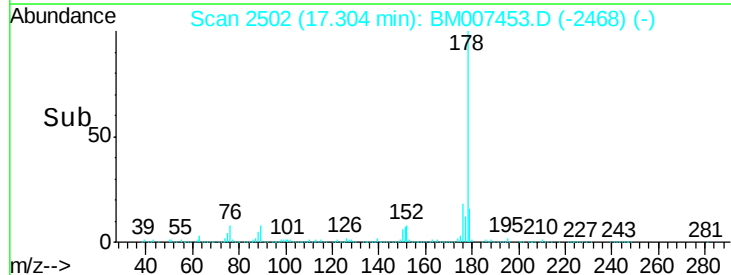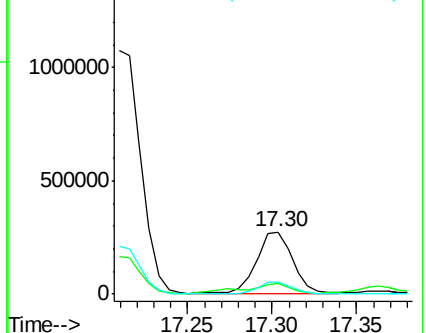



#72

Carbazole

Concen: 1.53 ng/ul

RT: 17.57 min Scan# 2548

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:167 Resp: 157329

Ion Ratio Lower Upper

167 100

166 22.9 16.6 25.0




139 14.3 10.2 15.4



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

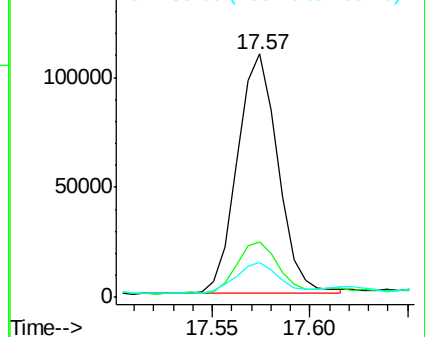

#74

Fluoranthene

Concen: 13.10 ng/ul

RT: 19.23 min Scan# 2829

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:202 Resp: 1882460

Ion Ratio Lower Upper

202 100

101 8.7 6.9 10.3



100 6.5 5.4 8.0




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

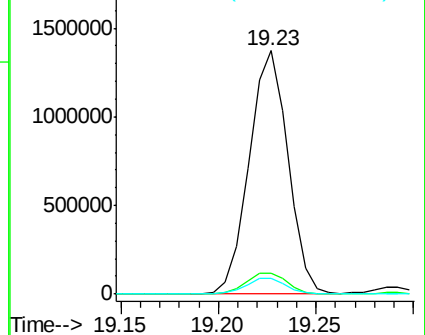

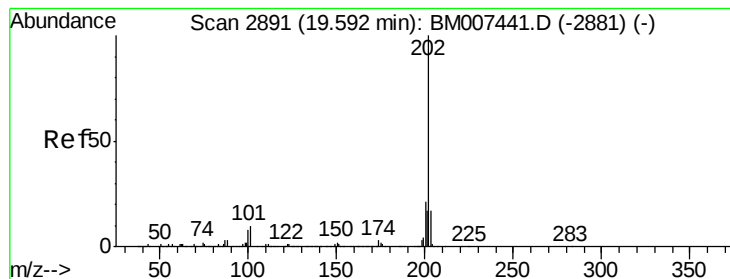

#77

Pyrene

Concen: 8.93 ng/ul

RT: 19.59 min Scan# 2891

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:202 Resp: 1133376

Ion Ratio Lower Upper

202 100

101 10.4 8.4 12.6




100 8.3 6.9 10.3



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

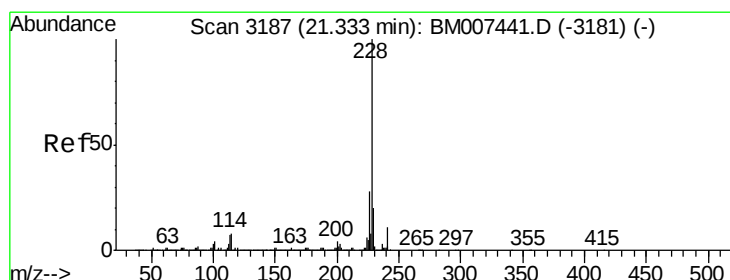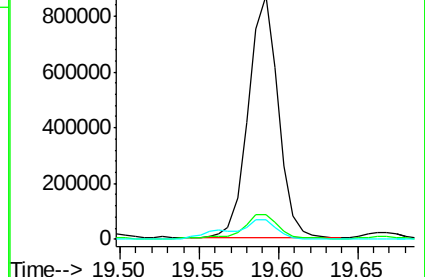

#80

Benzo(a)anthracene

Concen: 5.58 ng/ul

RT: 21.37 min Scan# 3193

Delta R.T. 0.04 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:228 Resp: 777982

Ion Ratio Lower Upper

228 100

229 23.1 15.6 23.4



226 31.4 21.8 32.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

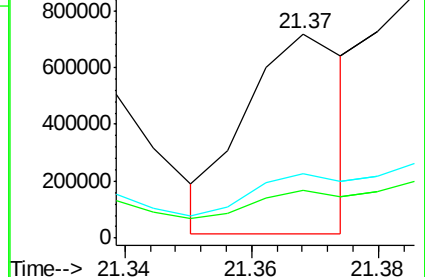

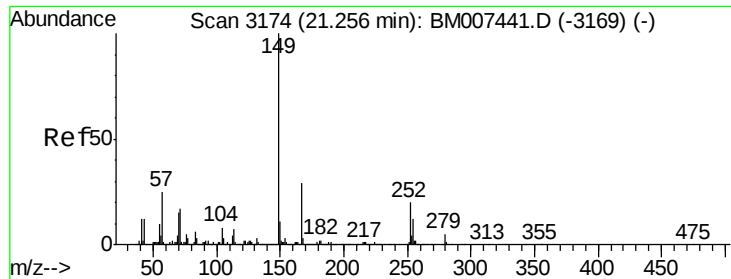

#81

Bis(2-ethylhexyl)phthalate

Concen: 1.18 ng/ul

RT: 21.26 min Scan# 3174

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:149 Resp: 90582

Ion Ratio Lower Upper

149 100

167 31.8 23.2 34.8




279 6.6 4.1 6.1#

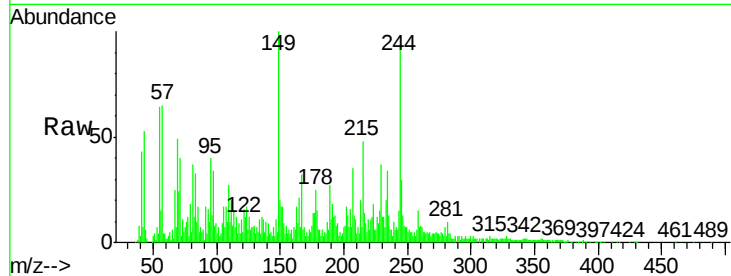

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

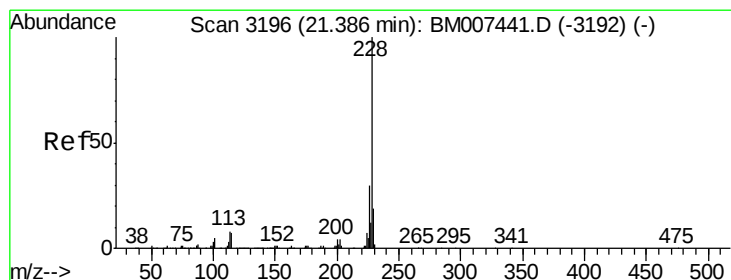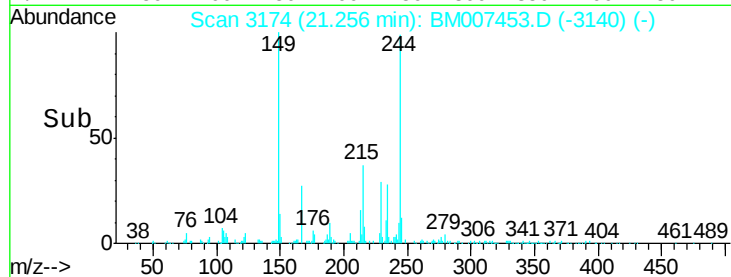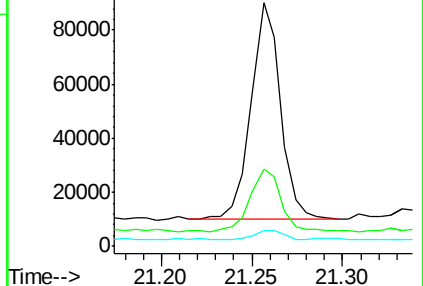

#82

Chrysene

Concen: 6.14 ng/ul

RT: 21.37 min Scan# 3193

Delta R.T. -0.02 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:228 Resp: 775267

Ion Ratio Lower Upper

228 100

226 31.4 23.4 35.2



229 23.1 15.5 23.3




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

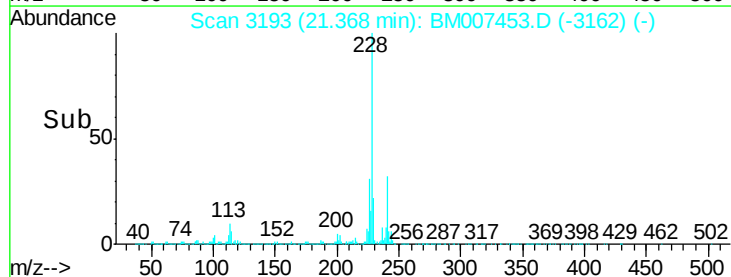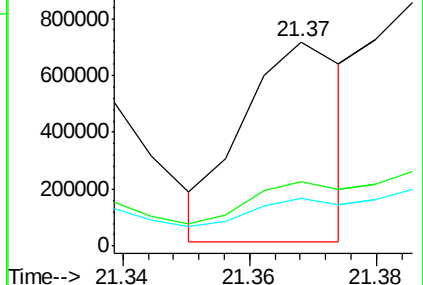

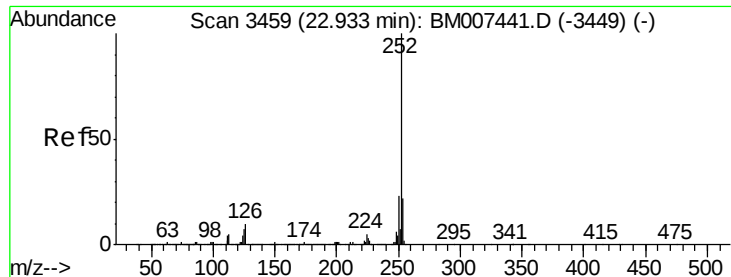

#85

Benzo(b)fluoranthene

Concen: 20.59 ng/ul

RT: 22.94 min Scan# 3461

Delta R.T. 0.01 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:252 Resp: 2433160

Ion Ratio Lower Upper

252 100

253 22.5 17.1 25.7




125 7.6 5.8 8.8



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

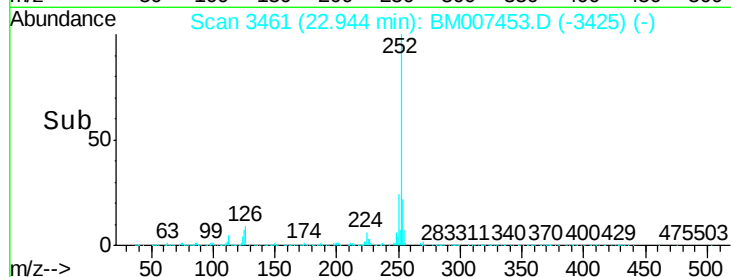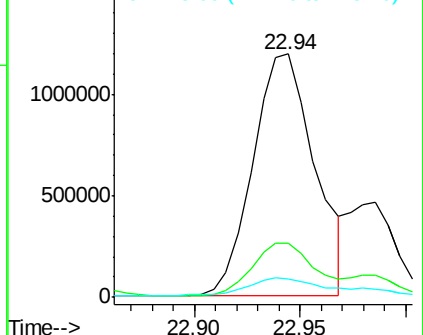

#86

Benzo(k)fluoranthene

Concen: 22.27 ng/ul

RT: 22.94 min Scan# 3461

Delta R.T. -0.04 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:252 Resp: 2431821

Ion Ratio Lower Upper

252 100

253 22.5 17.6 26.4



125 7.6 5.7 8.5




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

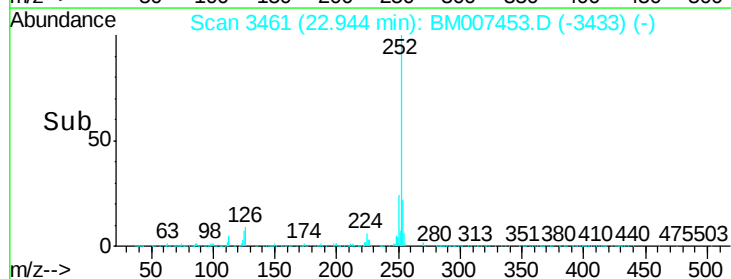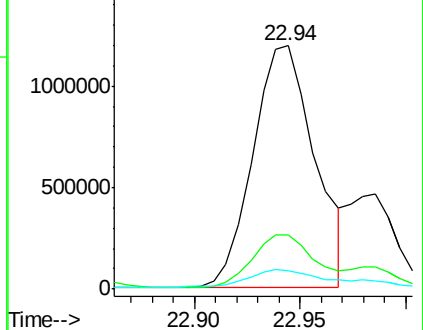



#88

Benzo(a)pyrene

Concen: 2.64 ng/ul

RT: 23.52 min Scan# 3559

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:252 Resp: 298684

Ion Ratio Lower Upper

252 100

253 26.3 17.7 26.5




125 14.5 6.6 9.8#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

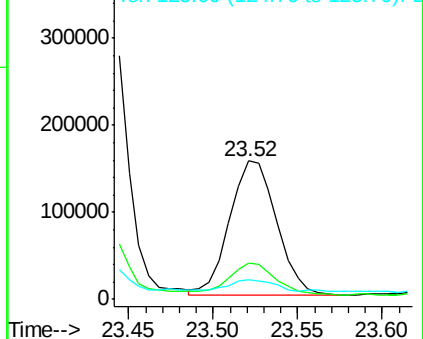

#89

Indeno(1,2,3-cd)pyrene

Concen: 3.18 ng/ul

RT: 25.91 min Scan# 3966

Delta R.T. 0.01 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:276 Resp: 440941

Ion Ratio Lower Upper

276 100

138 16.2 13.9 20.9



277 25.6 20.1 30.1




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

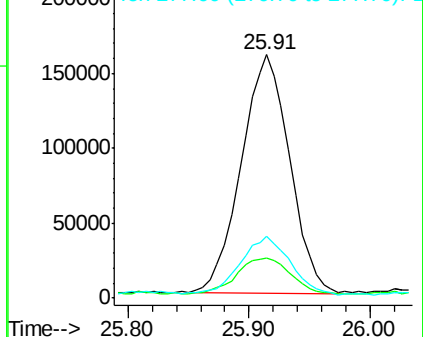

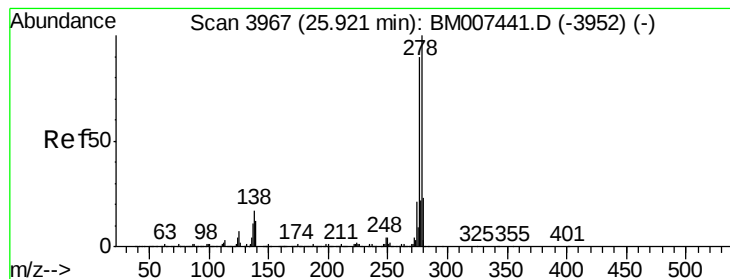

#90

Dibenzo(a,h)anthracene

Concen: 1.38 ng/ul

RT: 25.92 min Scan# 3967

Delta R.T. 0.00 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:278 Resp: 158977

Ion Ratio Lower Upper

278 100

139 21.1 9.5 14.3#




279 32.2 19.1 28.7#



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

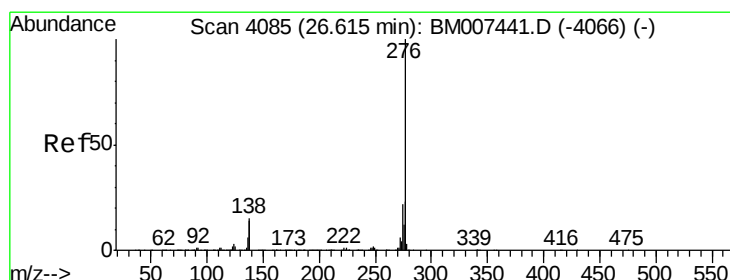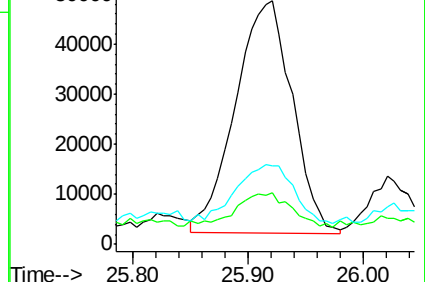

#91

Benzo(g,h,i)perylene

Concen: 2.50 ng/ul

RT: 26.62 min Scan# 4086

Delta R.T. 0.01 min

Lab File: BM007453.D

Acq: 07 Sep 2016 23:42


Tgt Ion:276 Resp: 295008

Ion Ratio Lower Upper

276 100

138 17.8 13.5 20.3

277 23.6 19.3 28.9

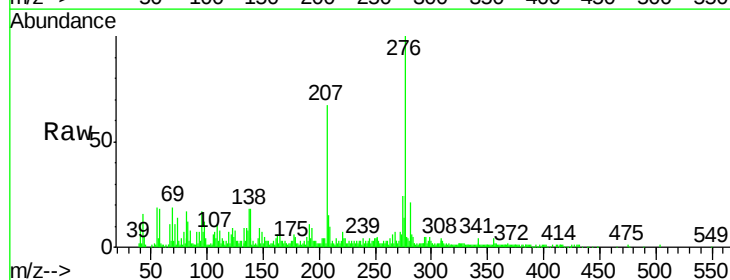

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

