

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
 Data File : BM007444.D
 Acq On : 07 Sep 2016 18:17
 Operator : UM/SJ
 Sample : H4666-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3A6

Quant Time: Sep 07 18:47:58 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 13:42:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	185232	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	910423	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	658490	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1737069	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	2203759	20.00	ng/ul	0.00
83) Perylene-d12	23.61	264	1976991	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	18766	5.18	ng/uL	0.00
5) Phenol-d5	6.96	99	439541	25.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	264081	28.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	346192	26.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	395992	25.95	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	193159	28.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	229158	29.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	412760	26.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	971988	50.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1603575	28.23	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1955075	29.69	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	258299	24.08	ng/ul	0.00
57) Fluorene-d10	15.42	176	1462346	29.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	260372	23.84	ng/ul	0.00
70) Anthracene-d10	17.27	188	2506019	30.88	ng/ul	0.00
76) Pyrene-d10	19.56	212	3122153	33.88	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	2839479	31.18	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	494979	8.75	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007444.D
Acq On : 07 Sep 2016 18:17
Operator : UM/SJ
Sample : H4666-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A6

Quant Time: Sep 07 18:47:58 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 13:42:00 2016
Response via : Initial Calibration

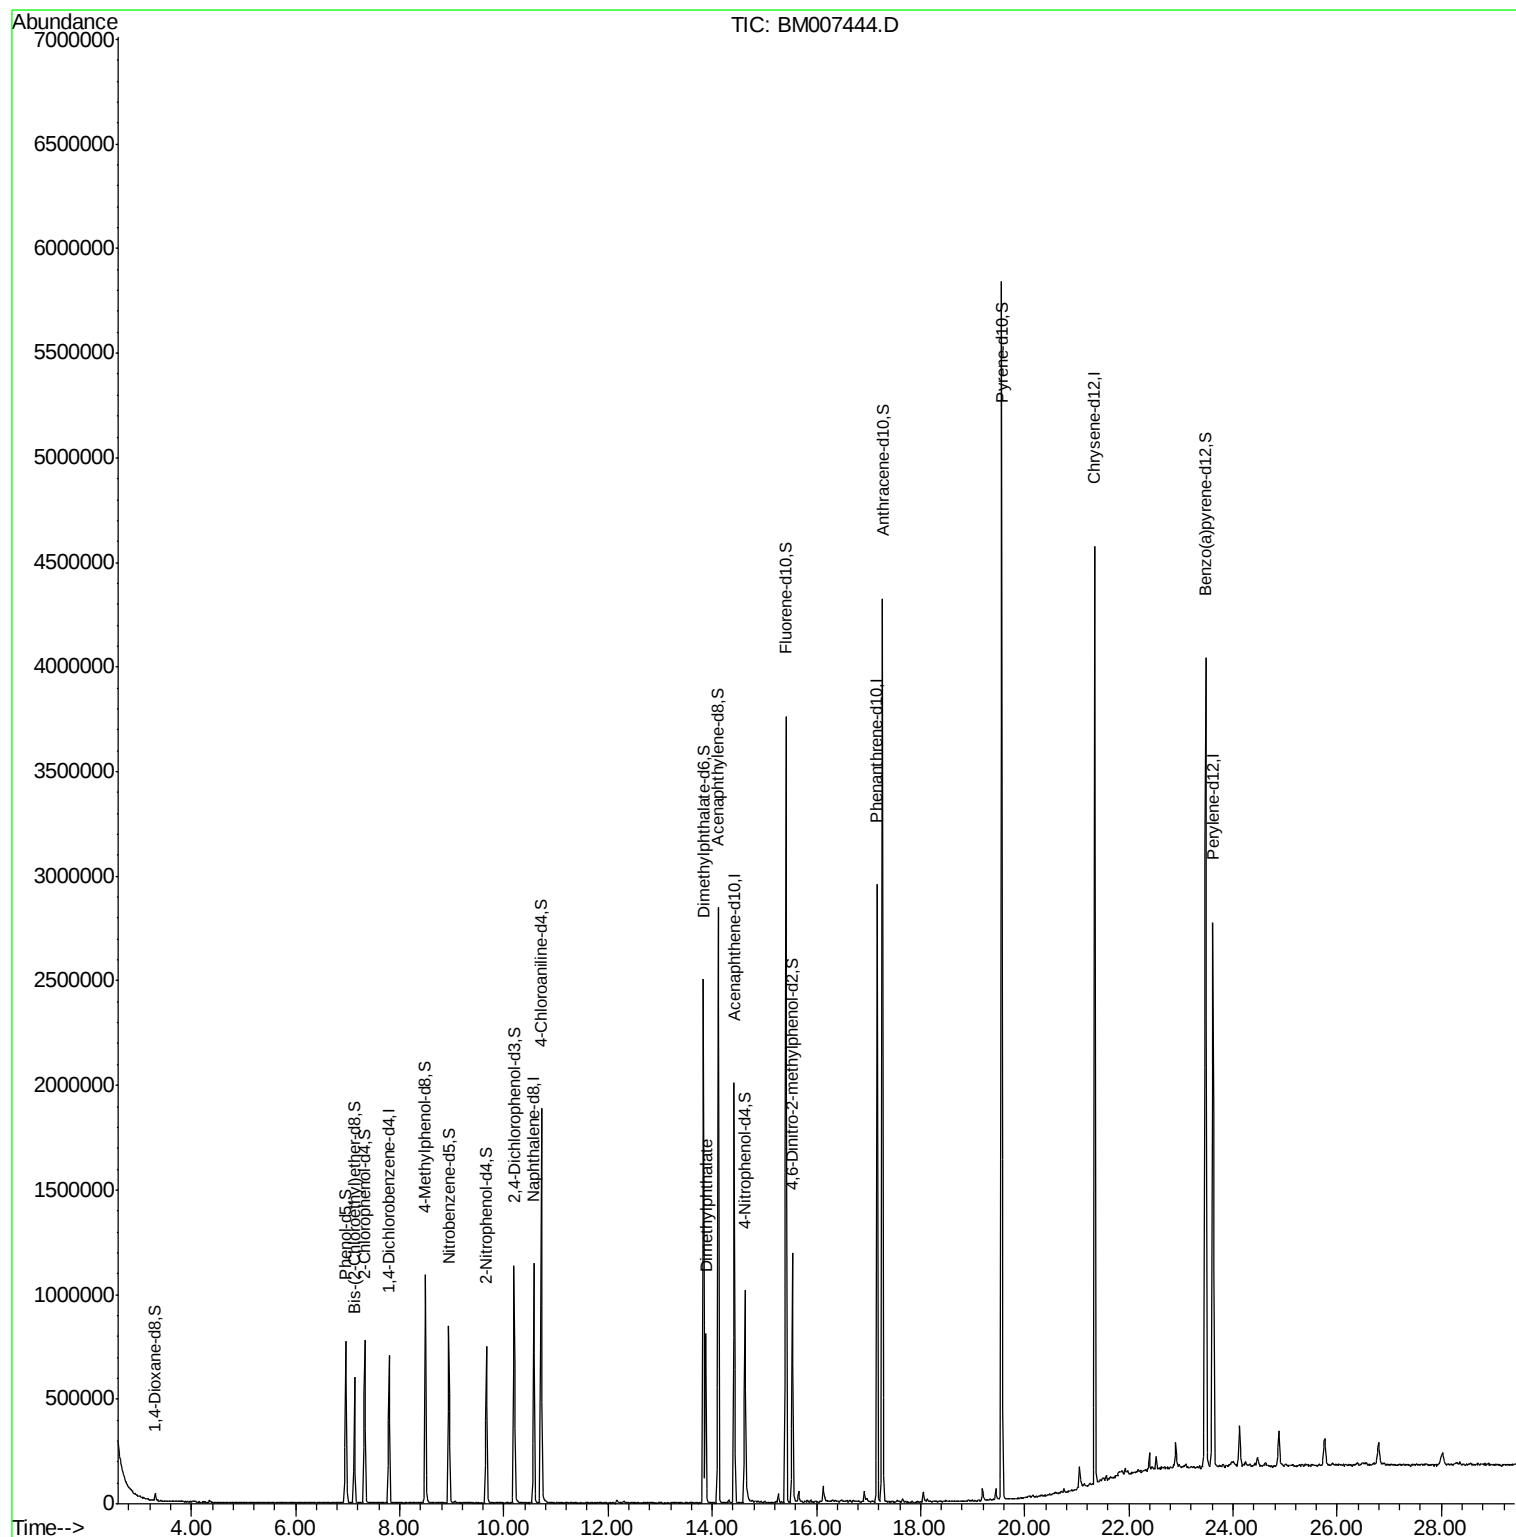

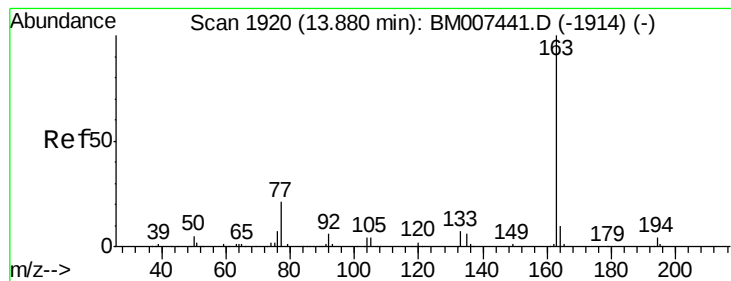

#44
 Dimethylphthalate
 Concen: 8.75 ng/ul
 RT: 13.88 min Scan# 1920
 Delta R.T. 0.00 min
 Lab File: BM007444.D
 Acq: 07 Sep 2016 18:17

Instrument :
 BNA_M
 ClientSampleId :
 BD3A6

Tgt Ion:	163	Resp:	494979
Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.2
164	10.3	7.8	11.8

